
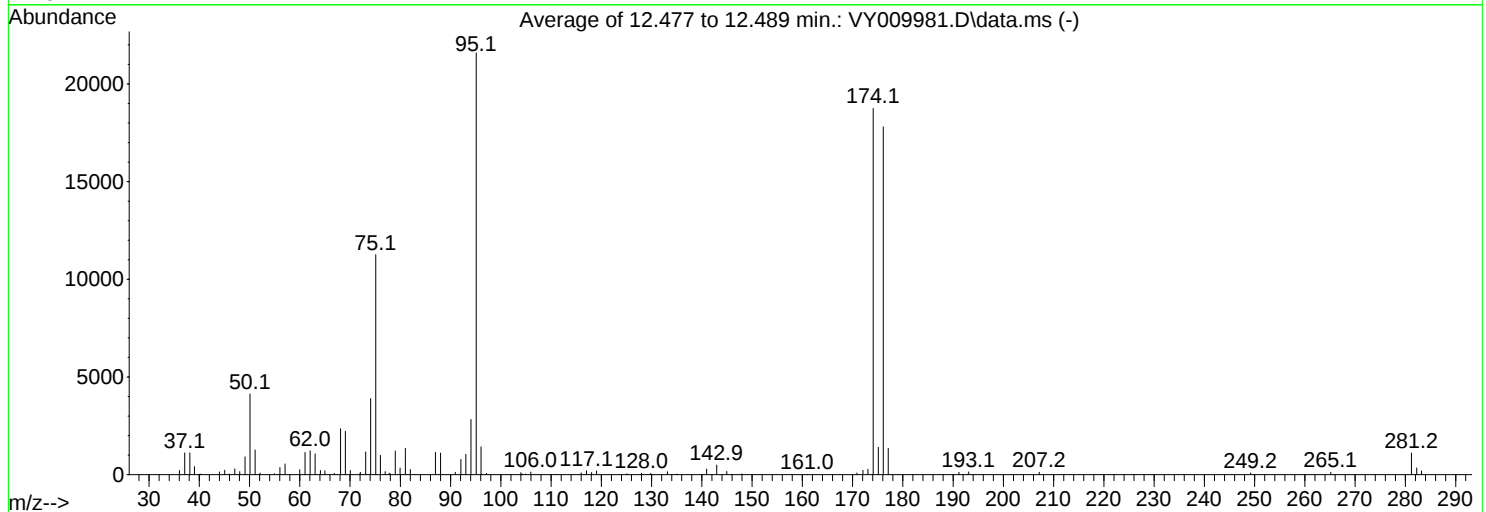


Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY081222\
Data File : VY009981.D
Acq On : 12 Aug 2022 09:06
Operator : KP/MD
Sample : BFB
Misc : 5.00g/5.0mL/MSVOA_Y/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_Y
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y081222S.M
Title : SW846 8260
Last Update : Sat Aug 13 02:54:57 2022

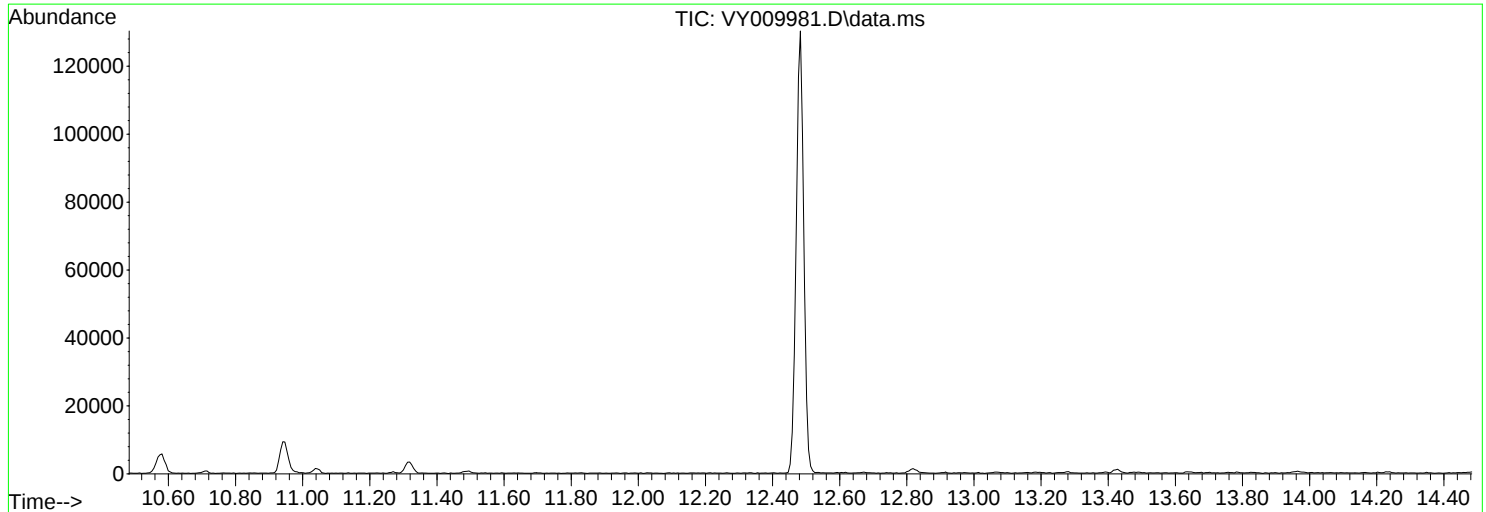

AutoFind: Scans 1748, 1749, 1750; Background Corrected with Scan 1740

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	19.1	4129	PASS
75	95	30	60	52.2	11263	PASS
95	95	100	100	100.0	21592	PASS
96	95	5	9	6.6	1427	PASS
173	174	0.00	2	1.5	277	PASS
174	95	50	100	86.8	18749	PASS
175	174	5	9	7.5	1397	PASS
176	174	95	101	95.0	17808	PASS
177	176	5	9	7.6	1346	PASS