



Dichlorodifluoromethane

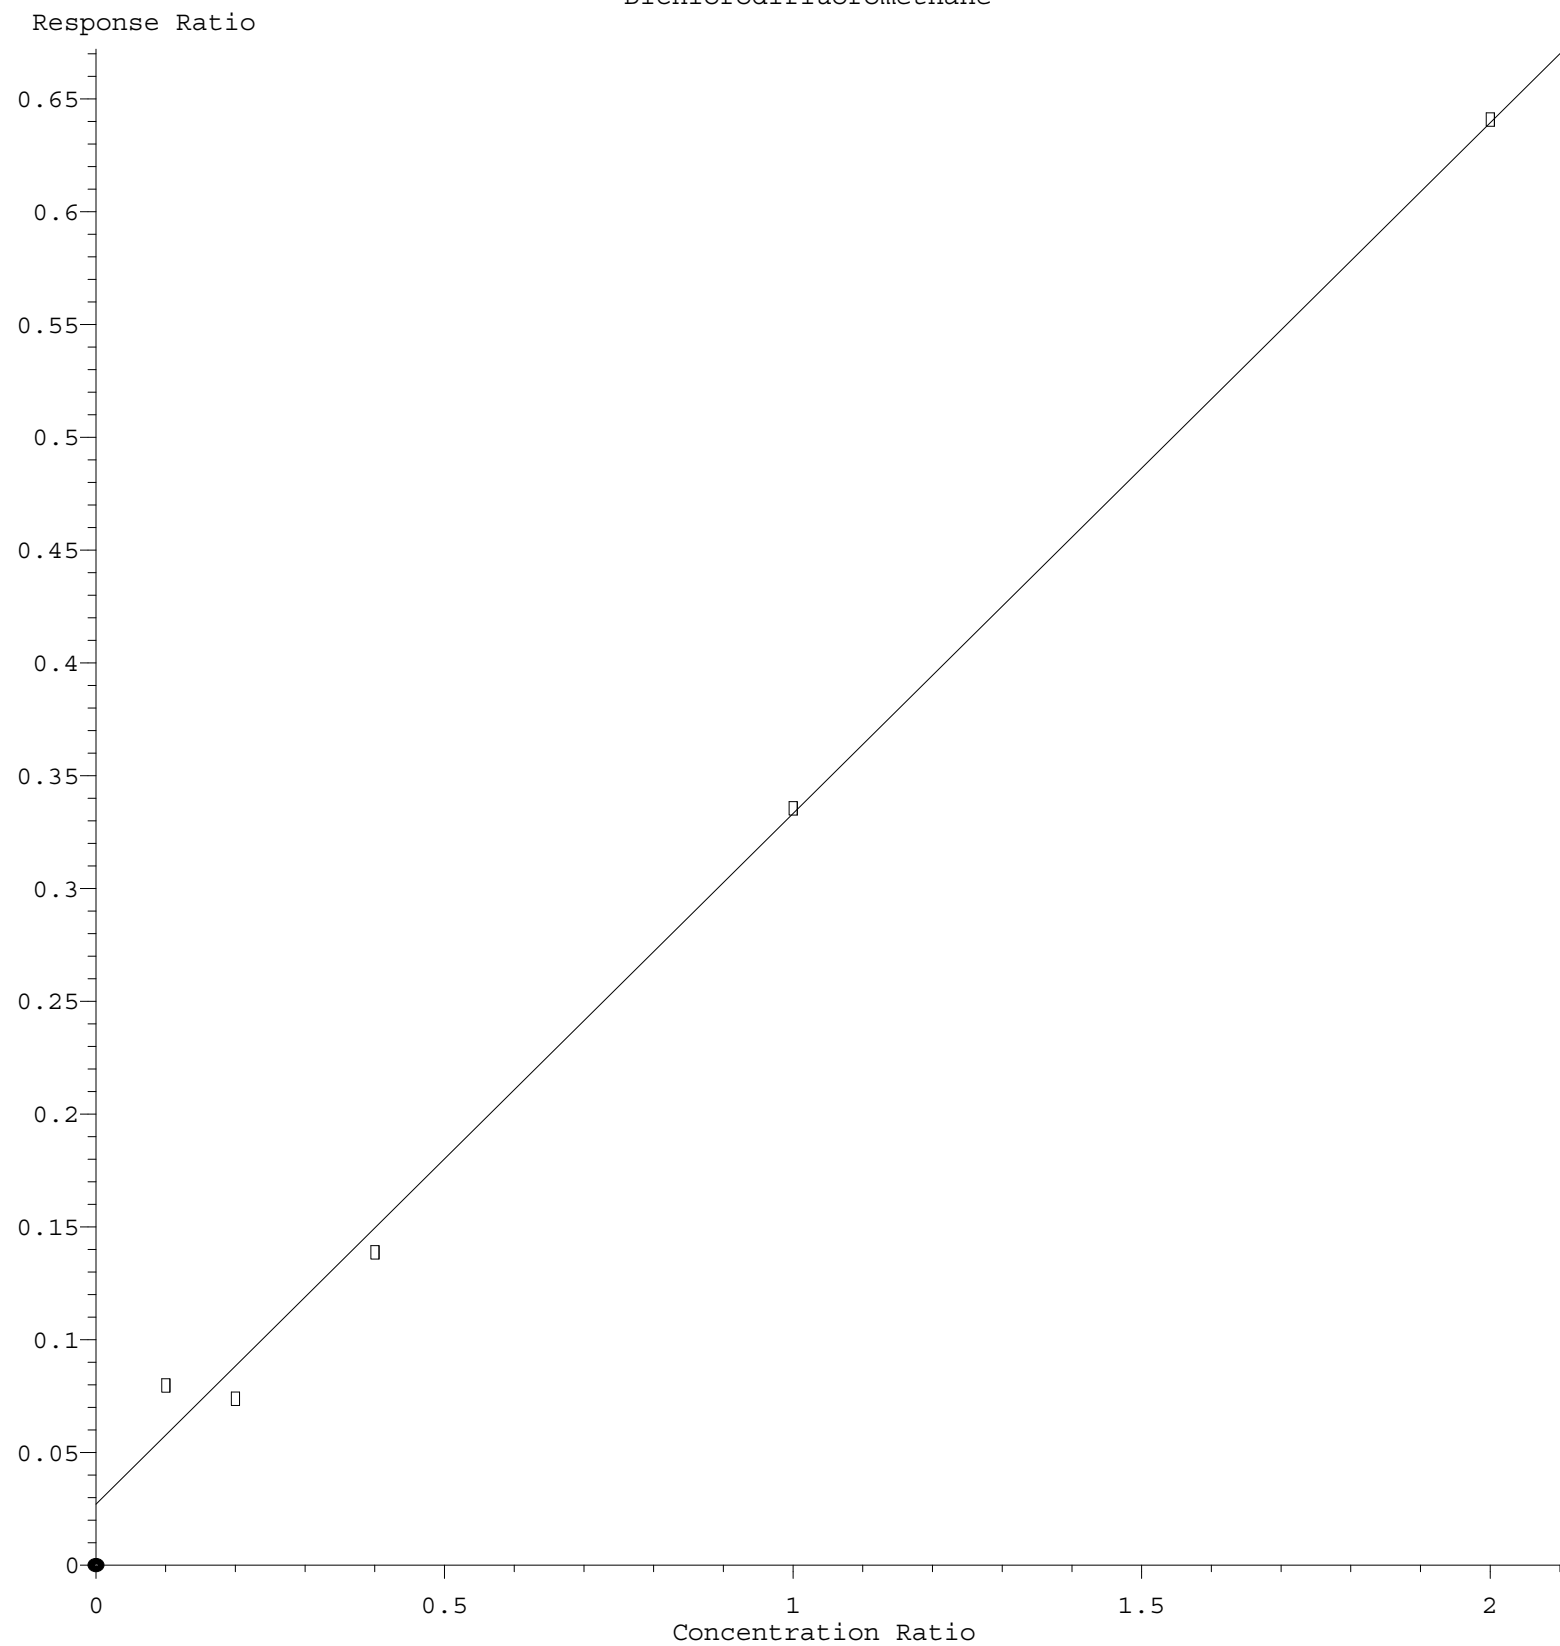


Response = 3.061e-001 * Amt + 2.713e-002
 Coef of Det (r^2) = 0.996476 Curve Fit: Linear
 Method Name: Z:\voasrv\HPCHEM1\MSVOA Y\methods\82Y082422S.M
 Calibration Table Last Updated: Fri Aug 26 06:12:05 2022

Trichlorofluoromethane

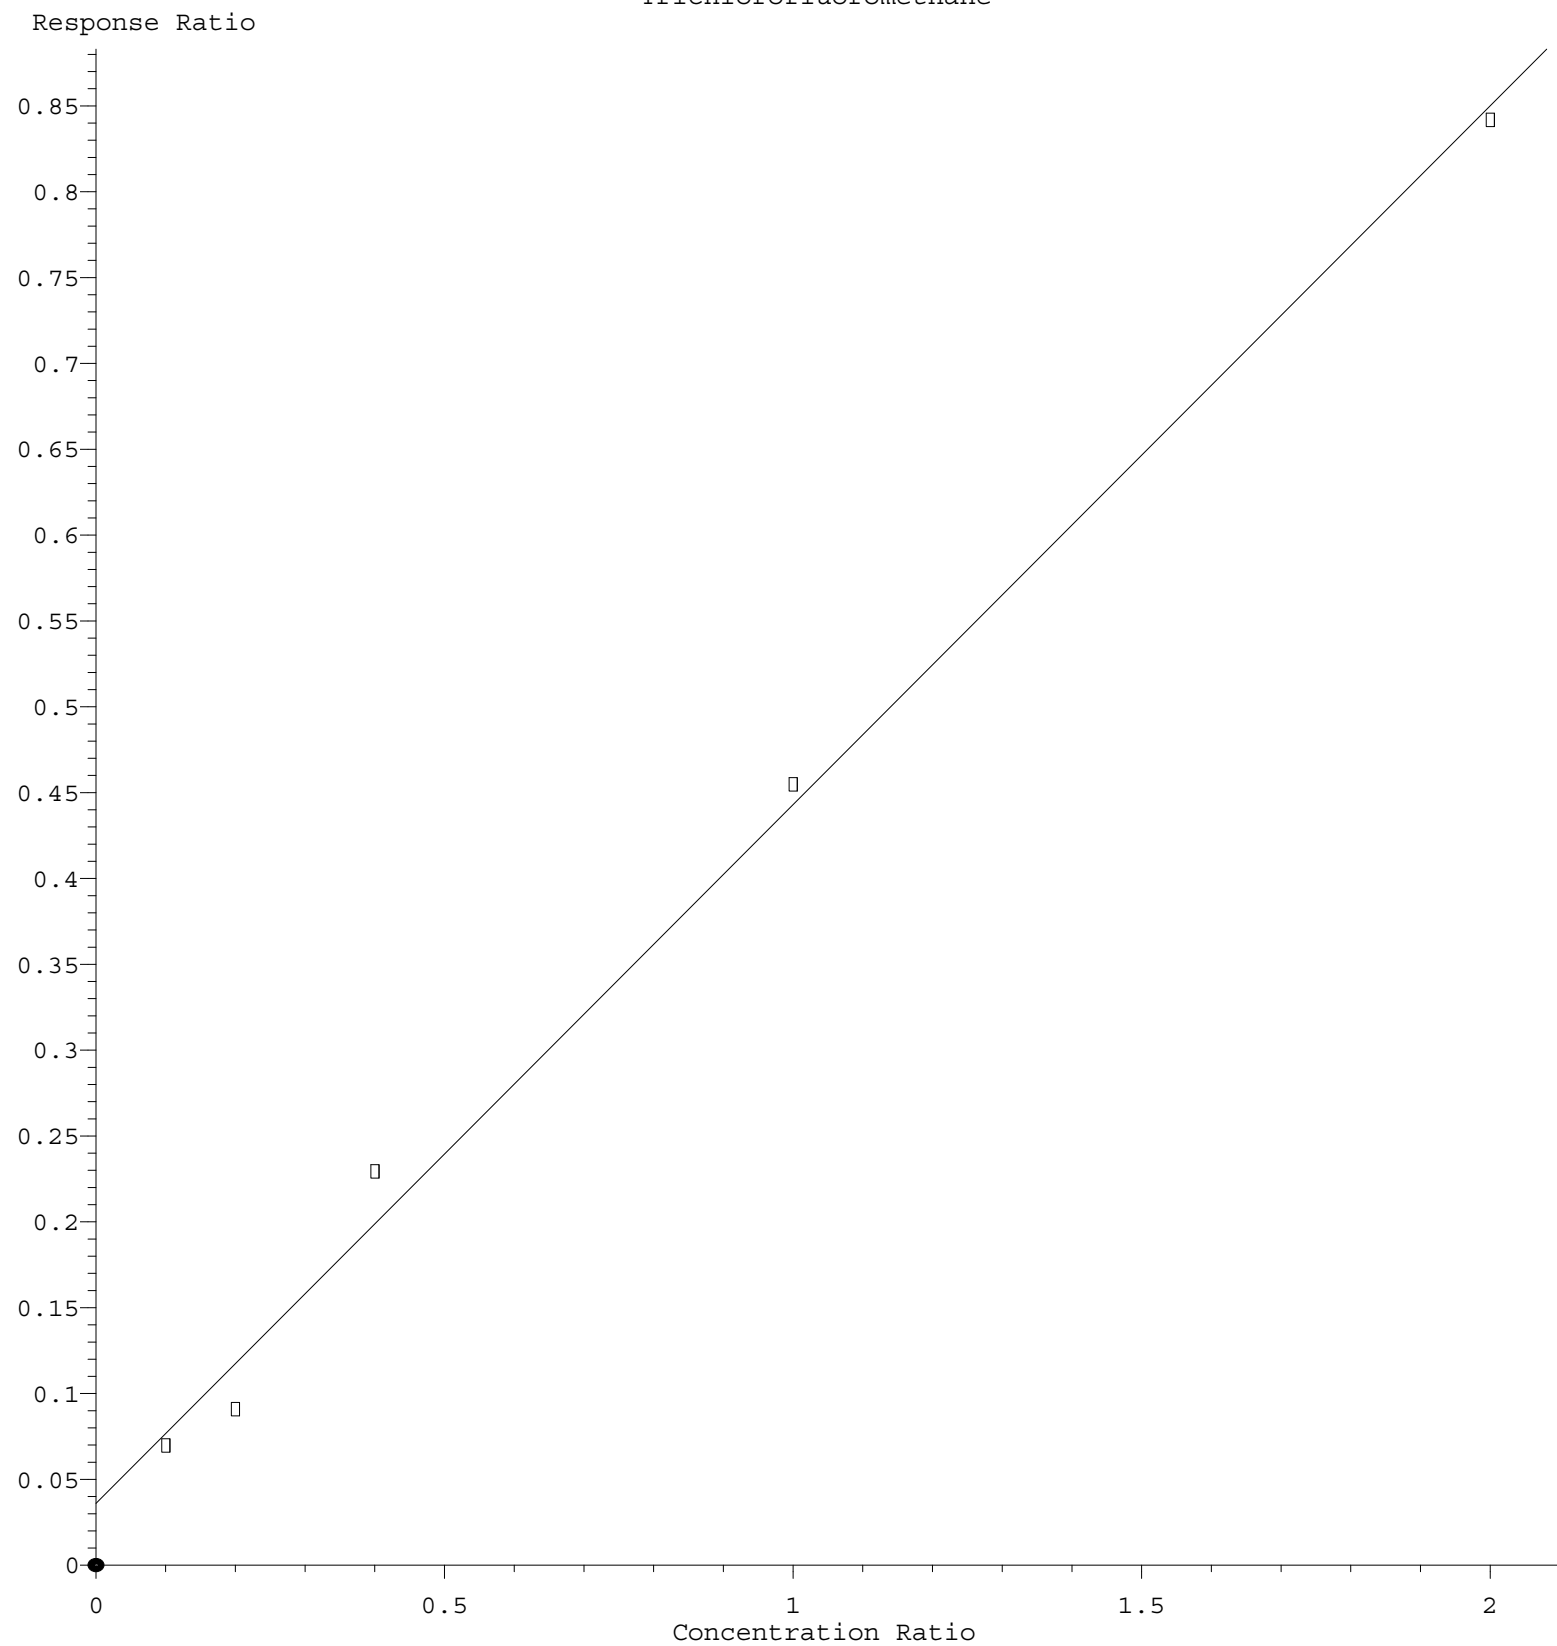


$\text{Response} = 4.074\text{e-}001 * \text{Amt} + 3.579\text{e-}002$
 Coef of Det (r^2) = 0.995421 Curve Fit: Linear
 Method Name: Z:\voasrv\HPCHEM1\MSVOA Y\methods\82Y082422S.M
 Calibration Table Last Updated: Fri Aug 26 06:12:05 2022

Tert butyl alcohol

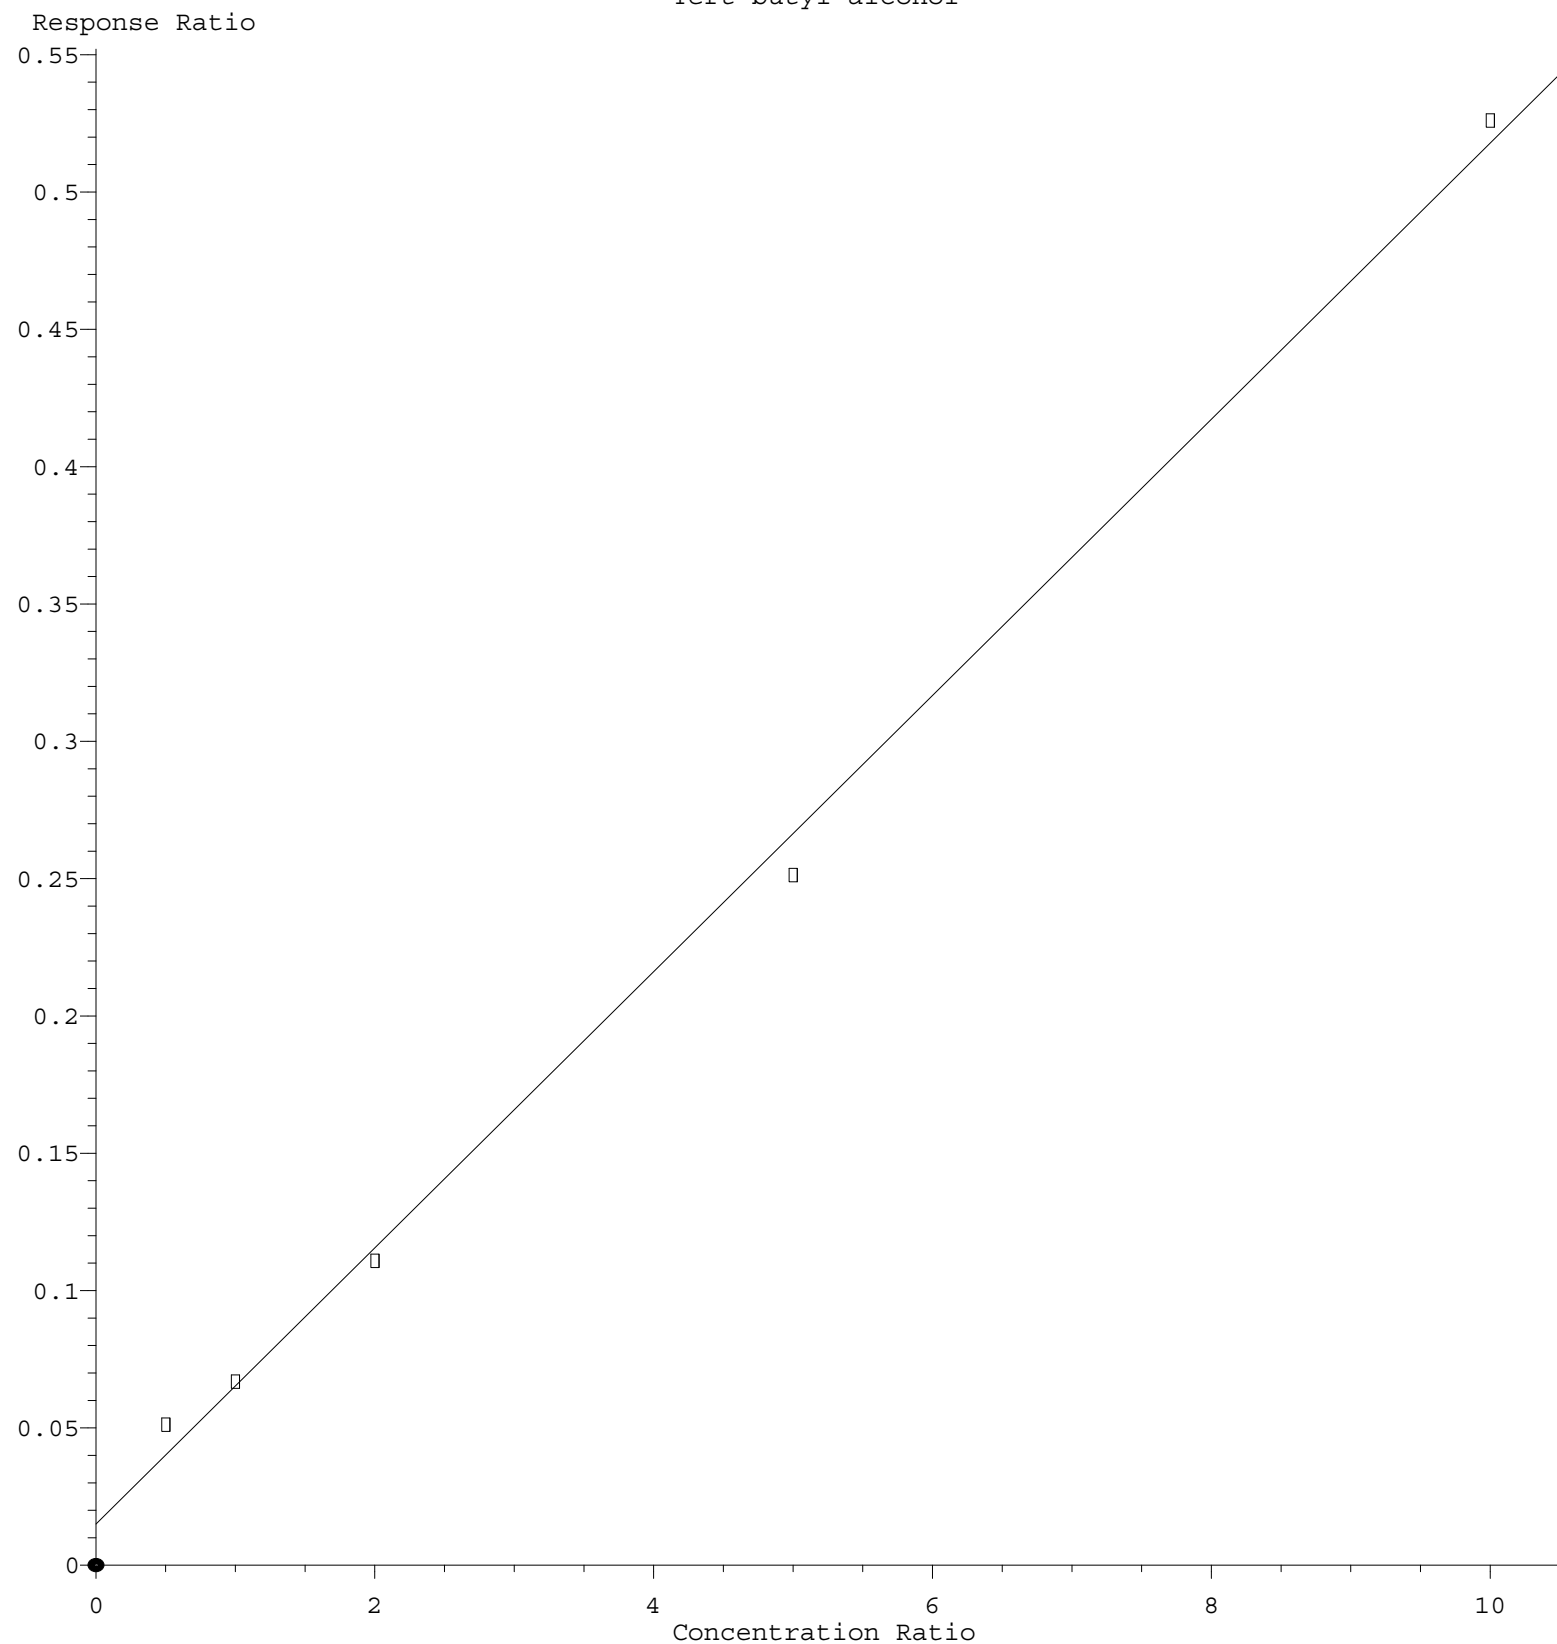

Response = 5.029e-002 * Amt + 1.515e-002
 Coef of Det (r^2) = 0.997174 Curve Fit: Linear
 Method Name: Z:\voasrv\HPCHEM1\MSVOA Y\methods\82Y082422S.M
 Calibration Table Last Updated: Fri Aug 26 06:12:05 2022


Methyl Acetate

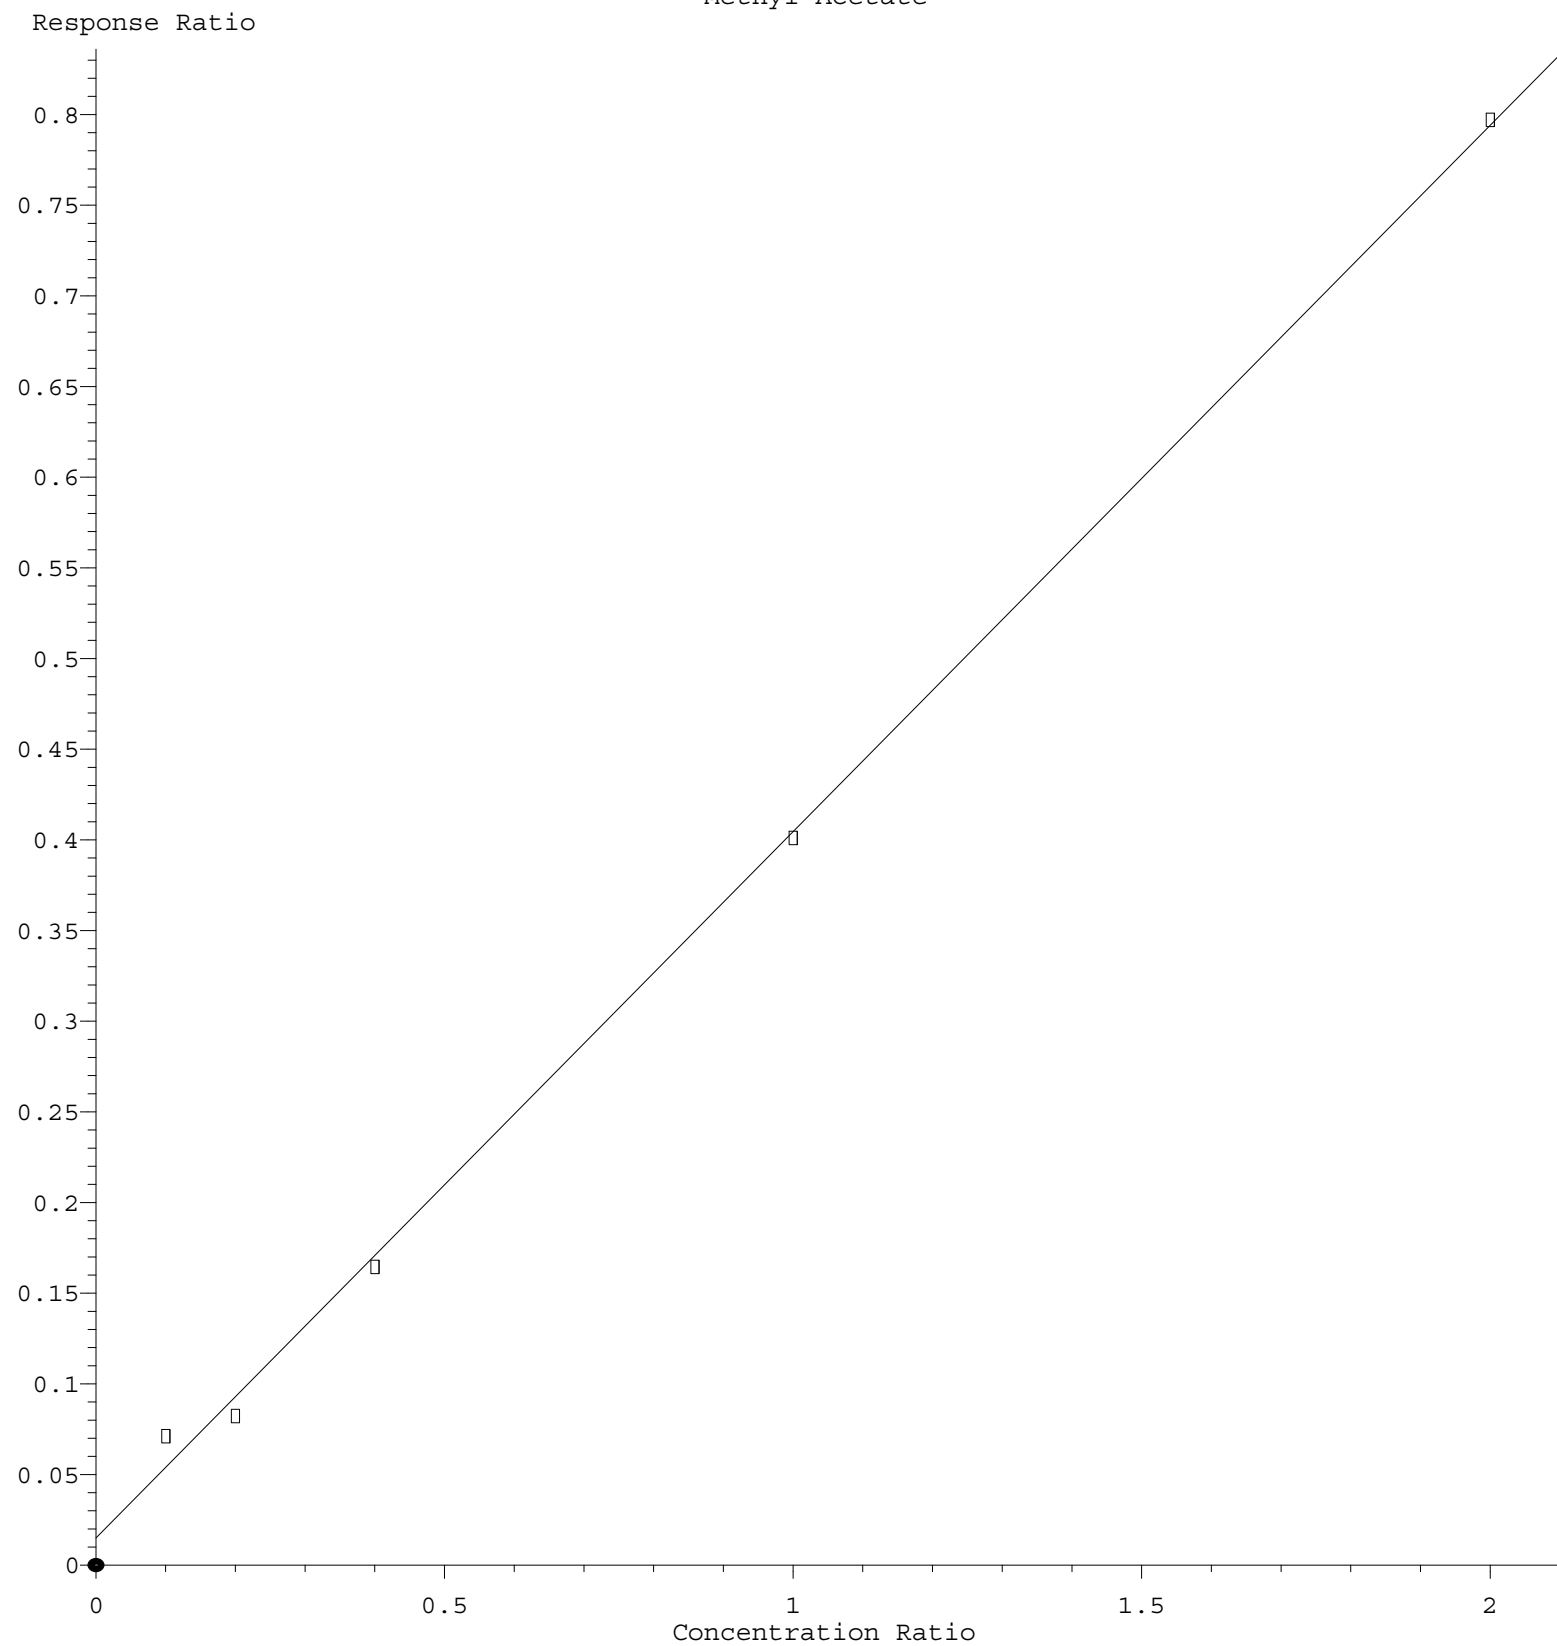

Response = $3.894 \times 10^{-1} \times \text{Amt} + 1.497 \times 10^{-2}$
Coef of Det (r^2) = 0.998751 Curve Fit: Linear
Method Name: Z:\voasrv\HPCHEM1\MSVOA Y\methods\82Y082422S.M
Calibration Table Last Updated: Fri Aug 26 06:12:05 2022

Methylene Chloride

Response Ratio

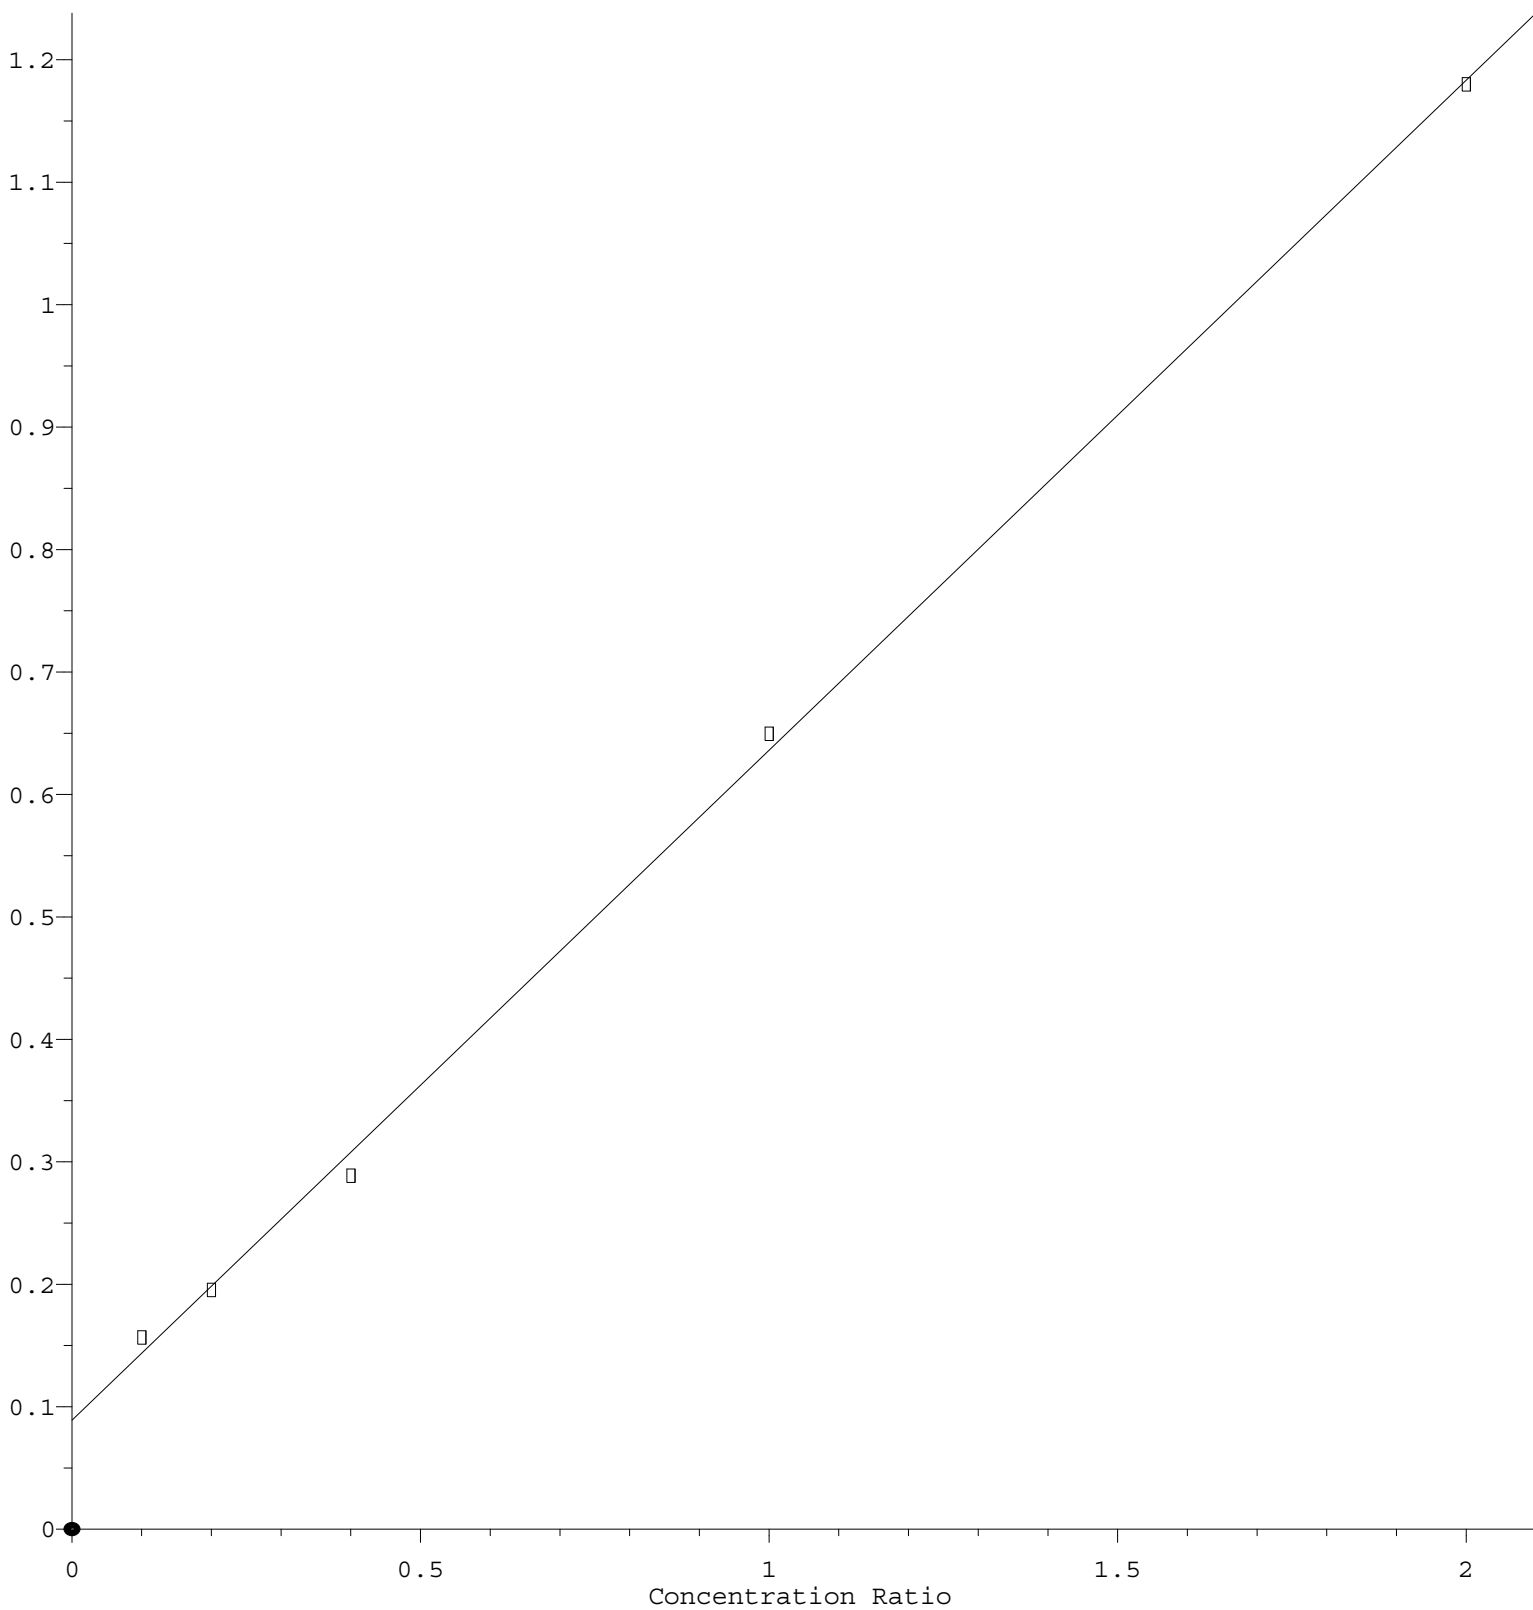


$$\text{Response} = 5.468\text{e-}001 * \text{Amt} + 8.932\text{e-}002$$

Coef of Det (r^2) = 0.999008 Curve Fit: Linear

Method Name: Z:\voasrv\HPCHEM1\MSVOA Y\methods\82Y082422S.M


Calibration Table Last Updated: Fri Aug 26 06:12:05 2022

1,2-Dichloroethane-d4

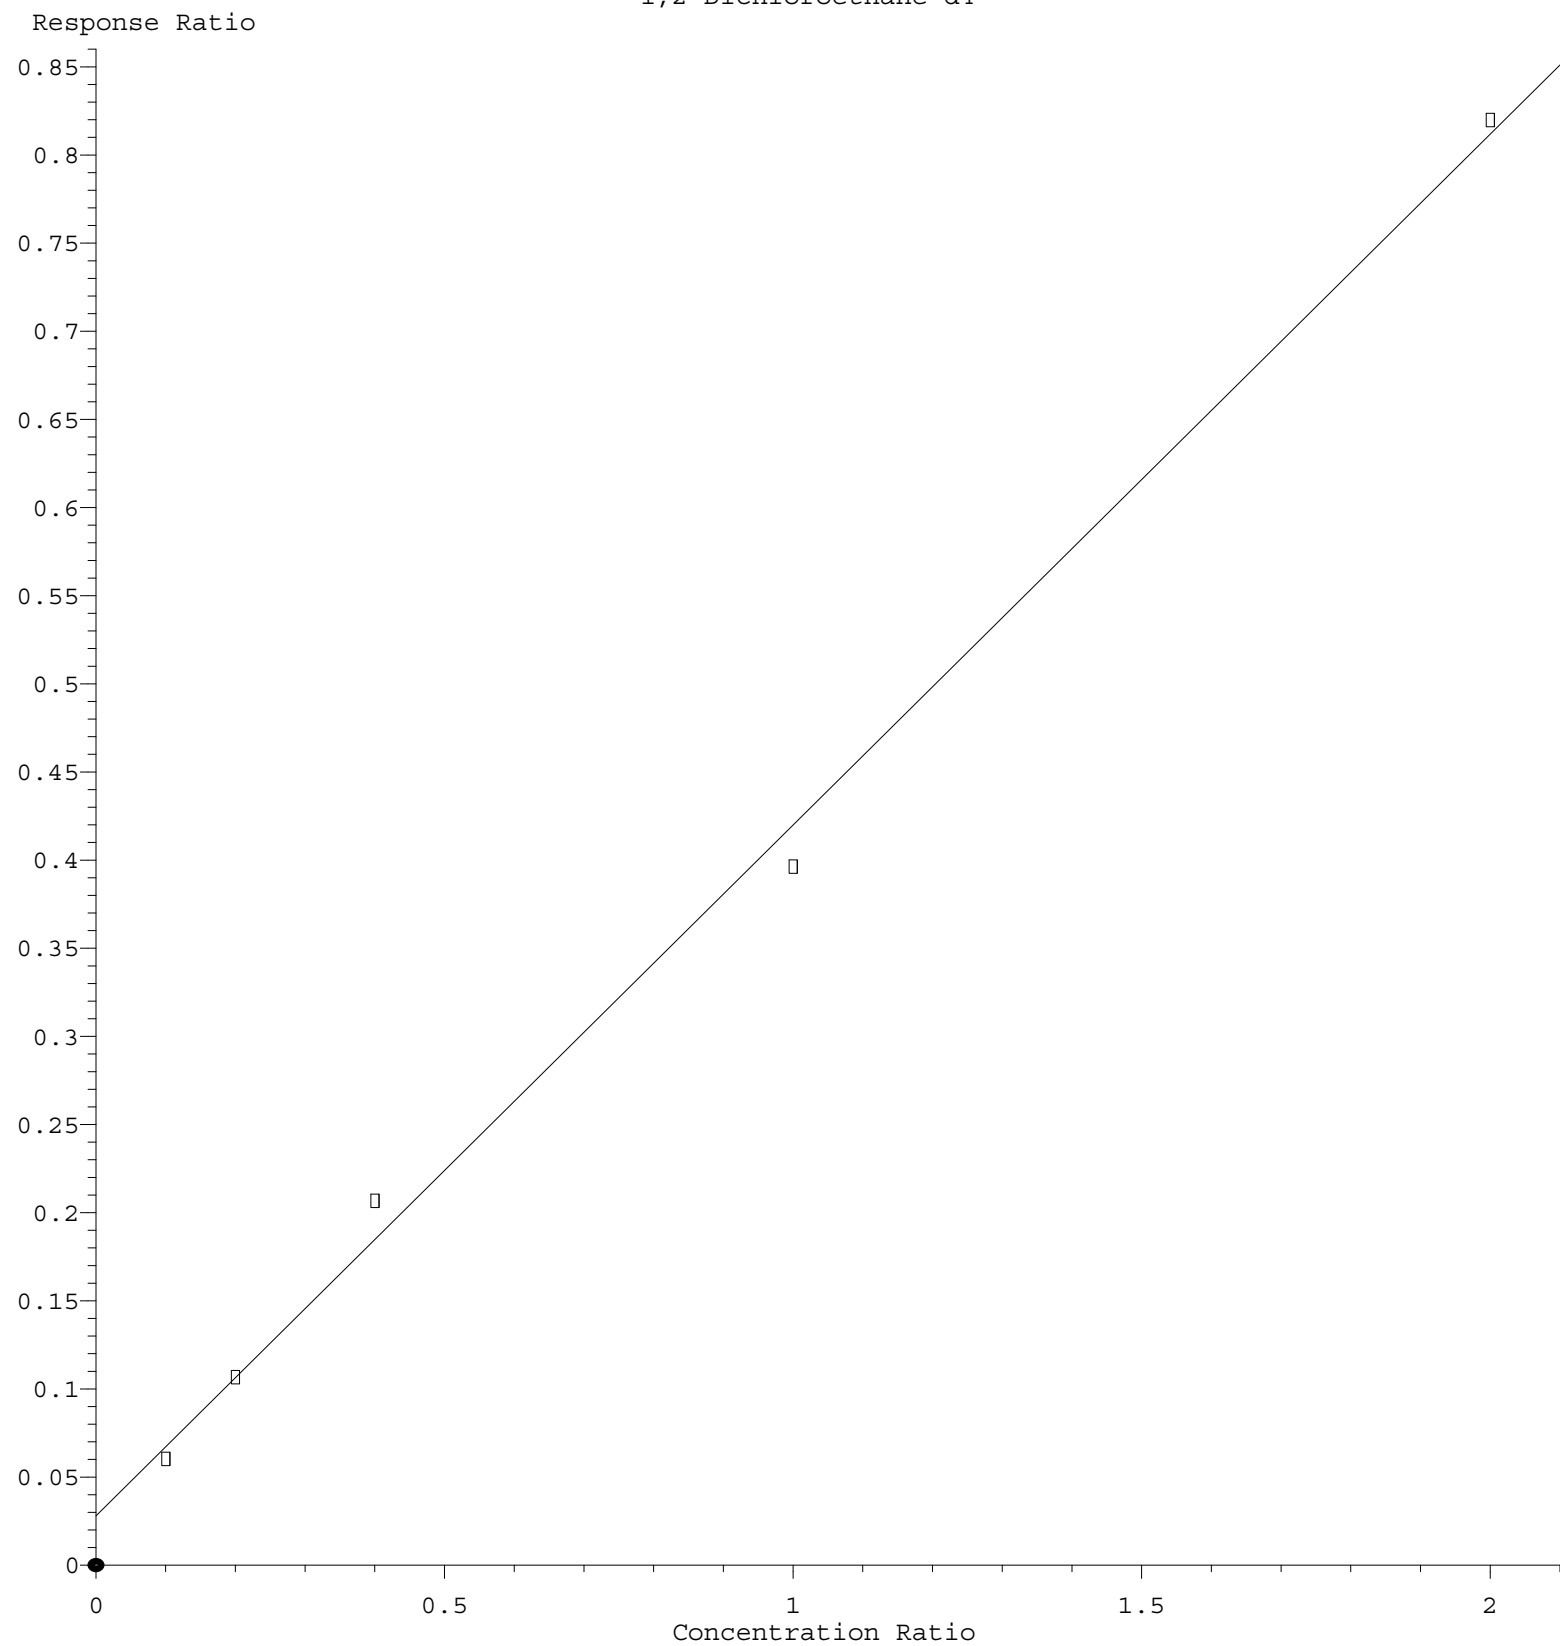

Response = 3.922e-001 * Amt + 2.771e-002
 Coef of Det (r^2) = 0.996986 Curve Fit: Linear
 Method Name: Z:\voasrv\HPCHEM1\MSVOA Y\methods\82Y082422S.M
 Calibration Table Last Updated: Fri Aug 26 06:12:05 2022


1,2-Dibromo-3-Chloropropane

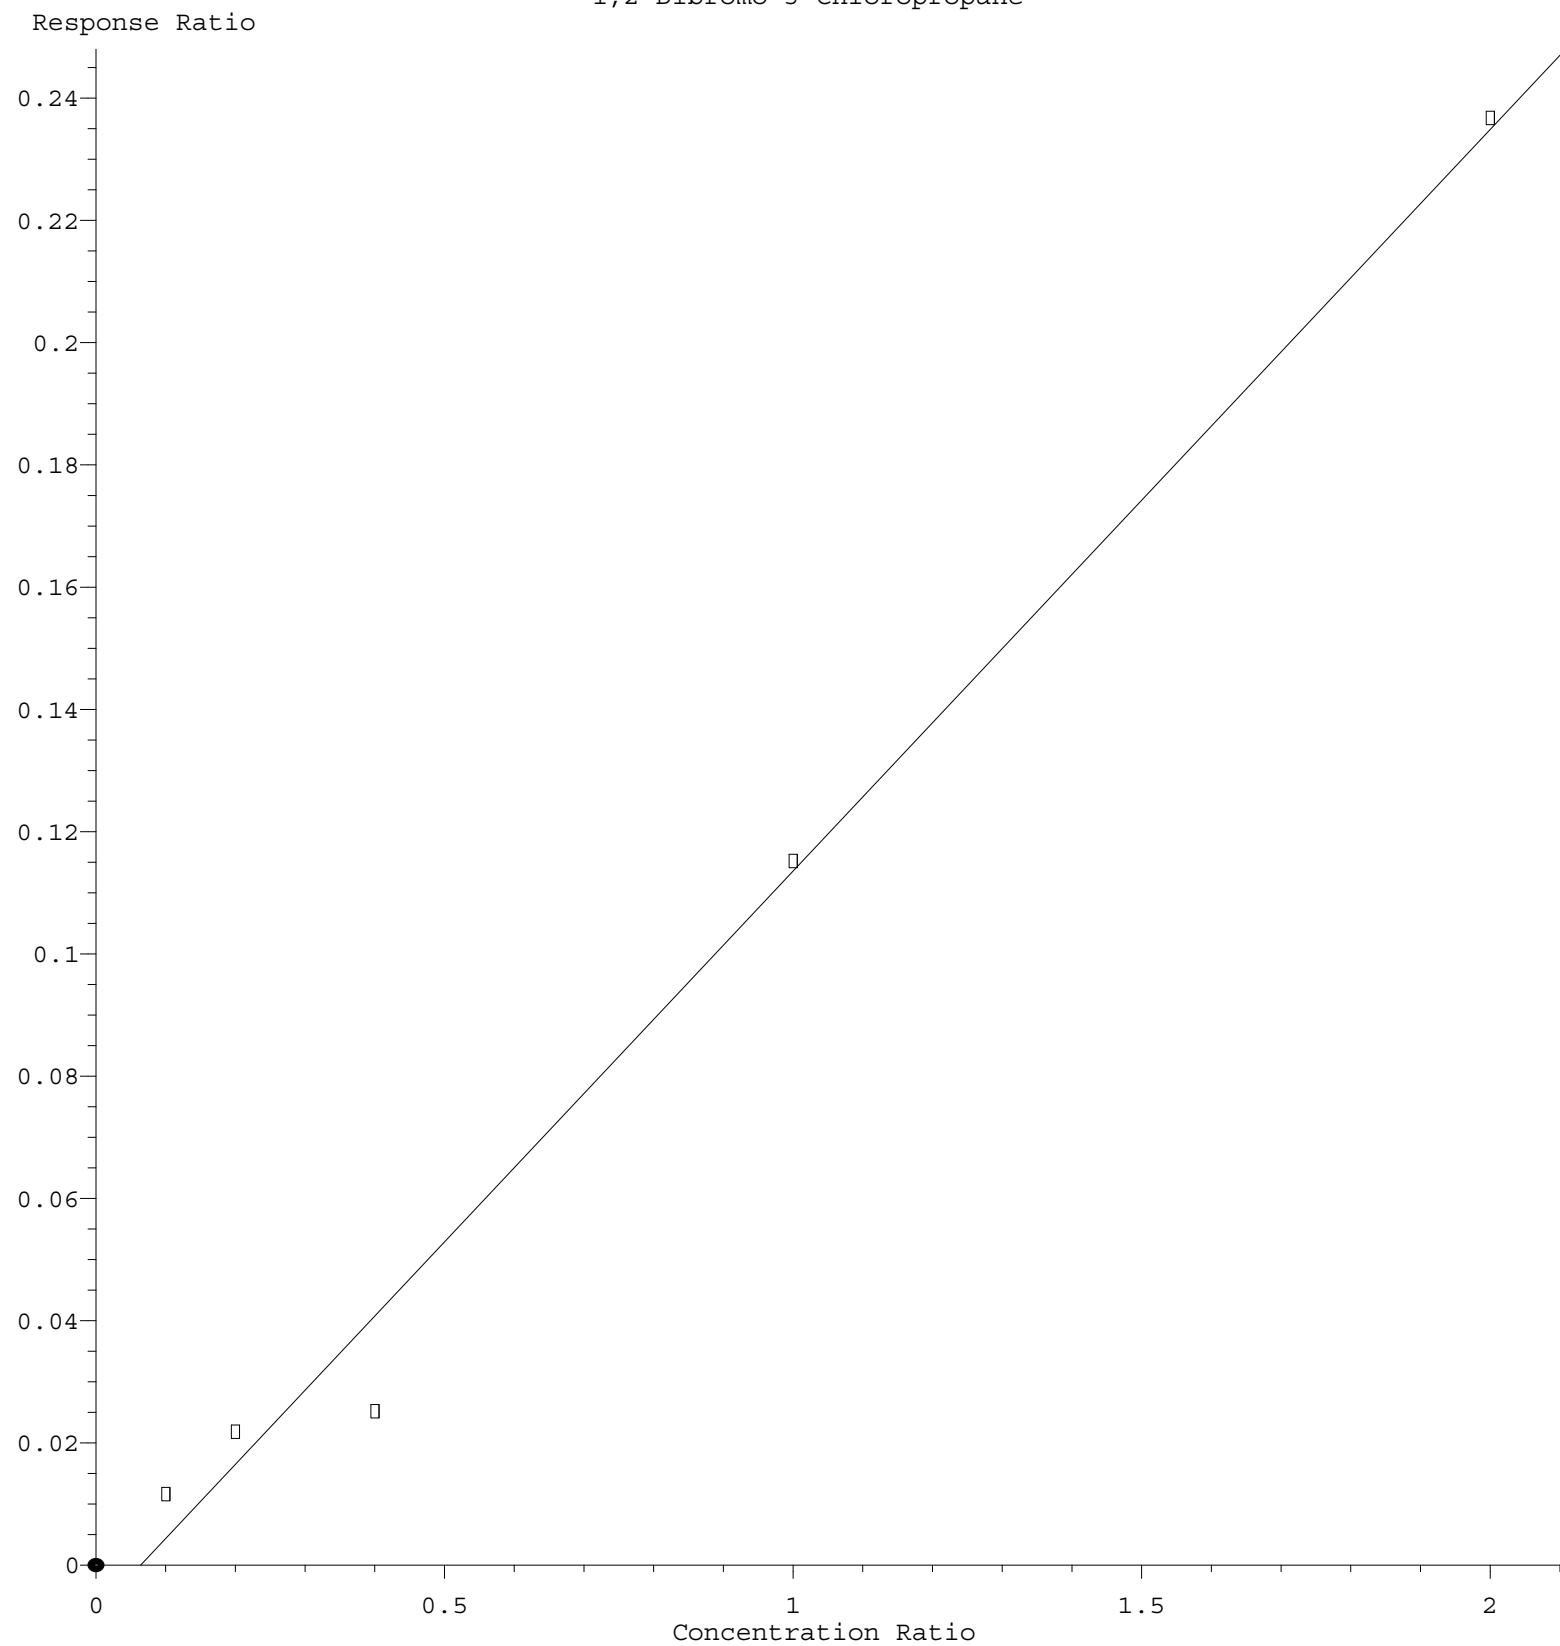

$\text{Response} = 1.215\text{e-}001 * \text{Amt} - 7.832\text{e-}003$
 Coef of Det (r^2) = 0.991048 Curve Fit: Linear
 Method Name: Z:\voasrv\HPCHEM1\MSVOA Y\methods\82Y082422S.M
 Calibration Table Last Updated: Fri Aug 26 06:12:05 2022

1,2,4-Trichlorobenzene

Response Ratio

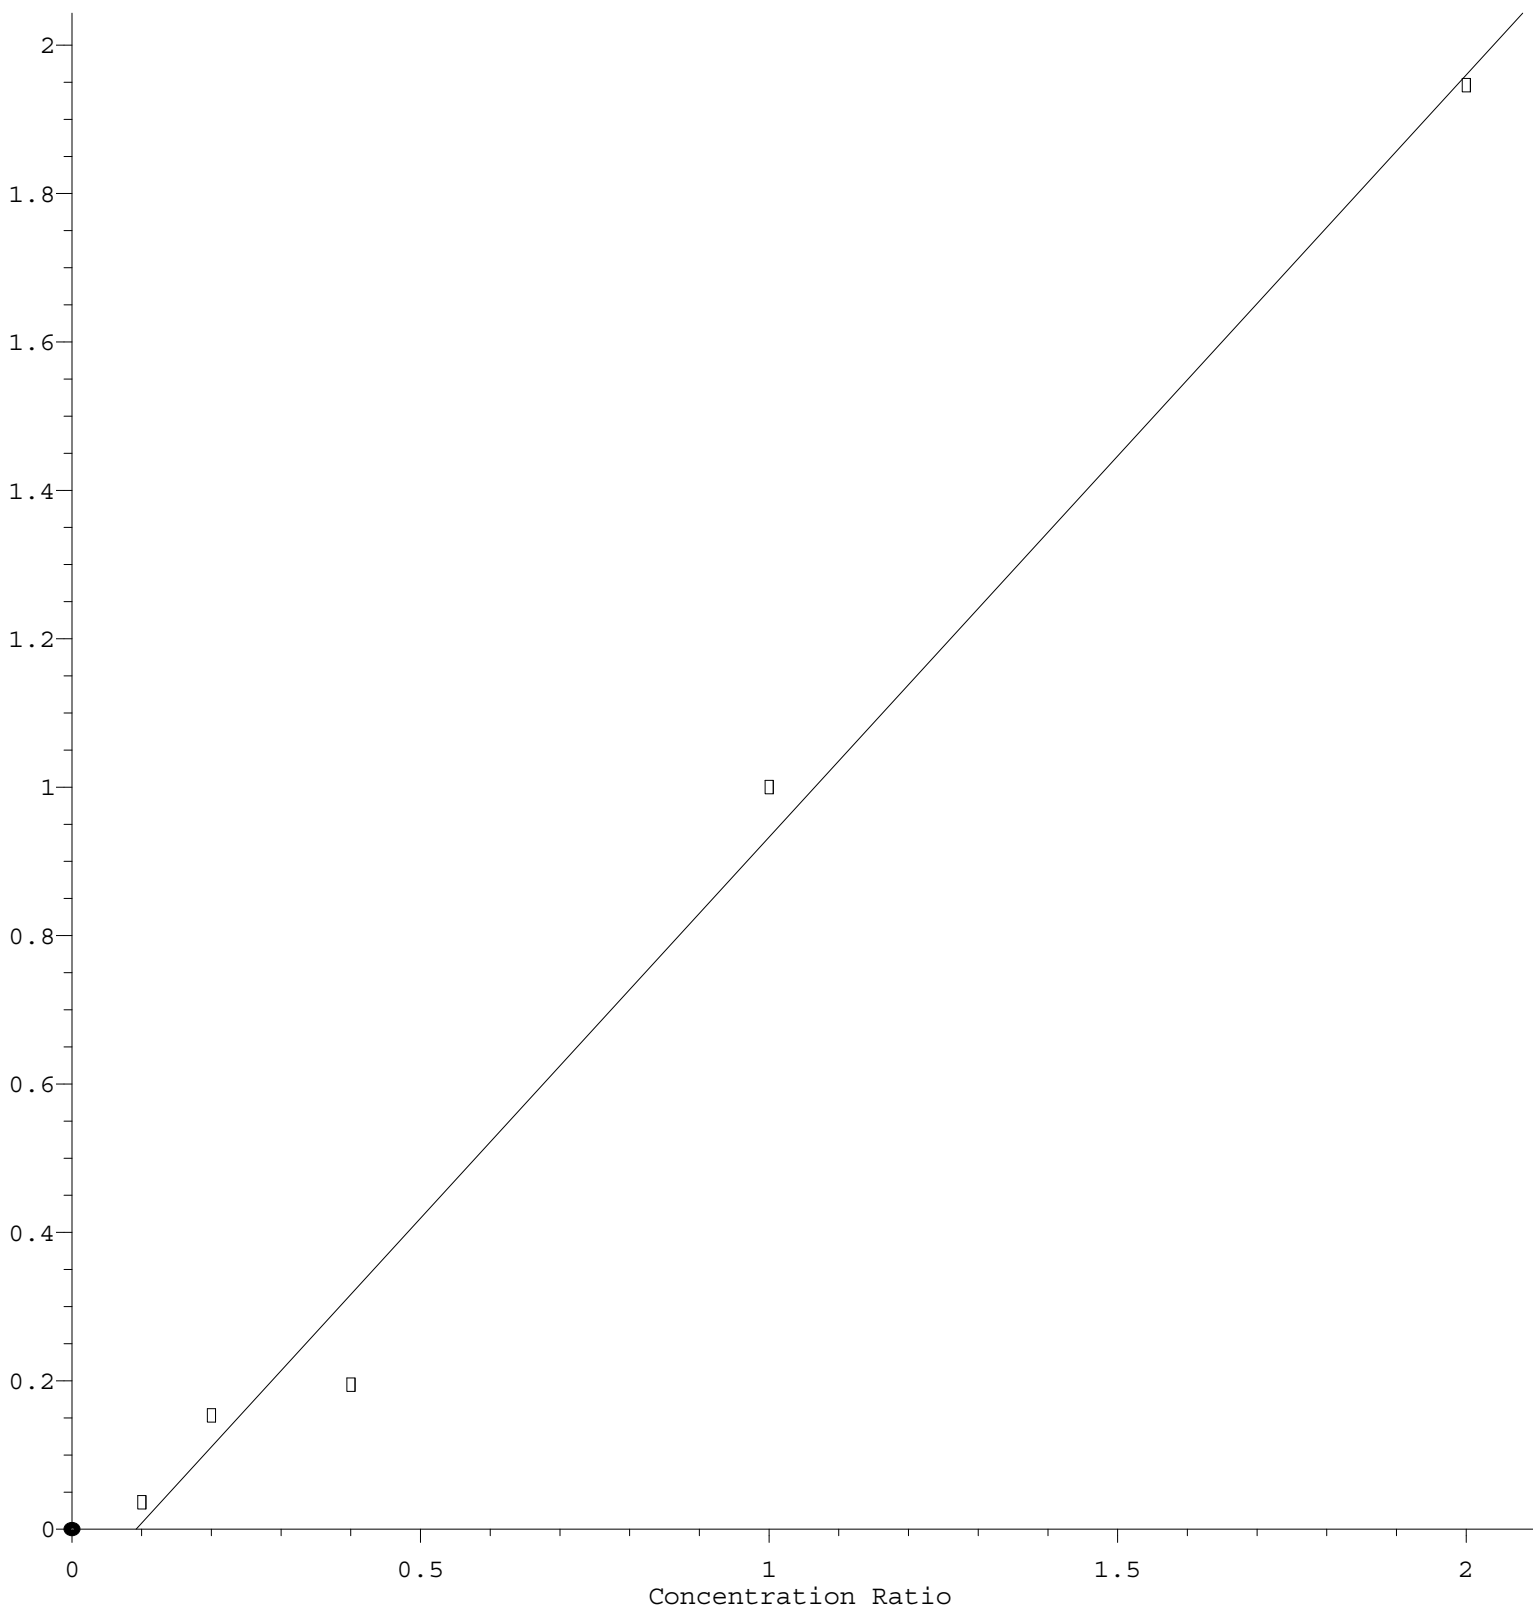

$$\text{Response} = 1.027\text{e}+000 * \text{Amt} - 9.416\text{e}-002$$


Coef of Det (r^2) = 0.991605 Curve Fit: Linear

Method Name: Z:\voasrv\HPCHEM1\MSVOA Y\methods\82Y082422S.M

Calibration Table Last Updated: Fri Aug 26 06:12:05 2022

Naphthalene


Response Ratio

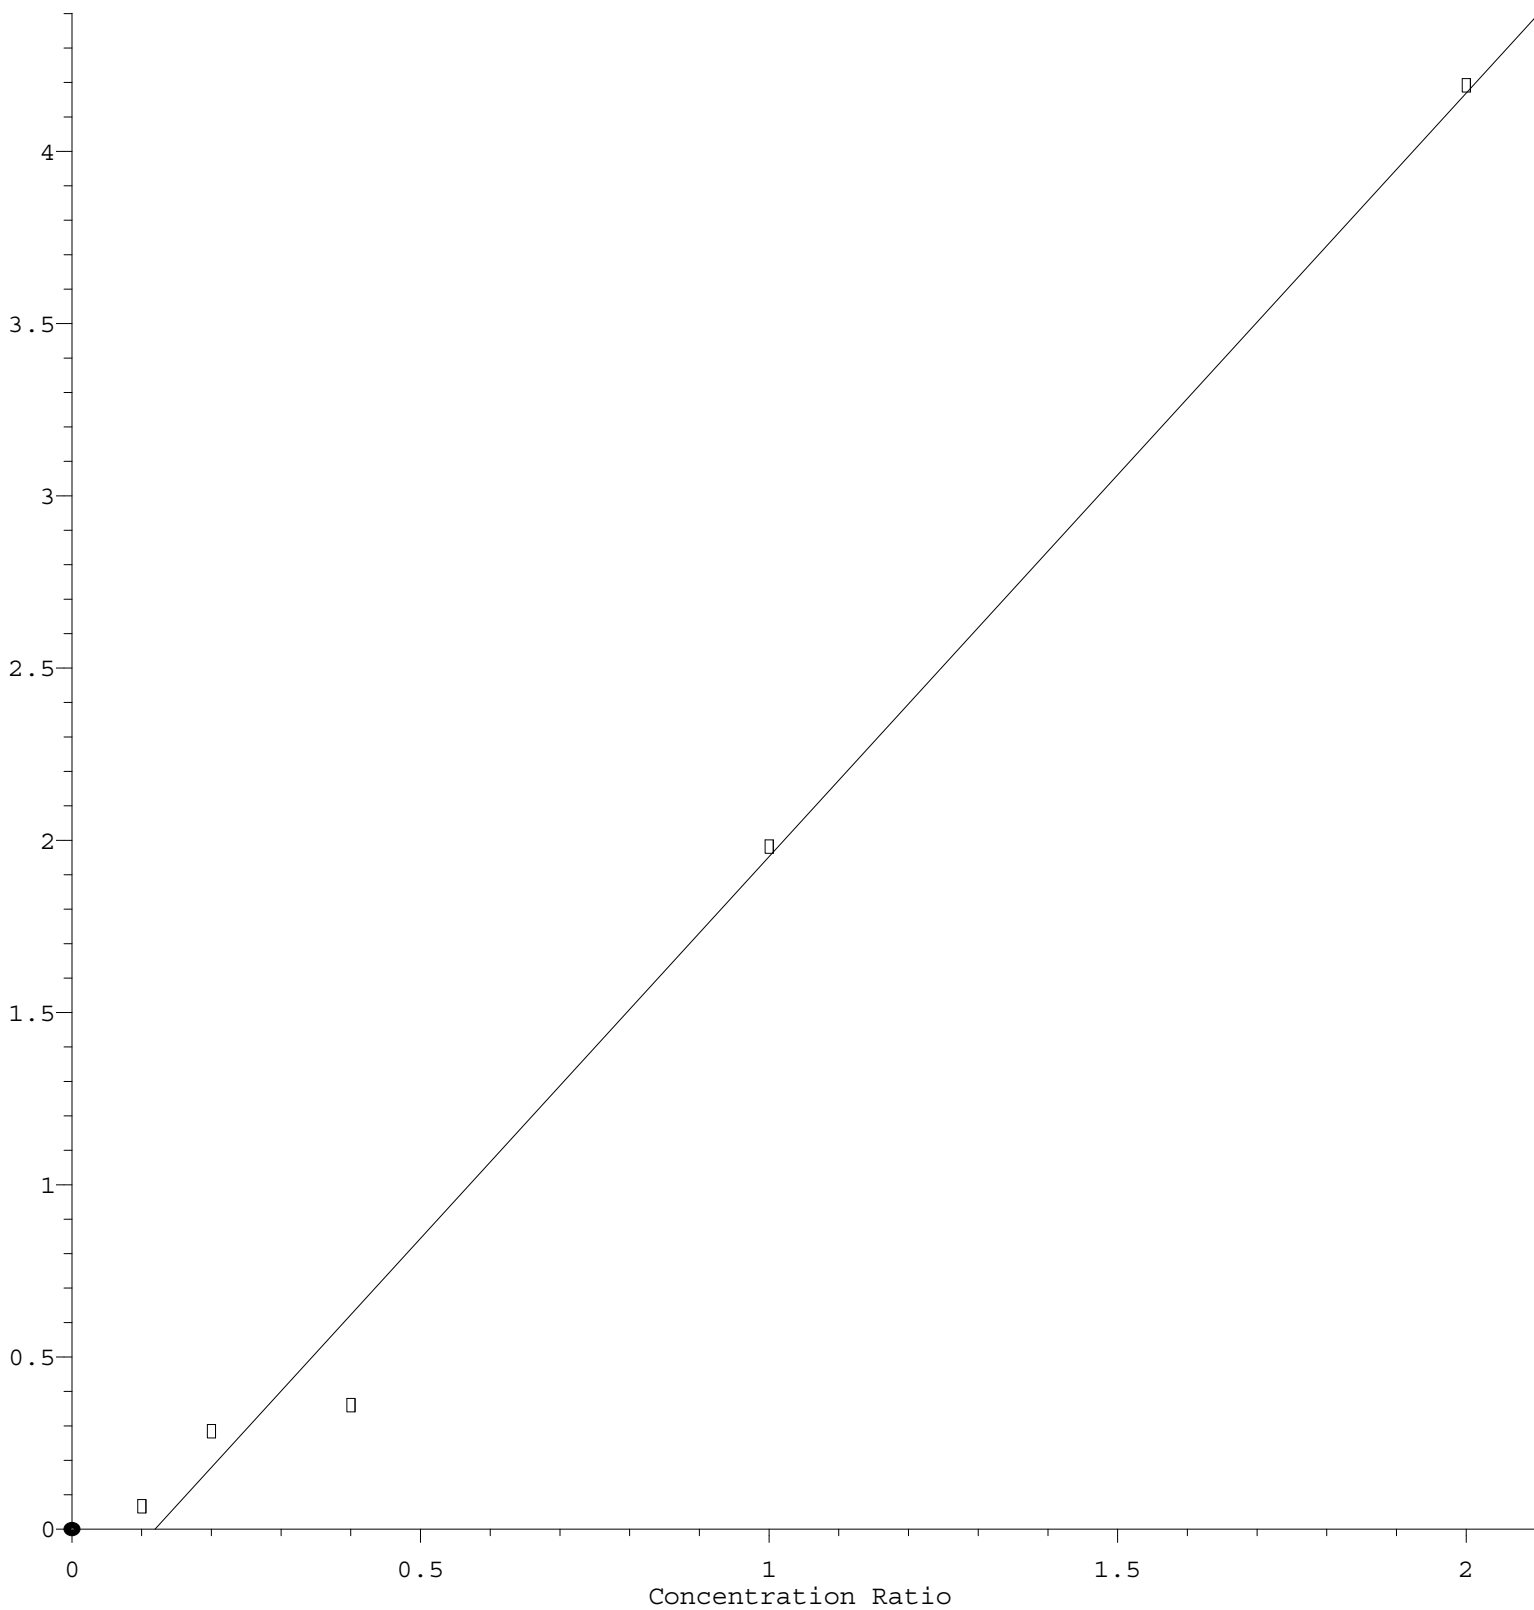

Response = 2.216e+000 * Amt - 2.631e-001
 Coef of Det (r^2) = 0.992388 Curve Fit: Linear
 Method Name: Z:\voasrv\HPCHEM1\MSVOA Y\methods\82Y082422S.M
 Calibration Table Last Updated: Fri Aug 26 06:12:05 2022

1,2,3-Trichlorobenzene

Response Ratio

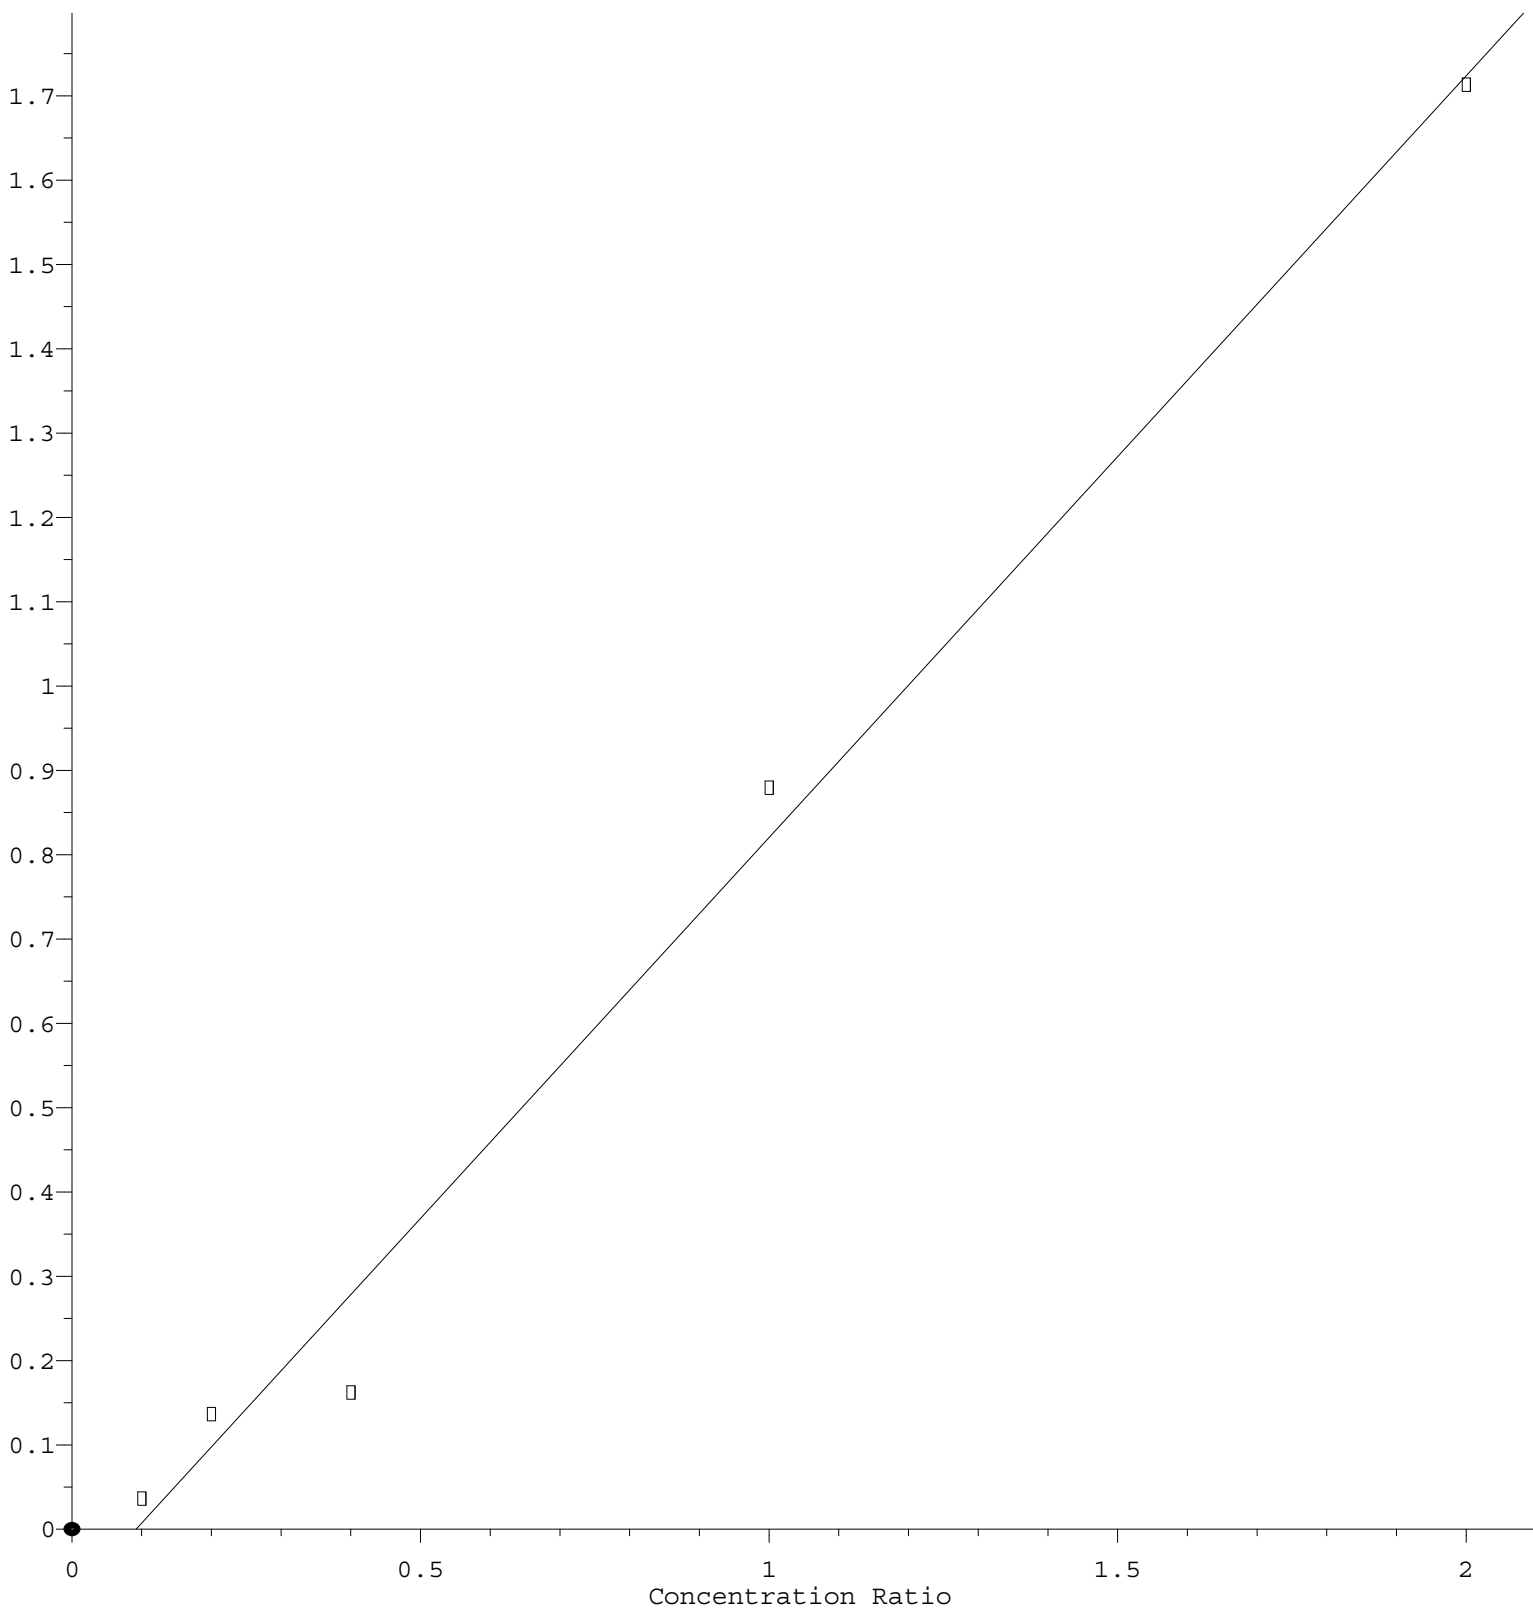

$$\text{Response} = 9.042\text{e-}001 * \text{Amt} - 8.364\text{e-}002$$

Coef of Det (r^2) = 0.990469 Curve Fit: Linear

Method Name: Z:\voasrv\HPCHEM1\MSVOA Y\methods\82Y082422S.M

Calibration Table Last Updated: Fri Aug 26 06:12:05 2022