
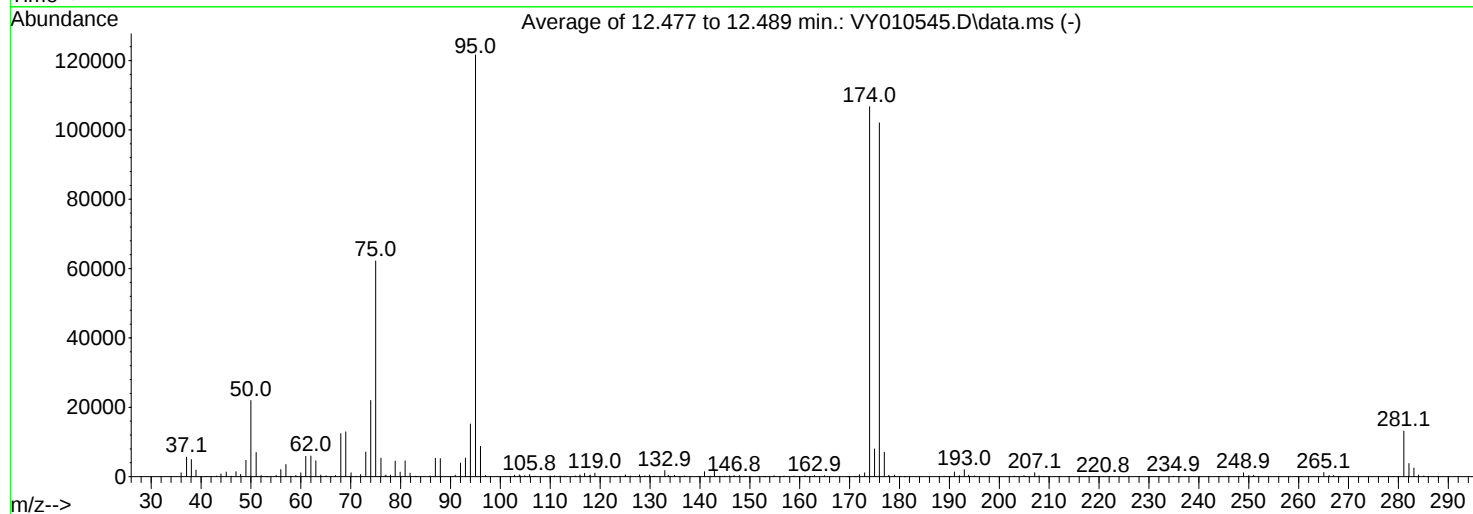


Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY091922\
 Data File : VY010545.D
 Acq On : 19 Sep 2022 10:00
 Operator : KP/MD
 Sample : BFB
 Misc : 5.00g/5.0mL/MSVOA_Y/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_Y
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y091922S.M
 Title : SW846 8260
 Last Update : Tue Sep 20 01:02:44 2022

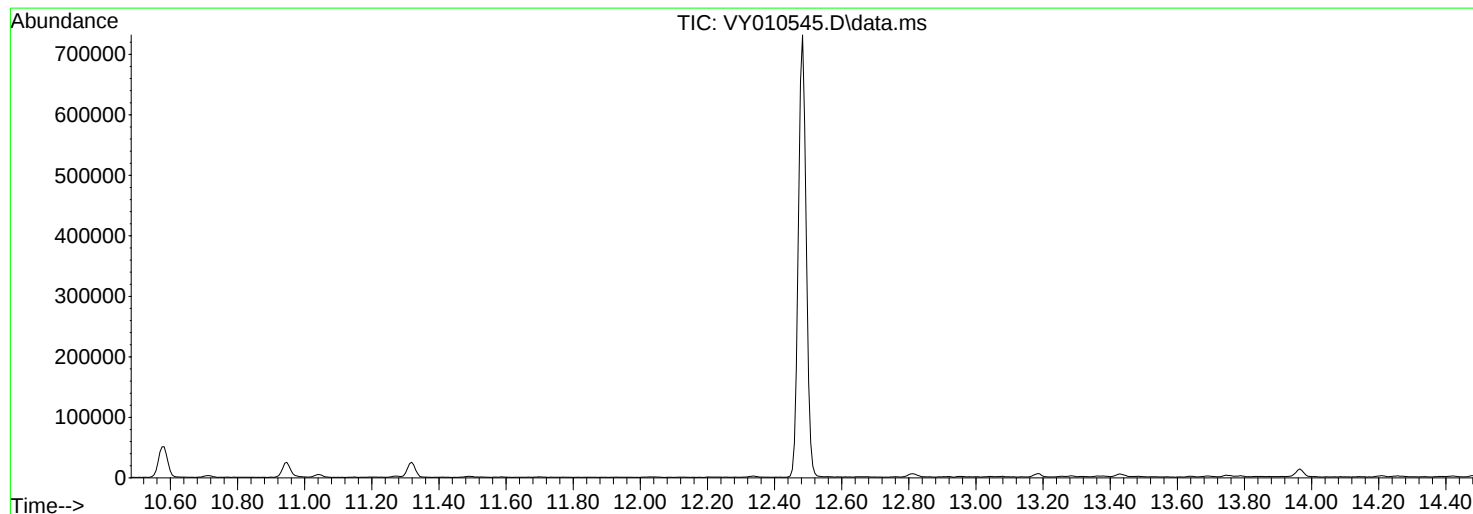

AutoFind: Scans 1748, 1749, 1750; Background Corrected with Scan 1739

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	18.1	21960	PASS
75	95	30	60	51.1	62205	PASS
95	95	100	100	100.0	121651	PASS
96	95	5	9	7.2	8726	PASS
173	174	0.00	2	1.0	1099	PASS
174	95	50	100	87.7	106669	PASS
175	174	5	9	7.5	7974	PASS
176	174	95	101	95.6	102011	PASS
177	176	5	9	6.9	7042	PASS