

Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY092122\
 Data File : VY010597.D
 Acq On : 21 Sep 2022 14:02
 Operator : KP/MD
 Sample : N4701-01
 Misc : 5.08g/5.0mL/MSVOA_Y/SOIL
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 MSVOA_Y
 ClientSampleId :
 OK-02-091622

Quant Time: Sep 21 15:36:09 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y091922S.M
 Quant Title : SW846 8260
 QLast Update : Tue Sep 20 01:02:44 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Pentafluorobenzene	7.783	168	160795	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	8.685	114	287276	50.000	ug/l	0.00
63) Chlorobenzene-d5	11.489	117	271005	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.422	152	120933	50.000	ug/l	0.00

System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.136	65	101074	65.719	ug/l	0.00
Spiked Amount	50.000	Range	50 - 163	Recovery	=	131.440%
35) Dibromofluoromethane	7.710	113	91274	49.784	ug/l	0.00
Spiked Amount	50.000	Range	54 - 147	Recovery	=	99.560%
50) Toluene-d8	10.179	98	344568	50.799	ug/l	0.00
Spiked Amount	50.000	Range	49 - 140	Recovery	=	101.600%
62) 4-Bromofluorobenzene	12.477	95	112324	44.363	ug/l	0.00
Spiked Amount	50.000	Range	25 - 144	Recovery	=	88.720%


Target Compounds	Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY092122\
Data File : VY010597.D
Acq On : 21 Sep 2022 14:02
Operator : KP/MD
Sample : N4701-01
Misc : 5.08g/5.0mL/MSVOA_Y/SOIL
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_Y
ClientSampleId :
OK-02-091622

Quant Time: Sep 21 15:36:09 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y091922S.M
Quant Title : SW846 8260
QLast Update : Tue Sep 20 01:02:44 2022
Response via : Initial Calibration




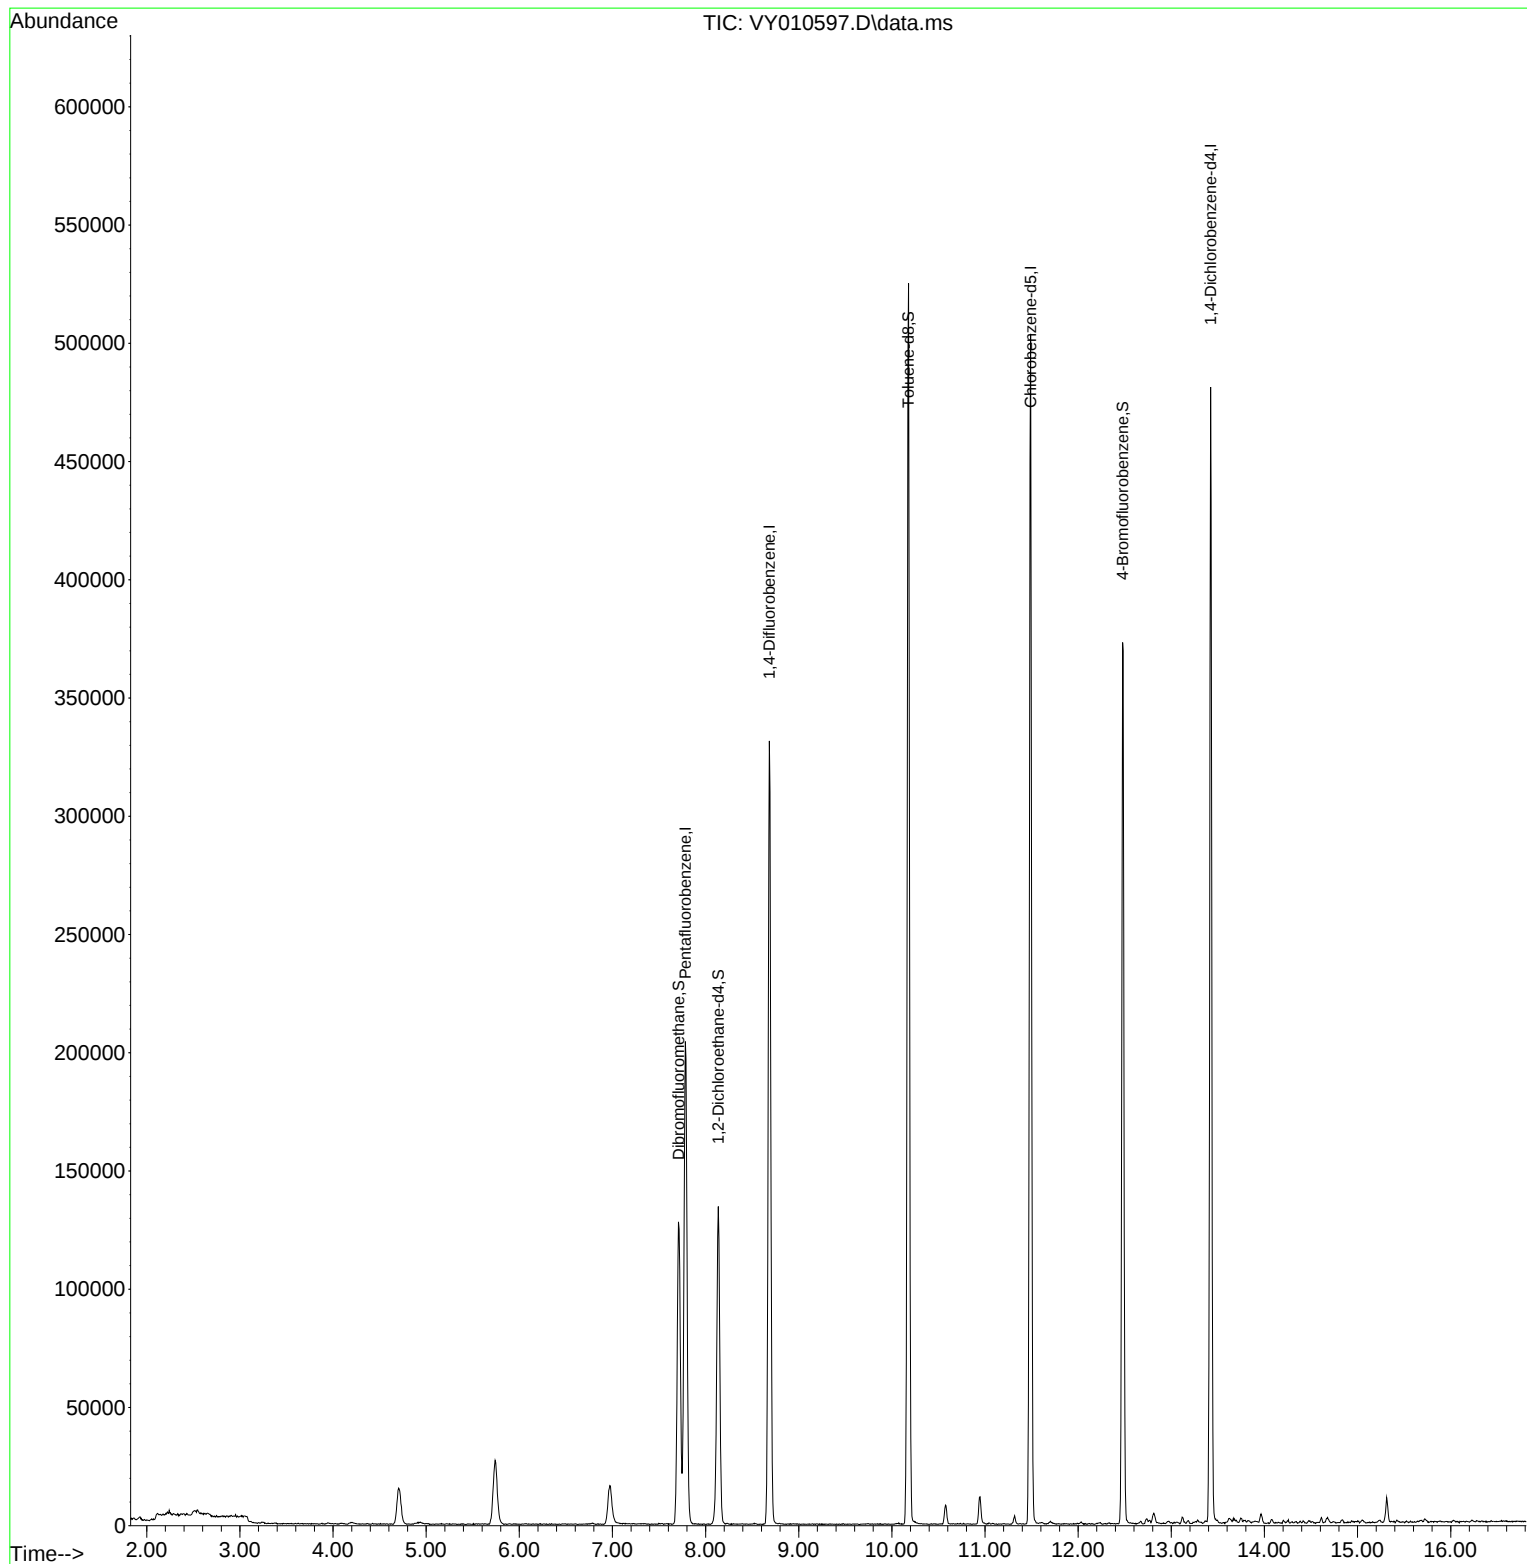


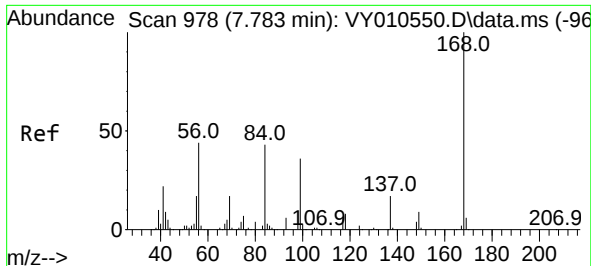

#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 7.783 min Scan# 91
Delta R.T. -0.000 min
Lab File: VY010597.D
Acq: 21 Sep 2022 14:02




Instrument :
MSVOA_Y
ClientSampleId :
OK-02-091622


Tgt Ion:168 Resp: 160795
Ion Ratio Lower Upper
168 100
99 54.4 46.9 70.3

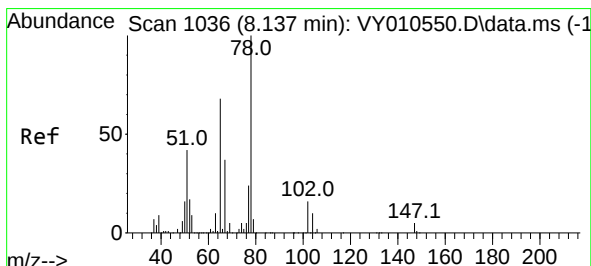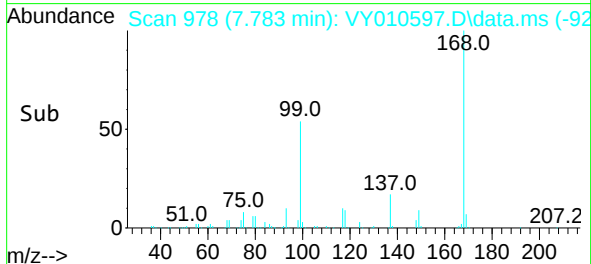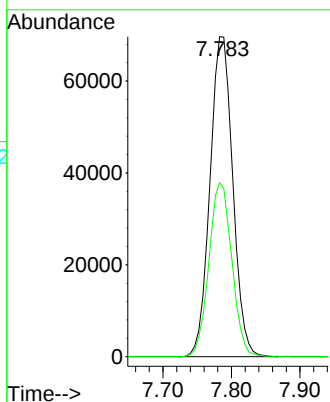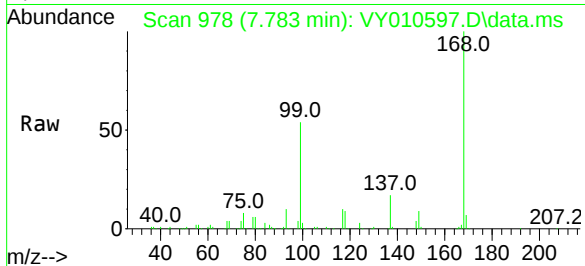

#33
1,2-Dichloroethane-d4
Concen: 65.719 ug/l
RT: 8.136 min Scan# 1036
Delta R.T. -0.001 min
Lab File: VY010597.D
Acq: 21 Sep 2022 14:02

Tgt Ion: 65 Resp: 101074
Ion Ratio Lower Upper
65 100
67 53.4 0.0 99.4

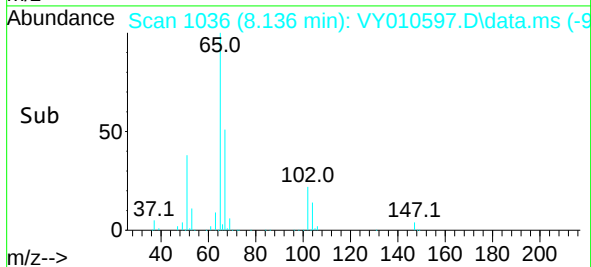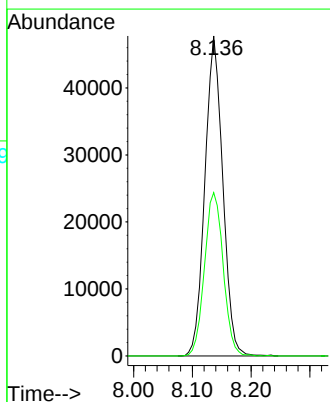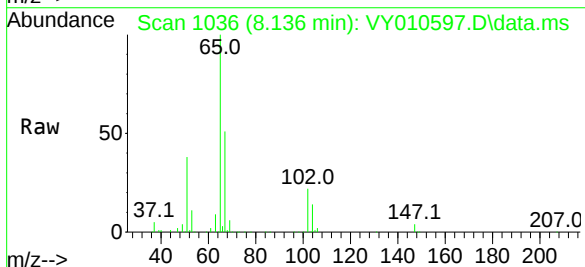

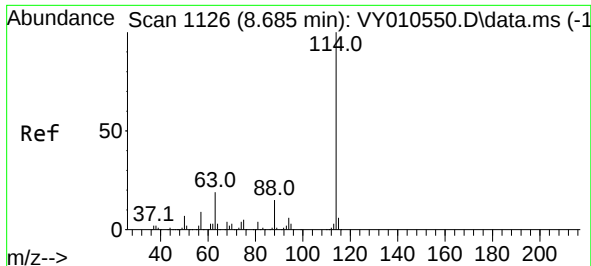

#34

1,4-Difluorobenzene

Concen: 50.000 ug/l

RT: 8.685 min Scan# 11

Delta R.T. 0.000 min

Lab File: VY010597.D

Acq: 21 Sep 2022 14:02

Instrument :

MSVOA_Y

ClientSampleId :

OK-02-091622





Tgt Ion:114 Resp: 287276

Ion Ratio Lower Upper

114 100

63 19.2 0.0 43.2

88 14.6 0.0 31.8

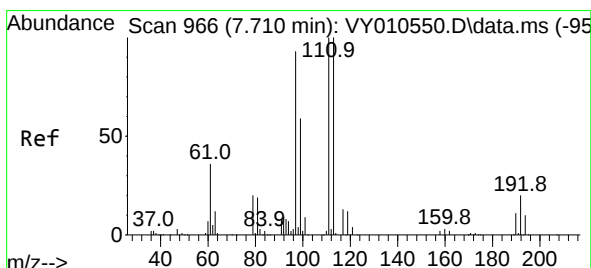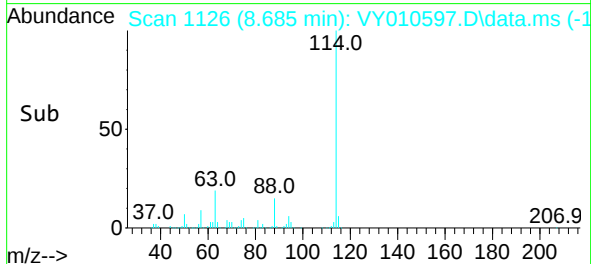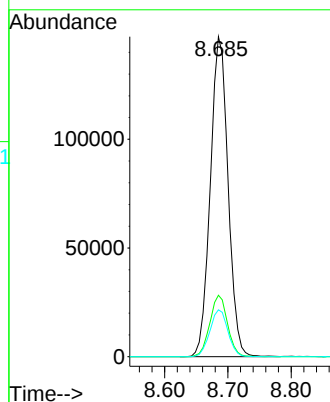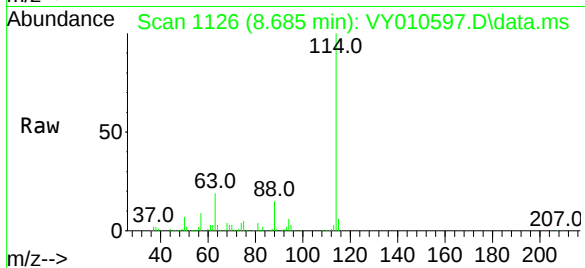

#35

Dibromofluoromethane

Concen: 49.784 ug/l

RT: 7.710 min Scan# 966

Delta R.T. -0.000 min

Lab File: VY010597.D

Acq: 21 Sep 2022 14:02




Tgt Ion:113 Resp: 91274


Ion Ratio Lower Upper

113 100

111 103.6 82.6 124.0

192 20.0 17.6 26.4


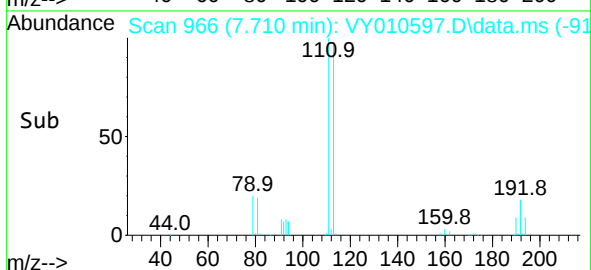
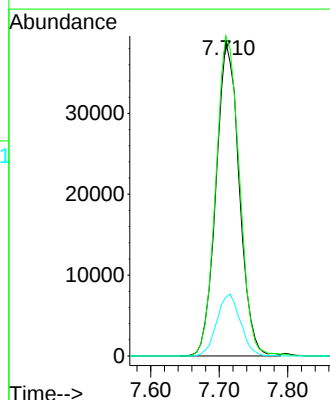
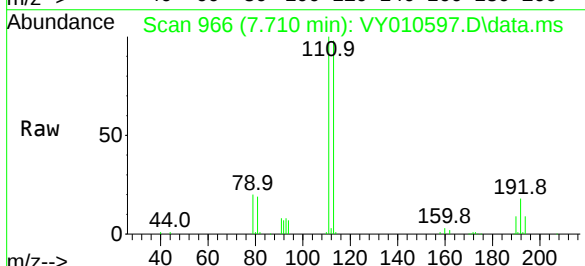


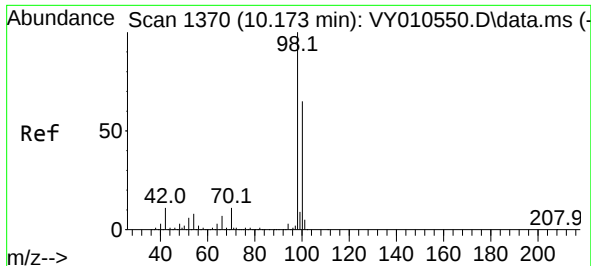

#50
Toluene-d8
Concen: 50.799 ug/l
RT: 10.179 min Scan# 11
Delta R.T. 0.006 min
Lab File: VY010597.D
Acq: 21 Sep 2022 14:02




Instrument :
MSVOA_Y
ClientSampleId :
OK-02-091622


Tgt Ion: 98 Resp: 344568
Ion Ratio Lower Upper
98 100
100 65.0 50.2 75.2

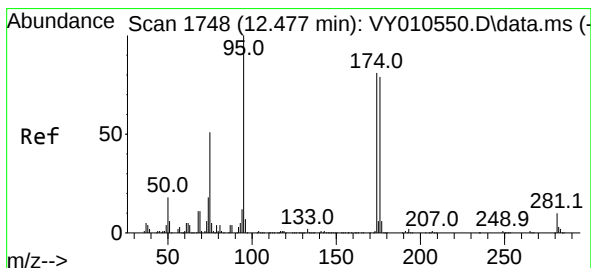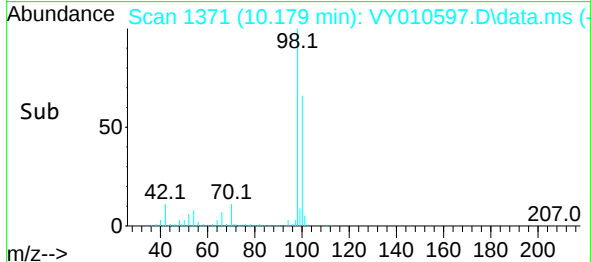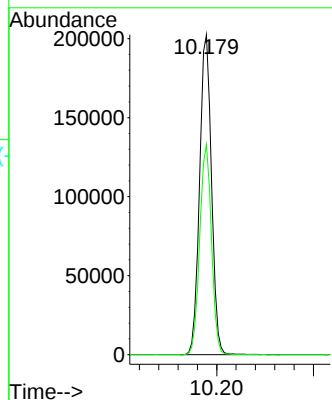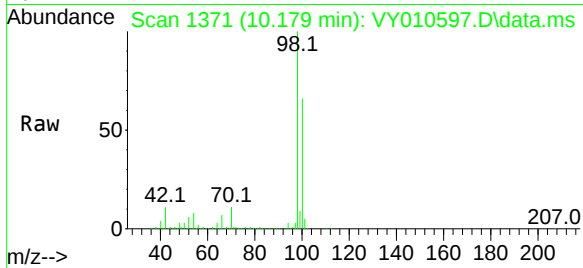

#62
4-Bromofluorobenzene
Concen: 44.363 ug/l
RT: 12.477 min Scan# 1748
Delta R.T. 0.000 min
Lab File: VY010597.D
Acq: 21 Sep 2022 14:02

Tgt Ion: 95 Resp: 112324
Ion Ratio Lower Upper
95 100
174 86.6 0.0 177.0
176 83.5 0.0 175.8


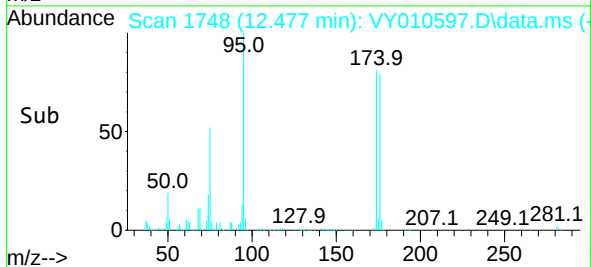
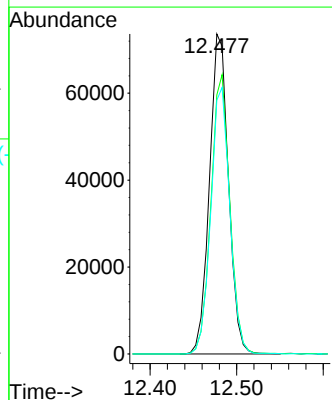
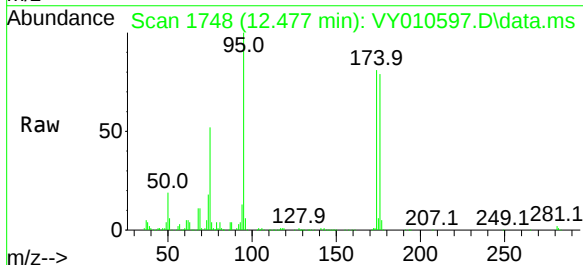


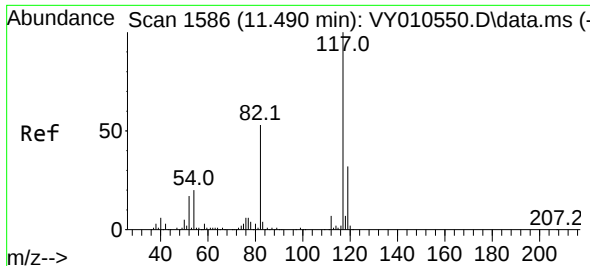

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 11.489 min Scan# 11
Delta R.T. -0.001 min
Lab File: VY010597.D
Acq: 21 Sep 2022 14:02

Instrument :
MSVOA_Y
ClientSampleId :
OK-02-091622

Tgt Ion:117 Resp: 271005
Ion Ratio Lower Upper
117 100
82 52.9 43.0 64.4
119 33.5 25.4 38.0

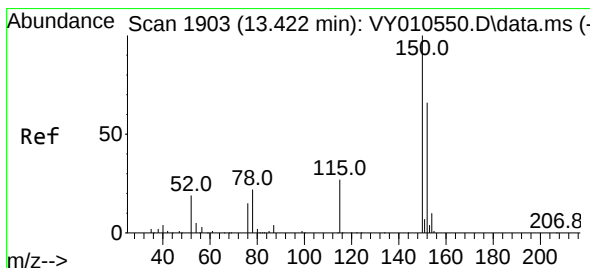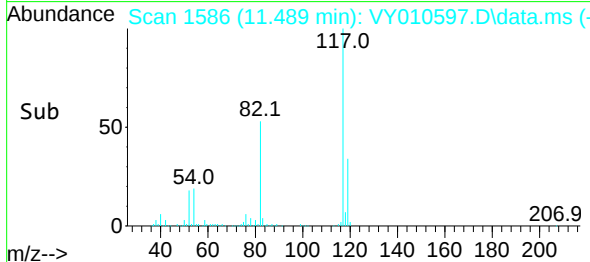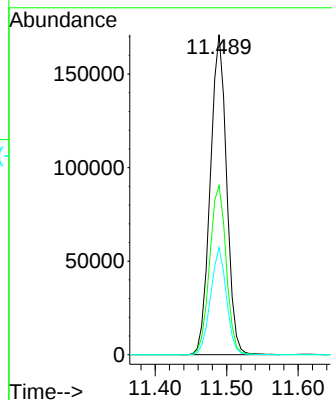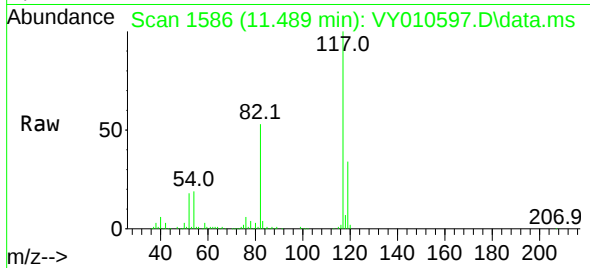

#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 13.422 min Scan# 1903
Delta R.T. 0.000 min
Lab File: VY010597.D
Acq: 21 Sep 2022 14:02

Tgt Ion:152 Resp: 120933
Ion Ratio Lower Upper
152 100
115 57.8 28.2 84.7
150 157.7 0.0 347.6

