


Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY101624\
Data File : VY019908.D
Acq On : 16 Oct 2024 09:37
Operator : SY/MD
Sample : BFB
Misc : 5.00g/5.0mL/MSVOA_Y/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_Y
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y100924S.M
Title : SW846 8260
Last Update : Wed Oct 16 05:44:48 2024

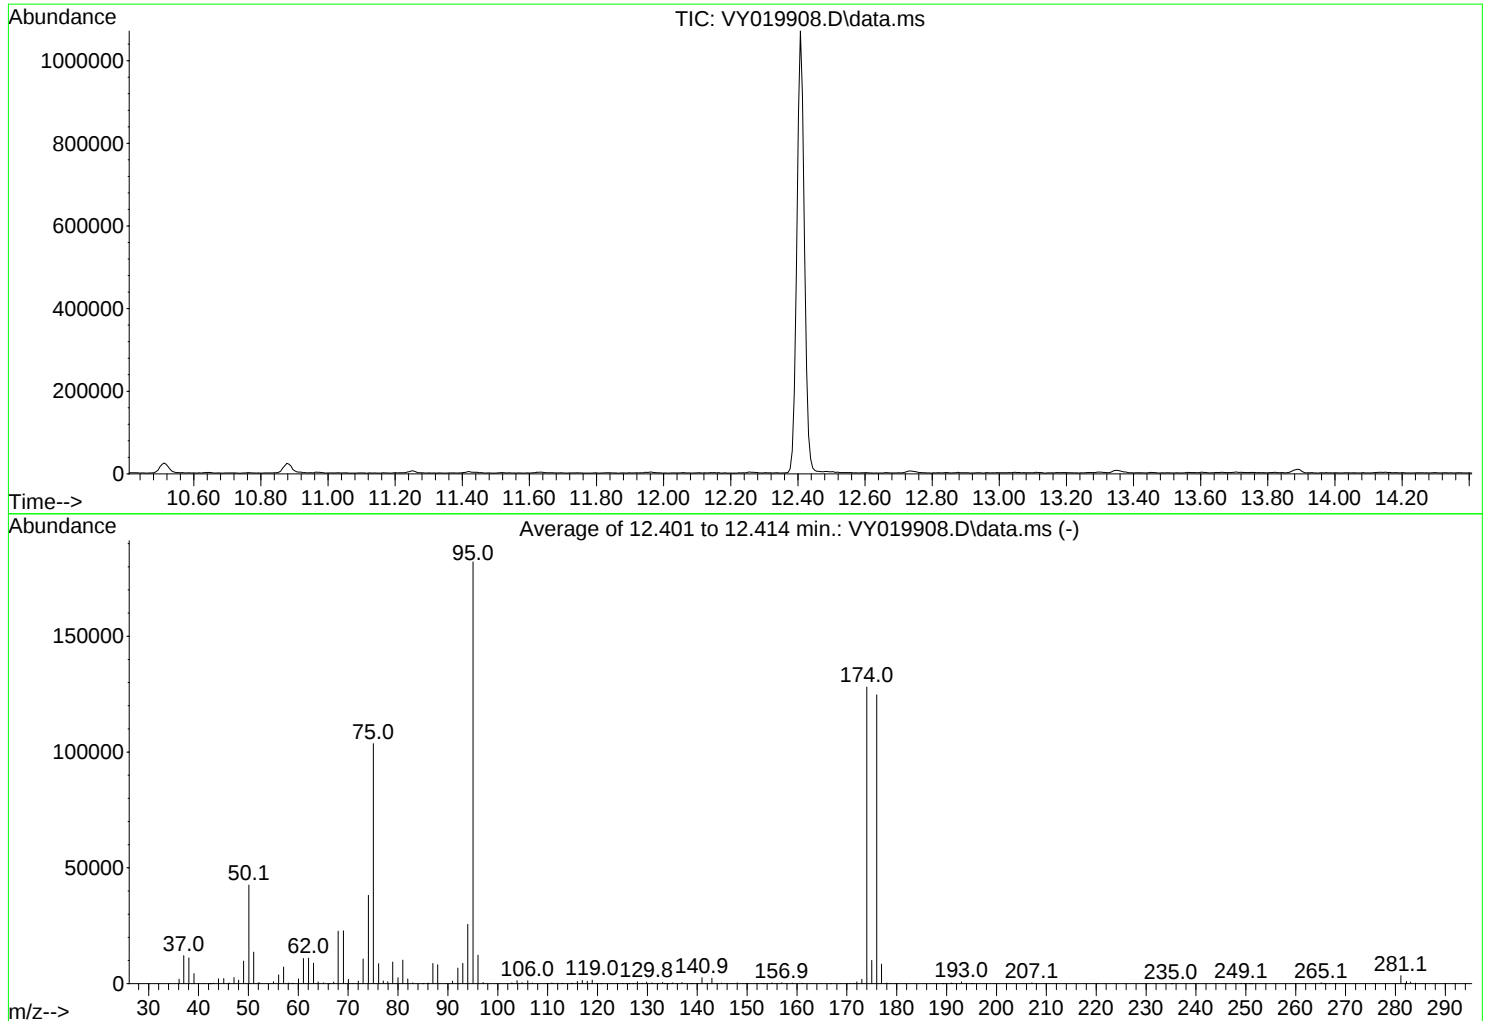

AutoFind: Scans 1752, 1753, 1754; Background Corrected with Scan 1744

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	23.4	42528	PASS
75	95	30	60	56.9	103656	PASS
95	95	100	100	100.0	182123	PASS
96	95	5	9	6.8	12325	PASS
173	174	0.00	2	1.5	1895	PASS
174	95	50	100	70.3	128061	PASS
175	174	5	9	7.8	10036	PASS
176	174	95	101	97.4	124699	PASS
177	176	5	9	6.8	8419	PASS