
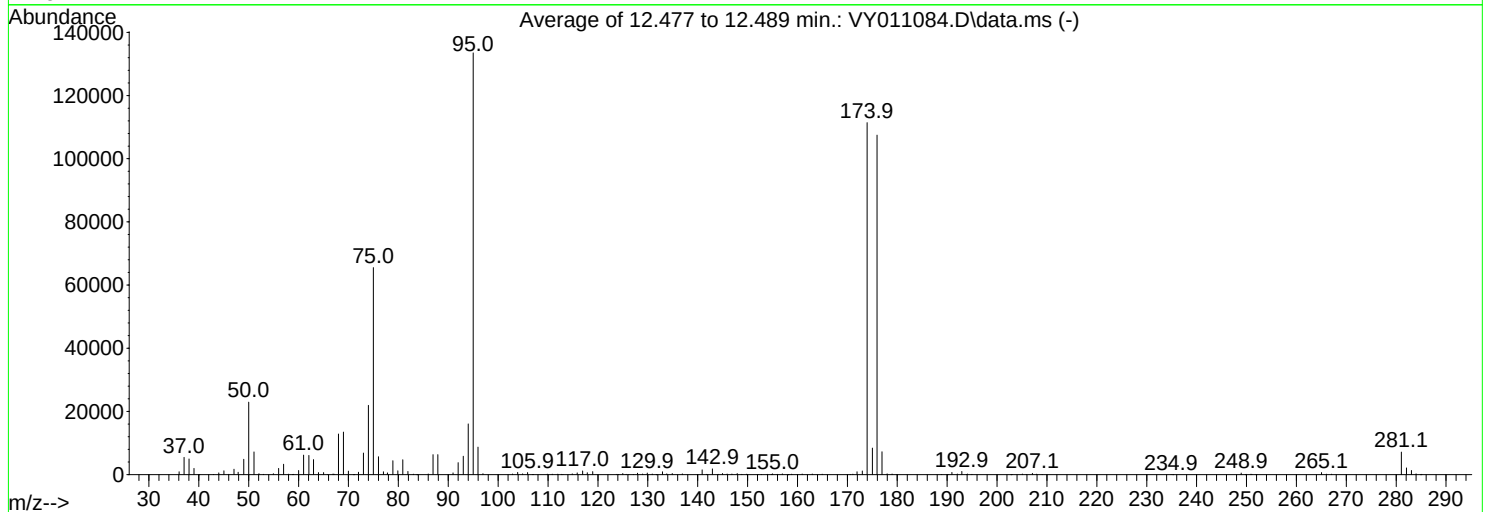


Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY102522\
Data File : VY011084.D
Acq On : 25 Oct 2022 09:11
Operator : KP/MD
Sample : BFB
Misc : 5.00g/5.0mL/MSVOA_Y/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_Y
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y101722S.M
Title : SW846 8260
Last Update : Tue Oct 18 01:42:42 2022

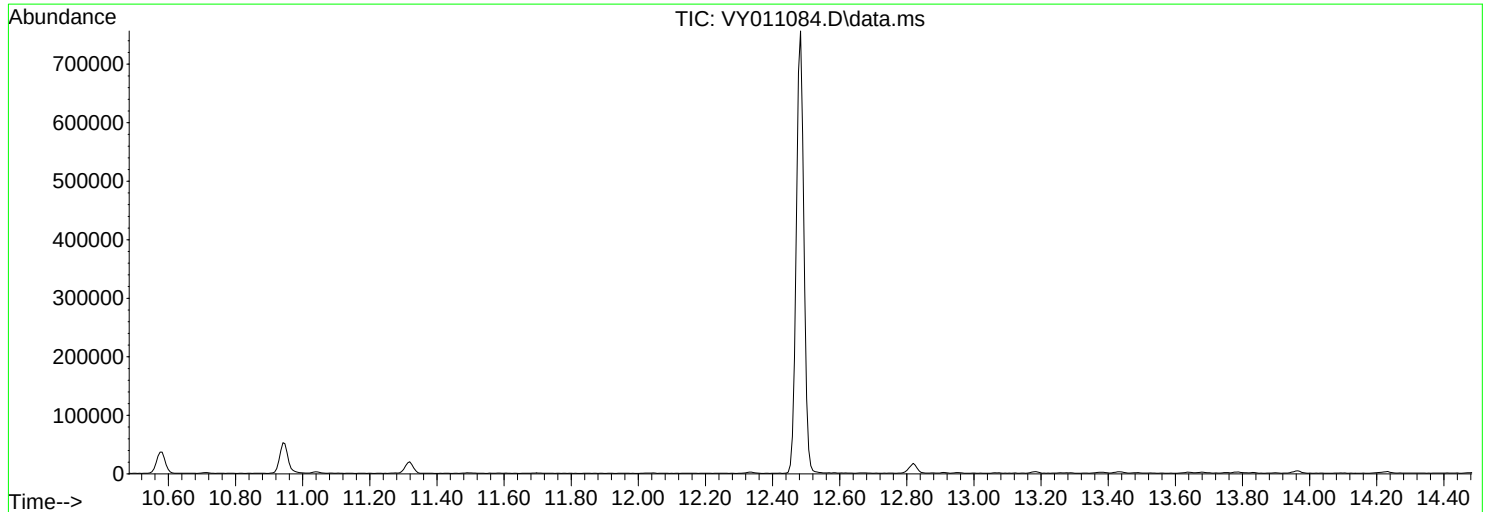

AutoFind: Scans 1748, 1749, 1750; Background Corrected with Scan 1739

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	17.2	22928	PASS
75	95	30	60	49.1	65565	PASS
95	95	100	100	100.0	133515	PASS
96	95	5	9	6.5	8689	PASS
173	174	0.00	2	1.0	1155	PASS
174	95	50	100	83.5	111437	PASS
175	174	5	9	7.5	8395	PASS
176	174	95	101	96.4	107475	PASS
177	176	5	9	6.7	7236	PASS