

Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY110222\
 Data File : VY011261.D
 Acq On : 02 Nov 2022 14:41
 Operator : KP/MD
 Sample : N5395-04
 Misc : 5.82g/5.0mL/MSVOA_Y/SOIL
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 MSVOA_Y
 ClientSampleId :
 S-10-103122

Quant Time: Nov 03 05:16:06 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y110122S.M
 Quant Title : SW846 8260
 QLast Update : Tue Nov 01 11:56:18 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) Pentafluorobenzene	7.789	168	229118	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	8.685	114	351196	50.000	ug/l	0.00
63) Chlorobenzene-d5	11.489	117	220052	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.422	152	57140	50.000	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.136	65	96304	39.301	ug/l	0.00
Spiked Amount	50.000	Range	50 - 163	Recovery	=	78.600%
35) Dibromofluoromethane	7.716	113	117794	52.204	ug/l	0.00
Spiked Amount	50.000	Range	54 - 147	Recovery	=	104.400%
50) Toluene-d8	10.179	98	393198	44.882	ug/l	0.00
Spiked Amount	50.000	Range	49 - 140	Recovery	=	89.760%
62) 4-Bromofluorobenzene	12.477	95	76659	25.205	ug/l	0.00
Spiked Amount	50.000	Range	25 - 144	Recovery	=	50.420%
Target Compounds						
16) Acetone	3.948	43	8937	12.082	ug/l	Qvalue # 77


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY110222\
Data File : VY011261.D
Acq On : 02 Nov 2022 14:41
Operator : KP/MD
Sample : N5395-04
Misc : 5.82g/5.0mL/MSVOA_Y/SOIL
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_Y
ClientSampleId :
S-10-103122

Quant Time: Nov 03 05:16:06 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y110122S.M
Quant Title : SW846 8260
QLast Update : Tue Nov 01 11:56:18 2022
Response via : Initial Calibration




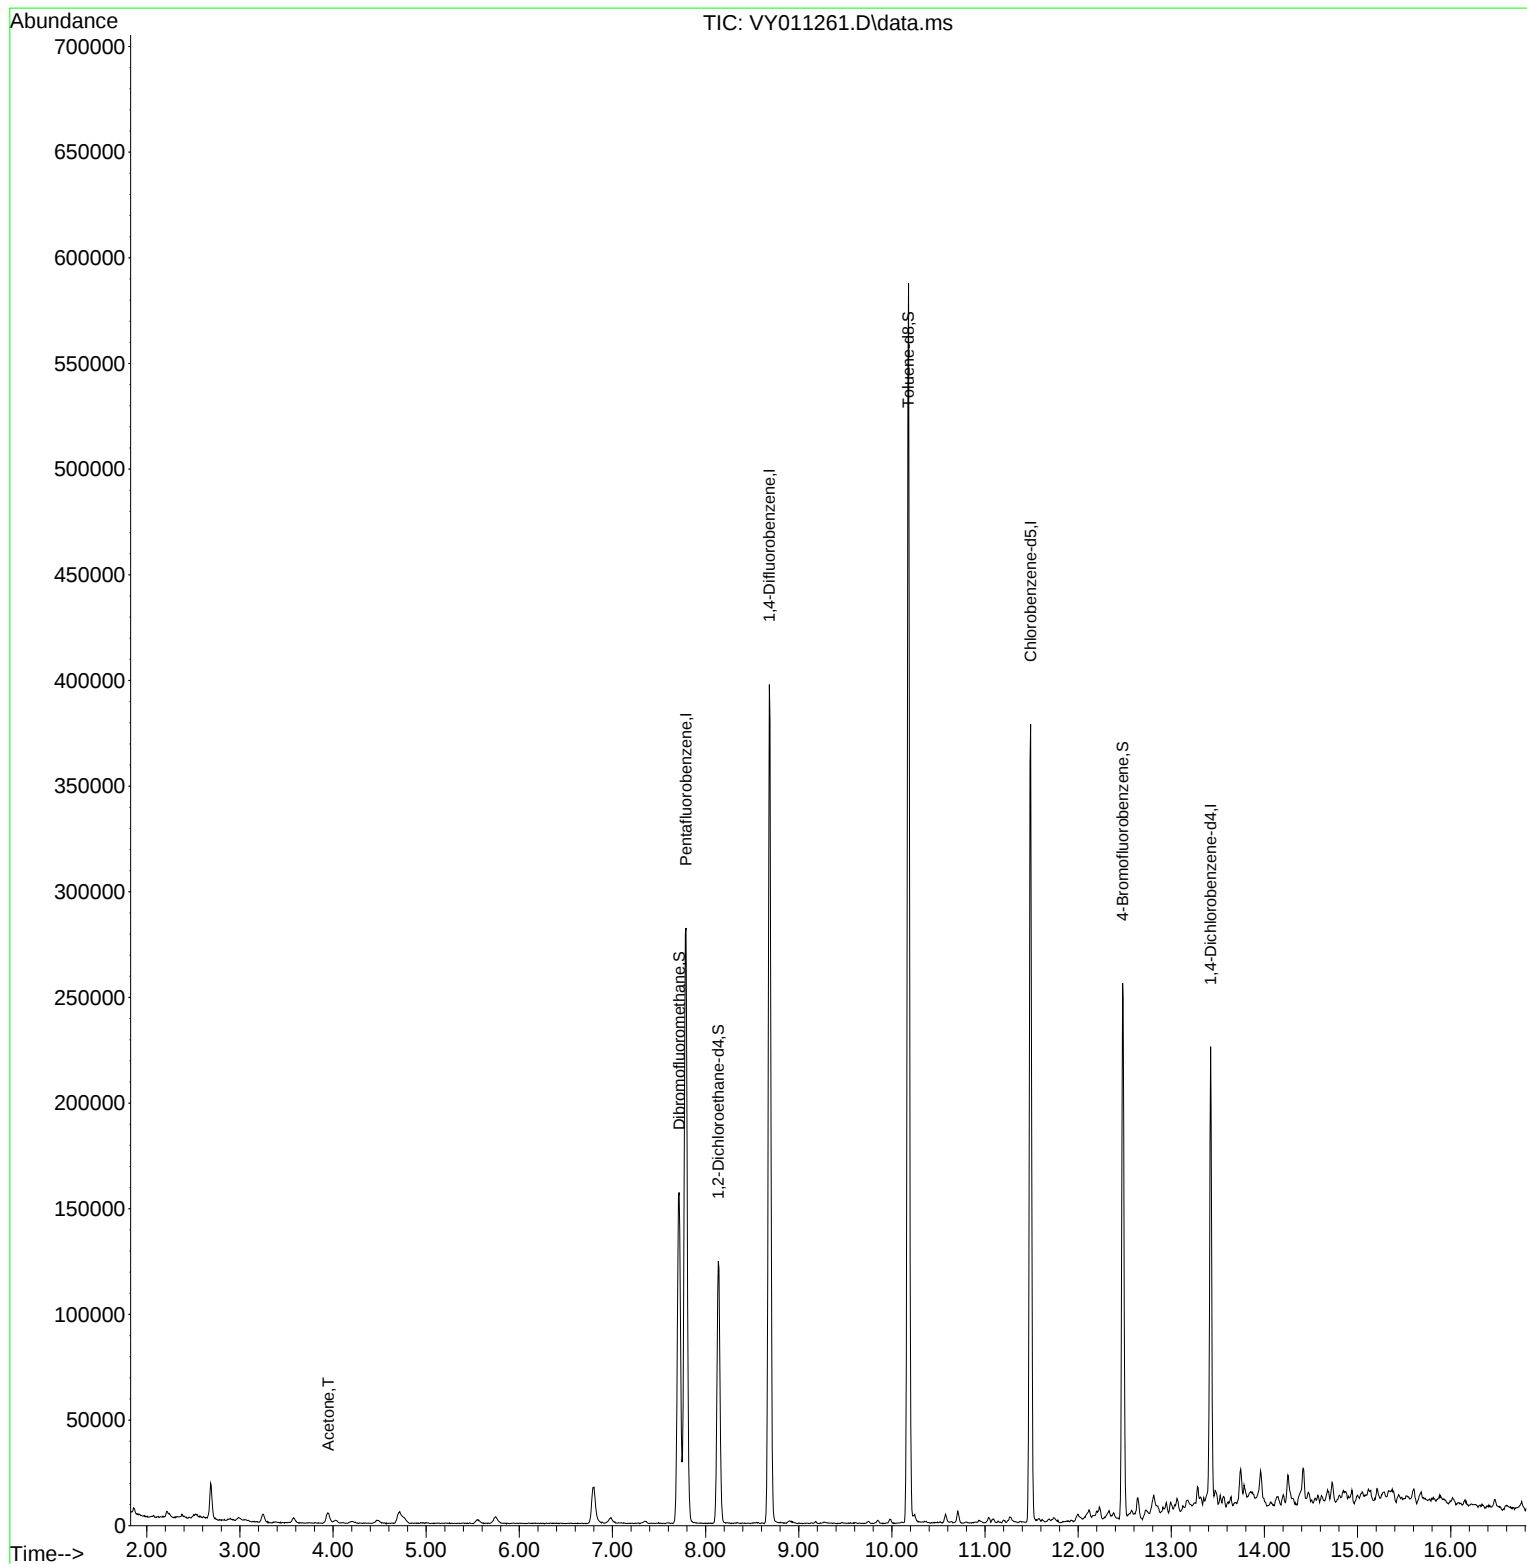


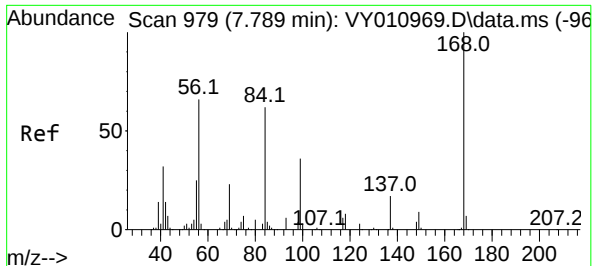

#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 7.789 min Scan# 91
Delta R.T. -0.000 min
Lab File: VY011261.D
Acq: 02 Nov 2022 14:41




Instrument :
MSVOA_Y
ClientSampleId :
S-10-103122


Tgt Ion:168 Resp: 229118
Ion Ratio Lower Upper
168 100
99 54.3 46.9 70.3

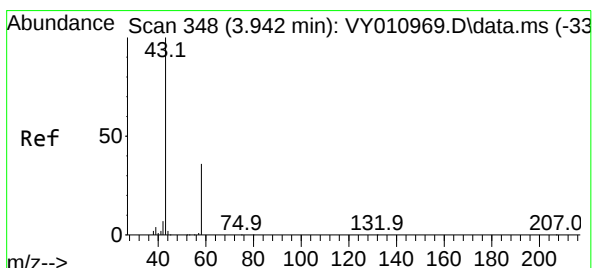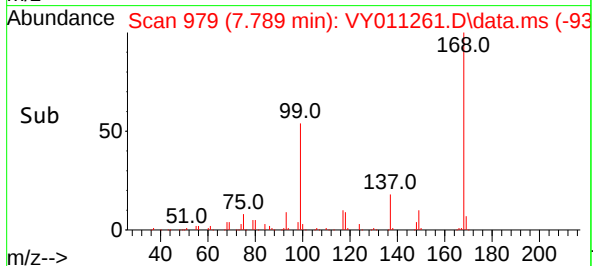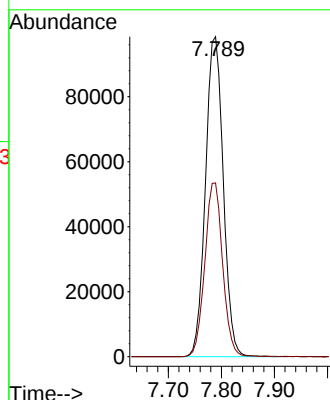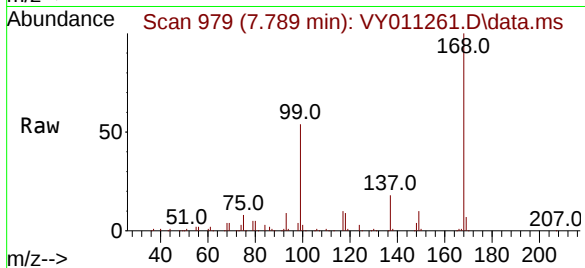

#16
Acetone
Concen: 12.082 ug/l
RT: 3.948 min Scan# 349
Delta R.T. 0.006 min
Lab File: VY011261.D
Acq: 02 Nov 2022 14:41

Tgt Ion: 43 Resp: 8937
Ion Ratio Lower Upper
43 100
58 39.7 22.0 33.0#

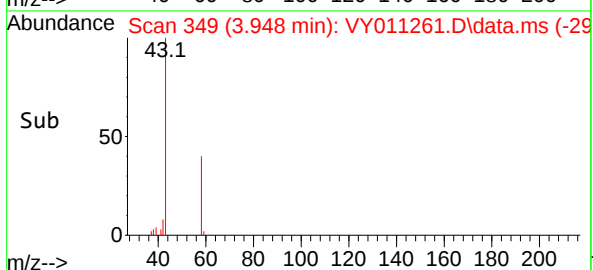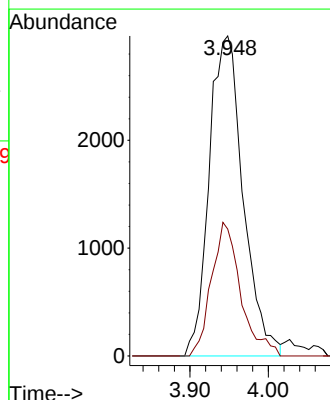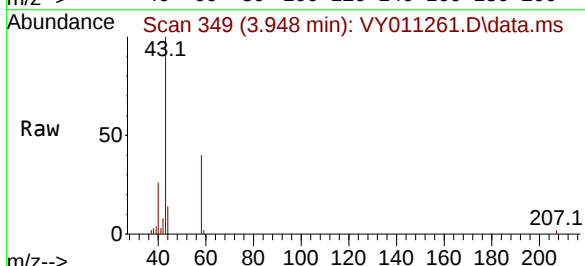

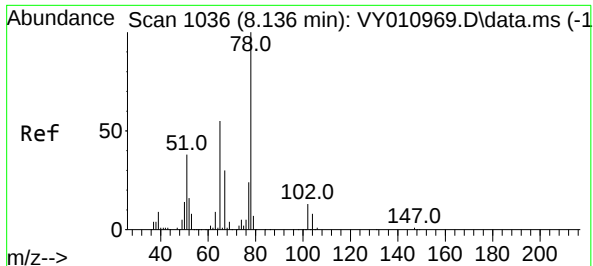

#33

1,2-Dichloroethane-d4

Concen: 39.301 ug/l

RT: 8.136 min Scan# 1103

Delta R.T. 0.000 min

Lab File: VY011261.D

Acq: 02 Nov 2022 14:41

Instrument :

MSVOA_Y

ClientSampleId :





S-10-103122

Tgt Ion: 65 Resp: 96304

Ion Ratio Lower Upper

65 100

67 55.3 0.0 99.4

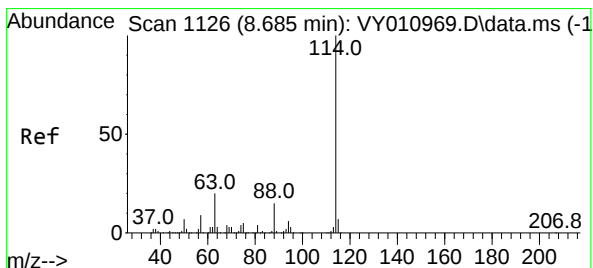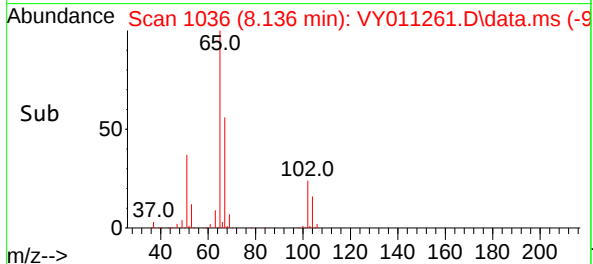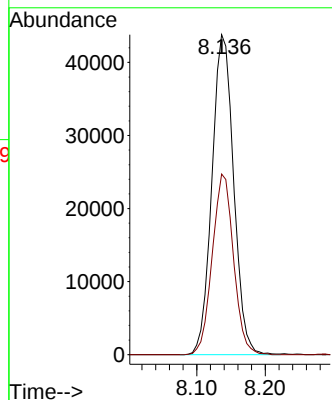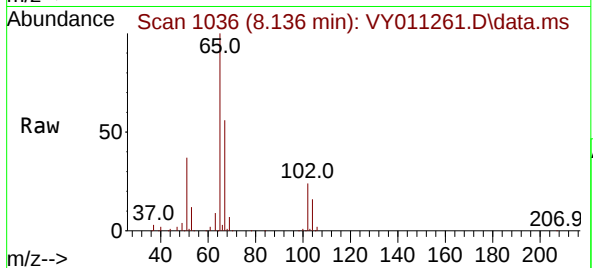

#34

1,4-Difluorobenzene

Concen: 50.000 ug/l

RT: 8.685 min Scan# 1126

Delta R.T. 0.000 min

Lab File: VY011261.D

Acq: 02 Nov 2022 14:41




Tgt Ion: 114 Resp: 351196


Ion Ratio Lower Upper

114 100

63 19.5 0.0 43.2

88 15.4 0.0 31.8


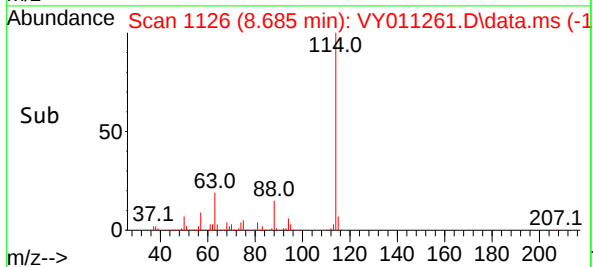
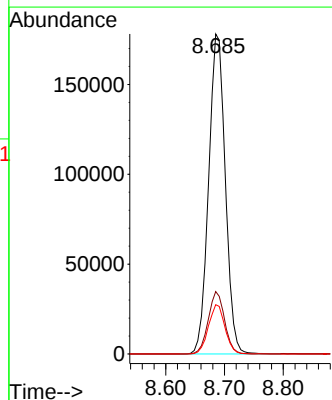
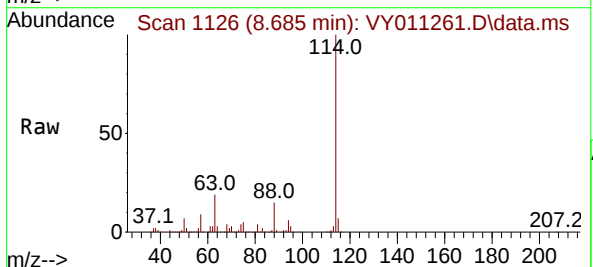


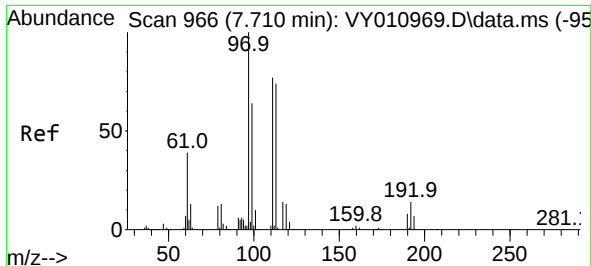

#35
Dibromofluoromethane
Concen: 52.204 ug/l
RT: 7.716 min Scan# 91
Delta R.T. 0.006 min
Lab File: VY011261.D
Acq: 02 Nov 2022 14:41




Instrument :
MSVOA_Y
ClientSampleId :
S-10-103122


Tgt Ion:113 Resp: 117794
Ion Ratio Lower Upper
113 100
111 102.2 82.6 124.0
192 19.5 17.6 26.4

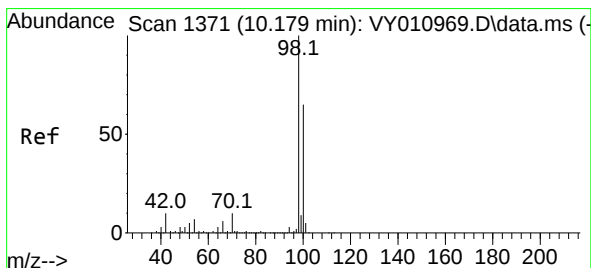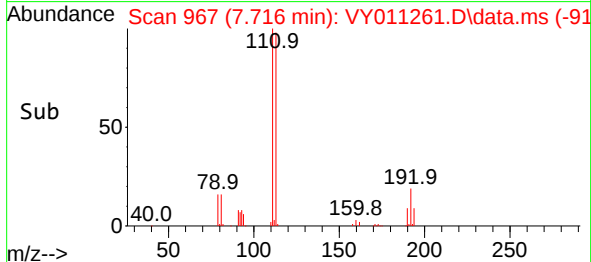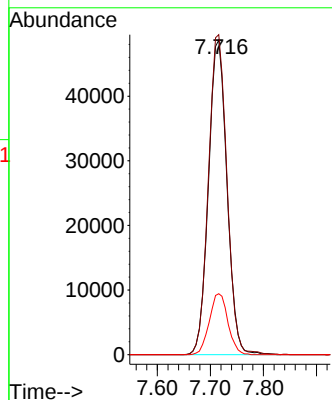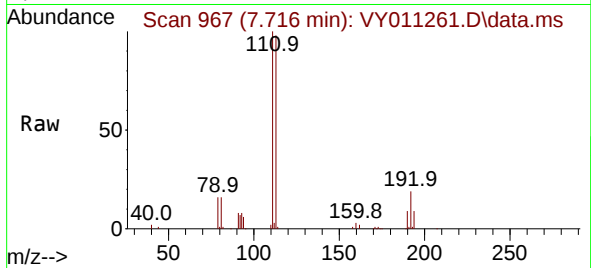

#50
Toluene-d8
Concen: 44.882 ug/l
RT: 10.179 min Scan# 1371
Delta R.T. -0.000 min
Lab File: VY011261.D
Acq: 02 Nov 2022 14:41

Tgt Ion: 98 Resp: 393198
Ion Ratio Lower Upper
98 100
100 65.2 50.2 75.2


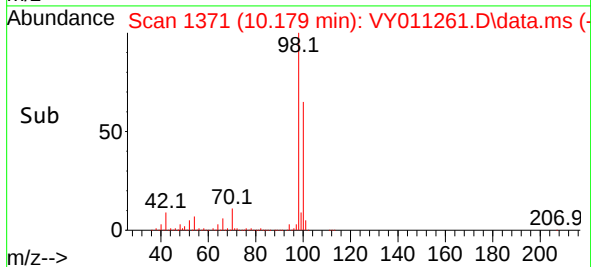
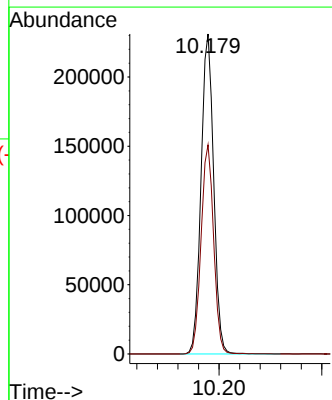
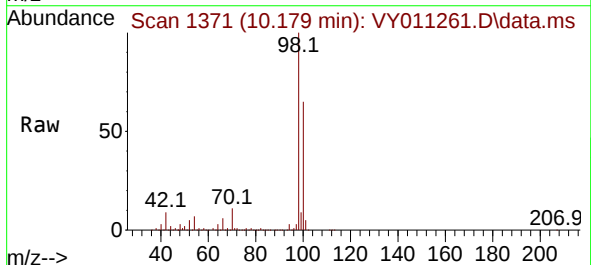


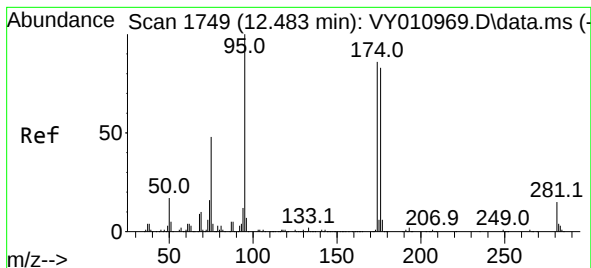

#62
4-Bromofluorobenzene
Concen: 25.205 ug/l
RT: 12.477 min Scan# 1748
Delta R.T. -0.006 min
Lab File: VY011261.D
Acq: 02 Nov 2022 14:41




Instrument :
MSVOA_Y
ClientSampleId :
S-10-103122


Tgt Ion: 95 Resp: 76659
Ion Ratio Lower Upper
95 100
174 86.0 0.0 177.0
176 82.0 0.0 175.8

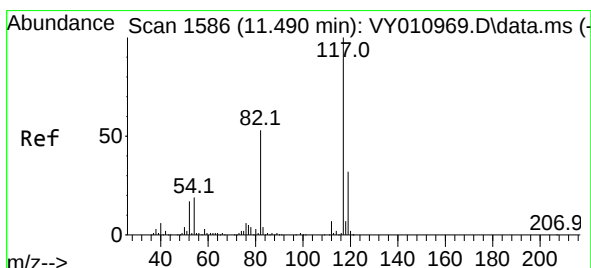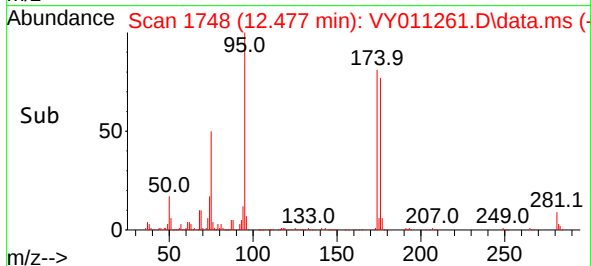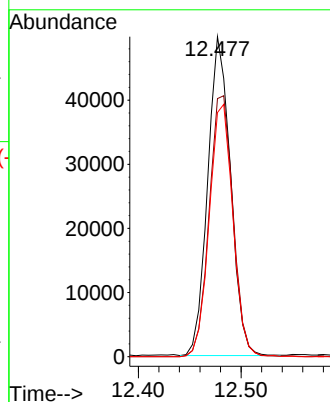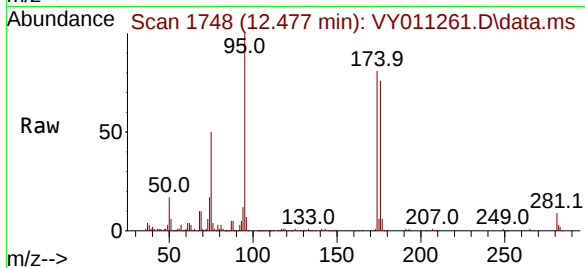

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 11.489 min Scan# 1586
Delta R.T. -0.001 min
Lab File: VY011261.D
Acq: 02 Nov 2022 14:41

Tgt Ion: 117 Resp: 220052
Ion Ratio Lower Upper
117 100
82 53.7 43.0 64.4
119 32.0 25.4 38.0

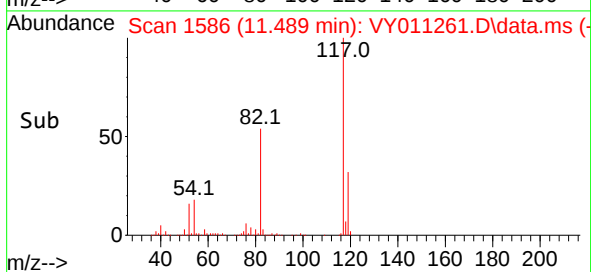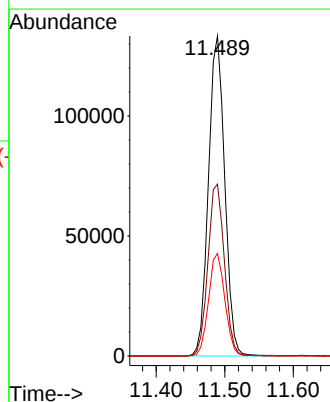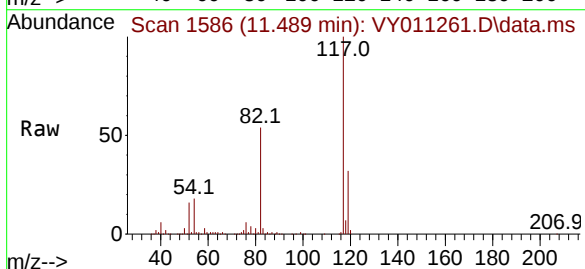

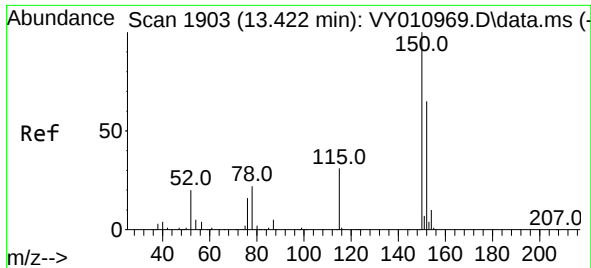

#72
 1,4-Dichlorobenzene-d4
 Concen: 50.000 ug/l
 RT: 13.422 min Scan# 1903
 Delta R.T. -0.000 min
 Lab File: VY011261.D
 Acq: 02 Nov 2022 14:41

Instrument :
 MSVOA_Y
 ClientSampleId :
 S-10-103122

Tgt Ion	Ratio	Lower	Upper
152	100		
115	58.3	28.2	84.7
150	153.5	0.0	347.6

