
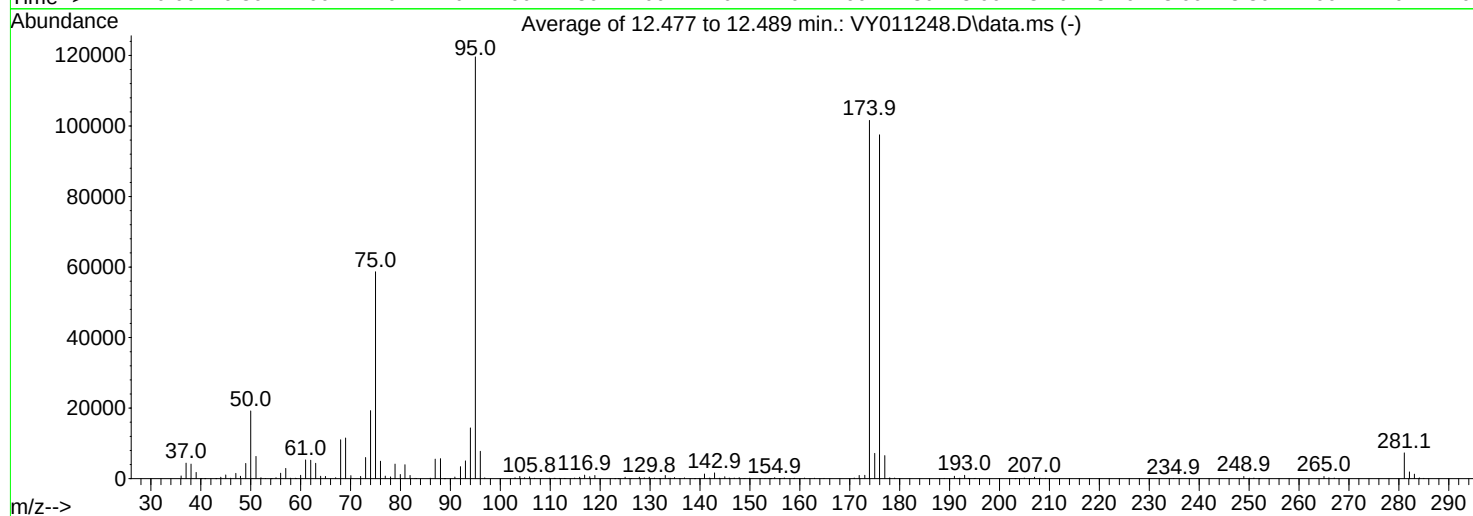


Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY110222\
 Data File : VY011248.D
 Acq On : 02 Nov 2022 08:40
 Operator : KP/MD
 Sample : BFB
 Misc : 5.00g/5.0mL/MSVOA_Y/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_Y
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y110122S.M
 Title : SW846 8260
 Last Update : Tue Nov 01 11:56:18 2022

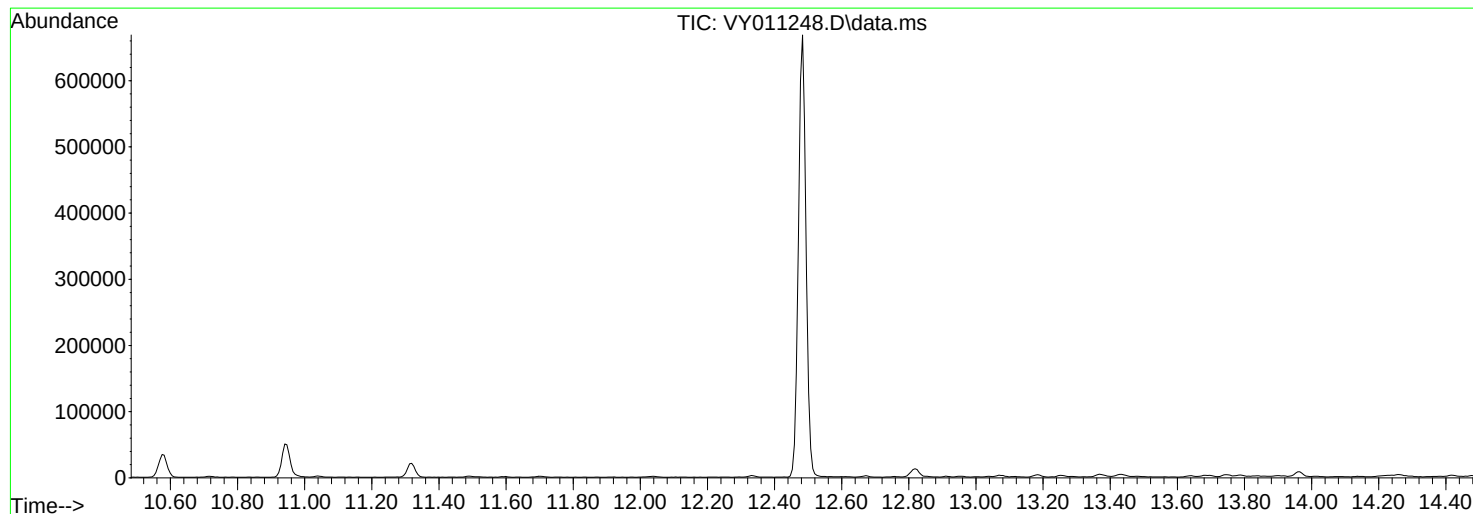

AutoFind: Scans 1748, 1749, 1750; Background Corrected with Scan 1740

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	16.0	19174	PASS
75	95	30	60	49.1	58672	PASS
95	95	100	100	100.0	119603	PASS
96	95	5	9	6.5	7744	PASS
173	174	0.00	2	1.0	966	PASS
174	95	50	100	85.0	101605	PASS
175	174	5	9	7.1	7191	PASS
176	174	95	101	95.9	97488	PASS
177	176	5	9	6.7	6516	PASS