


Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY110322\
Data File : VY011275.D
Acq On : 03 Nov 2022 08:54
Operator : KP/MD
Sample : BFB
Misc : 5.00g/5.0mL/MSVOA_Y/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_Y
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y110122S.M
Title : SW846 8260
Last Update : Tue Nov 01 11:56:18 2022

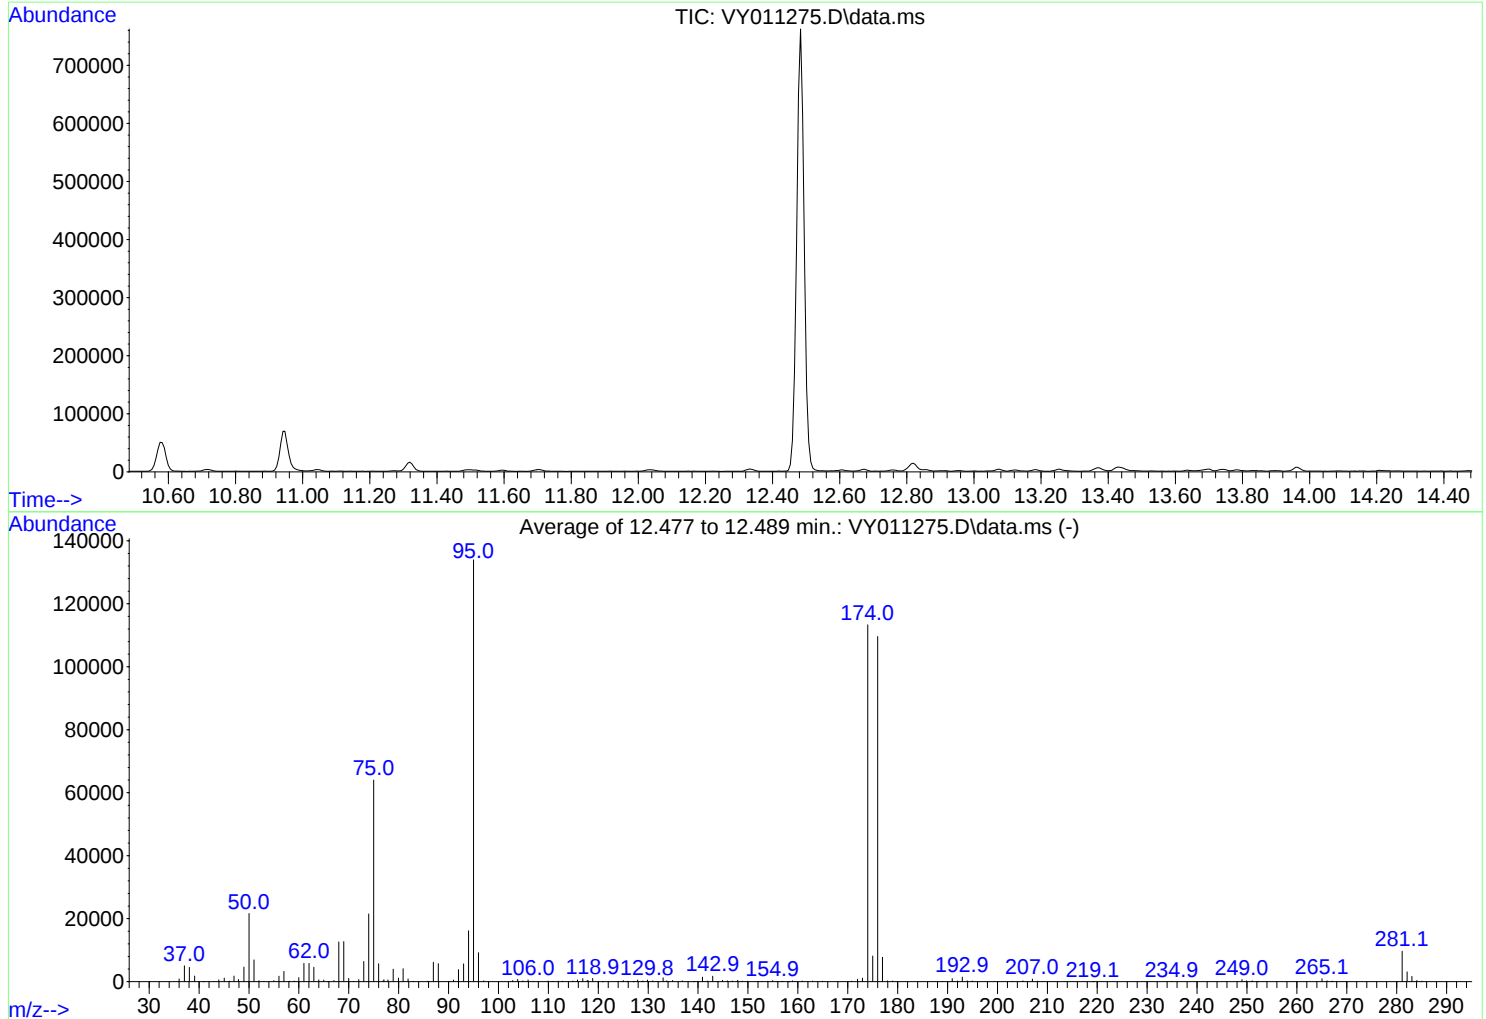

AutoFind: Scans 1748, 1749, 1750; Background Corrected with Scan 1740

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	16.2	21643	PASS
75	95	30	60	47.8	64045	PASS
95	95	100	100	100.0	133955	PASS
96	95	5	9	6.9	9185	PASS
173	174	0.00	2	1.0	1143	PASS
174	95	50	100	84.6	113317	PASS
175	174	5	9	7.2	8116	PASS
176	174	95	101	96.7	109592	PASS
177	176	5	9	7.0	7707	PASS