

Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY111324\
 Data File : VY020292.D
 Acq On : 13 Nov 2024 18:46
 Operator : SY/MD
 Sample : P4822-09
 Misc : 6.12g/5.0mL/MSVOA_Y/SOIL/A
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 MSVOA_Y
 ClientSampleId :
 SOIL-5

Quant Time: Nov 14 01:02:05 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y103024S.M
 Quant Title : SW846 8260
 QLast Update : Thu Oct 31 15:23:13 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Pentafluorobenzene	7.713	168	187862	50.000	ug/l	# 0.00
34) 1,4-Difluorobenzene	8.622	114	324534	50.000	ug/l	0.00
63) Chlorobenzene-d5	11.420	117	313306	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.347	152	137784	50.000	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.067	65	111434	47.527	ug/l	0.00
Spiked Amount	50.000	Range	50 - 163	Recovery	=	95.060%
35) Dibromofluoromethane	7.640	113	134823	65.341	ug/l	0.00
Spiked Amount	50.000	Range	54 - 147	Recovery	=	130.680%
50) Toluene-d8	10.109	98	398660	48.539	ug/l	0.00
Spiked Amount	50.000	Range	58 - 134	Recovery	=	97.080%
62) 4-Bromofluorobenzene	12.408	95	119036	44.620	ug/l	0.00
Spiked Amount	50.000	Range	29 - 146	Recovery	=	89.240%


Target Compounds Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY111324\
Data File : VY020292.D
Acq On : 13 Nov 2024 18:46
Operator : SY/MD
Sample : P4822-09
Misc : 6.12g/5.0mL/MSVOA_Y/SOIL/A
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_Y
ClientSampleId :
SOIL-5

Quant Time: Nov 14 01:02:05 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y103024S.M
Quant Title : SW846 8260
QLast Update : Thu Oct 31 15:23:13 2024
Response via : Initial Calibration




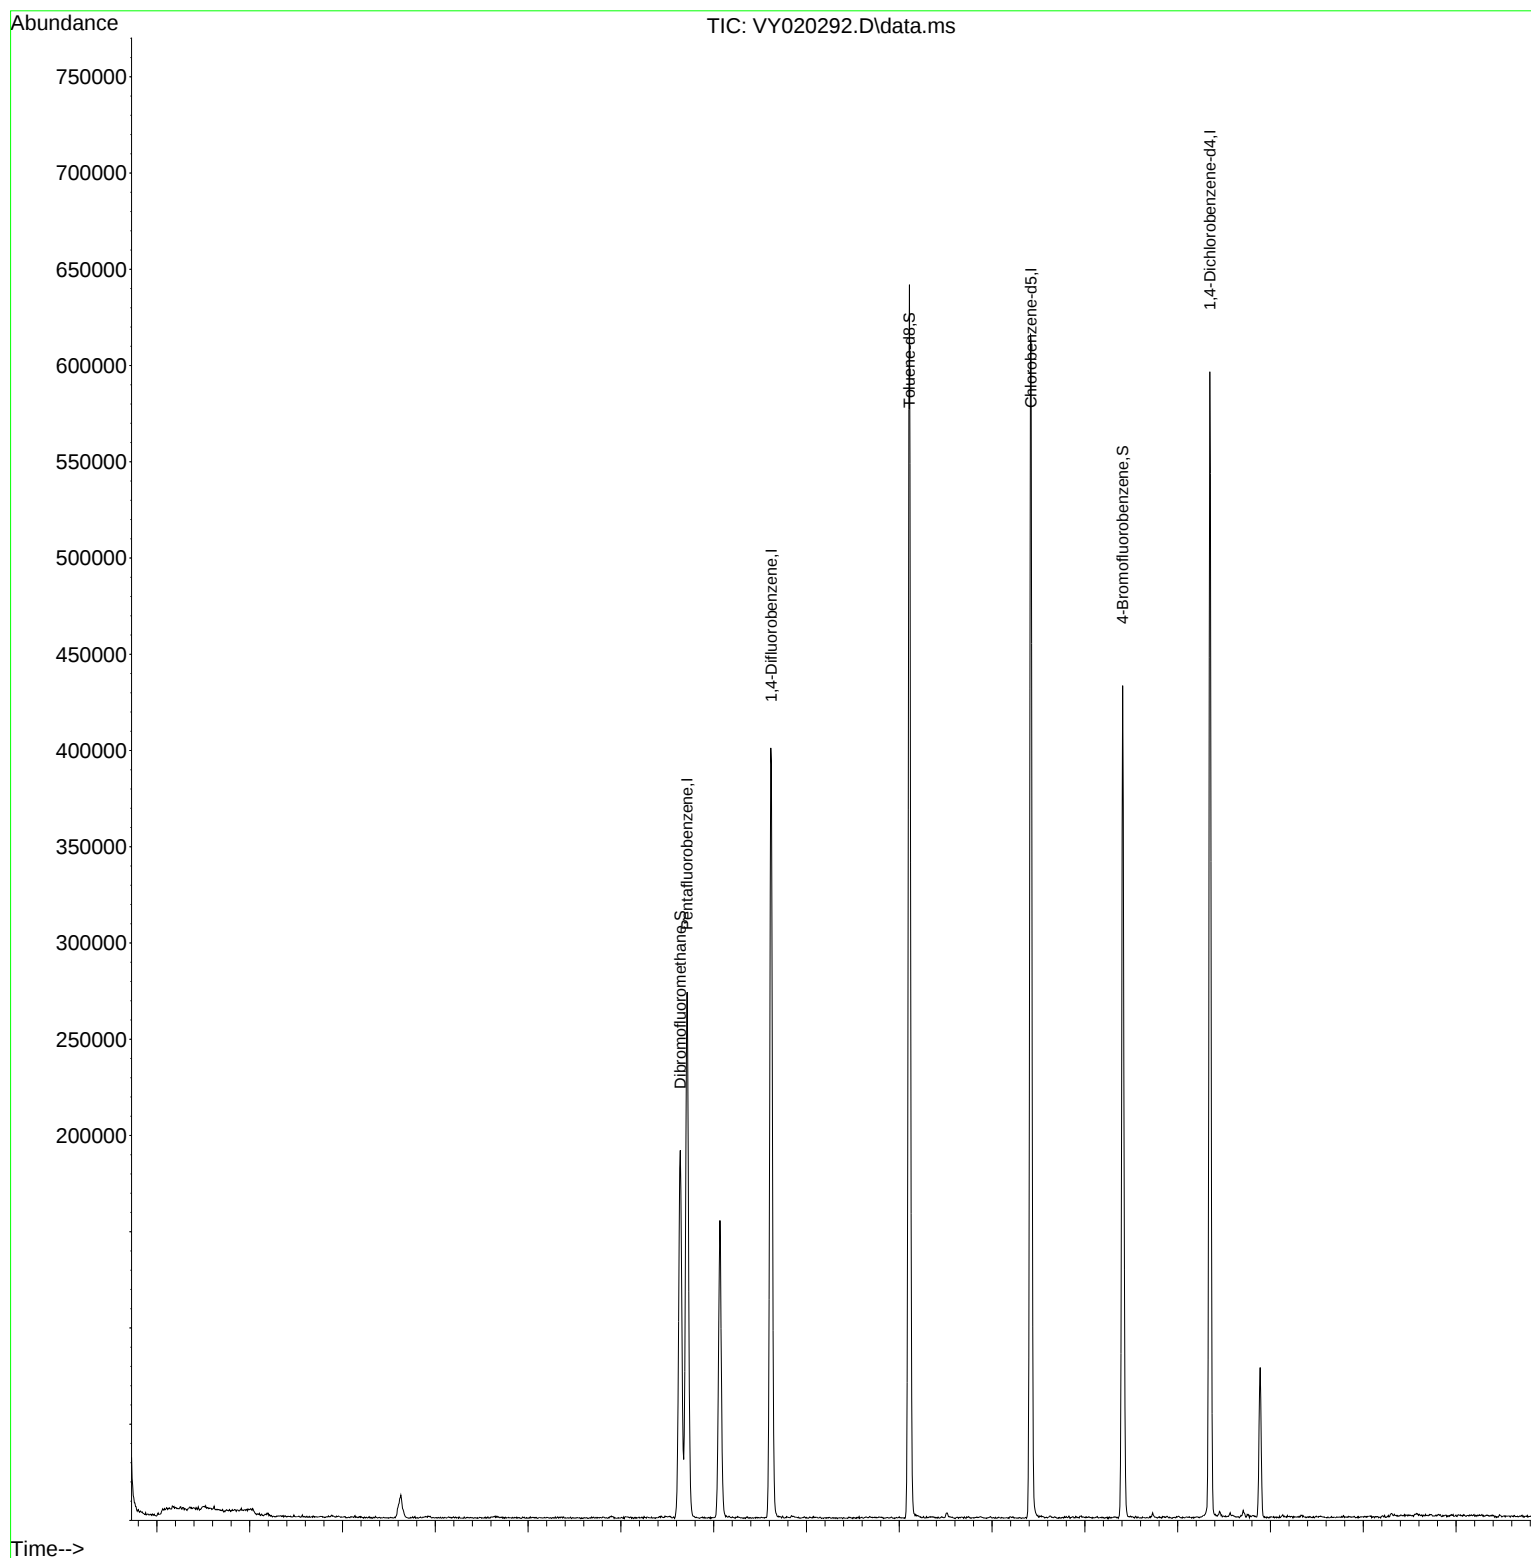


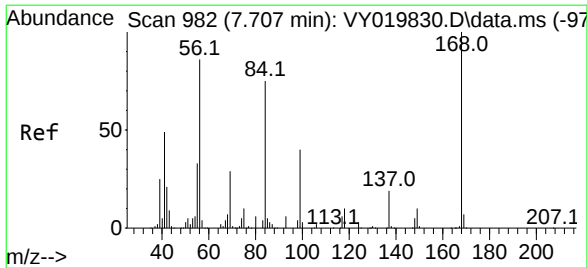

#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 7.713 min Scan# 98
Delta R.T. 0.006 min
Lab File: VY020292.D
Acq: 13 Nov 2024 18:46




Instrument :
MSVOA_Y
ClientSampleId :
SOIL-5


Tgt Ion:168 Resp: 187862
Ion Ratio Lower Upper
168 100
99 63.0 39.1 58.7#

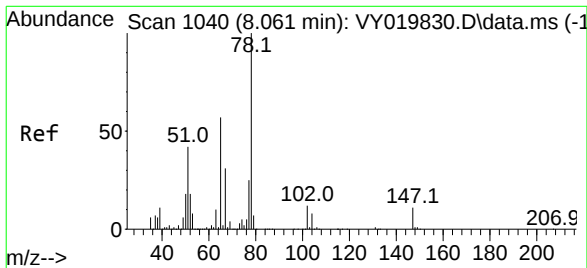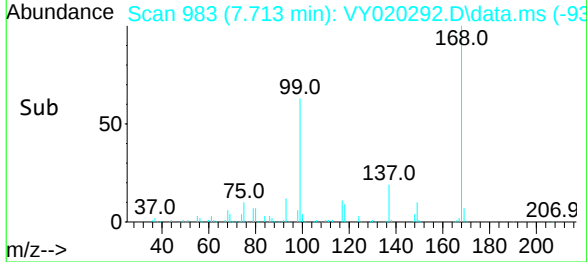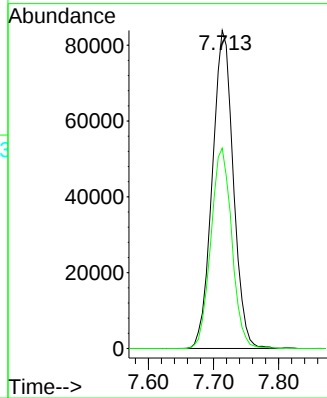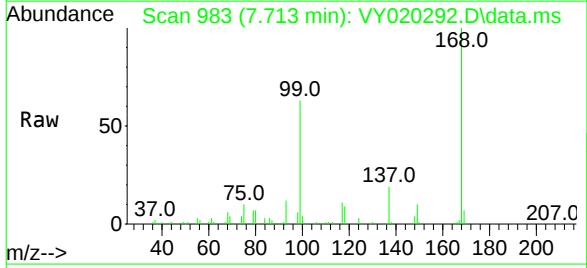

#33
1,2-Dichloroethane-d4
Concen: 47.527 ug/l
RT: 8.067 min Scan# 1041
Delta R.T. 0.006 min
Lab File: VY020292.D
Acq: 13 Nov 2024 18:46

Tgt Ion: 65 Resp: 111434
Ion Ratio Lower Upper
65 100
67 52.2 0.0 109.6


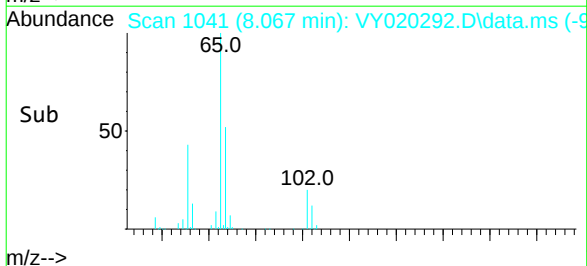
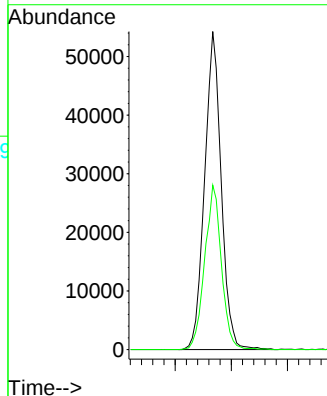
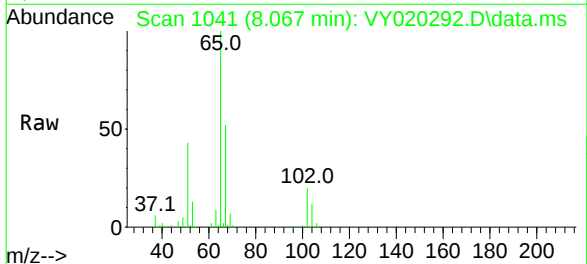


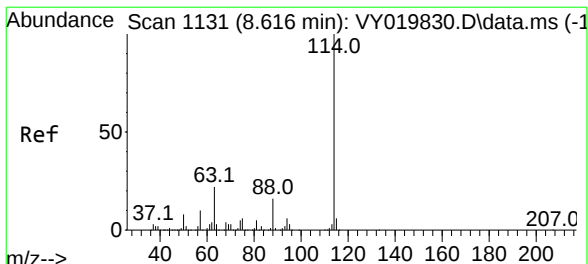

#34
1,4-Difluorobenzene
Concen: 50.000 ug/l
RT: 8.622 min Scan# 11
Delta R.T. 0.006 min
Lab File: VY020292.D
Acq: 13 Nov 2024 18:46




Instrument :
MSVOA_Y
ClientSampleId :
SOIL-5


Tgt Ion:	114	Resp:	324534
Ion	Ratio	Lower	Upper
114	100		
63	21.5	0.0	35.0
88	15.3	0.0	27.2

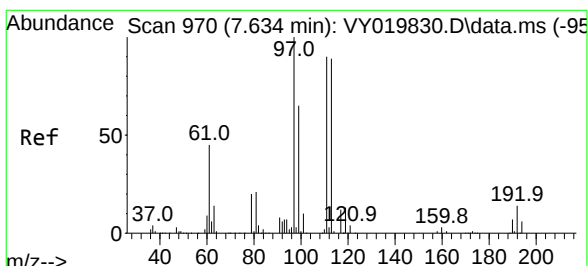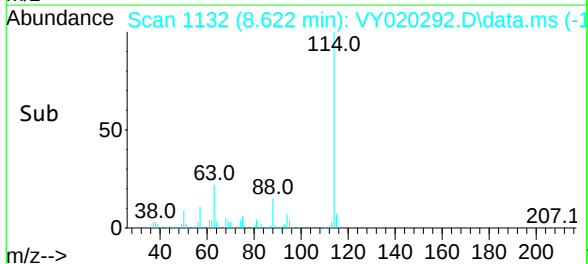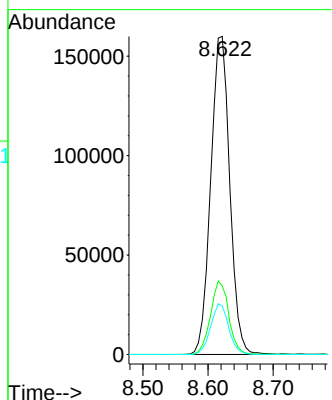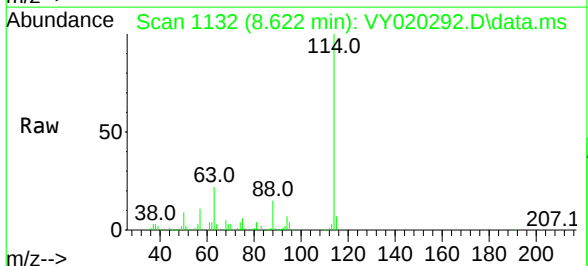

#35
Dibromofluoromethane
Concen: 65.341 ug/l
RT: 7.640 min Scan# 971
Delta R.T. 0.006 min
Lab File: VY020292.D
Acq: 13 Nov 2024 18:46

Tgt Ion:	113	Resp:	134823
Ion	Ratio	Lower	Upper
113	100		
111	104.0	82.2	123.4
192	16.6	15.9	23.9

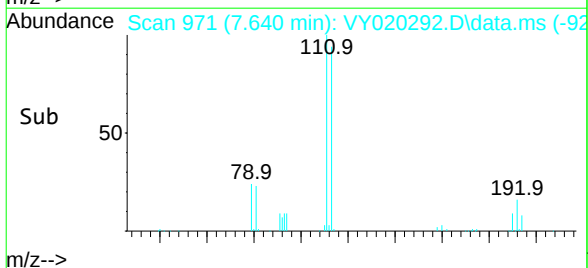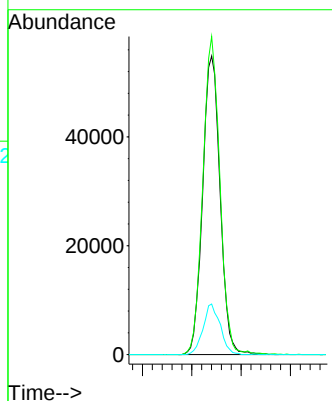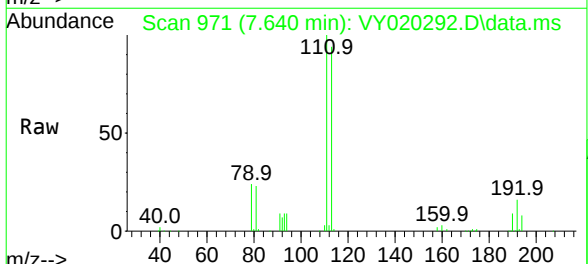

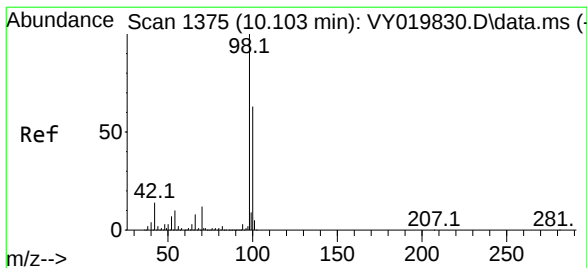

#50

Toluene-d8

Concen: 48.539 ug/l

RT: 10.109 min Scan# 1375

Delta R.T. 0.000 min

Lab File: VY020292.D

Acq: 13 Nov 2024 18:46

Instrument :

MSVOA_Y

ClientSampleId :





SOIL-5

Tgt Ion: 98 Resp: 398660

Ion Ratio Lower Upper

98 100

100 64.2 52.0 78.0

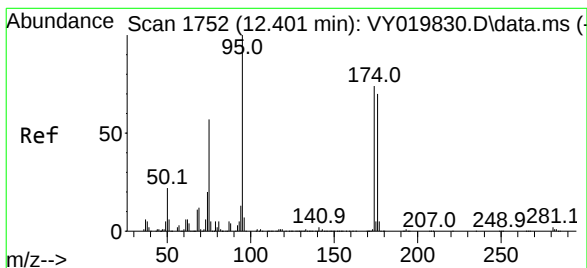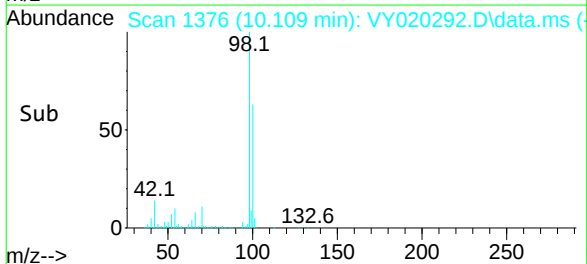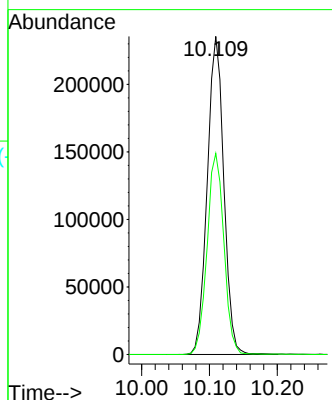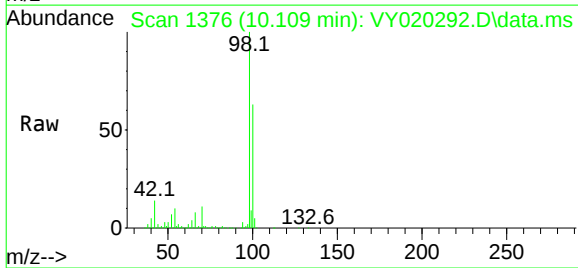

#62

4-Bromofluorobenzene

Concen: 44.620 ug/l

RT: 12.408 min Scan# 1753

Delta R.T. 0.000 min

Lab File: VY020292.D

Acq: 13 Nov 2024 18:46




Tgt Ion: 95 Resp: 119036


Ion Ratio Lower Upper

95 100

174 74.9 0.0 175.6

176 70.5 0.0 171.4

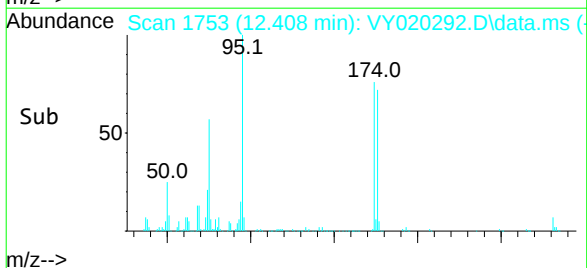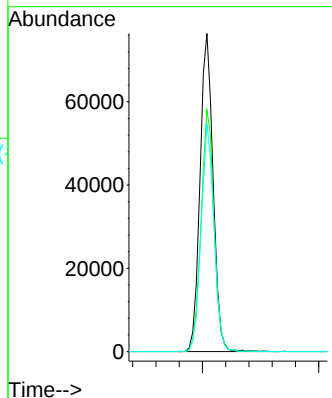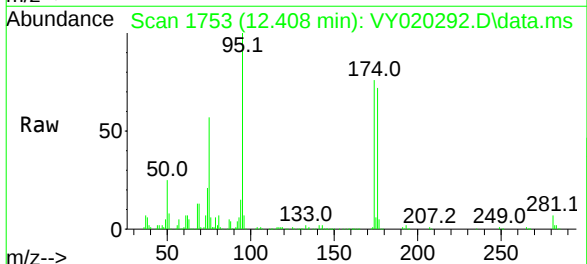

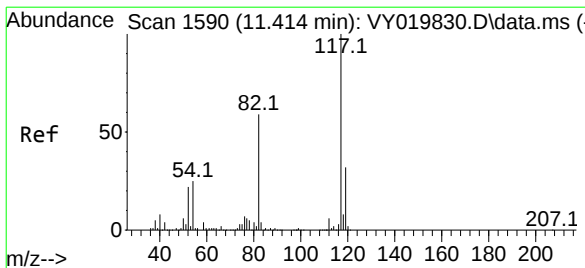

#63

Chlorobenzene-d5

Concen: 50.000 ug/l

RT: 11.420 min Scan# 1591

Delta R.T. 0.000 min

Lab File: VY020292.D

Acq: 13 Nov 2024 18:46

Instrument :

MSVOA_Y

ClientSampleId :

SOIL-5





Tgt Ion:117 Resp: 313306

Ion Ratio Lower Upper

117 100

82 59.0 42.4 63.6

119 31.1 25.9 38.9

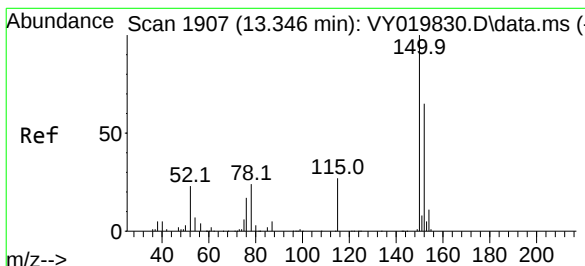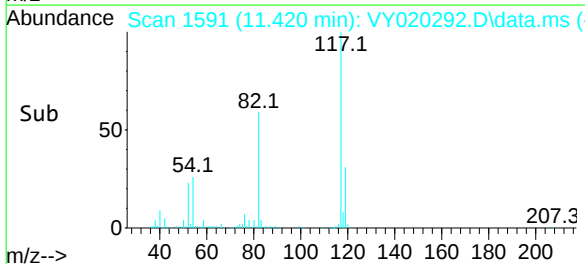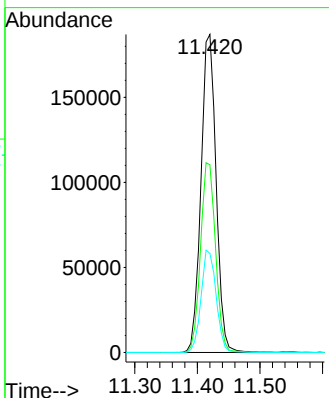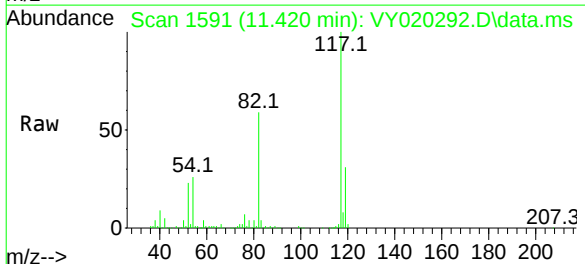

#72

1,4-Dichlorobenzene-d4

Concen: 50.000 ug/l

RT: 13.347 min Scan# 1907

Delta R.T. 0.000 min

Lab File: VY020292.D

Acq: 13 Nov 2024 18:46

Tgt Ion:152 Resp: 137784

Ion Ratio Lower Upper

152 100

115 61.7 28.2 84.7

150 155.5 0.0 345.6

