
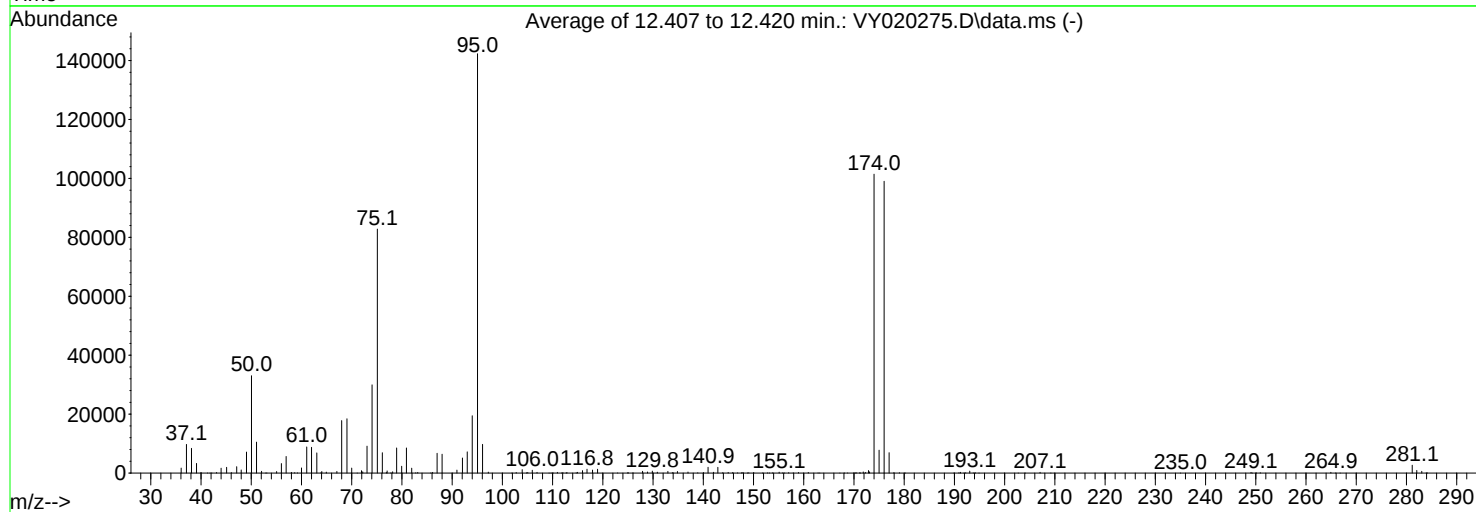


Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY111324\
Data File : VY020275.D
Acq On : 13 Nov 2024 09:22
Operator : SY/MD
Sample : BFB
Misc : 5.00g/5.0mL/MSVOA_Y/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_Y
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y103024S.M
Title : SW846 8260
Last Update : Thu Oct 31 15:23:13 2024

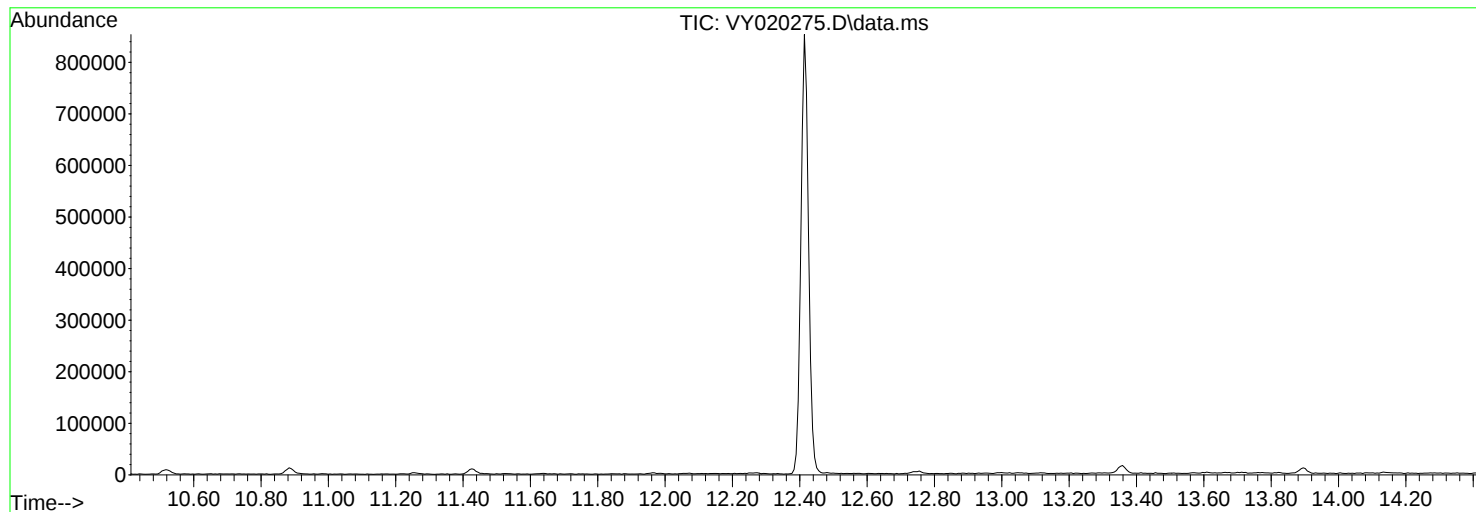

AutoFind: Scans 1753, 1754, 1755; Background Corrected with Scan 1744

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	23.2	33043	PASS
75	95	30	60	58.2	82803	PASS
95	95	100	100	100.0	142315	PASS
96	95	5	9	6.9	9749	PASS
173	174	0.00	2	0.8	860	PASS
174	95	50	100	71.3	101435	PASS
175	174	5	9	7.7	7768	PASS
176	174	95	101	97.6	99024	PASS
177	176	5	9	7.0	6934	PASS