

Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY121125\
 Data File : VY023945.D
 Acq On : 11 Dec 2025 11:09
 Operator : SY/MD
 Sample : Q3827-01
 Misc : 5.08g/5.0mL/MSVOA_Y/SOIL/A
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 MSVOA_Y
 ClientSampleId :
 RT4262

Quant Time: Dec 12 03:20:11 2025
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y121025S.M
 Quant Title : SW846 8260
 QLast Update : Thu Dec 11 03:57:51 2025
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Pentafluorobenzene	7.713	168	740700	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	8.615	114	1276389	50.000	ug/l	0.00
63) Chlorobenzene-d5	11.420	117	1087589	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.346	152	458740	50.000	ug/l	0.00

System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.067	65	352004	53.750	ug/l	0.00
Spiked Amount	50.000	Range	50 - 163	Recovery	=	107.500%
35) Dibromofluoromethane	7.640	113	396830	47.561	ug/l	0.00
Spiked Amount	50.000	Range	54 - 147	Recovery	=	95.120%
50) Toluene-d8	10.109	98	1462050	47.065	ug/l	0.00
Spiked Amount	50.000	Range	58 - 134	Recovery	=	94.140%
62) 4-Bromofluorobenzene	12.407	95	430846	41.531	ug/l	0.00
Spiked Amount	50.000	Range	30 - 143	Recovery	=	83.060%


Target Compounds	Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY121125\
Data File : VY023945.D
Acq On : 11 Dec 2025 11:09
Operator : SY/MD
Sample : Q3827-01
Misc : 5.08g/5.0mL/MSVOA_Y/SOIL/A
ALS Vial : 2 Sample Multiplier: 1

Instrument :
MSVOA_Y
ClientSampleId :
RT4262

Quant Time: Dec 12 03:20:11 2025
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y121025S.M
Quant Title : SW846 8260
QLast Update : Thu Dec 11 03:57:51 2025
Response via : Initial Calibration




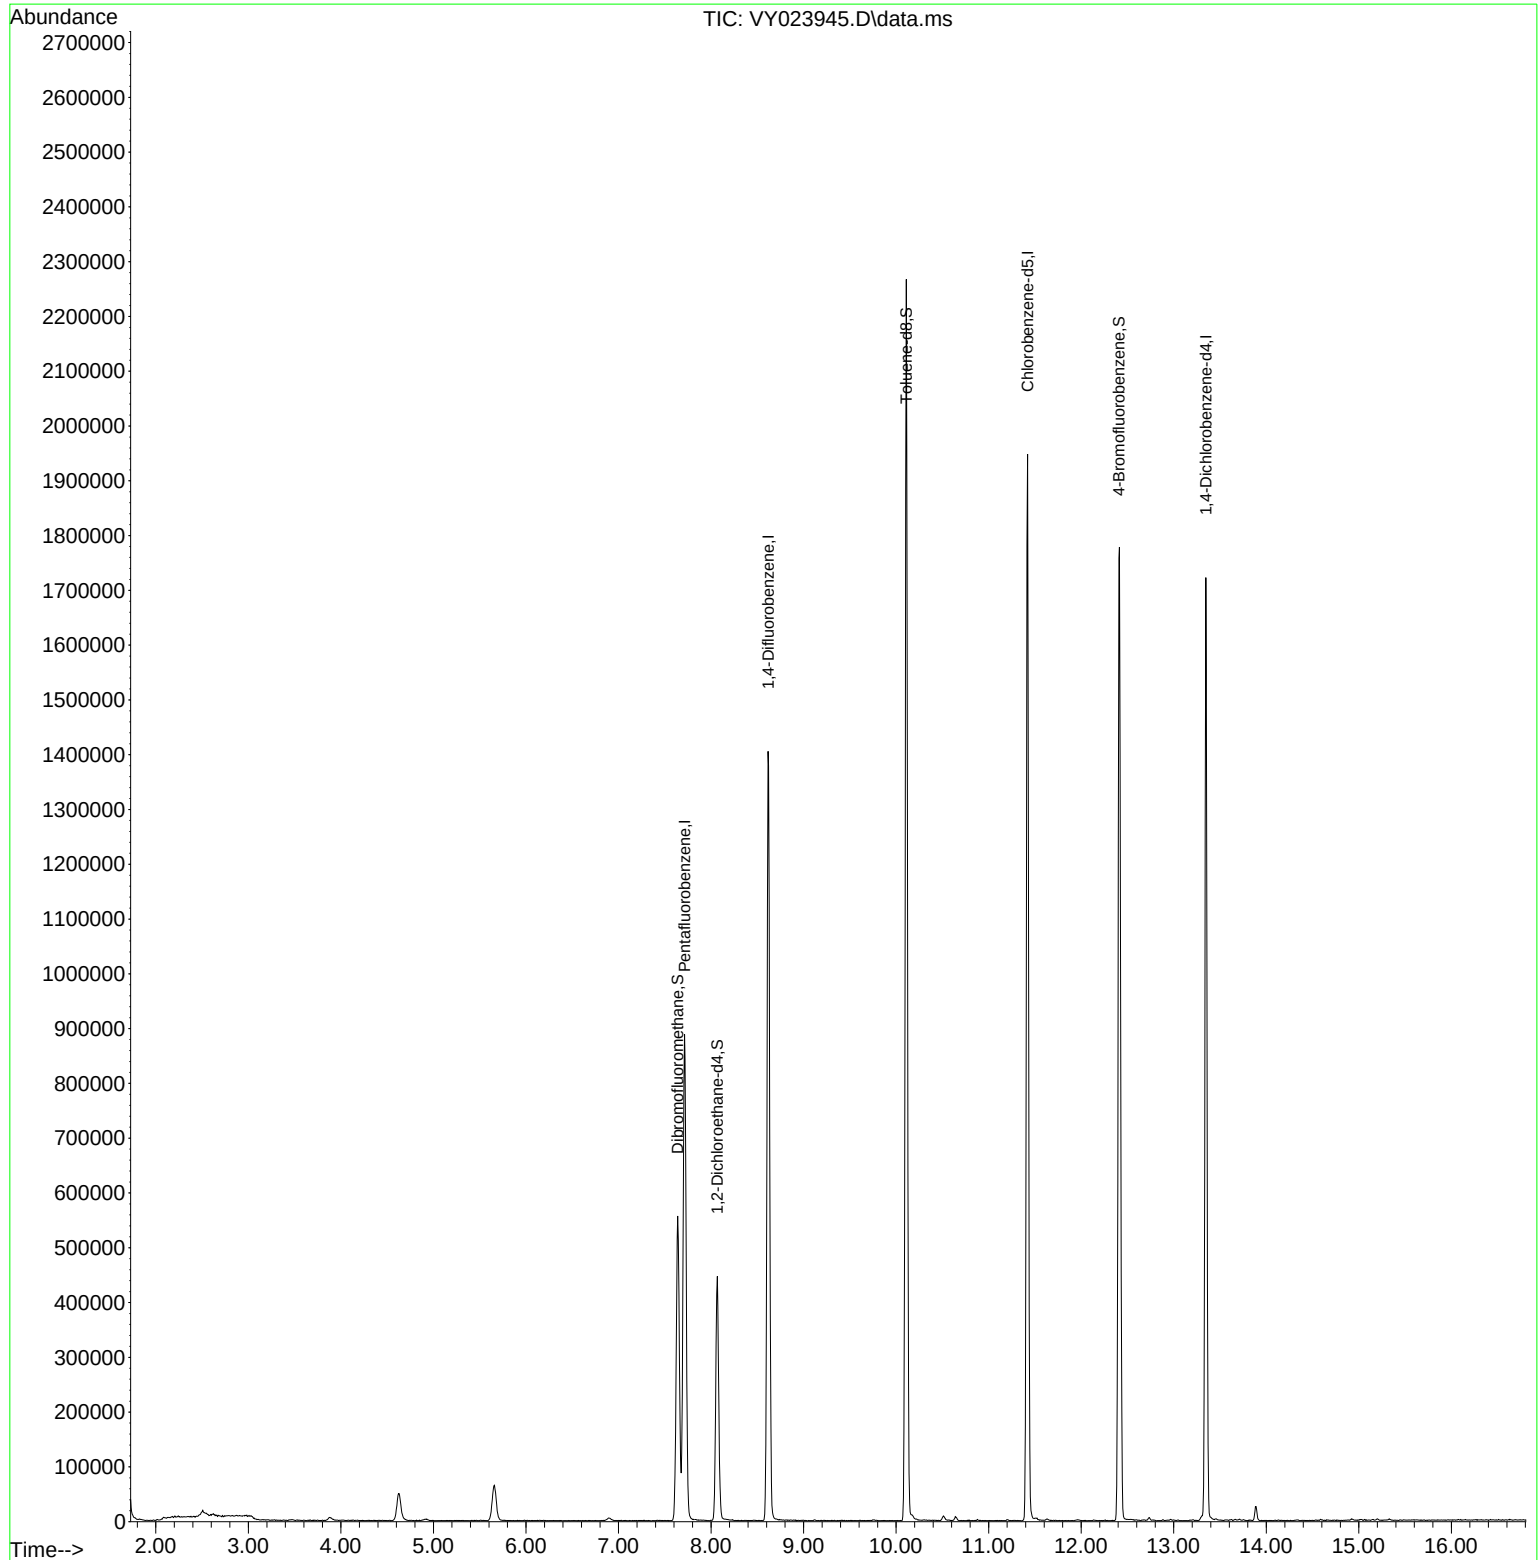


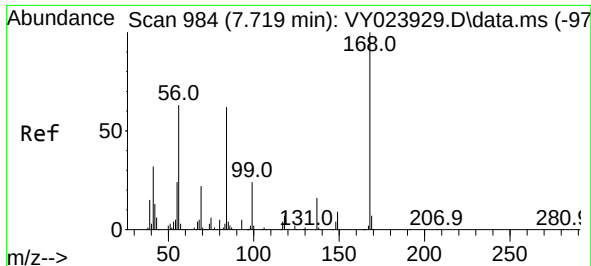

#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 7.713 min Scan# 984
Delta R.T. -0.006 min
Lab File: VY023945.D
Acq: 11 Dec 2025 11:09




Instrument :
MSVOA_Y
ClientSampleId :
RT4262


Tgt Ion:168 Resp: 740700
Ion Ratio Lower Upper
168 100
99 50.8 38.9 58.3

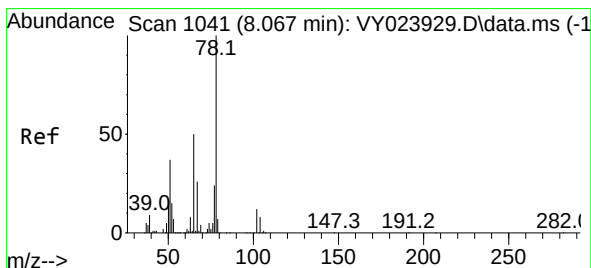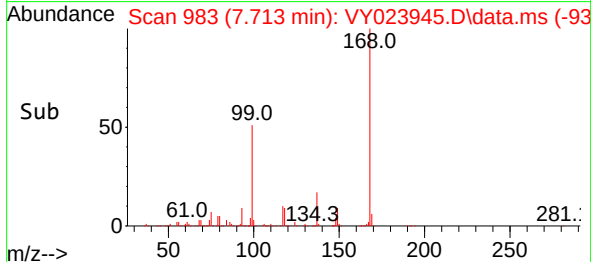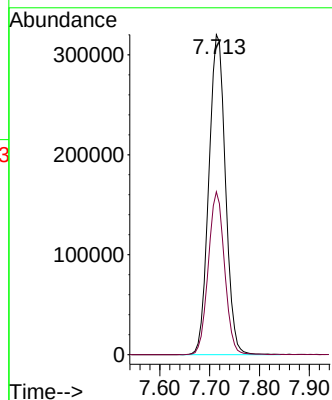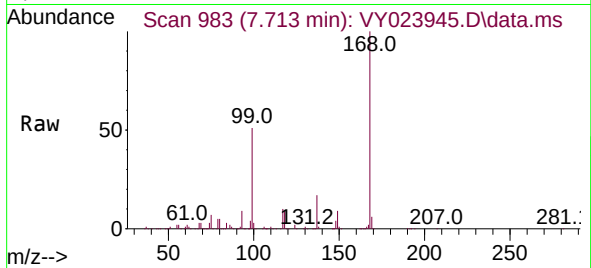

#33
1,2-Dichloroethane-d4
Concen: 53.750 ug/l
RT: 8.067 min Scan# 1041
Delta R.T. -0.000 min
Lab File: VY023945.D
Acq: 11 Dec 2025 11:09

Tgt Ion: 65 Resp: 352004
Ion Ratio Lower Upper
65 100
67 52.7 0.0 106.2

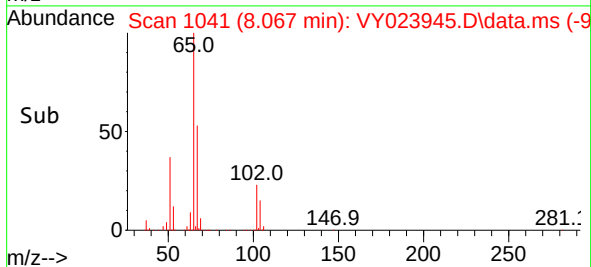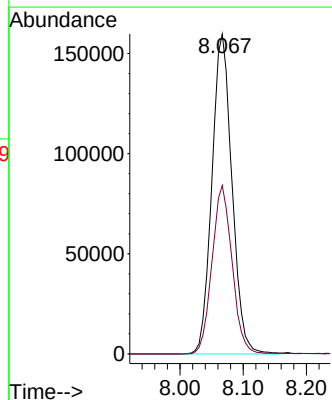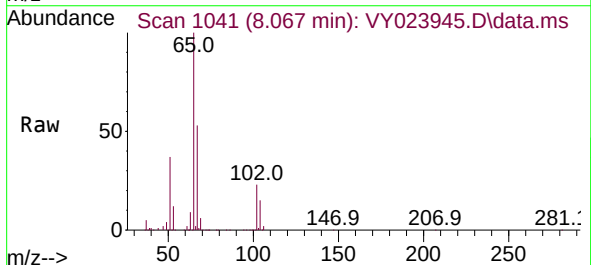

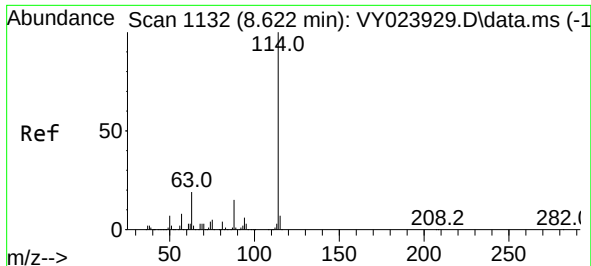

#34

1,4-Difluorobenzene

Concen: 50.000 ug/l

RT: 8.615 min Scan# 1131

Delta R.T. -0.006 min

Lab File: VY023945.D

Acq: 11 Dec 2025 11:09

Instrument :

MSVOA_Y

ClientSampleId :

RT4262





Tgt Ion:114 Resp: 1276389

Ion Ratio Lower Upper

114 100

63 18.1 0.0 37.2

88 14.8 0.0 29.4

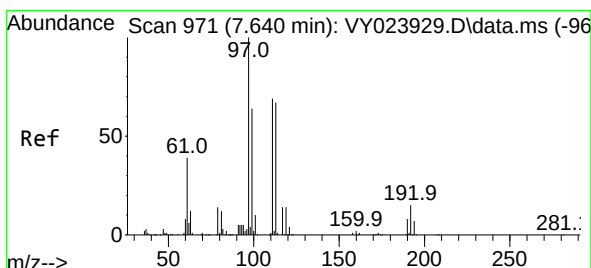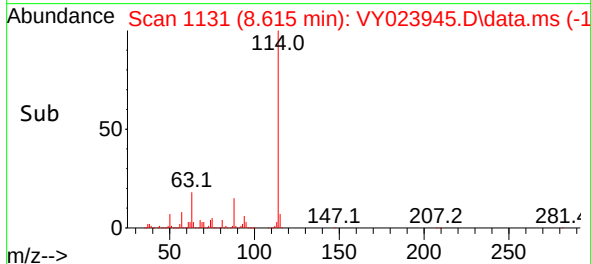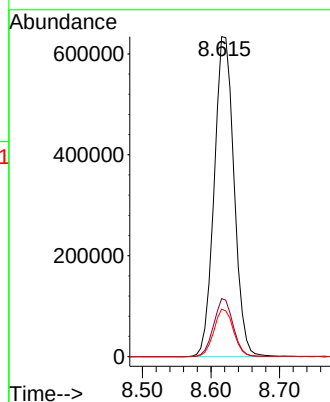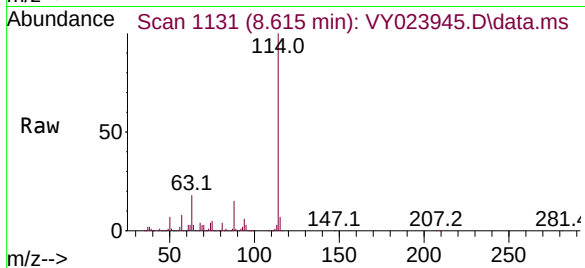

#35

Dibromofluoromethane

Concen: 47.561 ug/l

RT: 7.640 min Scan# 971

Delta R.T. -0.000 min

Lab File: VY023945.D

Acq: 11 Dec 2025 11:09




Tgt Ion:113 Resp: 396830


Ion Ratio Lower Upper

113 100

111 102.7 82.4 123.6

192 22.2 17.9 26.9


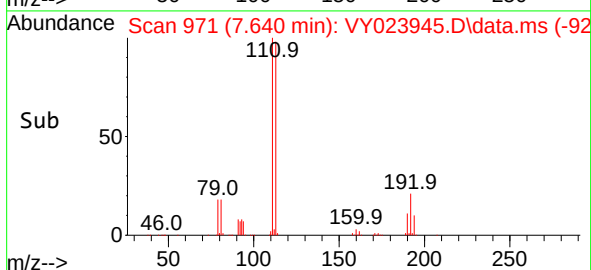
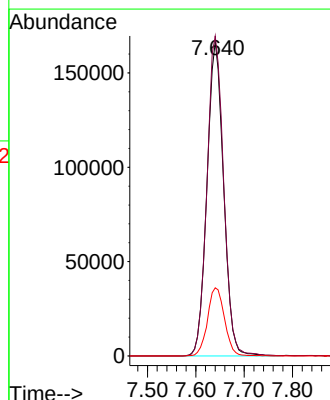
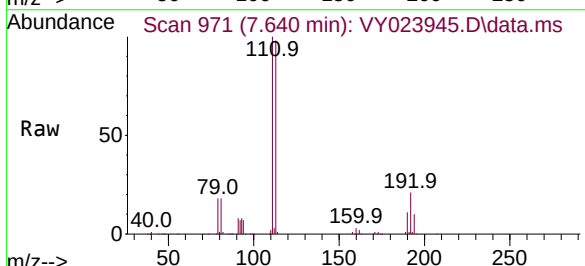


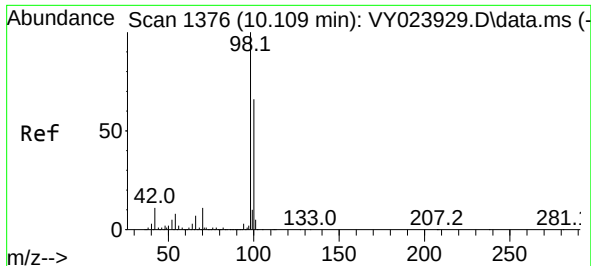

#50
Toluene-d8
Concen: 47.065 ug/l
RT: 10.109 min Scan# 1376
Delta R.T. -0.000 min
Lab File: VY023945.D
Acq: 11 Dec 2025 11:09




Instrument :
MSVOA_Y
ClientSampleId :
RT4262


Tgt Ion: 98 Resp: 1462050
Ion Ratio Lower Upper
98 100
100 65.5 52.8 79.2

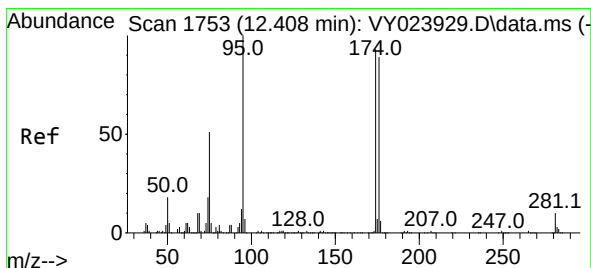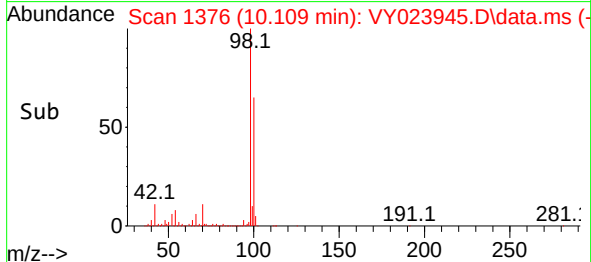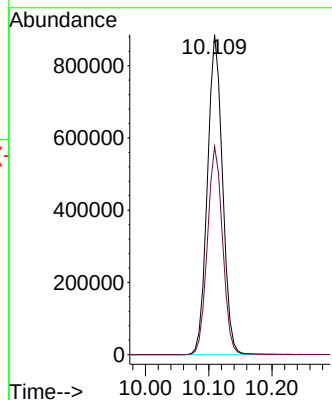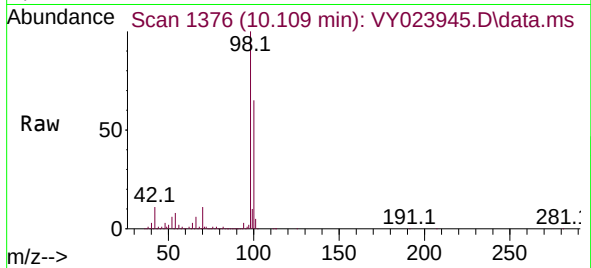

#62
4-Bromofluorobenzene
Concen: 41.531 ug/l
RT: 12.407 min Scan# 1753
Delta R.T. -0.000 min
Lab File: VY023945.D
Acq: 11 Dec 2025 11:09

Tgt Ion: 95 Resp: 430846
Ion Ratio Lower Upper
95 100
174 95.3 0.0 187.4
176 93.0 0.0 179.6


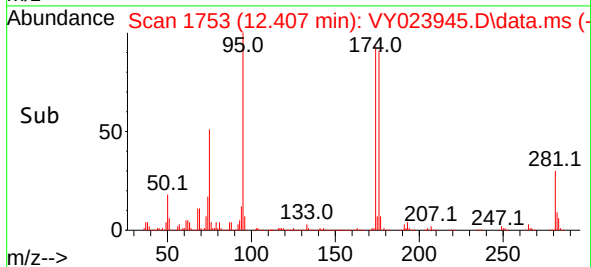
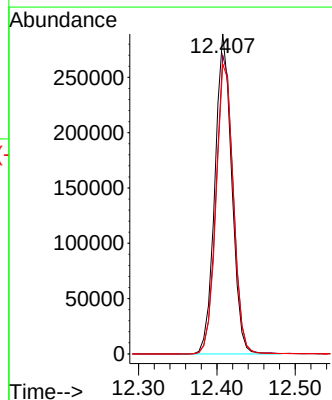
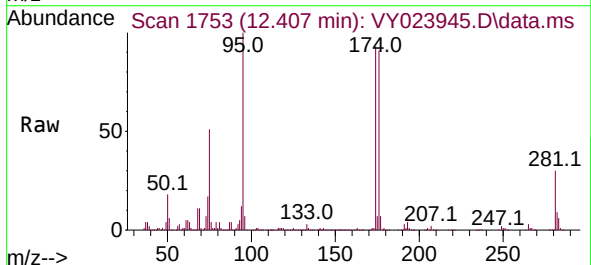


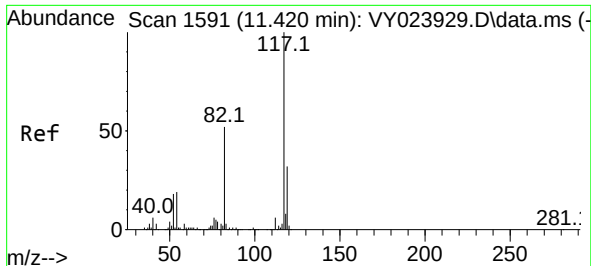

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 11.420 min Scan# 11
Delta R.T. -0.000 min
Lab File: VY023945.D
Acq: 11 Dec 2025 11:09

Instrument :
MSVOA_Y
ClientSampleId :
RT4262

Tgt Ion:117 Resp: 1087589
Ion Ratio Lower Upper
117 100
82 51.3 41.4 62.2
119 32.1 25.5 38.3

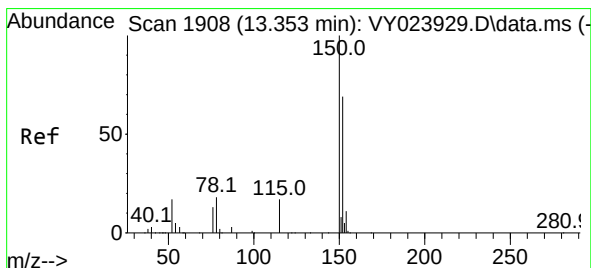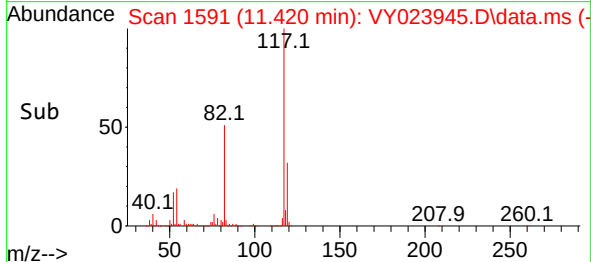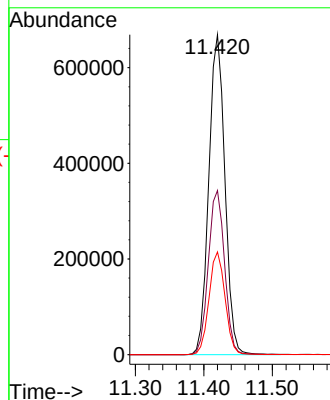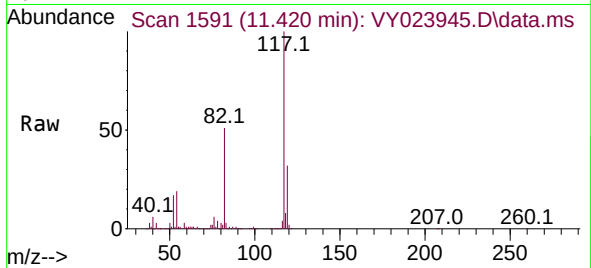

#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 13.346 min Scan# 1907
Delta R.T. -0.006 min
Lab File: VY023945.D
Acq: 11 Dec 2025 11:09

Tgt Ion:152 Resp: 458740
Ion Ratio Lower Upper
152 100
115 54.1 27.3 81.9
150 155.9 0.0 347.6

