

Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY122222\
 Data File : VY011971.D
 Acq On : 22 Dec 2022 13:51
 Operator : KP/MD
 Sample : N6160-04
 Misc : 5.40g/5.0mL/MSVOA_Y/SOIL
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_Y
 ClientSampleId :
 VOC-8-3051

Quant Time: Dec 23 04:32:00 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y122022S.M
 Quant Title : SW846 8260
 QLast Update : Tue Dec 20 12:37:37 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) Pentafluorobenzene	7.789	168	193071	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	8.691	114	336948	50.000	ug/l	0.00
63) Chlorobenzene-d5	11.489	117	308269	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.428	152	134179	50.000	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.143	65	115414	59.334	ug/l	0.00
Spiked Amount	50.000	Range	50 - 163	Recovery	=	118.660%
35) Dibromofluoromethane	7.716	113	104789	51.658	ug/l	0.00
Spiked Amount	50.000	Range	54 - 147	Recovery	=	103.320%
50) Toluene-d8	10.179	98	409419	49.746	ug/l	0.00
Spiked Amount	50.000	Range	49 - 140	Recovery	=	99.500%
62) 4-Bromofluorobenzene	12.483	95	125698	45.411	ug/l	0.00
Spiked Amount	50.000	Range	25 - 144	Recovery	=	90.820%
Target Compounds						
29) Tetrahydrofuran	7.350	42	3264	8.891	ug/l	96


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY122222\
Data File : VY011971.D
Acq On : 22 Dec 2022 13:51
Operator : KP/MD
Sample : N6160-04
Misc : 5.40g/5.0mL/MSVOA_Y/SOIL
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_Y
ClientSampleId :
VOC-8-3051

Quant Time: Dec 23 04:32:00 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y122022S.M
Quant Title : SW846 8260
QLast Update : Tue Dec 20 12:37:37 2022
Response via : Initial Calibration




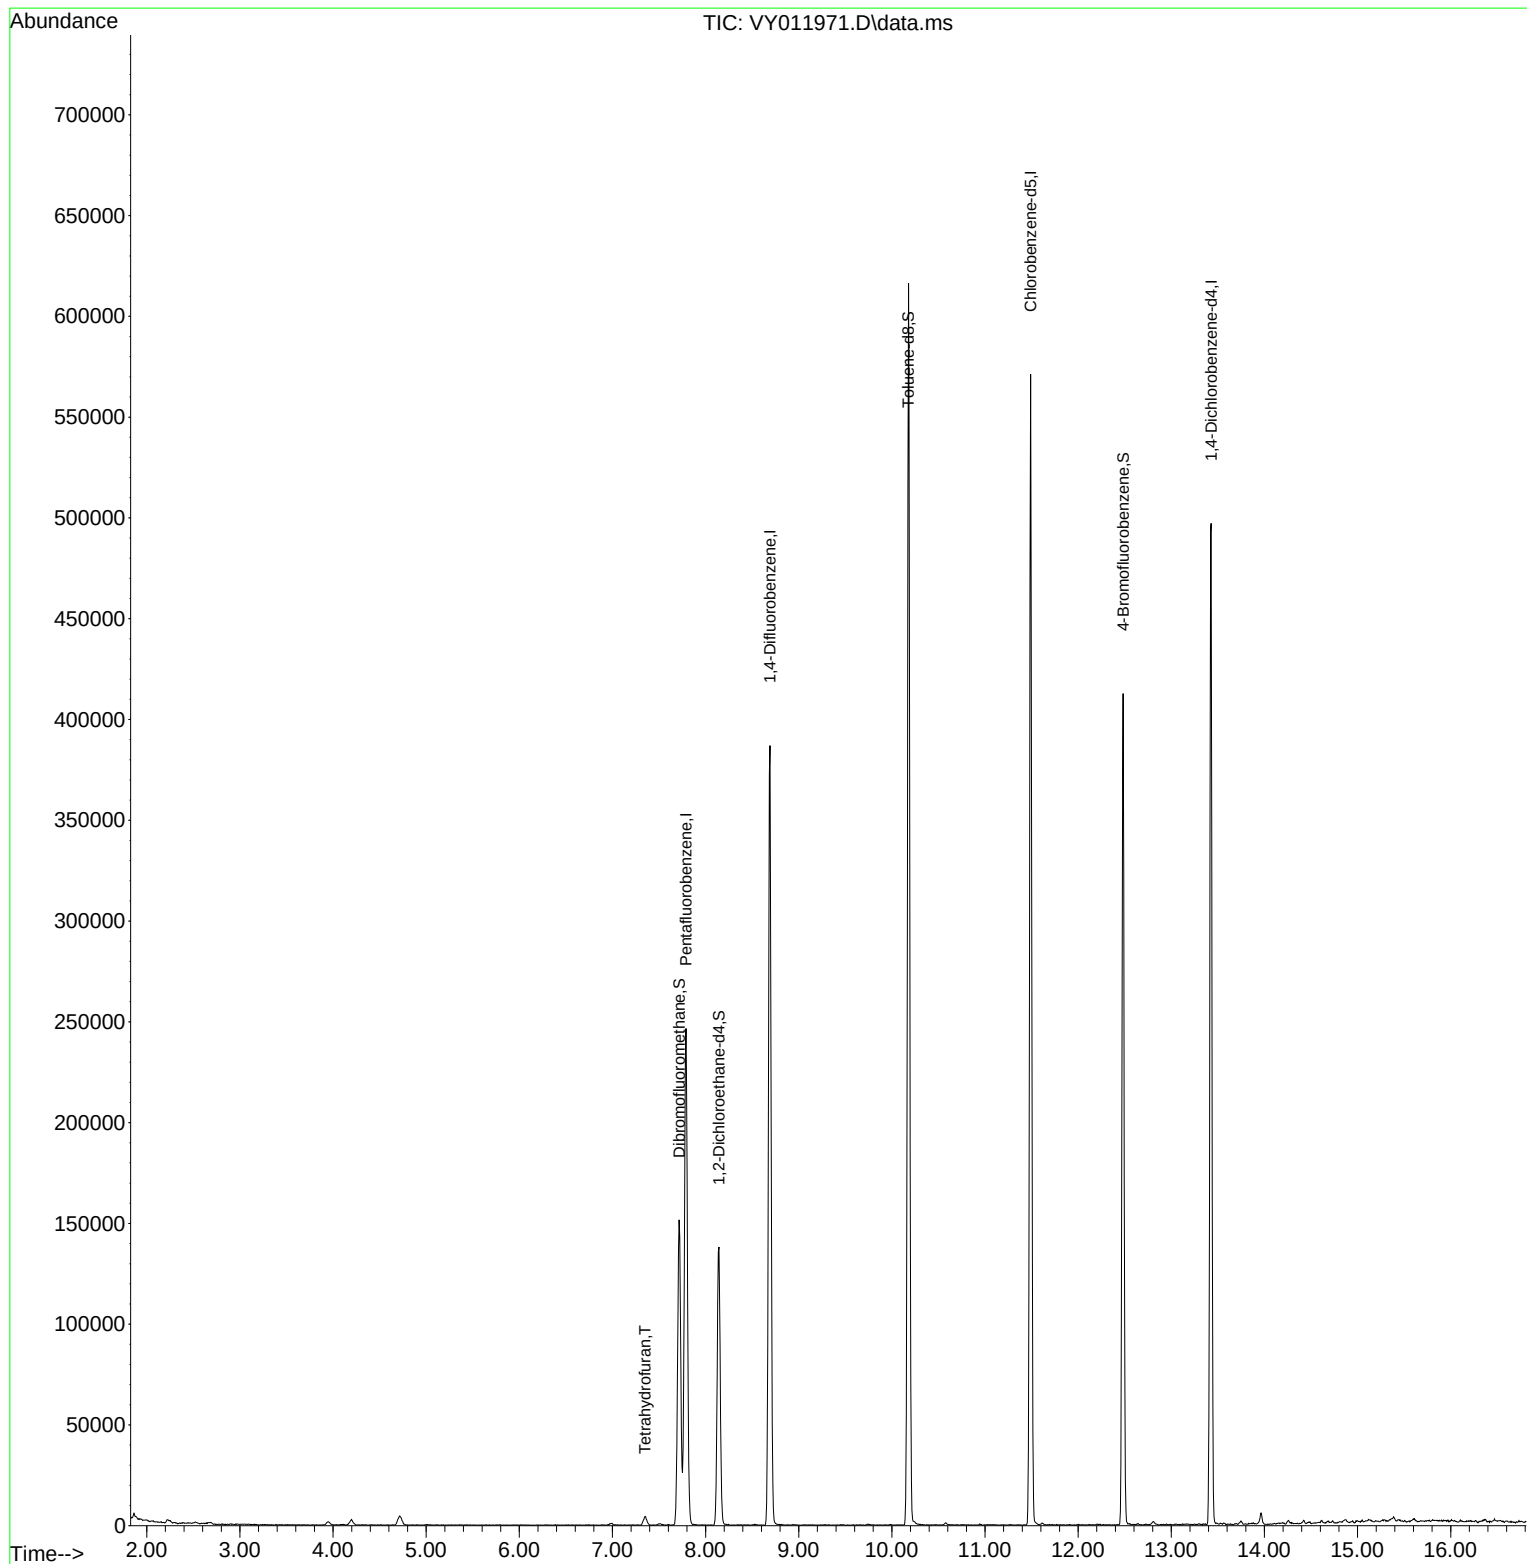


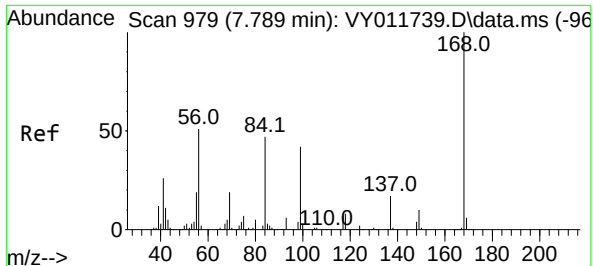

#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 7.789 min Scan# 91
Delta R.T. -0.000 min
Lab File: VY011971.D
Acq: 22 Dec 2022 13:51




Instrument :
MSVOA_Y
ClientSampleId :
VOC-8-3051


Tgt Ion:168 Resp: 193071
Ion Ratio Lower Upper
168 100
99 55.5 44.0 66.0

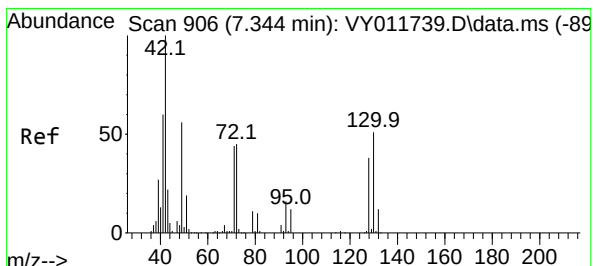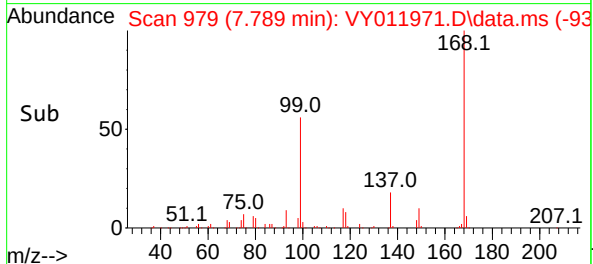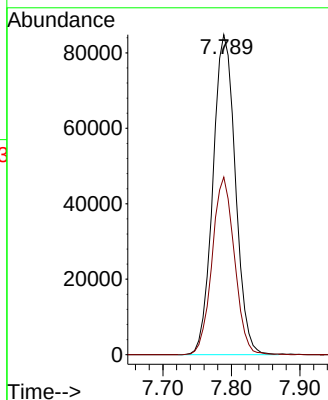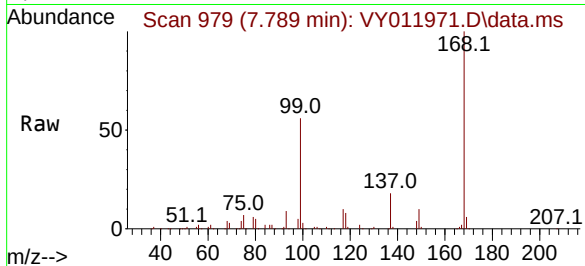

#29
Tetrahydrofuran
Concen: 8.891 ug/l
RT: 7.350 min Scan# 907
Delta R.T. 0.006 min
Lab File: VY011971.D
Acq: 22 Dec 2022 13:51

Tgt Ion: 42 Resp: 3264
Ion Ratio Lower Upper
42 100
72 49.8 37.0 55.6
71 45.7 34.9 52.3

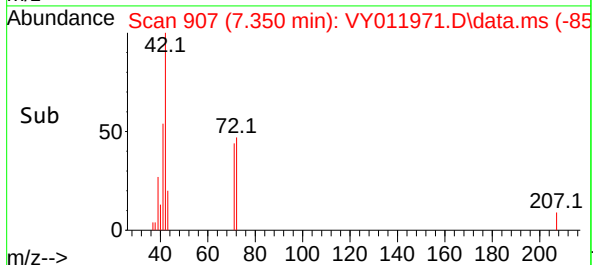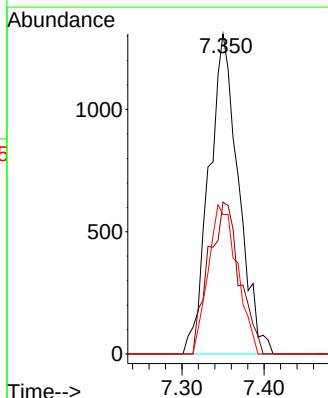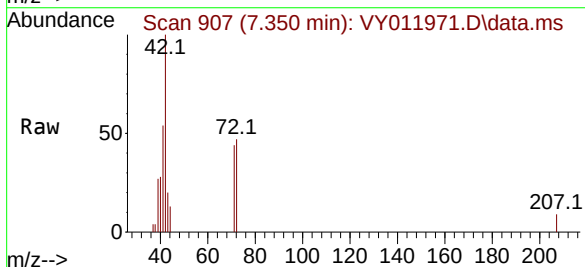

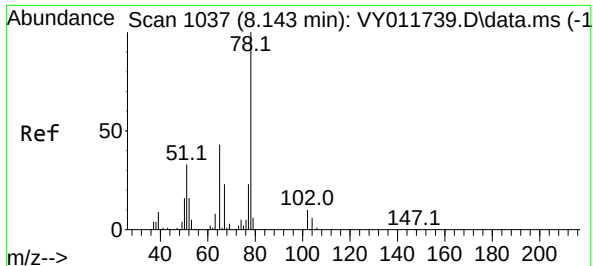

#33

1,2-Dichloroethane-d4

Concen: 59.334 ug/l

RT: 8.143 min Scan# 1037

Delta R.T. -0.001 min

Lab File: VY011971.D

Acq: 22 Dec 2022 13:51

Instrument :

MSVOA_Y

ClientSampleId :





VOC-8-3051

Tgt Ion: 65 Resp: 115414

Ion Ratio Lower Upper

65 100

67 50.6 0.0 103.2

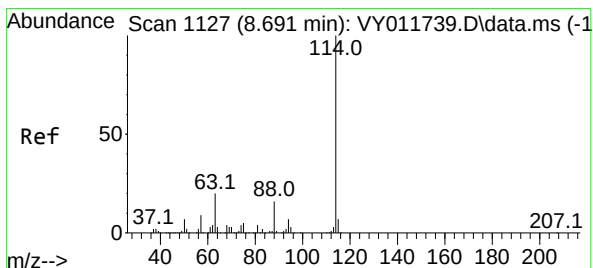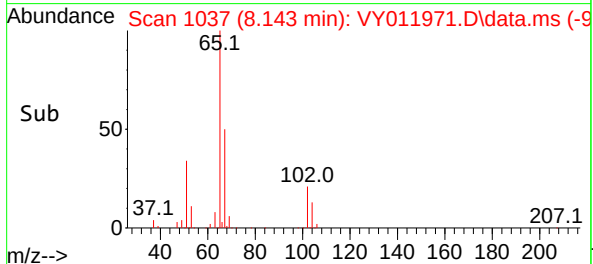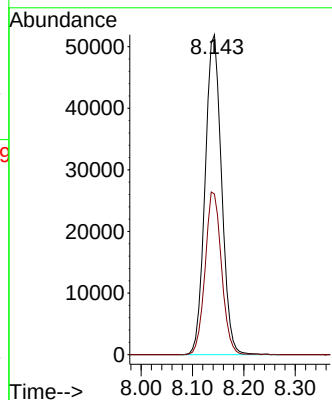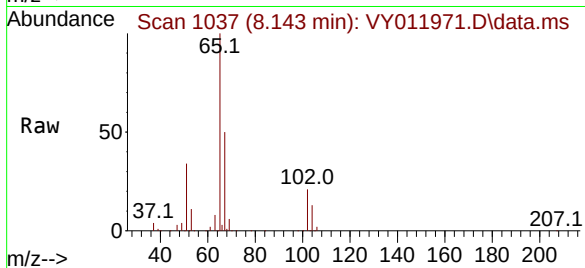

#34

1,4-Difluorobenzene

Concen: 50.000 ug/l

RT: 8.691 min Scan# 1127

Delta R.T. 0.000 min

Lab File: VY011971.D

Acq: 22 Dec 2022 13:51




Tgt Ion: 114 Resp: 336948


Ion Ratio Lower Upper

114 100

63 18.2 0.0 39.6

88 15.3 0.0 32.2


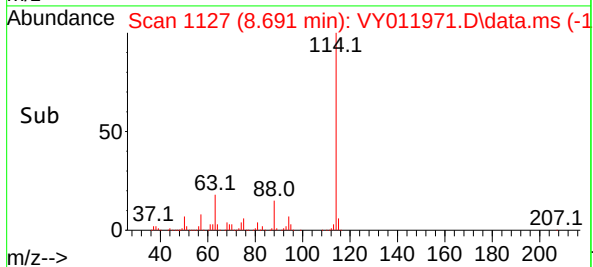
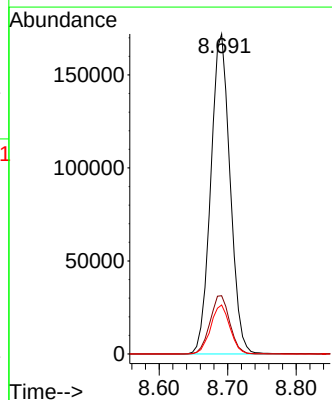
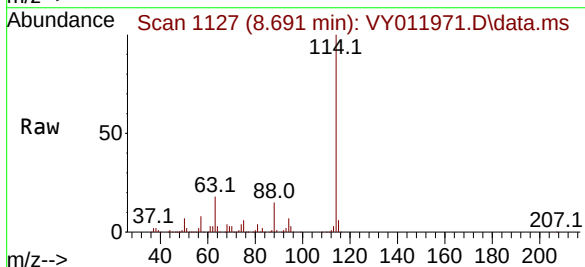


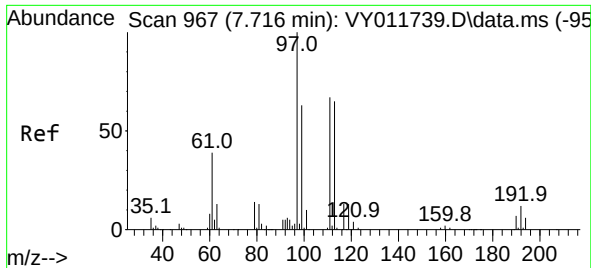

#35
Dibromofluoromethane
Concen: 51.658 ug/l
RT: 7.716 min Scan# 967
Delta R.T. -0.000 min
Lab File: VY011971.D
Acq: 22 Dec 2022 13:51




Instrument :
MSVOA_Y
ClientSampleId :
VOC-8-3051


Tgt Ion:113 Resp: 104789
Ion Ratio Lower Upper
113 100
111 102.1 83.0 124.4
192 21.1 16.0 24.0

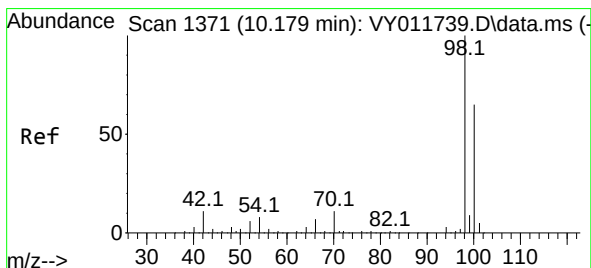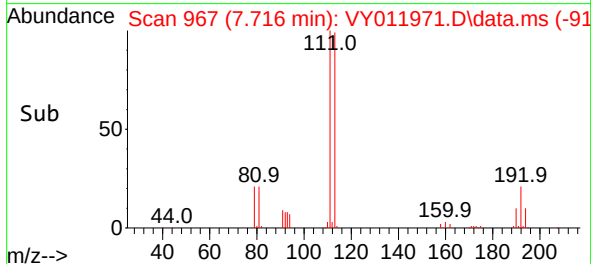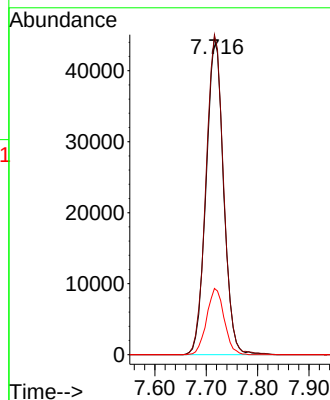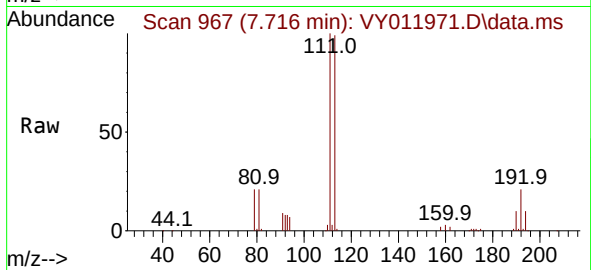

#50
Toluene-d8
Concen: 49.746 ug/l
RT: 10.179 min Scan# 1371
Delta R.T. -0.000 min
Lab File: VY011971.D
Acq: 22 Dec 2022 13:51

Tgt Ion: 98 Resp: 409419
Ion Ratio Lower Upper
98 100
100 64.1 51.9 77.9


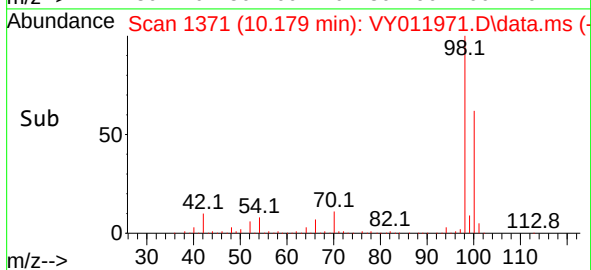
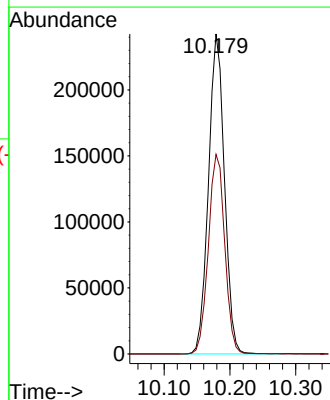
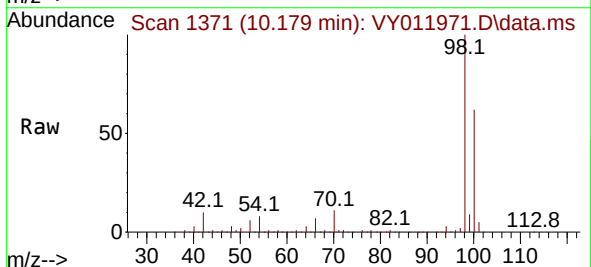


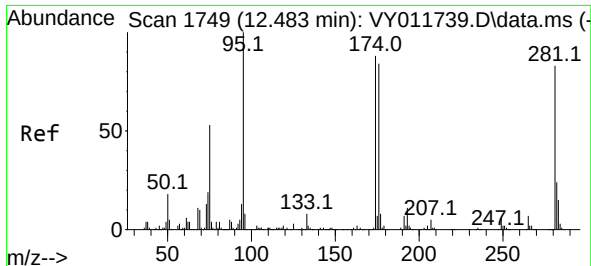

#62
4-Bromofluorobenzene
Concen: 45.411 ug/l
RT: 12.483 min Scan# 1749
Delta R.T. 0.000 min
Lab File: VY011971.D
Acq: 22 Dec 2022 13:51




Instrument :
MSVOA_Y
ClientSampleId :
VOC-8-3051


Tgt Ion: 95 Resp: 125698
Ion Ratio Lower Upper
95 100
174 87.6 0.0 172.0
176 85.5 0.0 167.6

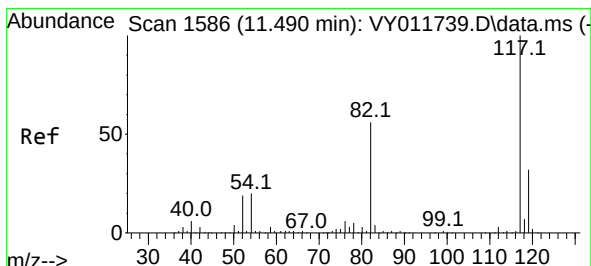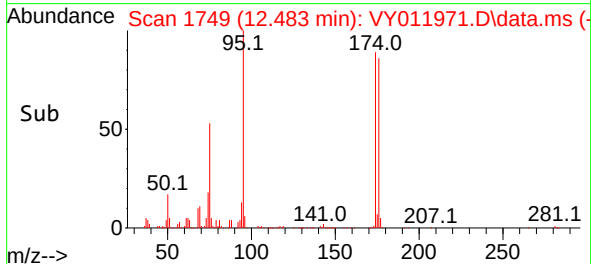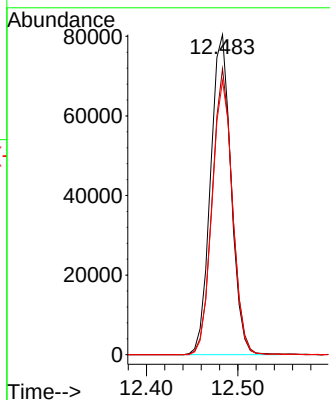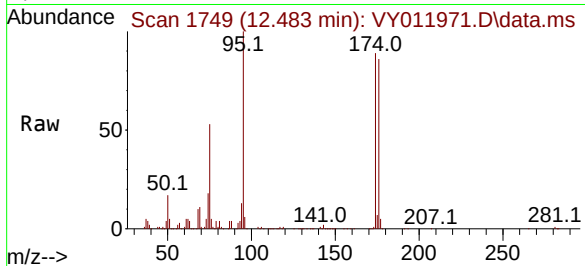

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 11.489 min Scan# 1586
Delta R.T. -0.000 min
Lab File: VY011971.D
Acq: 22 Dec 2022 13:51


Tgt Ion: 117 Resp: 308269
Ion Ratio Lower Upper
117 100
82 54.2 44.8 67.2
119 32.5 25.4 38.2

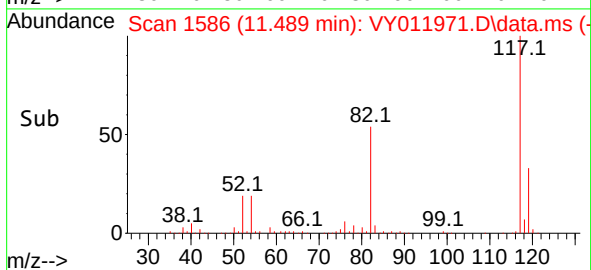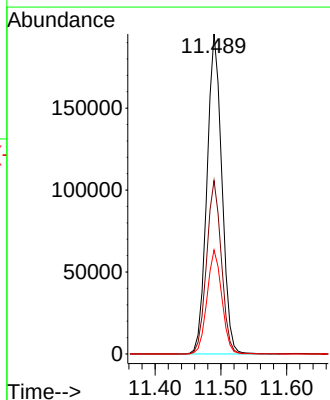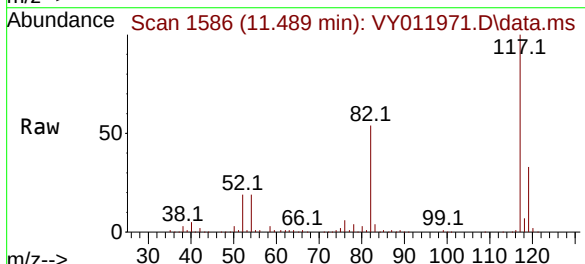

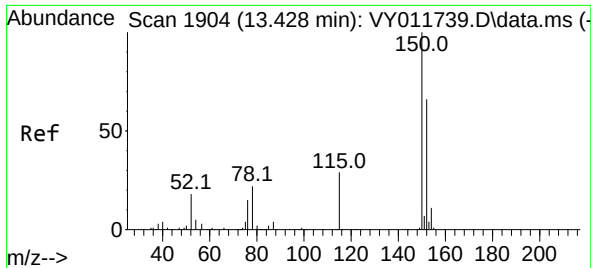

#72
 1,4-Dichlorobenzene-d4
 Concen: 50.000 ug/l
 RT: 13.428 min Scan# 1904
 Delta R.T. -0.000 min
 Lab File: VY011971.D
 Acq: 22 Dec 2022 13:51

Instrument :
 MSVOA_Y
 ClientSampleId :
 VOC-8-3051

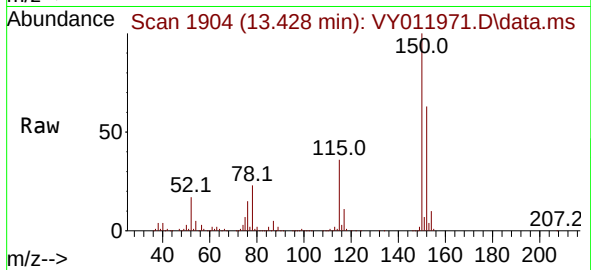

Tgt Ion:152 Resp: 134179
 Ion Ratio Lower Upper
 152 100
 115 57.7 29.1 87.3
 150 157.8 0.0 342.6

