


Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY122222\
Data File : VY011962.D
Acq On : 22 Dec 2022 09:28
Operator : KP/MD
Sample : BFB
Misc : 5.00g/5.0mL/MSVOA_Y/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_Y
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y122022S.M
Title : SW846 8260
Last Update : Tue Dec 20 12:37:37 2022

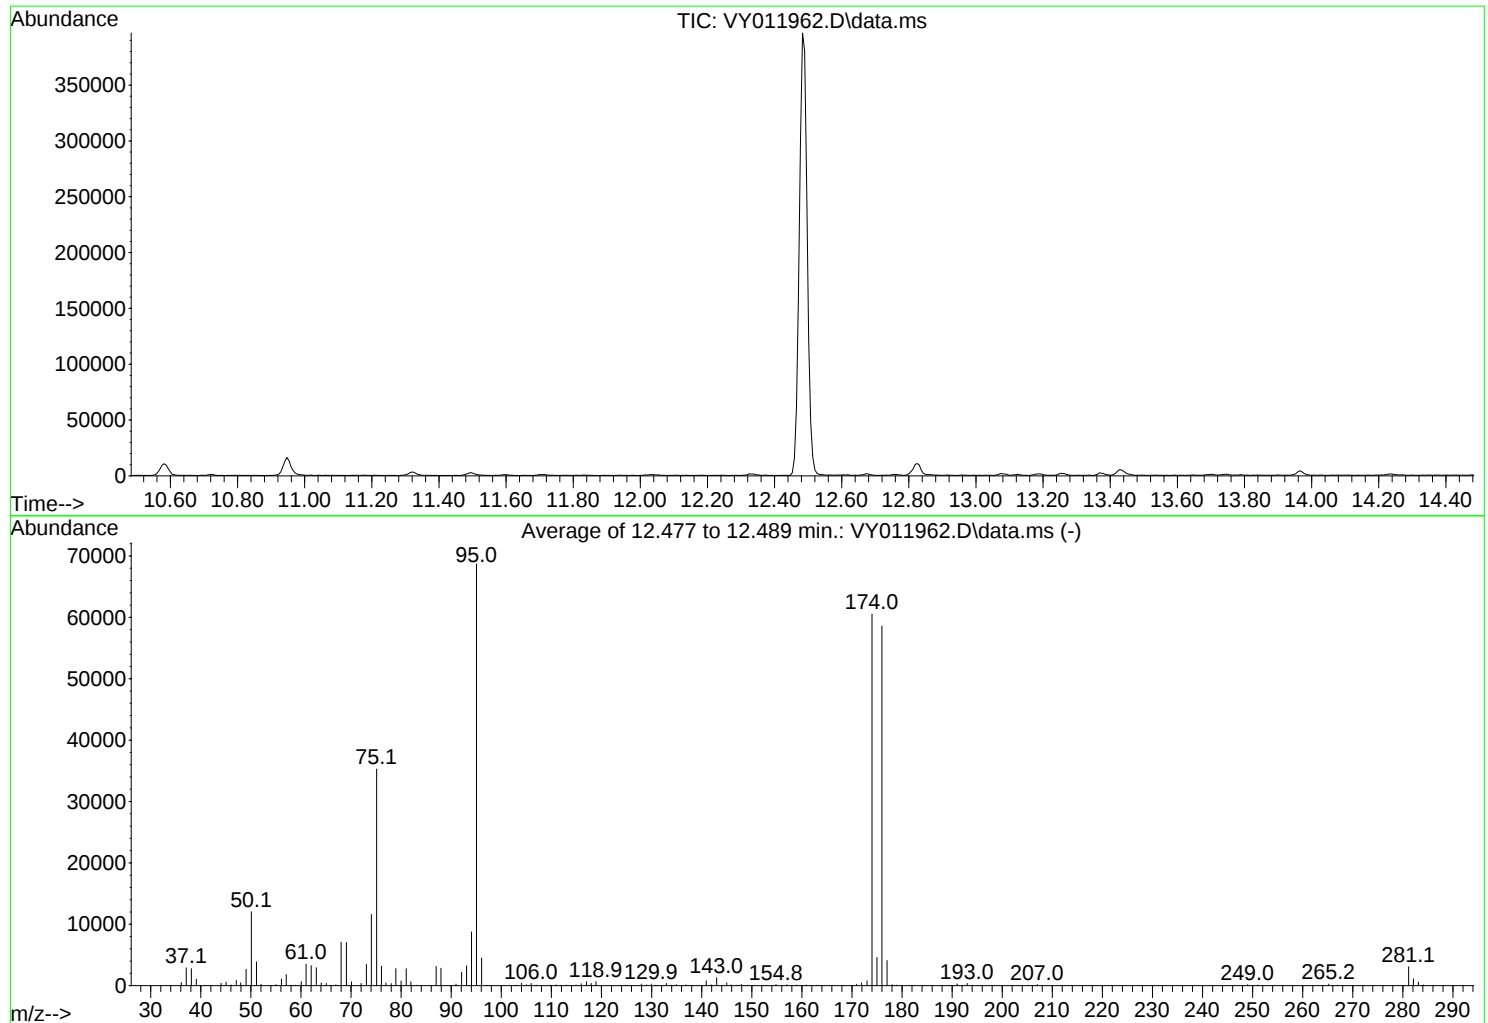

AutoFind: Scans 1748, 1749, 1750; Background Corrected with Scan 1740

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	17.5	12049	PASS
75	95	30	60	51.3	35283	PASS
95	95	100	100	100.0	68723	PASS
96	95	5	9	6.5	4475	PASS
173	174	0.00	2	1.3	795	PASS
174	95	50	100	88.1	60544	PASS
175	174	5	9	7.6	4588	PASS
176	174	95	101	96.8	58587	PASS
177	176	5	9	7.0	4094	PASS