
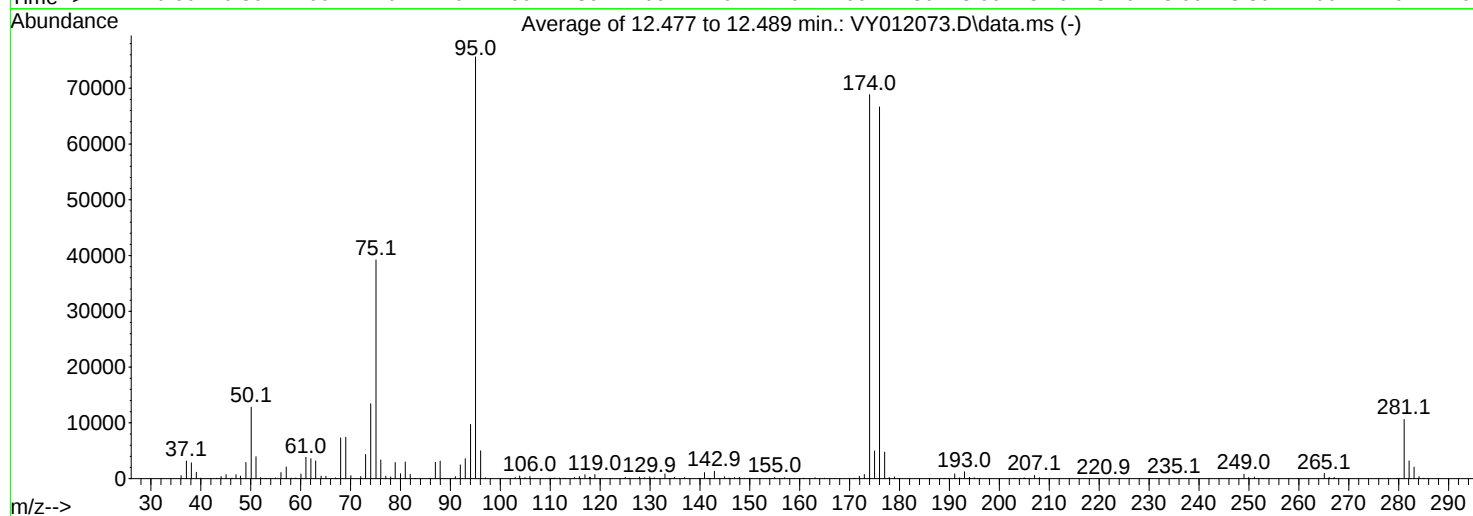


Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY010523\
Data File : VY012073.D
Acq On : 05 Jan 2023 09:20
Operator : KP/MD
Sample : BFB
Misc : 5.00g/5.0mL/MSVOA_Y/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_Y
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y122022S.M
Title : SW846 8260
Last Update : Tue Dec 20 12:37:37 2022

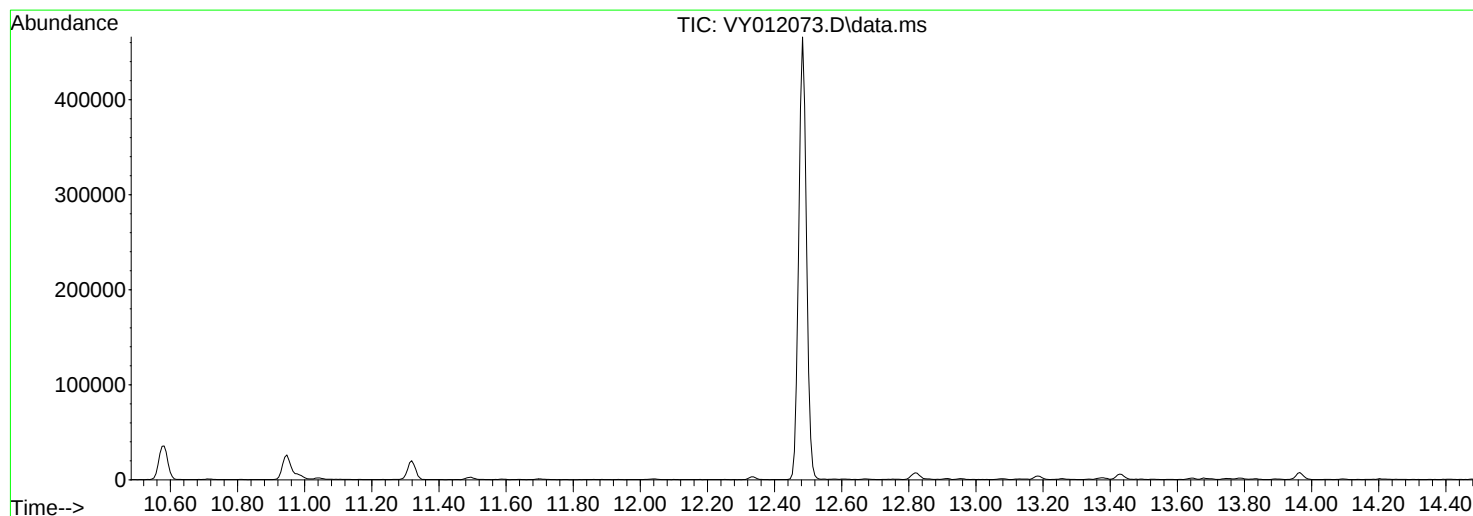

AutoFind: Scans 1748, 1749, 1750; Background Corrected with Scan 1740

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	17.0	12834	PASS
75	95	30	60	51.9	39219	PASS
95	95	100	100	100.0	75629	PASS
96	95	5	9	6.6	4990	PASS
173	174	0.00	2	1.1	743	PASS
174	95	50	100	91.0	68848	PASS
175	174	5	9	7.2	4960	PASS
176	174	95	101	96.8	66640	PASS
177	176	5	9	7.2	4772	PASS