

Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY010923\
 Data File : VY012117.D
 Acq On : 09 Jan 2023 17:44
 Operator : KP/MD
 Sample : 01067-02
 Misc : 5.04g/5.0mL/MSVOA_Y/SOIL
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 MSVOA_Y
 ClientSampleId :
 7822

Quant Time: Jan 10 01:49:19 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y010623S.M
 Quant Title : SW846 8260
 QLast Update : Sat Jan 07 01:46:48 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Pentafluorobenzene	7.789	168	168766	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	8.691	114	285006	50.000	ug/l	0.00
63) Chlorobenzene-d5	11.496	117	268560	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.428	152	123479	50.000	ug/l	0.00

System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.142	65	100496	52.994	ug/l	0.00
Spiked Amount	50.000	Range	50 - 163	Recovery	=	105.980%
35) Dibromofluoromethane	7.722	113	86161	45.994	ug/l	0.00
Spiked Amount	50.000	Range	54 - 147	Recovery	=	91.980%
50) Toluene-d8	10.179	98	338784	45.819	ug/l	0.00
Spiked Amount	50.000	Range	49 - 140	Recovery	=	91.640%
62) 4-Bromofluorobenzene	12.483	95	109013	42.179	ug/l	0.00
Spiked Amount	50.000	Range	25 - 144	Recovery	=	84.360%


Target Compounds	Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY010923\
Data File : VY012117.D
Acq On : 09 Jan 2023 17:44
Operator : KP/MD
Sample : 01067-02
Misc : 5.04g/5.0mL/MSVOA_Y/SOIL
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_Y
ClientSampleId :
7822

Quant Time: Jan 10 01:49:19 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y010623S.M
Quant Title : SW846 8260
QLast Update : Sat Jan 07 01:46:48 2023
Response via : Initial Calibration




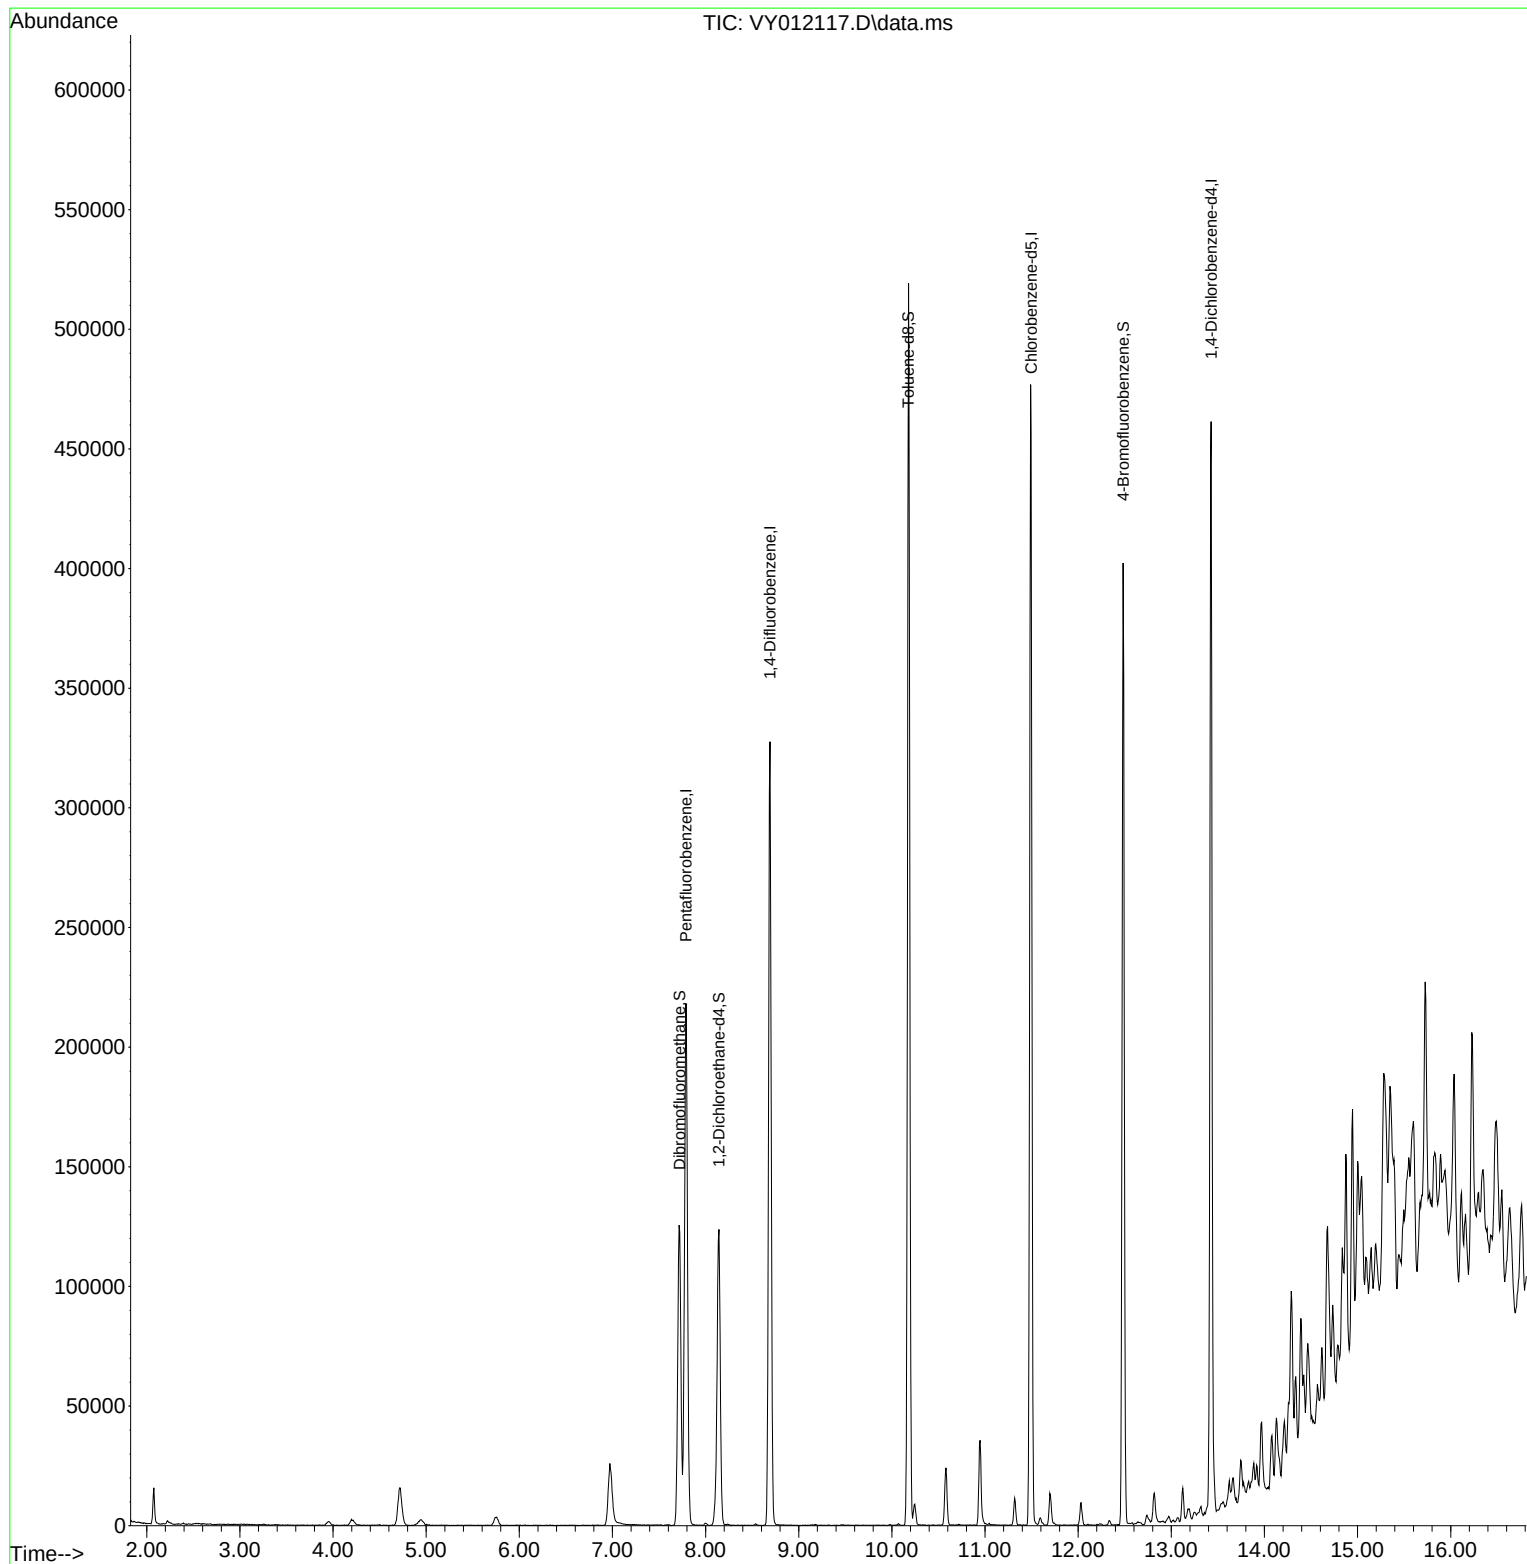


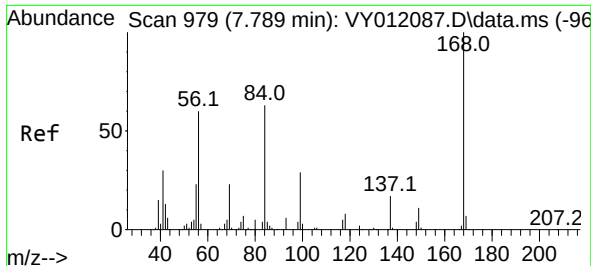

#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 7.789 min Scan# 91
Delta R.T. -0.000 min
Lab File: VY012117.D
Acq: 09 Jan 2023 17:44




Instrument :
MSVOA_Y
ClientSampleId :
7822


Tgt Ion:168 Resp: 168766
Ion Ratio Lower Upper
168 100
99 53.7 44.0 66.0

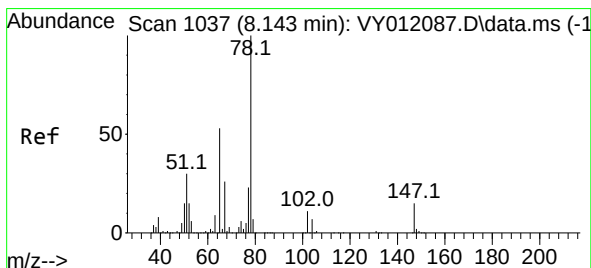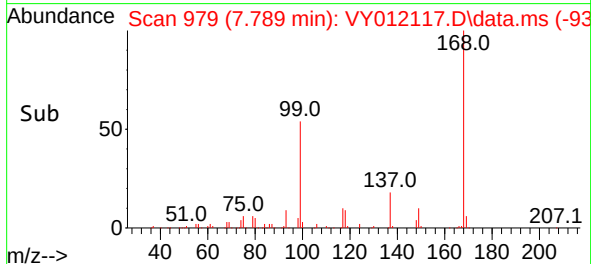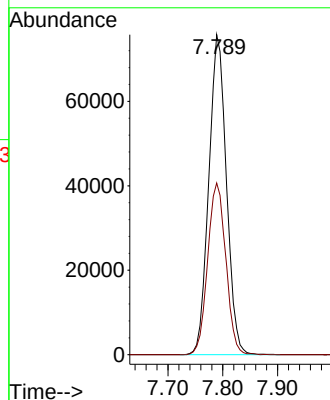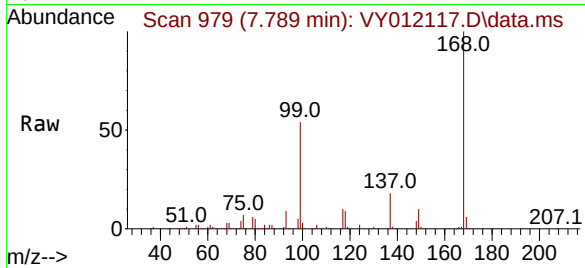

#33
1,2-Dichloroethane-d4
Concen: 52.994 ug/l
RT: 8.142 min Scan# 1037
Delta R.T. -0.001 min
Lab File: VY012117.D
Acq: 09 Jan 2023 17:44

Tgt Ion: 65 Resp: 100496
Ion Ratio Lower Upper
65 100
67 50.0 0.0 103.2

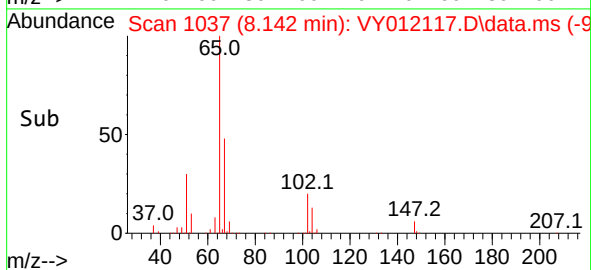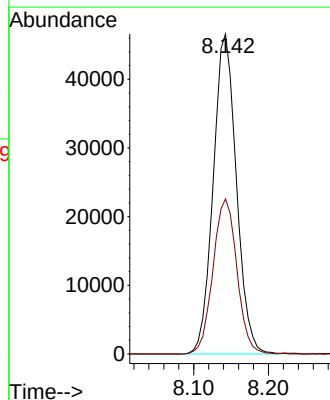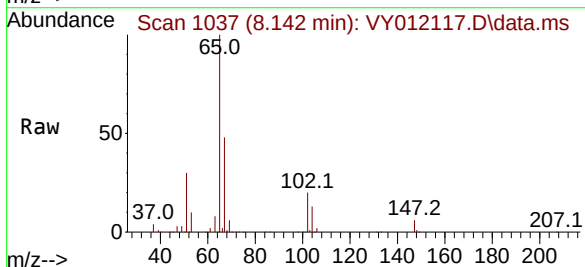

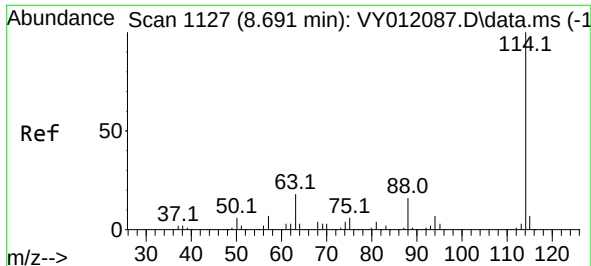

#34

1,4-Difluorobenzene

Concen: 50.000 ug/l

RT: 8.691 min Scan# 1127

Delta R.T. 0.000 min

Lab File: VY012117.D

Acq: 09 Jan 2023 17:44

Instrument :

MSVOA_Y

ClientSampleId :

7822





Tgt Ion:114 Resp: 285006

Ion Ratio Lower Upper

114 100

63 18.2 0.0 39.6

88 15.1 0.0 32.2

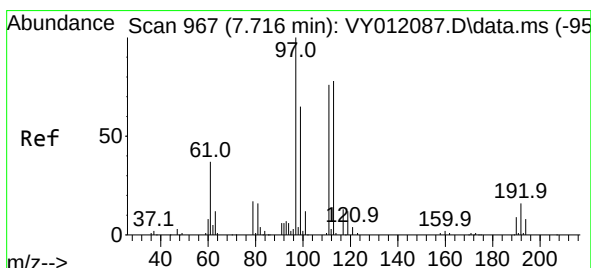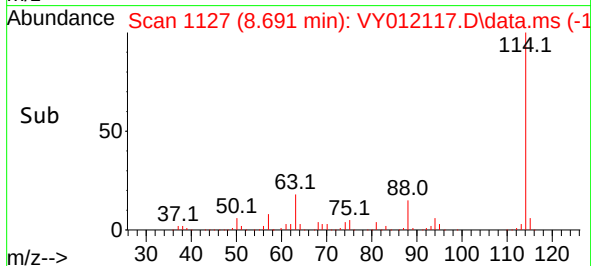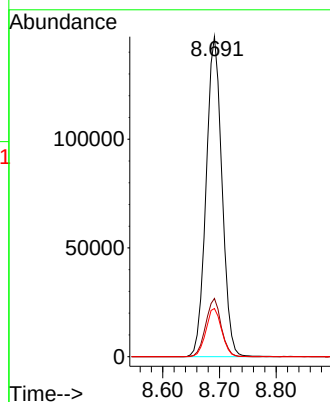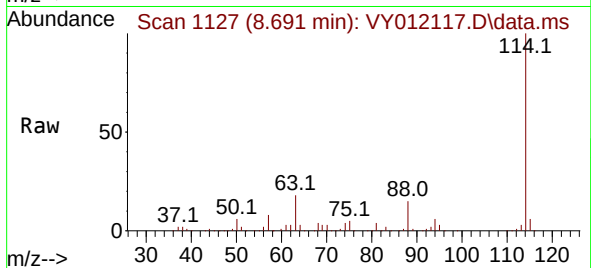

#35

Dibromofluoromethane

Concen: 45.994 ug/l

RT: 7.722 min Scan# 968

Delta R.T. 0.006 min

Lab File: VY012117.D

Acq: 09 Jan 2023 17:44




Tgt Ion:113 Resp: 86161


Ion Ratio Lower Upper

113 100

111 102.9 83.0 124.4

192 21.8 16.0 24.0


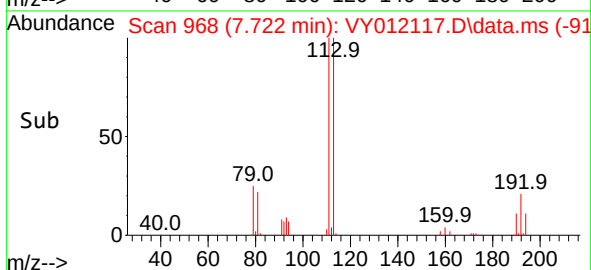
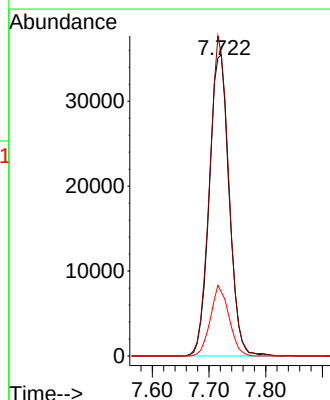
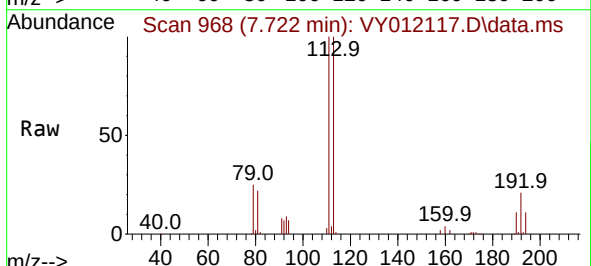


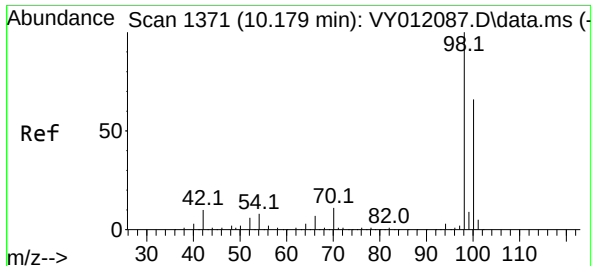

#50
Toluene-d8
Concen: 45.819 ug/l
RT: 10.179 min Scan# 11
Delta R.T. -0.000 min
Lab File: VY012117.D
Acq: 09 Jan 2023 17:44




Instrument :
MSVOA_Y
ClientSampleId :
7822


Tgt Ion: 98 Resp: 338784
Ion Ratio Lower Upper
98 100
100 64.2 51.9 77.9

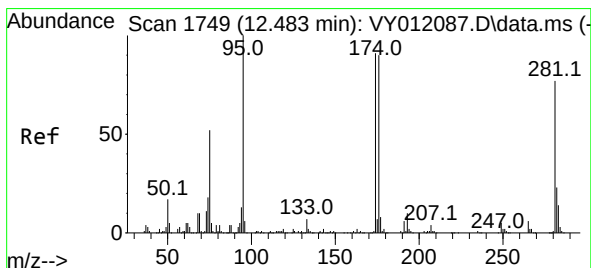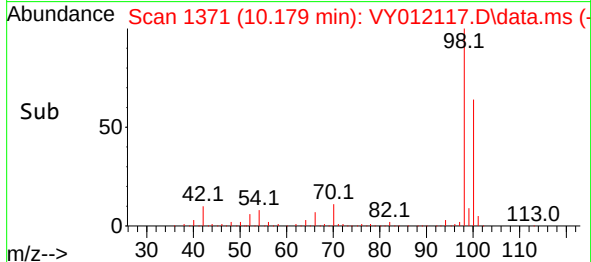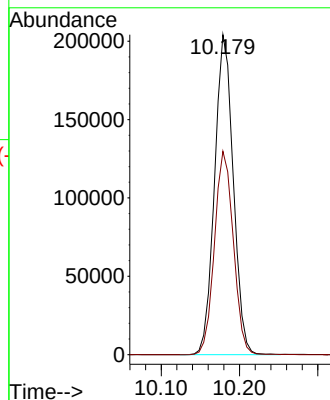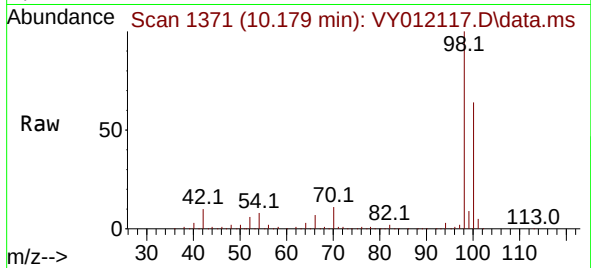

#62
4-Bromofluorobenzene
Concen: 42.179 ug/l
RT: 12.483 min Scan# 1749
Delta R.T. 0.000 min
Lab File: VY012117.D
Acq: 09 Jan 2023 17:44

Tgt Ion: 95 Resp: 109013
Ion Ratio Lower Upper
95 100
174 92.9 0.0 172.0
176 90.0 0.0 167.6

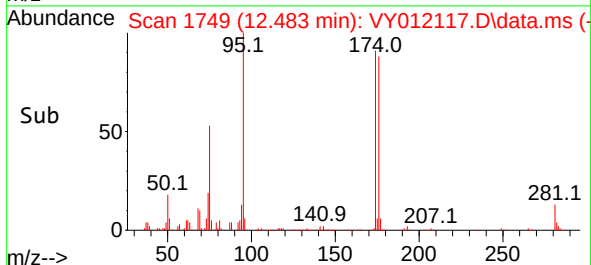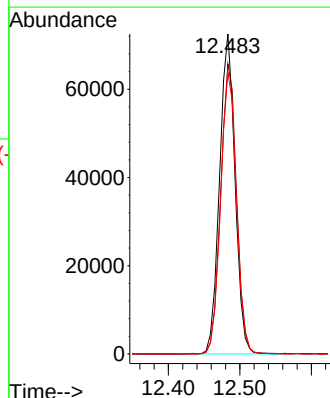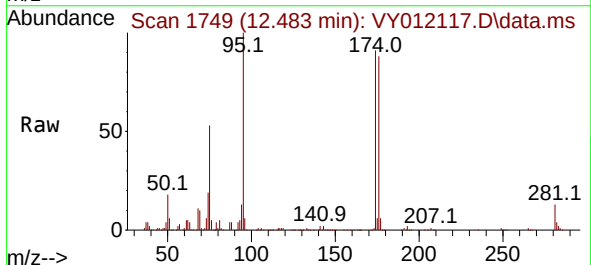

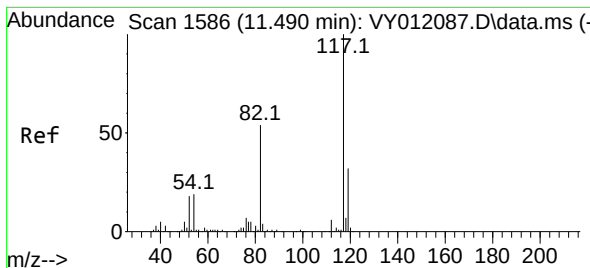

#63

Chlorobenzene-d5

Concen: 50.000 ug/l

RT: 11.496 min Scan# 11

Delta R.T. 0.006 min

Lab File: VY012117.D

Acq: 09 Jan 2023 17:44

Instrument :

MSVOA_Y

ClientSampleId :

7822





Tgt Ion:117 Resp: 268560

Ion Ratio Lower Upper

117 100

82 50.4 44.8 67.2

119 31.4 25.4 38.2

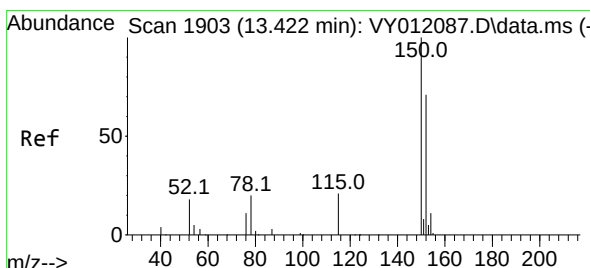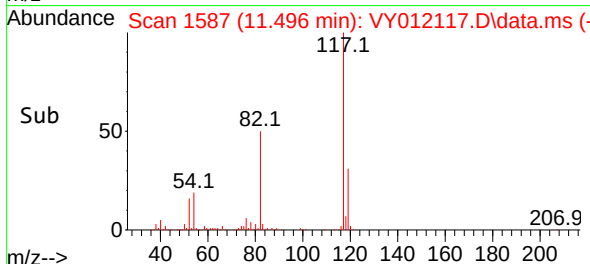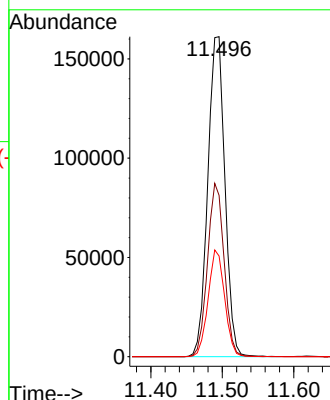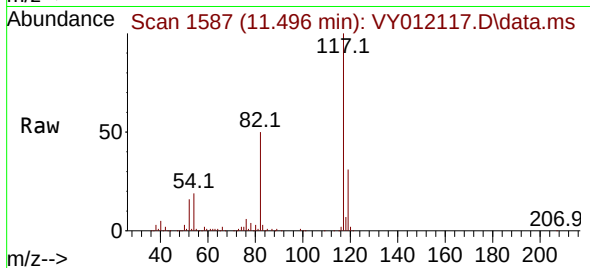

#72

1,4-Dichlorobenzene-d4

Concen: 50.000 ug/l

RT: 13.428 min Scan# 1904

Delta R.T. 0.006 min

Lab File: VY012117.D

Acq: 09 Jan 2023 17:44

Tgt Ion:152 Resp: 123479

Ion Ratio Lower Upper

152 100

115 56.8 29.1 87.3

150 154.5 0.0 342.6

