

Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY011023\
 Data File : VY012131.D
 Acq On : 10 Jan 2023 10:40
 Operator : KP/MD
 Sample : VY0110SBL01
 Misc : 5.00g/5.0mL/MSVOA_Y/SOIL
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_Y
 ClientSampleId :
 VY0110SBL01

Quant Time: Jan 11 03:07:09 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y010623S.M
 Quant Title : SW846 8260
 QLast Update : Sat Jan 07 01:46:48 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Pentafluorobenzene	7.795	168	174060	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	8.691	114	295083	50.000	ug/l	0.00
63) Chlorobenzene-d5	11.489	117	281211	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.428	152	128690	50.000	ug/l	0.00

System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.143	65	104883	53.625	ug/l	0.00
Spiked Amount	50.000	Range	50 - 163	Recovery	=	107.260%
35) Dibromofluoromethane	7.722	113	89562	46.177	ug/l	0.00
Spiked Amount	50.000	Range	54 - 147	Recovery	=	92.360%
50) Toluene-d8	10.179	98	353240	46.143	ug/l	0.00
Spiked Amount	50.000	Range	49 - 140	Recovery	=	92.280%
62) 4-Bromofluorobenzene	12.483	95	115689	43.234	ug/l	0.00
Spiked Amount	50.000	Range	25 - 144	Recovery	=	86.460%


Target Compounds	Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY011023\
Data File : VY012131.D
Acq On : 10 Jan 2023 10:40
Operator : KP/MD
Sample : VY0110SBL01
Misc : 5.00g/5.0mL/MSVOA_Y/SOIL
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_Y
ClientSampleId :
VY0110SBL01

Quant Time: Jan 11 03:07:09 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y010623S.M
Quant Title : SW846 8260
QLast Update : Sat Jan 07 01:46:48 2023
Response via : Initial Calibration




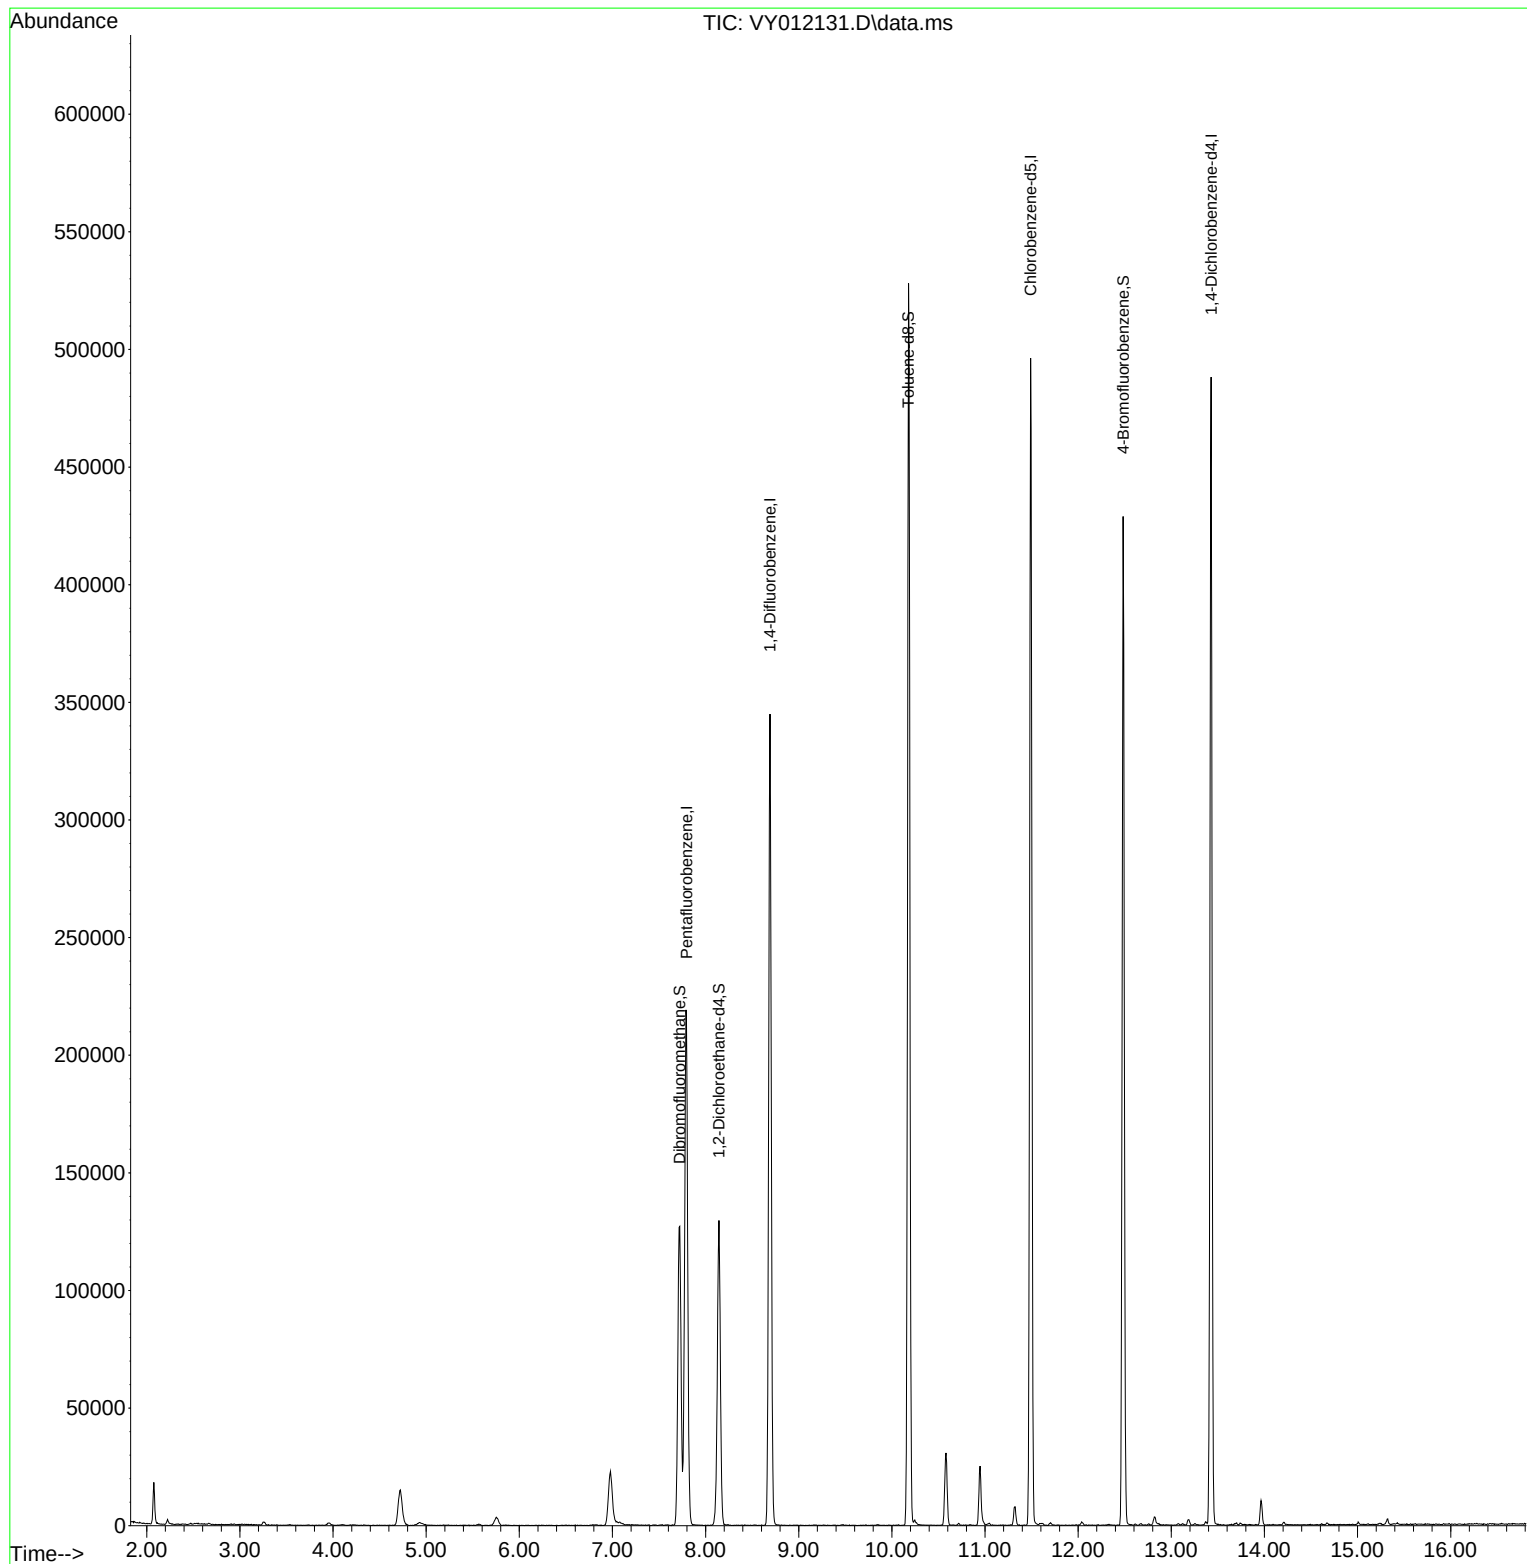


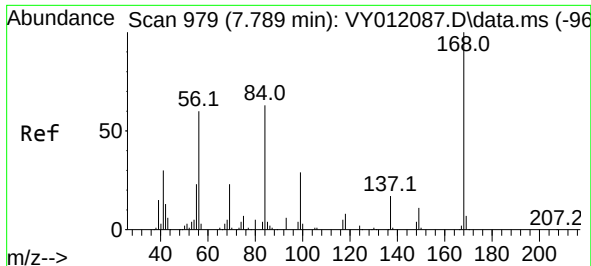

#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 7.795 min Scan# 979
Delta R.T. 0.006 min
Lab File: VY012131.D
Acq: 10 Jan 2023 10:40




Instrument :
MSVOA_Y
ClientSampleId :
VY0110SBL01


Tgt Ion:168 Resp: 174060
Ion Ratio Lower Upper
168 100
99 54.1 44.0 66.0

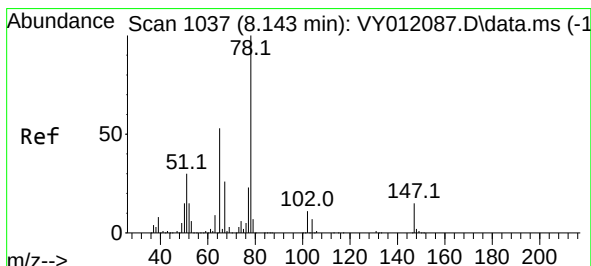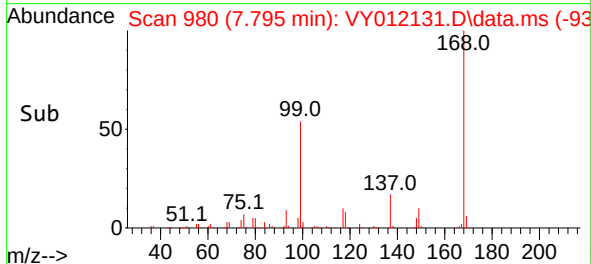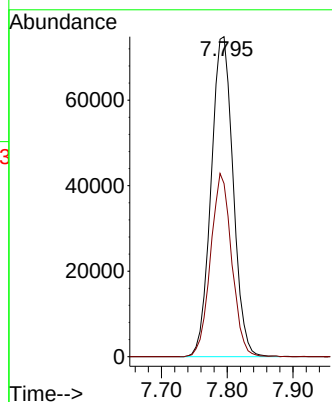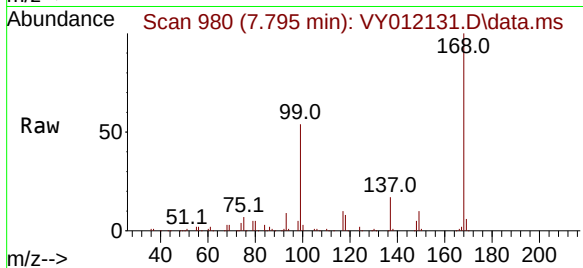

#33
1,2-Dichloroethane-d4
Concen: 53.625 ug/l
RT: 8.143 min Scan# 1037
Delta R.T. -0.000 min
Lab File: VY012131.D
Acq: 10 Jan 2023 10:40

Tgt Ion: 65 Resp: 104883
Ion Ratio Lower Upper
65 100
67 49.0 0.0 103.2


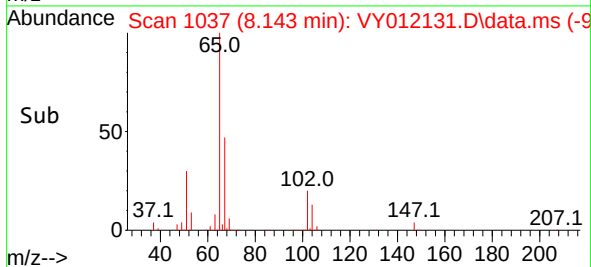
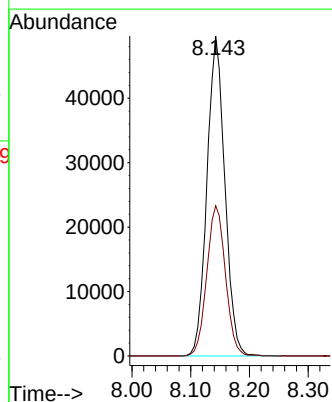
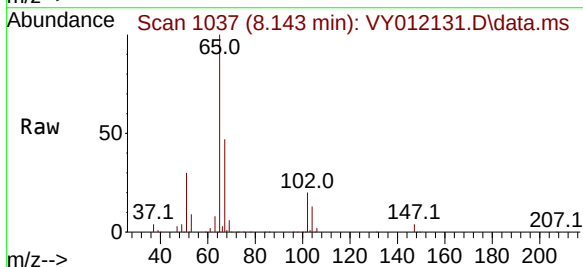


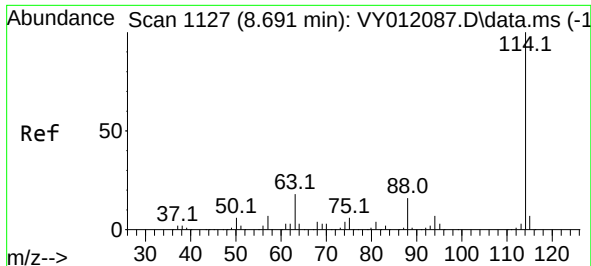

#34
1,4-Difluorobenzene
Concen: 50.000 ug/l
RT: 8.691 min Scan# 1127
Delta R.T. 0.000 min
Lab File: VY012131.D
Acq: 10 Jan 2023 10:40




Instrument :
MSVOA_Y
ClientSampleId :
VY0110SBL01


Tgt Ion:114 Resp: 295083
Ion Ratio Lower Upper
114 100
63 17.8 0.0 39.6
88 15.0 0.0 32.2

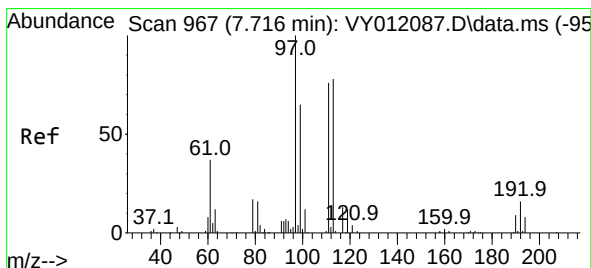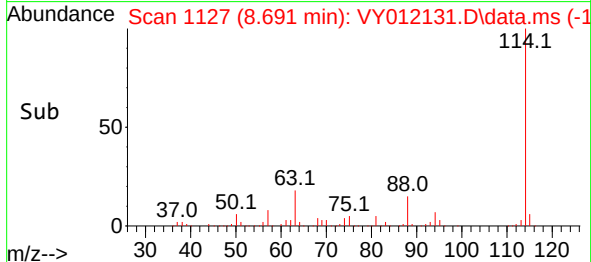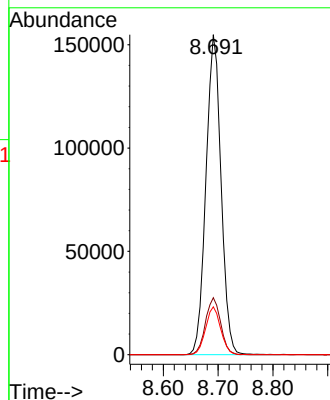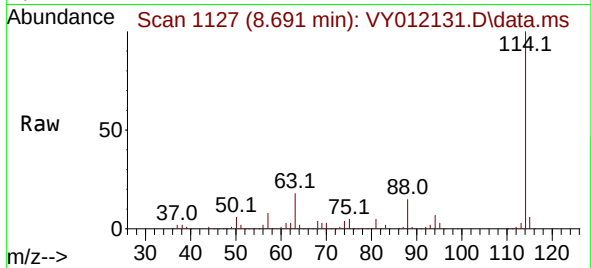

#35
Dibromofluoromethane
Concen: 46.177 ug/l
RT: 7.722 min Scan# 968
Delta R.T. 0.006 min
Lab File: VY012131.D
Acq: 10 Jan 2023 10:40

Tgt Ion:113 Resp: 89562
Ion Ratio Lower Upper
113 100
111 102.2 83.0 124.4
192 21.3 16.0 24.0


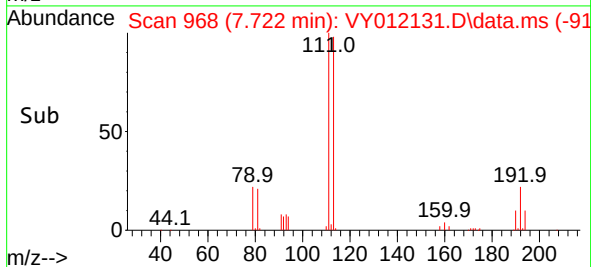
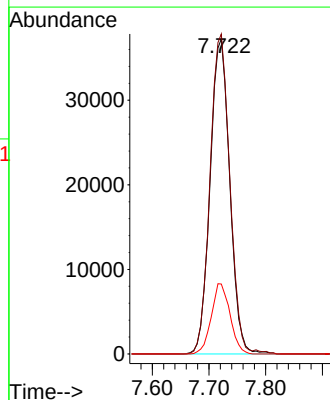
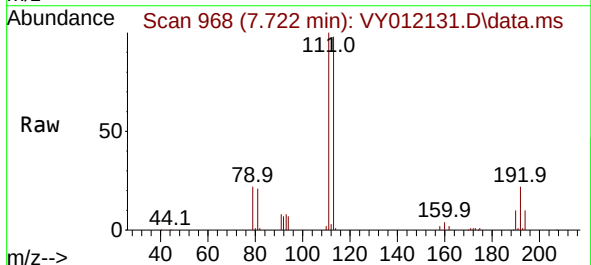


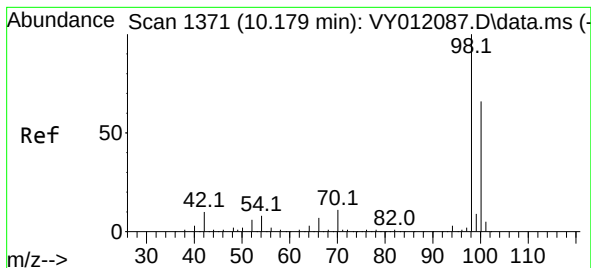

#50
Toluene-d8
Concen: 46.143 ug/l
RT: 10.179 min Scan# 1371
Delta R.T. -0.000 min
Lab File: VY012131.D
Acq: 10 Jan 2023 10:40




Instrument :
MSVOA_Y
ClientSampleId :
VY0110SBL01


Tgt Ion: 98 Resp: 353240
Ion Ratio Lower Upper
98 100
100 64.8 51.9 77.9

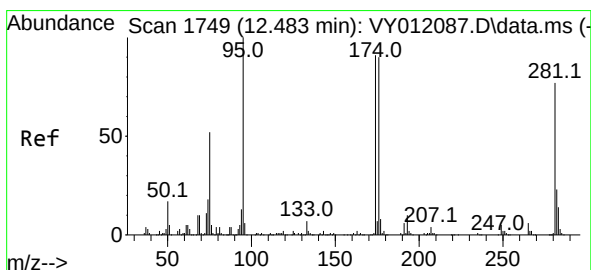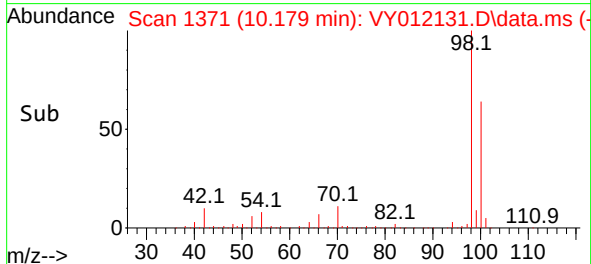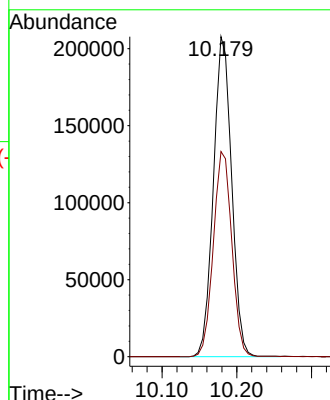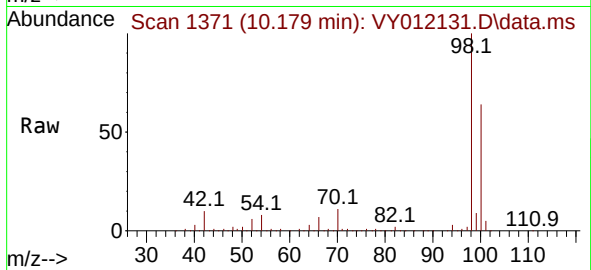

#62
4-Bromofluorobenzene
Concen: 43.234 ug/l
RT: 12.483 min Scan# 1749
Delta R.T. 0.000 min
Lab File: VY012131.D
Acq: 10 Jan 2023 10:40

Tgt Ion: 95 Resp: 115689
Ion Ratio Lower Upper
95 100
174 93.2 0.0 172.0
176 88.7 0.0 167.6


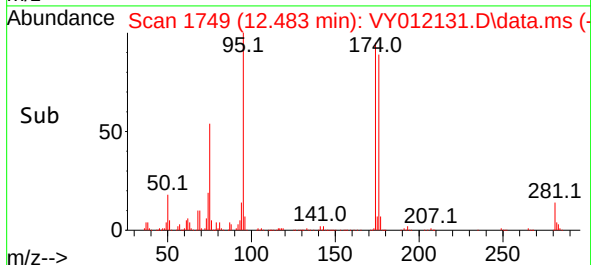
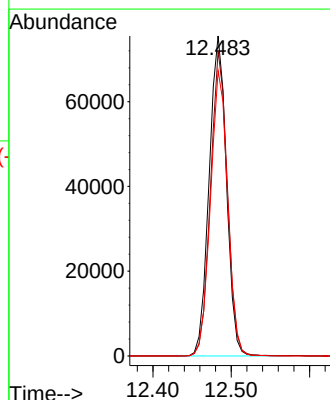
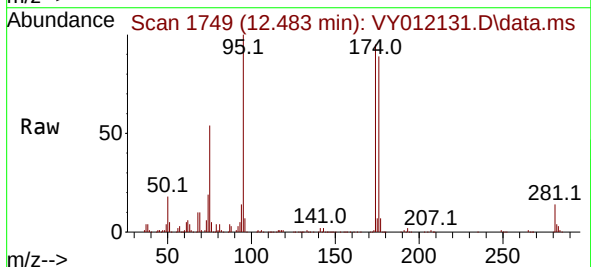


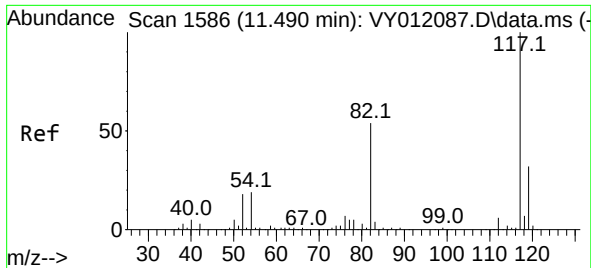

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 11.489 min Scan# 11
Delta R.T. -0.001 min
Lab File: VY012131.D
Acq: 10 Jan 2023 10:40

Instrument :
MSVOA_Y
ClientSampleId :
VY0110SBL01

Tgt Ion:117 Resp: 281211
Ion Ratio Lower Upper
117 100
82 53.5 44.8 67.2
119 32.2 25.4 38.2

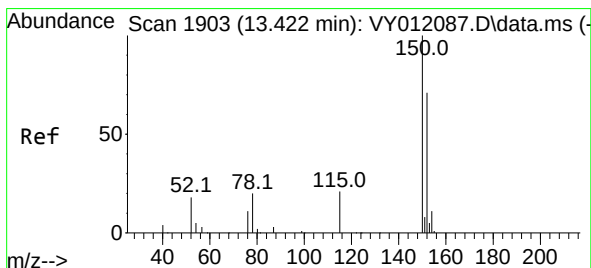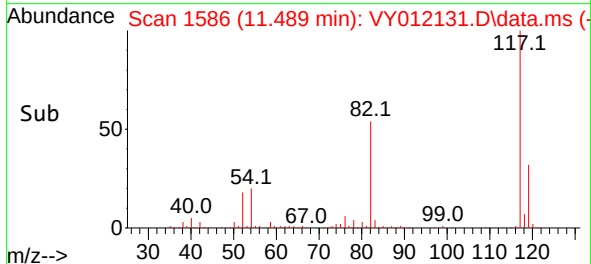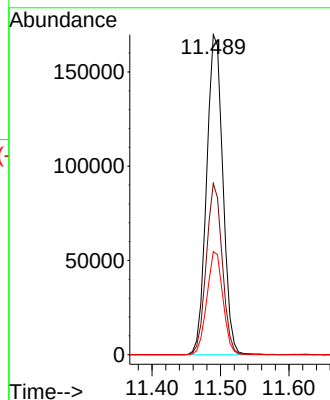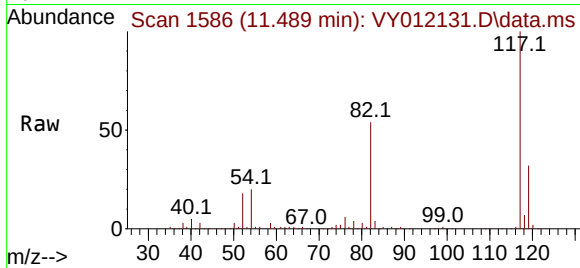

#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 13.428 min Scan# 1904
Delta R.T. 0.006 min
Lab File: VY012131.D
Acq: 10 Jan 2023 10:40

Tgt Ion:152 Resp: 128690
Ion Ratio Lower Upper
152 100
115 56.7 29.1 87.3
150 157.8 0.0 342.6

