


Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY011023\
Data File : VY012129.D
Acq On : 10 Jan 2023 09:01
Operator : KP/MD
Sample : BFB
Misc : 5.00g/5.0mL/MSVOA_Y/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_Y
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y010623S.M
Title : SW846 8260
Last Update : Sat Jan 07 01:46:48 2023

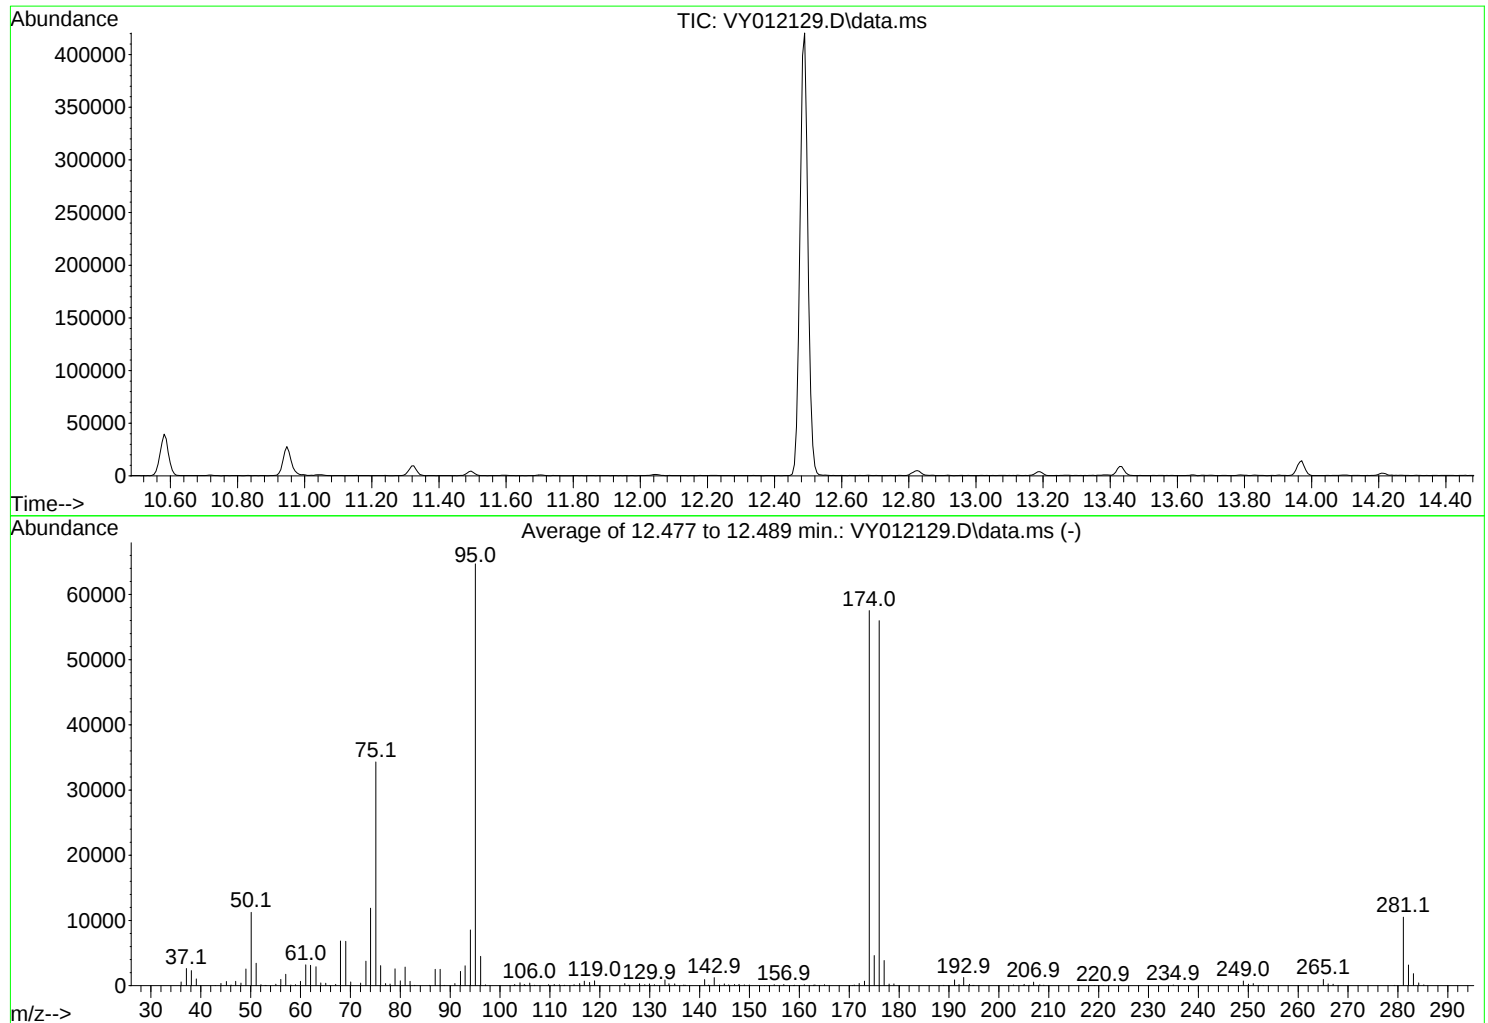

AutoFind: Scans 1748, 1749, 1750; Background Corrected with Scan 1740

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	17.4	11253	PASS
75	95	30	60	53.0	34320	PASS
95	95	100	100	100.0	64701	PASS
96	95	5	9	6.9	4488	PASS
173	174	0.00	2	1.2	697	PASS
174	95	50	100	88.9	57539	PASS
175	174	5	9	8.0	4627	PASS
176	174	95	101	97.3	55973	PASS
177	176	5	9	6.9	3849	PASS