

Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY011221\
 Data File : VY003904.D
 Acq On : 12 Jan 2021 16:30
 Operator : SY/MD
 Sample : M1055-01
 Misc : 5.89G/5ML/MSVOA_Y/SOIL
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 MSVOA_Y
 ClientSampleId :
 SA-01-010821

Quant Time: Jan 13 02:34:03 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y011221S.M
 Quant Title : SW846 8260
 QLast Update : Tue Jan 12 11:47:10 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) Pentafluorobenzene	7.795	168	143187	50.00	ug/l	0.00
34) 1,4-Difluorobenzene	8.691	114	242686	50.00	ug/l	0.00
63) Chlorobenzene-d5	11.489	117	231025	50.00	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.422	152	123649	50.00	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.143	65	109146	49.07	ug/l	0.00
Spiked Amount	50.000	Range	50 - 163	Recovery	=	98.14%
35) Dibromofluoromethane	7.722	113	79280	39.97	ug/l	0.00
Spiked Amount	50.000	Range	54 - 147	Recovery	=	79.94%
50) Toluene-d8	10.179	98	309266	38.48	ug/l	0.00
Spiked Amount	50.000	Range	49 - 140	Recovery	=	76.96%
62) 4-Bromofluorobenzene	12.477	95	112303	38.26	ug/l	0.00
Spiked Amount	50.000	Range	25 - 144	Recovery	=	76.52%
Target Compounds						
16) Acetone	3.954	43	19568	35.58	ug/l	Qvalue 92


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY011221\
Data File : VY003904.D
Acq On : 12 Jan 2021 16:30
Operator : SY/MD
Sample : M1055-01
Misc : 5.89G/5ML/MSVOA_Y/SOIL
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_Y
ClientSampleId :
SA-01-010821

Quant Time: Jan 13 02:34:03 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y011221S.M
Quant Title : SW846 8260
QLast Update : Tue Jan 12 11:47:10 2021
Response via : Initial Calibration




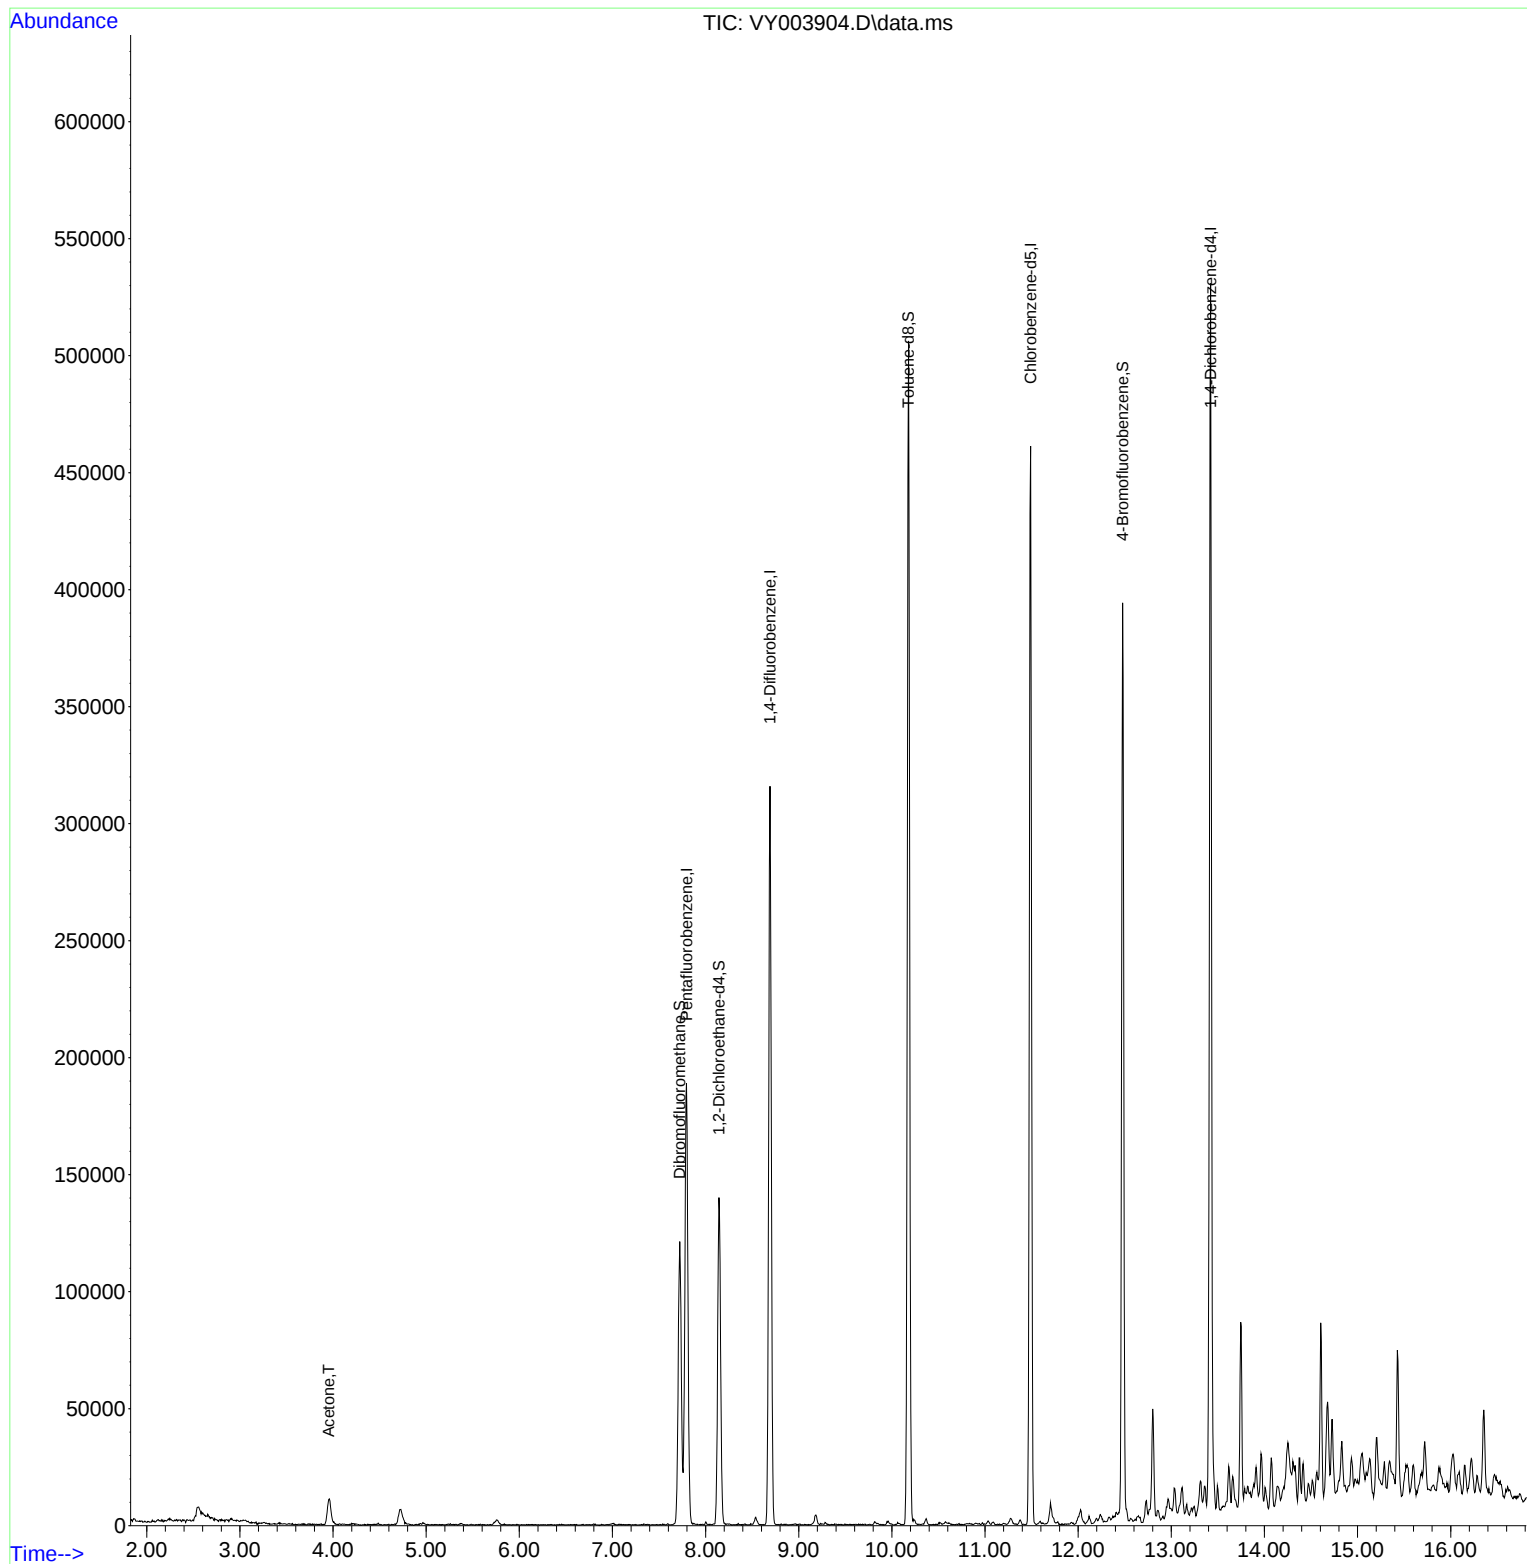


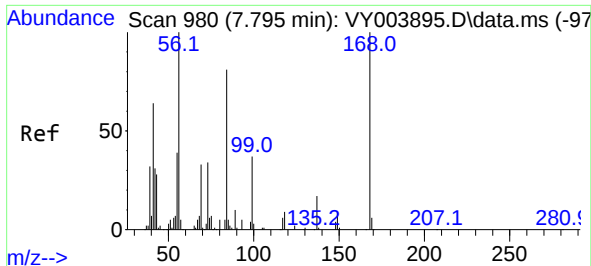

#1
Pentafluorobenzene
Concen: 50.00 ug/l
RT: 7.795 min Scan# 980
Delta R.T. 0.000 min
Lab File: VY003904.D
Acq: 12 Jan 2021 16:30




Instrument :
MSVOA_Y
ClientSampleId :
SA-01-010821


Tgt Ion:168 Resp: 143187
Ion Ratio Lower Upper
168 100
99 58.1 40.4 60.6

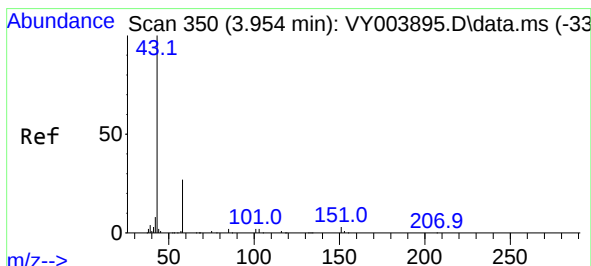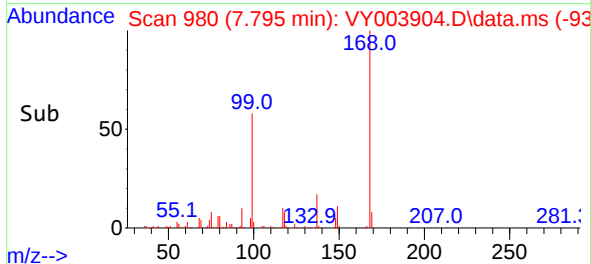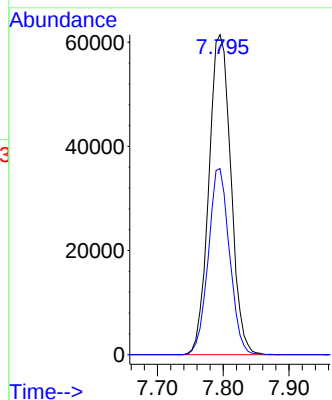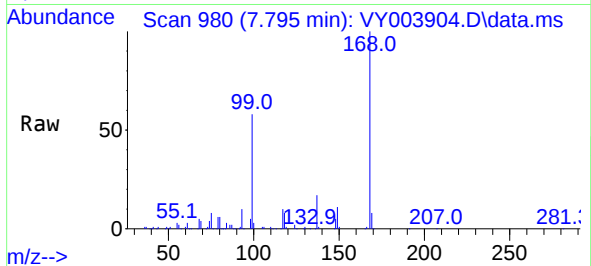

#16
Acetone
Concen: 35.58 ug/l
RT: 3.954 min Scan# 350
Delta R.T. 0.000 min
Lab File: VY003904.D
Acq: 12 Jan 2021 16:30

Tgt Ion: 43 Resp: 19568
Ion Ratio Lower Upper
43 100
58 26.4 24.5 36.7


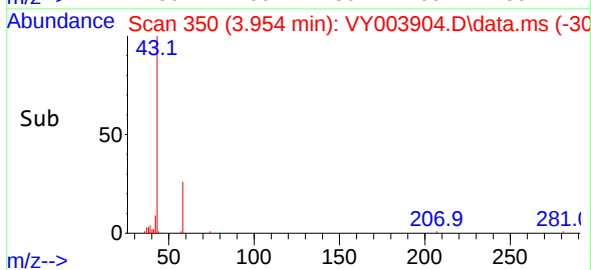
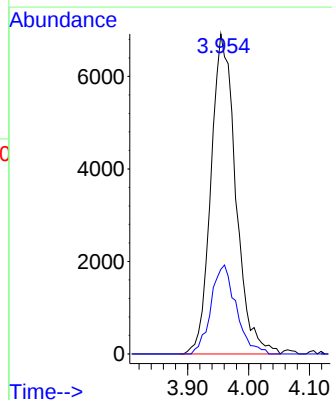
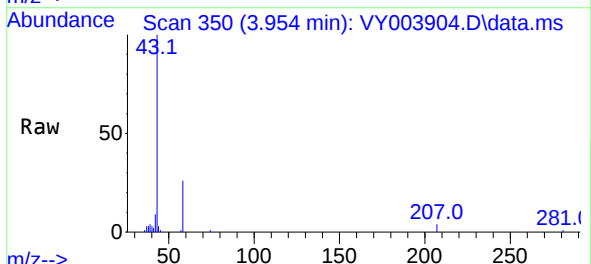


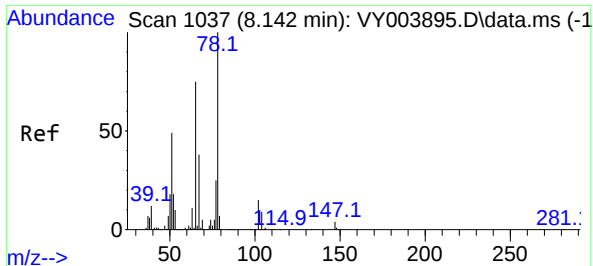

#33
1,2-Dichloroethane-d4
Concen: 49.07 ug/l
RT: 8.143 min Scan# 1037
Delta R.T. 0.000 min
Lab File: VY003904.D
Acq: 12 Jan 2021 16:30




Instrument :
MSVOA_Y
ClientSampleId :
SA-01-010821


Tgt Ion: 65 Resp: 109146
Ion Ratio Lower Upper
65 100
67 50.2 0.0 102.2

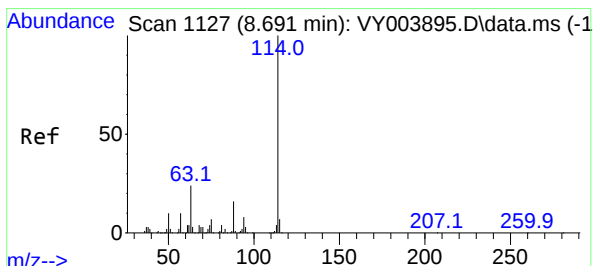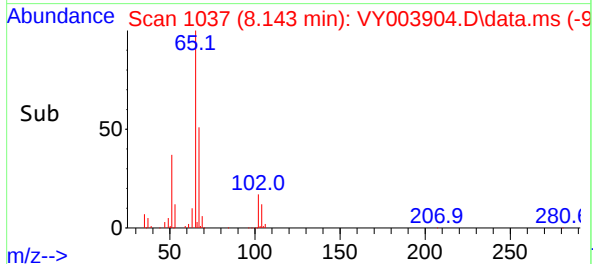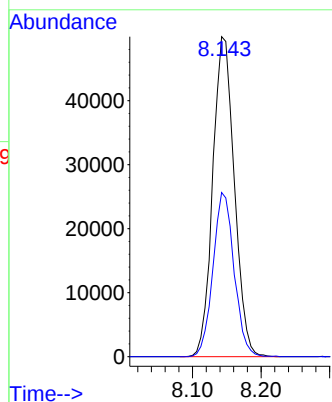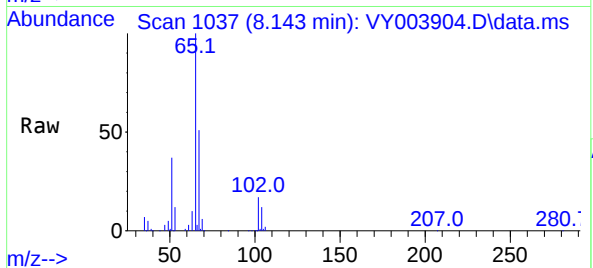

#34
1,4-Difluorobenzene
Concen: 50.00 ug/l
RT: 8.691 min Scan# 1127
Delta R.T. 0.000 min
Lab File: VY003904.D
Acq: 12 Jan 2021 16:30

Tgt Ion: 114 Resp: 242686
Ion Ratio Lower Upper
114 100
63 23.3 0.0 38.8
88 15.9 0.0 31.4


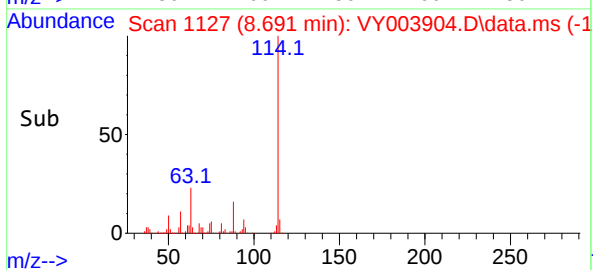
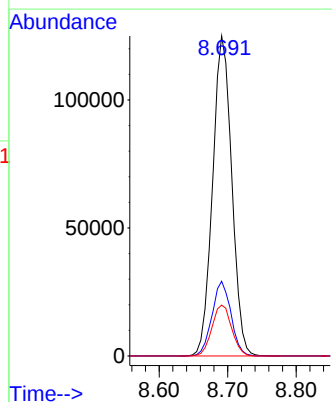
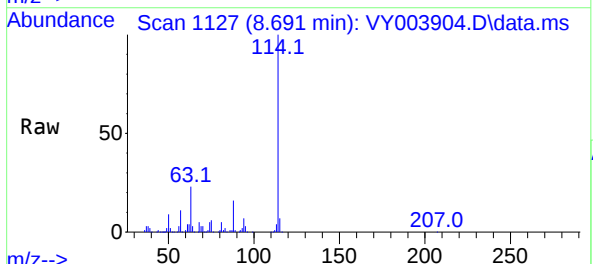


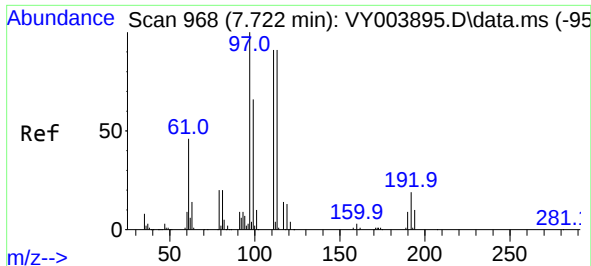

#35
Dibromofluoromethane
Concen: 39.97 ug/l
RT: 7.722 min Scan# 968
Delta R.T. 0.000 min
Lab File: VY003904.D
Acq: 12 Jan 2021 16:30




Instrument :
MSVOA_Y
ClientSampleId :
SA-01-010821


Tgt Ion:113 Resp: 79280
Ion Ratio Lower Upper
113 100
111 104.4 83.0 124.6
192 23.2 19.8 29.6

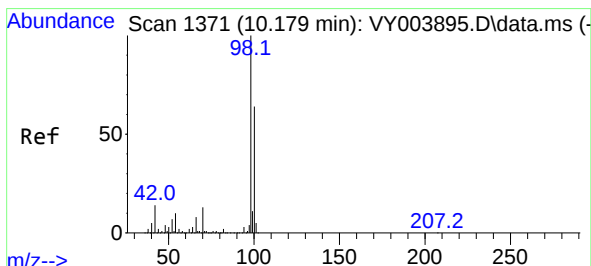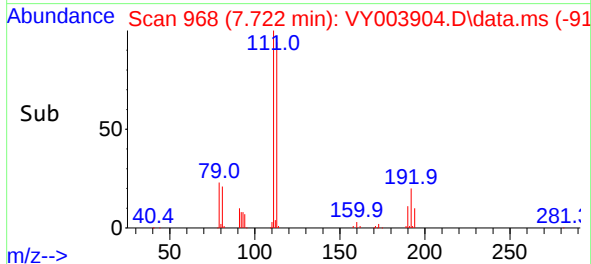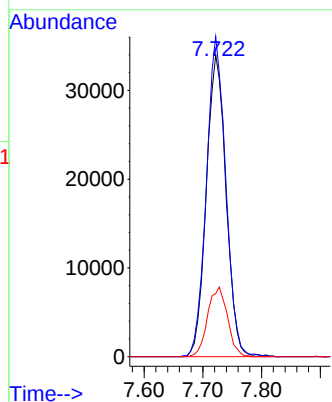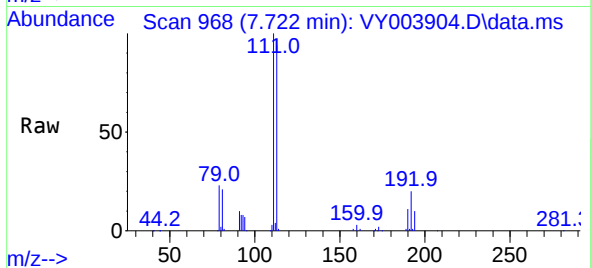

#50
Toluene-d8
Concen: 38.48 ug/l
RT: 10.179 min Scan# 1371
Delta R.T. 0.000 min
Lab File: VY003904.D
Acq: 12 Jan 2021 16:30

Tgt Ion: 98 Resp: 309266
Ion Ratio Lower Upper
98 100
100 62.9 51.4 77.0

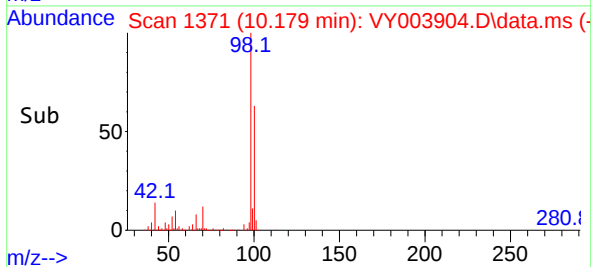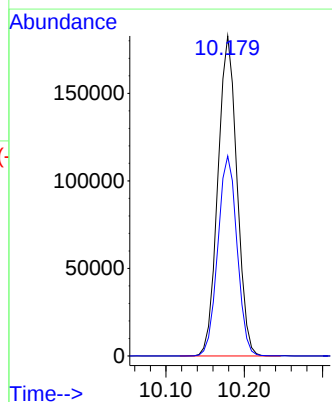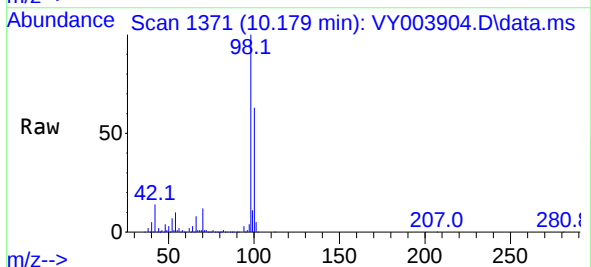




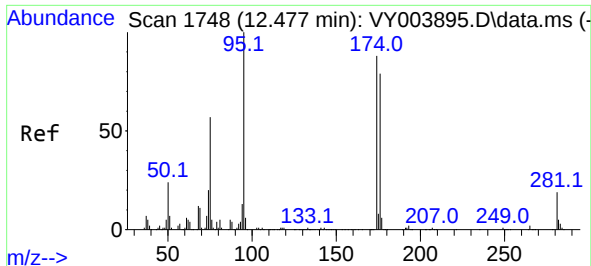


#62
4-Bromofluorobenzene
Concen: 38.26 ug/l
RT: 12.477 min Scan# 1748
Delta R.T. 0.000 min
Lab File: VY003904.D
Acq: 12 Jan 2021 16:30

Instrument :
MSVOA_Y
ClientSampleId :
SA-01-010821

Tgt Ion: 95 Resp: 112303




Ion	Ratio	Lower	Upper
95	100		
174	87.2	0.0	193.2
176	85.0	0.0	187.0

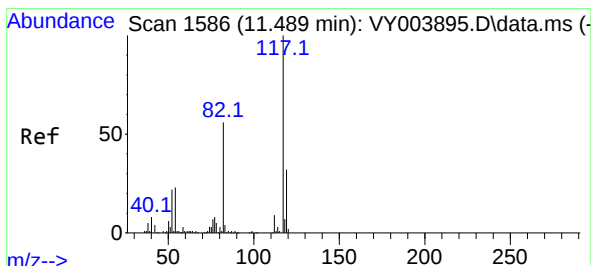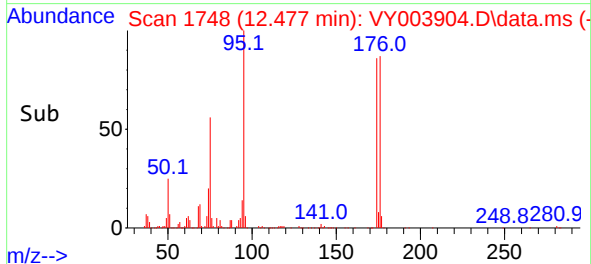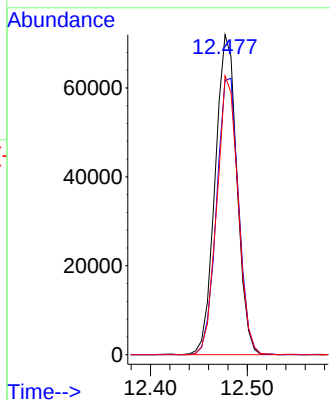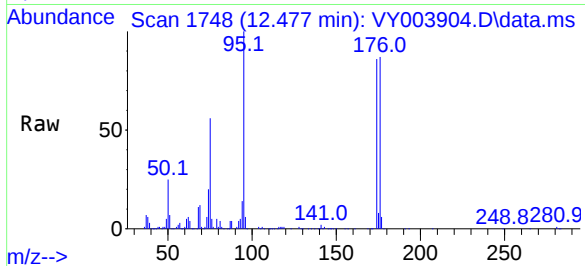


#63
Chlorobenzene-d5
Concen: 50.00 ug/l
RT: 11.489 min Scan# 1586
Delta R.T. 0.000 min
Lab File: VY003904.D
Acq: 12 Jan 2021 16:30

Tgt Ion: 117 Resp: 231025

Ion	Ratio	Lower	Upper
117	100		
82	57.2	43.9	65.9
119	30.8	26.2	39.4

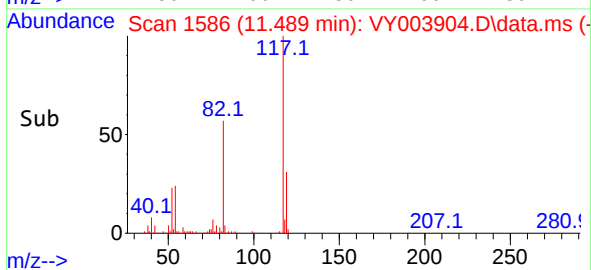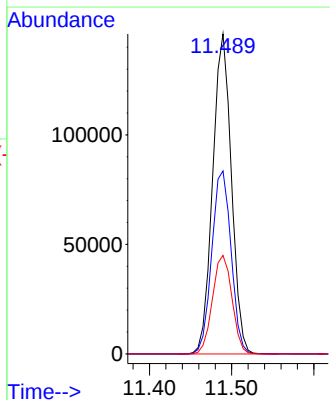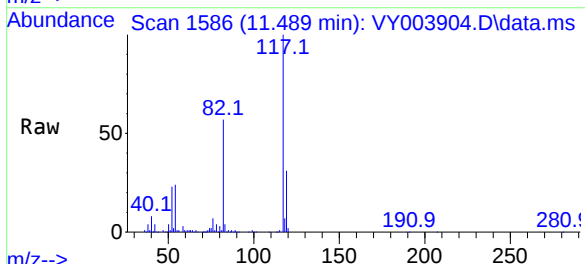

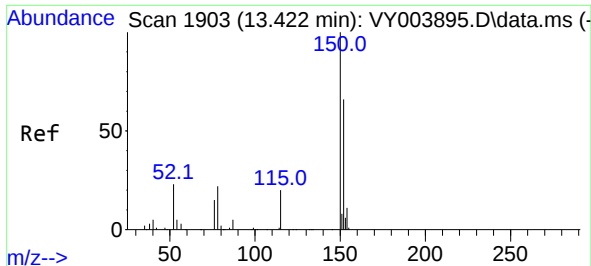

#72
 1,4-Dichlorobenzene-d4
 Concen: 50.00 ug/l
 RT: 13.422 min Scan# 1903
 Delta R.T. 0.000 min
 Lab File: VY003904.D
 Acq: 12 Jan 2021 16:30

Instrument :
 MSVOA_Y
 ClientSampleId :
 SA-01-010821

Tgt Ion:152 Resp: 123649
 Ion Ratio Lower Upper
 152 100
 115 55.9 27.9 83.7
 150 156.2 0.0 356.4

