
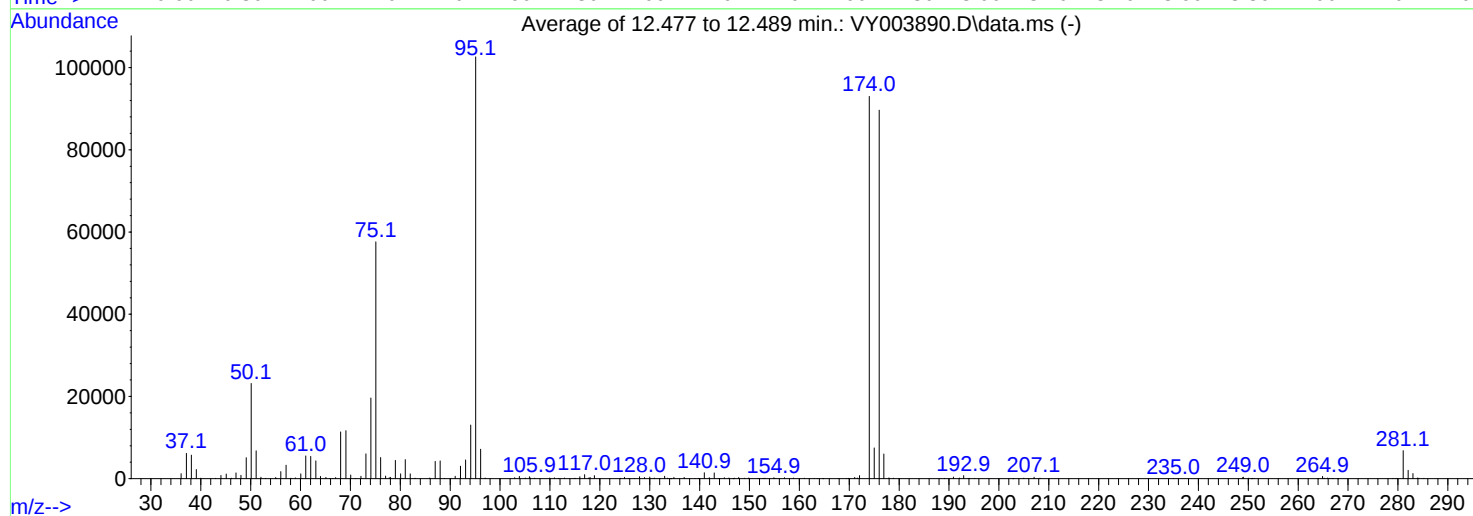


Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY011221\
 Data File : VY003890.D
 Acq On : 12 Jan 2021 08:01
 Operator : SY/MD
 Sample : BFB
 Misc : 5.00G/5ML/MSVOA_Y/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_Y
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y011221S.M
 Title : SW846 8260
 Last Update : Tue Jan 12 11:47:10 2021

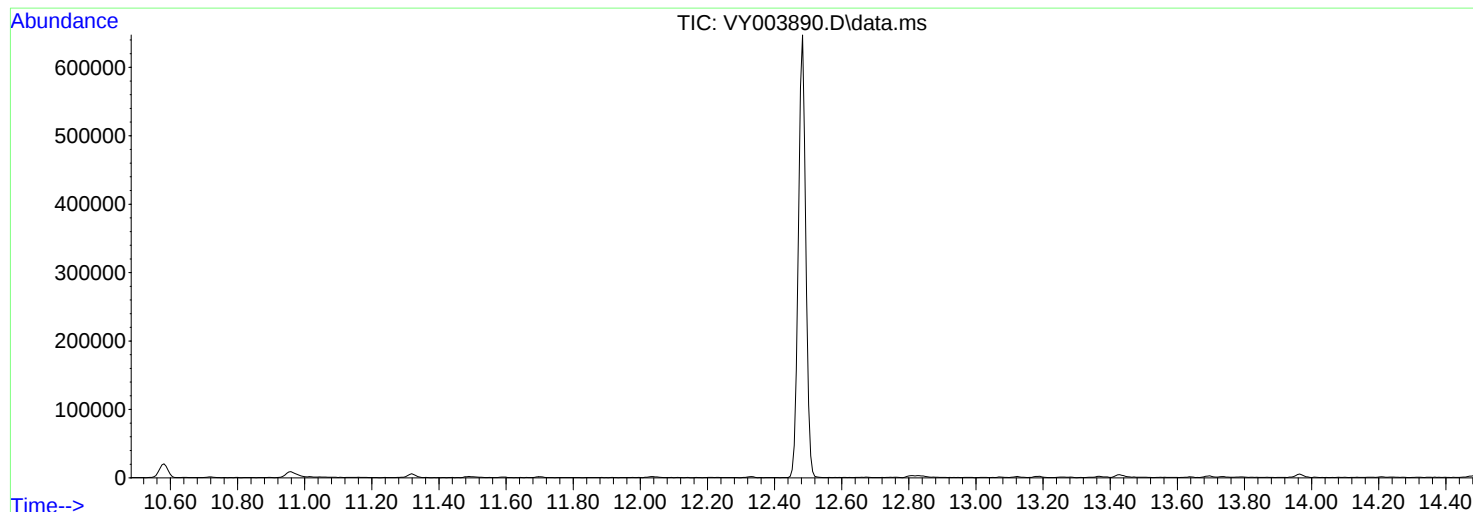

AutoFind: Scans 1748, 1749, 1750; Background Corrected with Scan 1739

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	22.6	23152	PASS
75	95	30	60	56.1	57616	PASS
95	95	100	100	100.0	102616	PASS
96	95	5	9	7.0	7164	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	100	90.6	93013	PASS
175	174	5	9	8.0	7486	PASS
176	174	95	101	96.4	89667	PASS
177	176	5	9	6.7	5981	PASS