
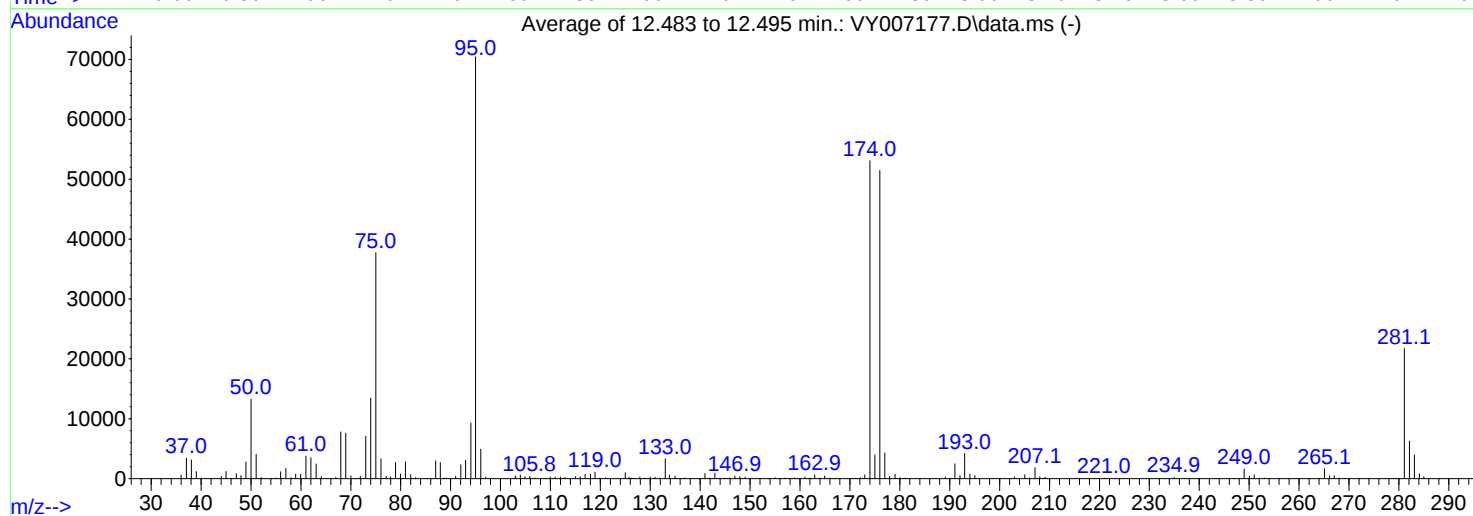


Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY011722\
 Data File : VY007177.D
 Acq On : 17 Jan 2022 09:00
 Operator : SY/MD
 Sample : BFB
 Misc : 5.00g/5.0mL/MSVOA_Y/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_Y
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y011322S.M
 Title : SW846 8260
 Last Update : Fri Jan 18 05:48:29 2022

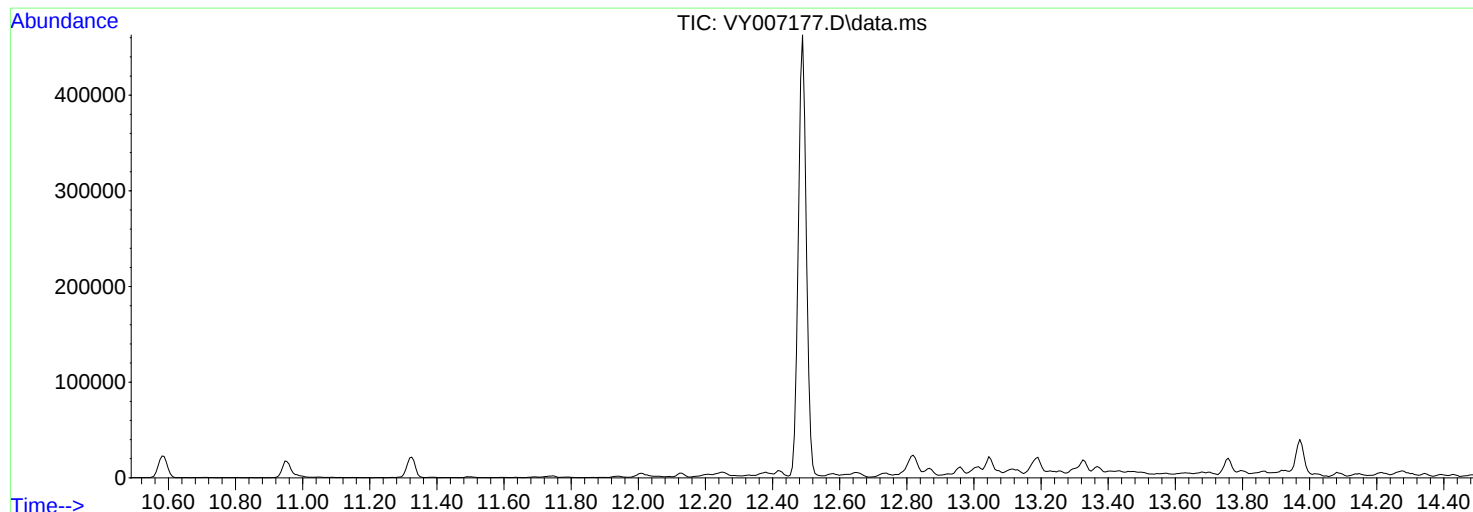

AutoFind: Scans 1749, 1750, 1751; Background Corrected with Scan 1736

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	18.9	13283	PASS
75	95	30	60	53.6	37739	PASS
95	95	100	100	100.0	70432	PASS
96	95	5	9	7.0	4924	PASS
173	174	0.00	2	1.2	613	PASS
174	95	50	100	75.4	53083	PASS
175	174	5	9	7.5	3966	PASS
176	174	95	101	96.9	51448	PASS
177	176	5	9	8.3	4290	PASS