
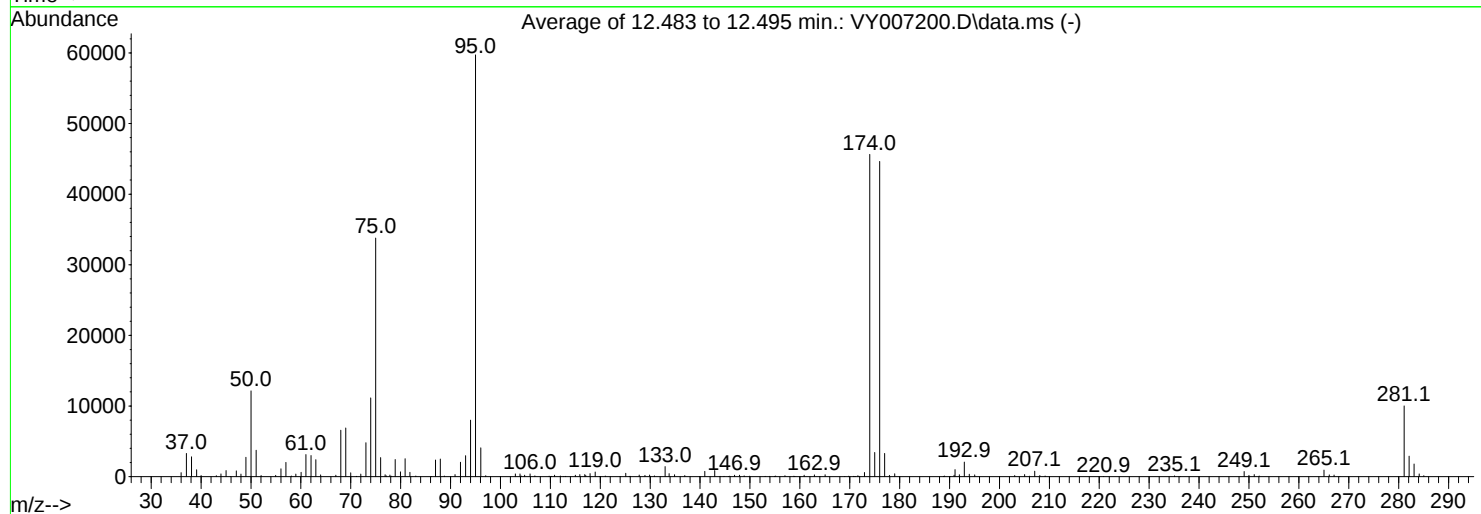


Data Path : Z:\voasrv\HPCHEM1\MSVOA\_Y\Data\VY011822\  
Data File : VY007200.D  
Acq On : 18 Jan 2022 09:14  
Operator : SY/MD  
Sample : BFB  
Misc : 5.00g/5.0mL/MSVOA\_Y/SOIL  
ALS Vial : 1 Sample Multiplier: 1

Instrument :  
MSVOA\_Y  
ClientSampleId :  
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA\_Y\methods\82Y011322S.M  
Title : SW846 8260  
Last Update : Fri Jan 14 05:48:29 2022

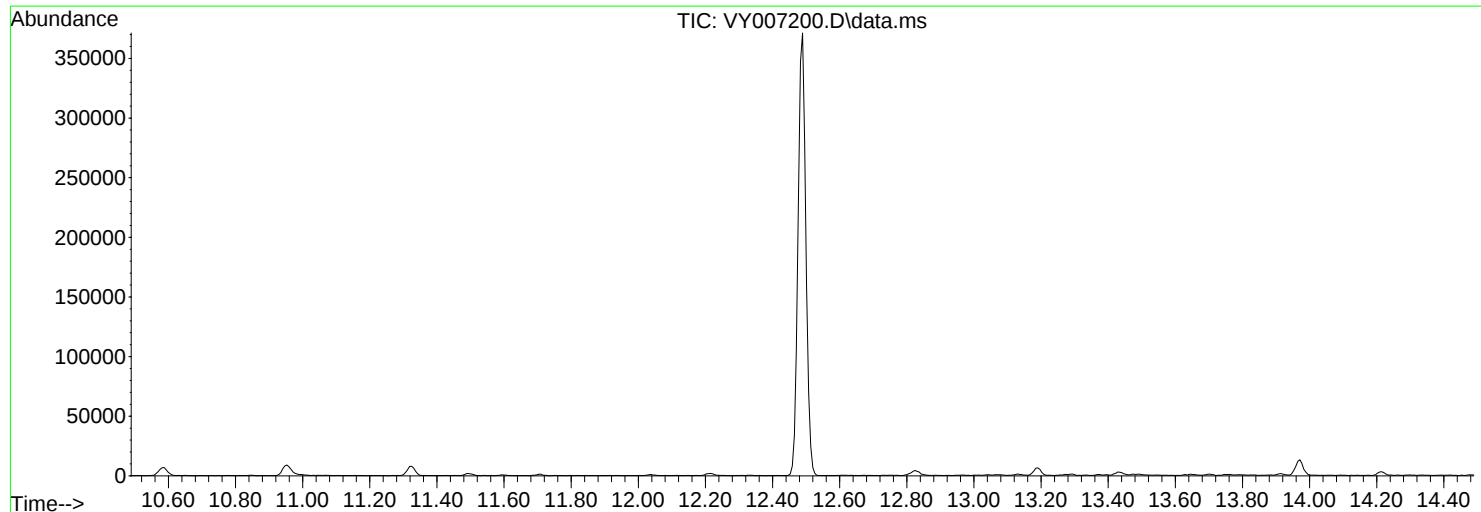

AutoFind: Scans 1749, 1750, 1751; Background Corrected with Scan 1740

| Target | Rel. to | Lower  | Upper  | Rel.  | Raw   | Result    |
|--------|---------|--------|--------|-------|-------|-----------|
| Mass   | Mass    | Limit% | Limit% | Abn%  | Abn   | Pass/Fail |
| 50     | 95      | 15     | 40     | 20.4  | 12157 | PASS      |
| 75     | 95      | 30     | 60     | 56.6  | 33787 | PASS      |
| 95     | 95      | 100    | 100    | 100.0 | 59728 | PASS      |
| 96     | 95      | 5      | 9      | 6.8   | 4087  | PASS      |
| 173    | 174     | 0.00   | 2      | 1.3   | 601   | PASS      |
| 174    | 95      | 50     | 100    | 76.4  | 45629 | PASS      |
| 175    | 174     | 5      | 9      | 7.5   | 3413  | PASS      |
| 176    | 174     | 95     | 101    | 97.8  | 44637 | PASS      |
| 177    | 176     | 5      | 9      | 7.4   | 3286  | PASS      |