
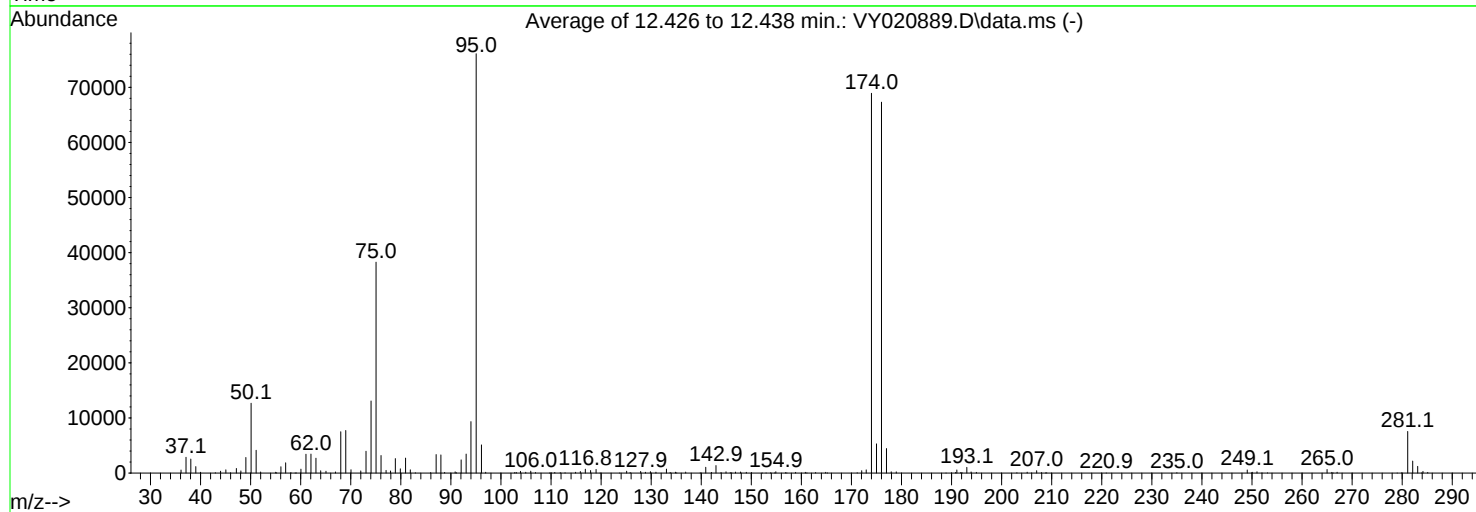


Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY012225\
Data File : VY020889.D
Acq On : 22 Jan 2025 08:30
Operator : SY/MD
Sample : BFB
Misc : 5.00g/5.0mL/MSVOA_Y/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_Y
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y010625S.M
Title : SW846 8260
Last Update : Thu Jan 23 00:38:42 2025

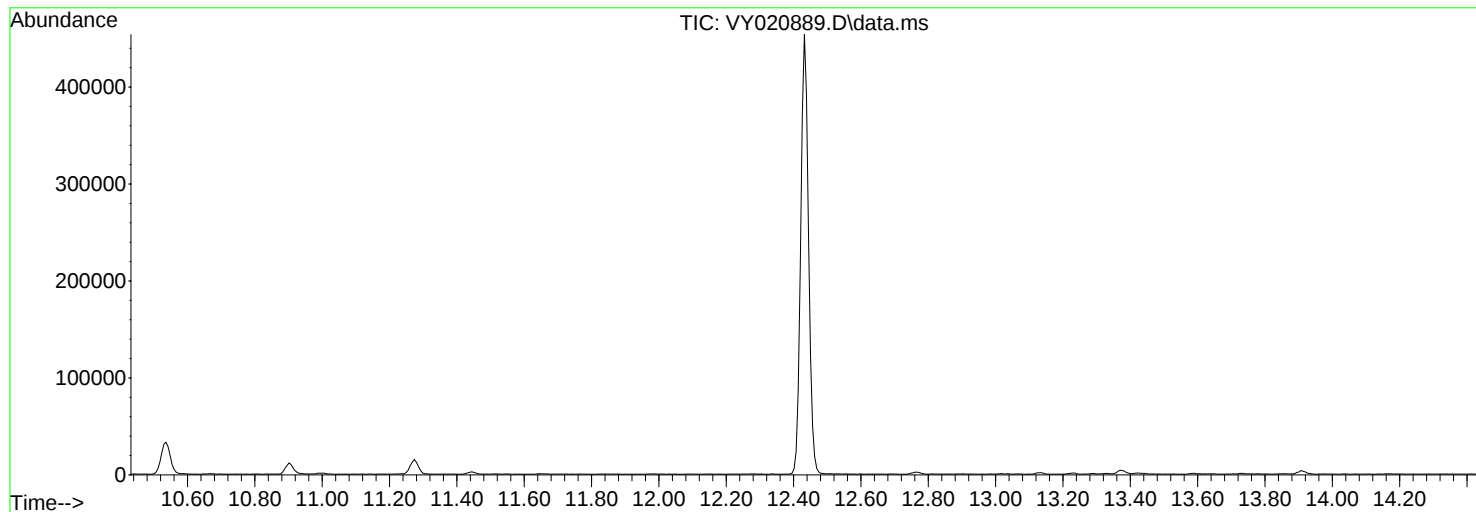

AutoFind: Scans 1756, 1757, 1758; Background Corrected with Scan 1747

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	16.7	12672	PASS
75	95	30	60	50.3	38275	PASS
95	95	100	100	100.0	76096	PASS
96	95	5	9	6.7	5115	PASS
173	174	0.00	2	0.8	582	PASS
174	95	50	100	90.6	68923	PASS
175	174	5	9	7.7	5311	PASS
176	174	95	101	97.7	67307	PASS
177	176	5	9	6.6	4451	PASS