

Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY012522\
 Data File : VY007286.D
 Acq On : 25 Jan 2022 10:59
 Operator : SY/MD
 Sample : VY0125SBL01
 Misc : 5.00g/5.0mL/MSVOA_Y/SOIL
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 MSVOA_Y
 ClientSampleId :
 VY0125SBL01

Quant Time: Jan 26 03:56:11 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y011322S.M
 Quant Title : SW846 8260
 QLast Update : Fri Jan 14 05:48:29 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Pentafluorobenzene	7.789	168	83038	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	8.691	114	156625	50.000	ug/l	0.00
63) Chlorobenzene-d5	11.495	117	145972	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.428	152	64022	50.000	ug/l	0.00

System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.142	65	46046	45.192	ug/l	0.00
Spiked Amount	50.000	Range	50 - 163	Recovery	=	90.380%
35) Dibromofluoromethane	7.722	113	50416	47.604	ug/l	0.00
Spiked Amount	50.000	Range	54 - 147	Recovery	=	95.200%
50) Toluene-d8	10.179	98	189612	48.998	ug/l	0.00
Spiked Amount	50.000	Range	49 - 140	Recovery	=	98.000%
62) 4-Bromofluorobenzene	12.483	95	66732	48.478	ug/l	0.00
Spiked Amount	50.000	Range	25 - 144	Recovery	=	96.960%


Target Compounds	Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY012522\
Data File : VY007286.D
Acq On : 25 Jan 2022 10:59
Operator : SY/MD
Sample : VY0125SBL01
Misc : 5.00g/5.0mL/MSVOA_Y/SOIL
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_Y
ClientSampleId :
VY0125SBL01

Quant Time: Jan 26 03:56:11 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y011322S.M
Quant Title : SW846 8260
QLast Update : Fri Jan 14 05:48:29 2022
Response via : Initial Calibration




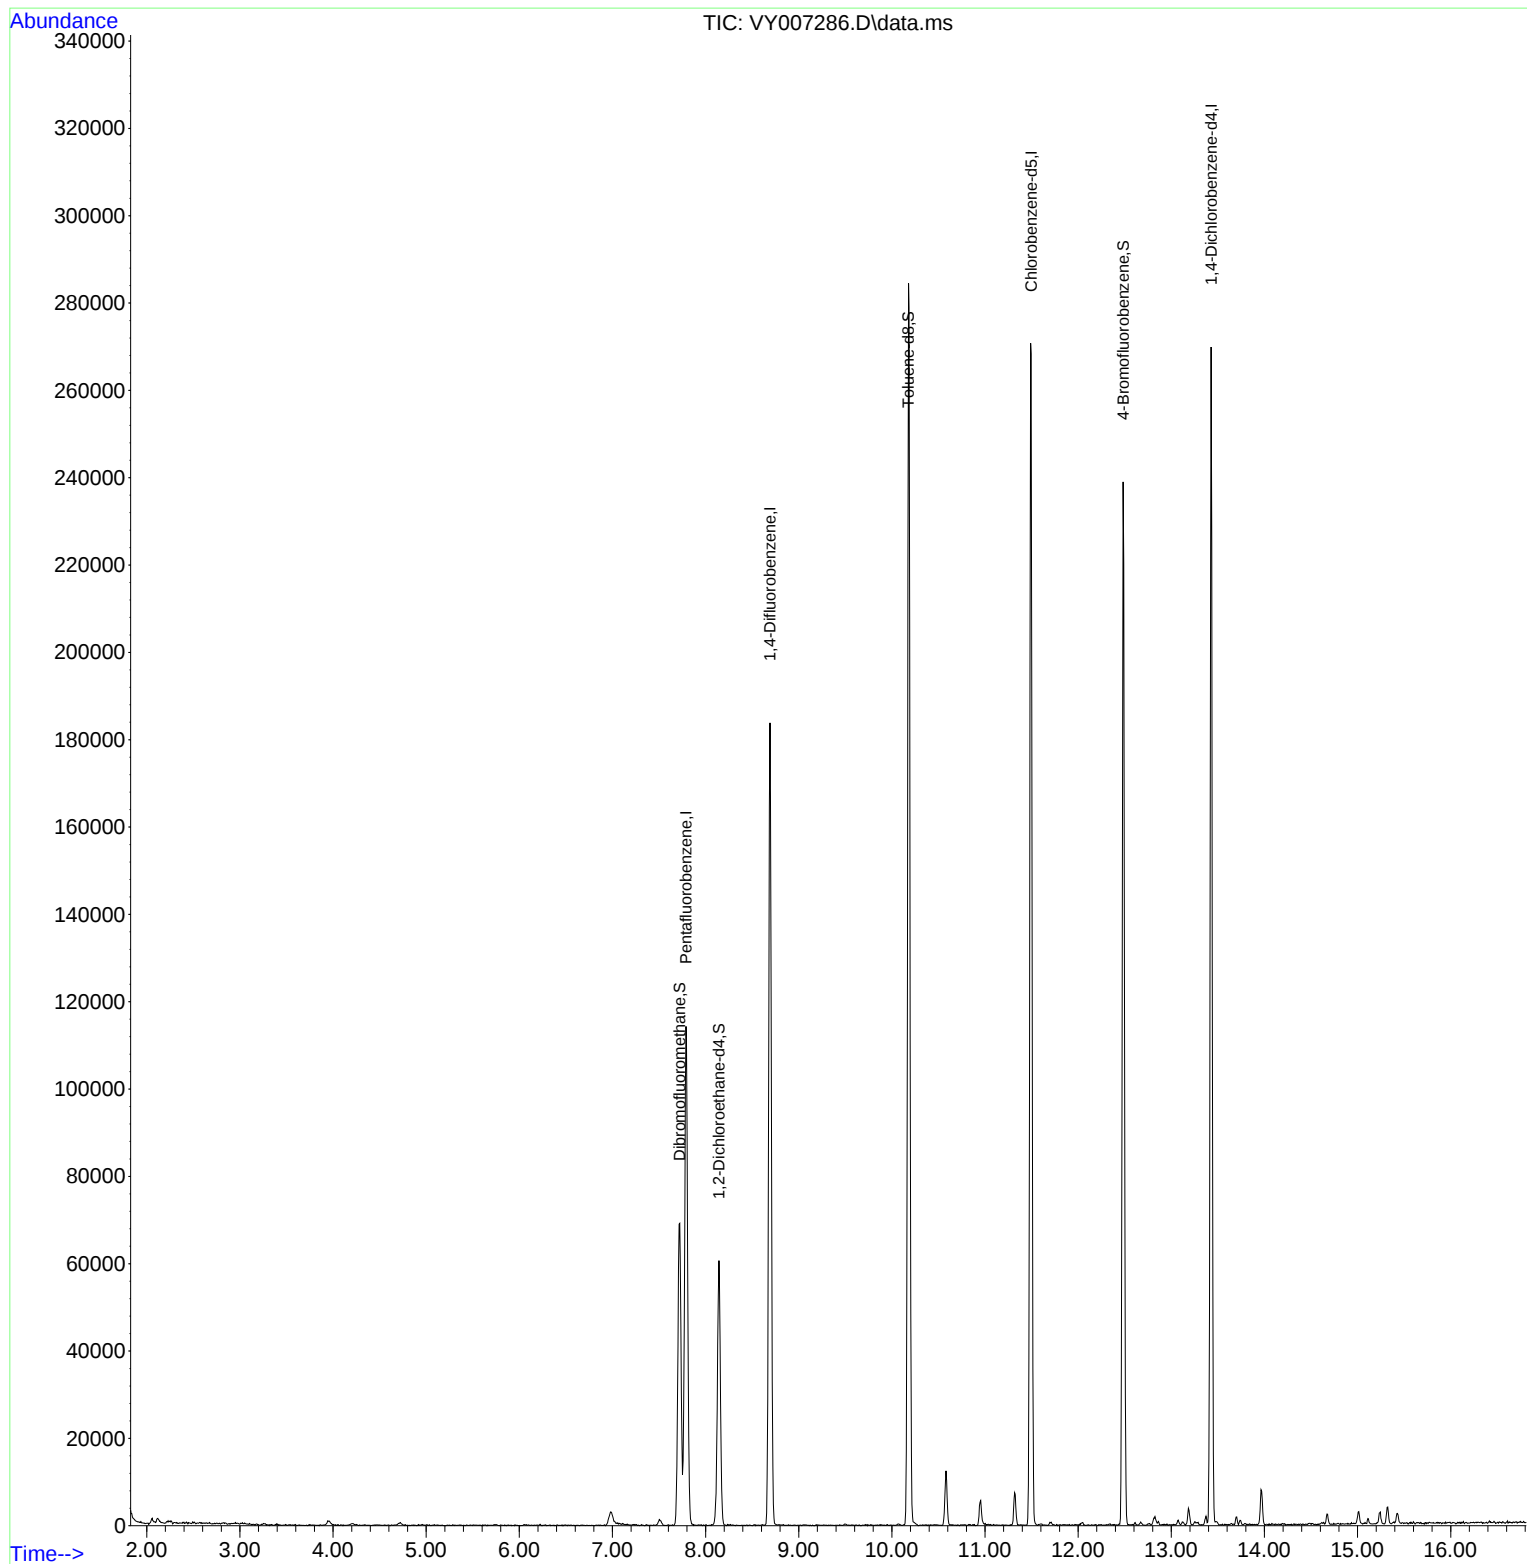


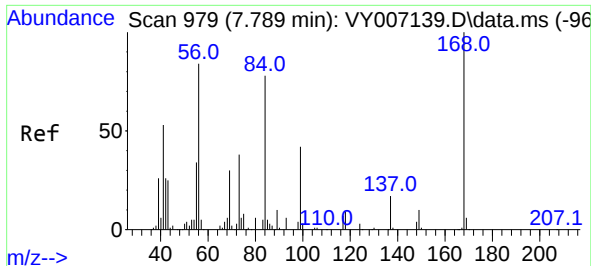

#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 7.789 min Scan# 91
Delta R.T. -0.000 min
Lab File: VY007286.D
Acq: 25 Jan 2022 10:59




Instrument :
MSVOA_Y
ClientSampleId :
VY0125SBL01


Tgt Ion:168 Resp: 83038
Ion Ratio Lower Upper
168 100
99 60.6 49.1 73.7

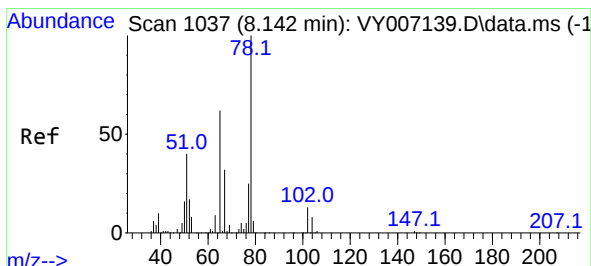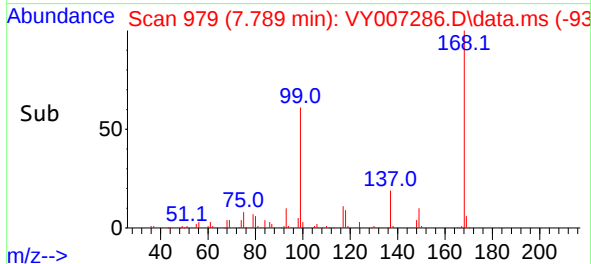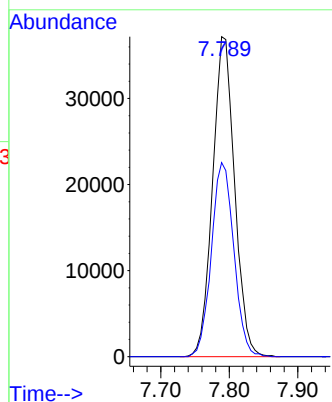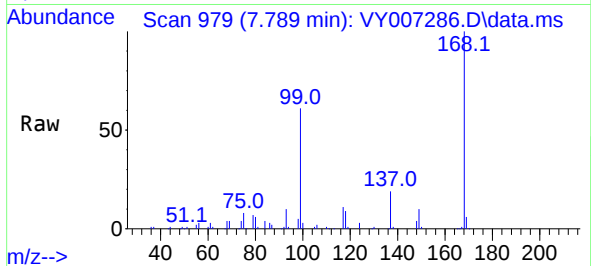

#33
1,2-Dichloroethane-d4
Concen: 45.192 ug/l
RT: 8.142 min Scan# 1037
Delta R.T. 0.000 min
Lab File: VY007286.D
Acq: 25 Jan 2022 10:59

Tgt Ion: 65 Resp: 46046
Ion Ratio Lower Upper
65 100
67 52.9 0.0 105.6


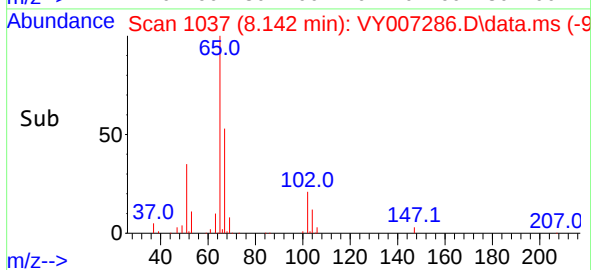
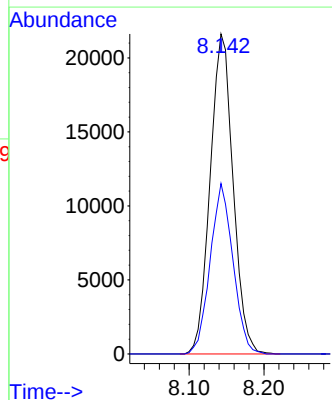
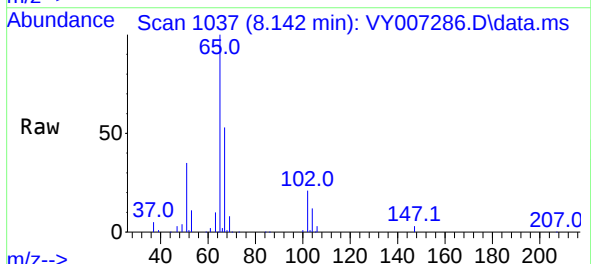


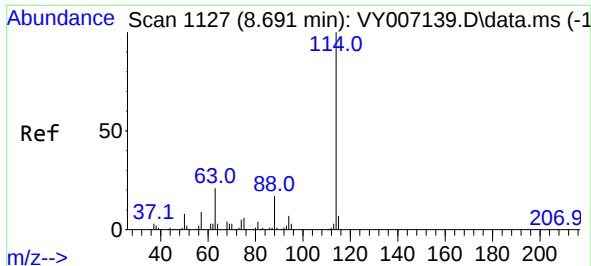

#34
1,4-Difluorobenzene
Concen: 50.000 ug/l
RT: 8.691 min Scan# 1127
Delta R.T. 0.000 min
Lab File: VY007286.D
Acq: 25 Jan 2022 10:59




Instrument :
MSVOA_Y
ClientSampleId :
VY0125SBL01


Tgt Ion:114 Resp: 156625
Ion Ratio Lower Upper
114 100
63 18.9 0.0 39.2
88 15.6 0.0 31.0

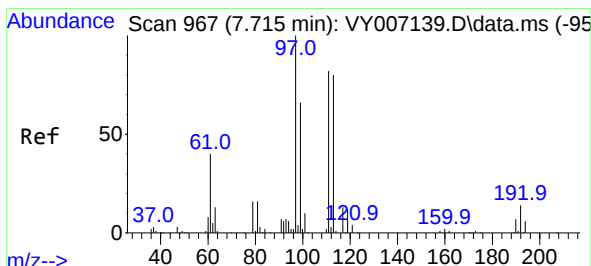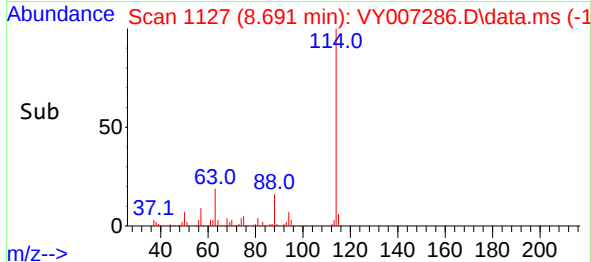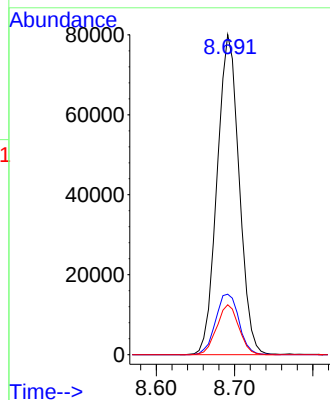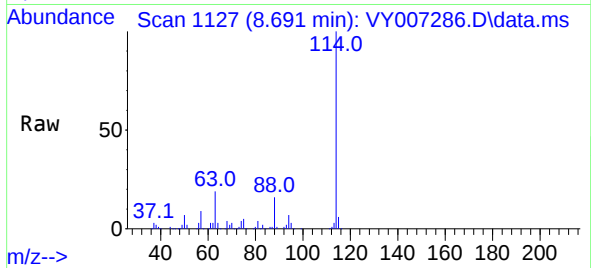

#35
Dibromofluoromethane
Concen: 47.604 ug/l
RT: 7.722 min Scan# 968
Delta R.T. 0.006 min
Lab File: VY007286.D
Acq: 25 Jan 2022 10:59

Tgt Ion:113 Resp: 50416
Ion Ratio Lower Upper
113 100
111 103.9 82.2 123.4
192 17.7 14.2 21.4


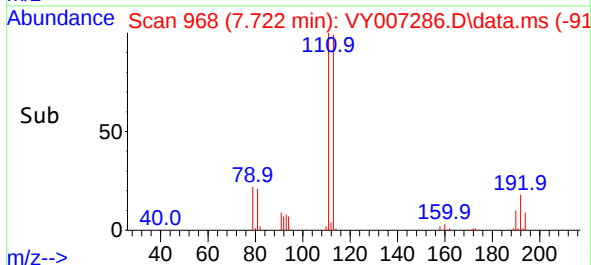
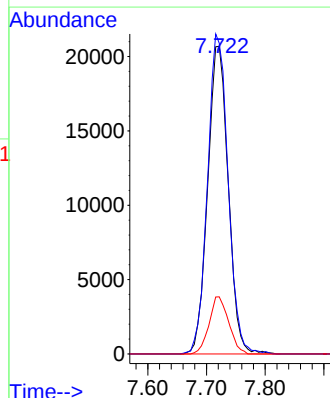
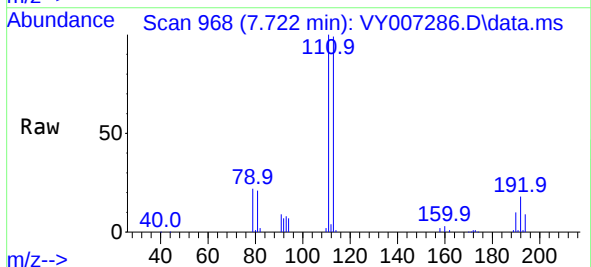


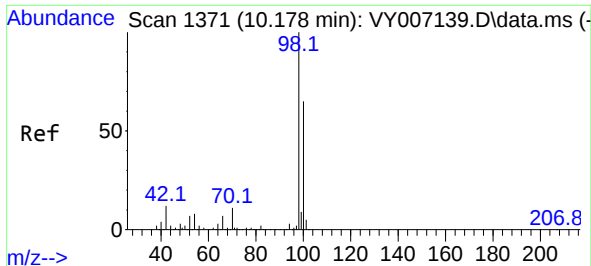

#50
Toluene-d8
Concen: 48.998 ug/l
RT: 10.179 min Scan# 11
Delta R.T. 0.000 min
Lab File: VY007286.D
Acq: 25 Jan 2022 10:59




Instrument :
MSVOA_Y
ClientSampleId :
VY0125SBL01


Tgt Ion: 98 Resp: 189612
Ion Ratio Lower Upper
98 100
100 64.4 52.2 78.2

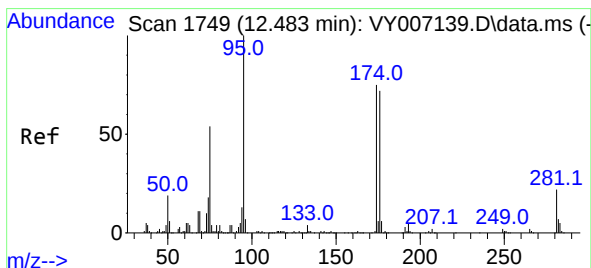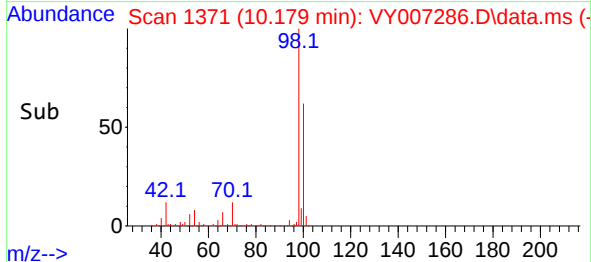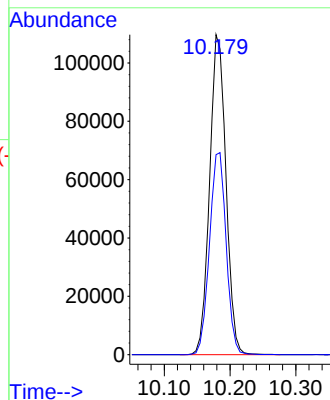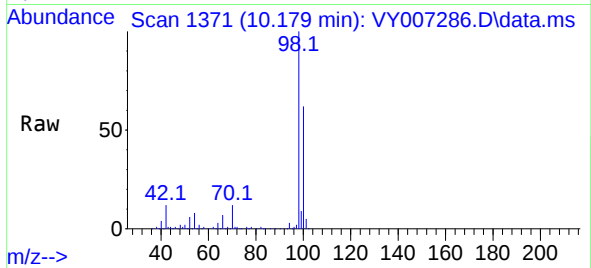

#62
4-Bromofluorobenzene
Concen: 48.478 ug/l
RT: 12.483 min Scan# 1749
Delta R.T. 0.000 min
Lab File: VY007286.D
Acq: 25 Jan 2022 10:59

Tgt Ion: 95 Resp: 66732
Ion Ratio Lower Upper
95 100
174 76.1 0.0 148.4
176 74.5 0.0 146.6


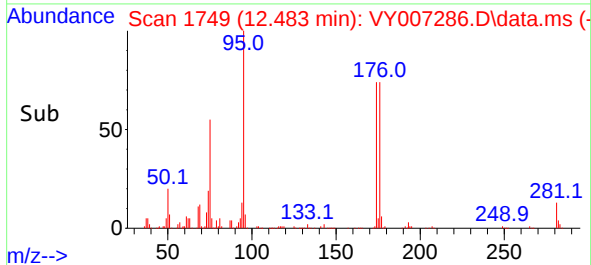
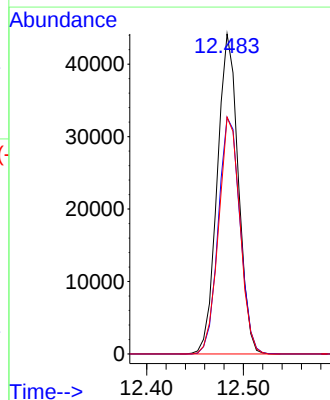
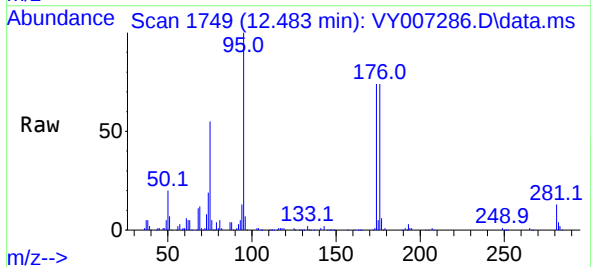


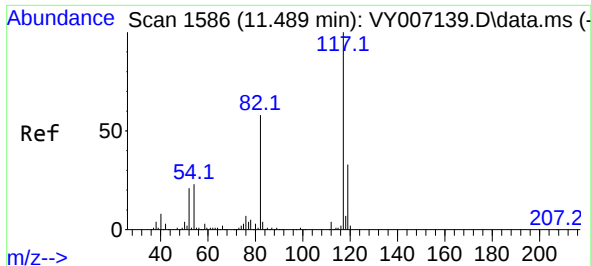

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 11.495 min Scan# 11
Delta R.T. 0.006 min
Lab File: VY007286.D
Acq: 25 Jan 2022 10:59

Instrument :
MSVOA_Y
ClientSampleId :
VY0125SBL01

Tgt Ion:117 Resp: 145972
Ion Ratio Lower Upper
117 100
82 54.4 45.4 68.0
119 32.2 26.4 39.6

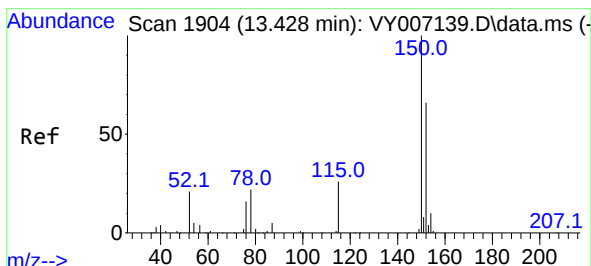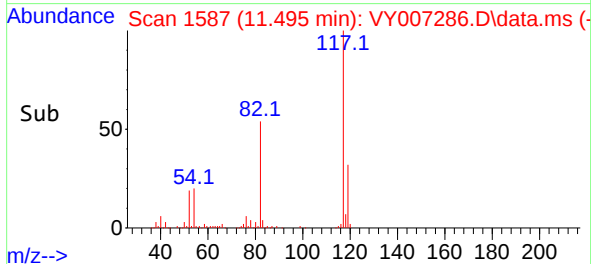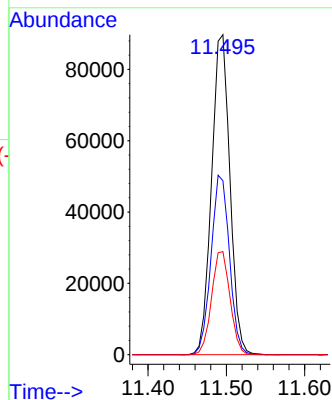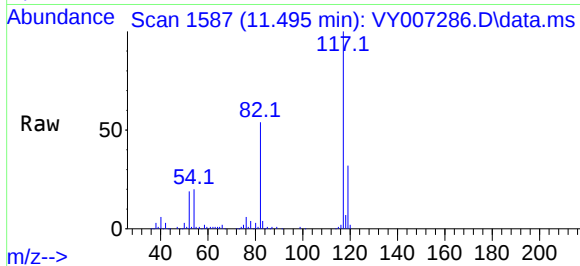

#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 13.428 min Scan# 1904
Delta R.T. 0.000 min
Lab File: VY007286.D
Acq: 25 Jan 2022 10:59

Tgt Ion:152 Resp: 64022
Ion Ratio Lower Upper
152 100
115 60.8 31.4 94.0
150 157.5 0.0 348.4

