


Data Path : Z:\voasrv\HPCHEM1\MSVOA\_Y\Data\VY012522\  
 Data File : VY007284.D  
 Acq On : 25 Jan 2022 09:08  
 Operator : SY/MD  
 Sample : BFB  
 Misc : 5.00g/5.0mL/MSVOA\_Y/SOIL  
 ALS Vial : 1 Sample Multiplier: 1

Instrument :  
 MSVOA\_Y  
 ClientSampleId :  
 BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA\_Y\methods\82Y011322S.M  
 Title : SW846 8260  
 Last Update : Fri Jan 14 05:48:29 2022

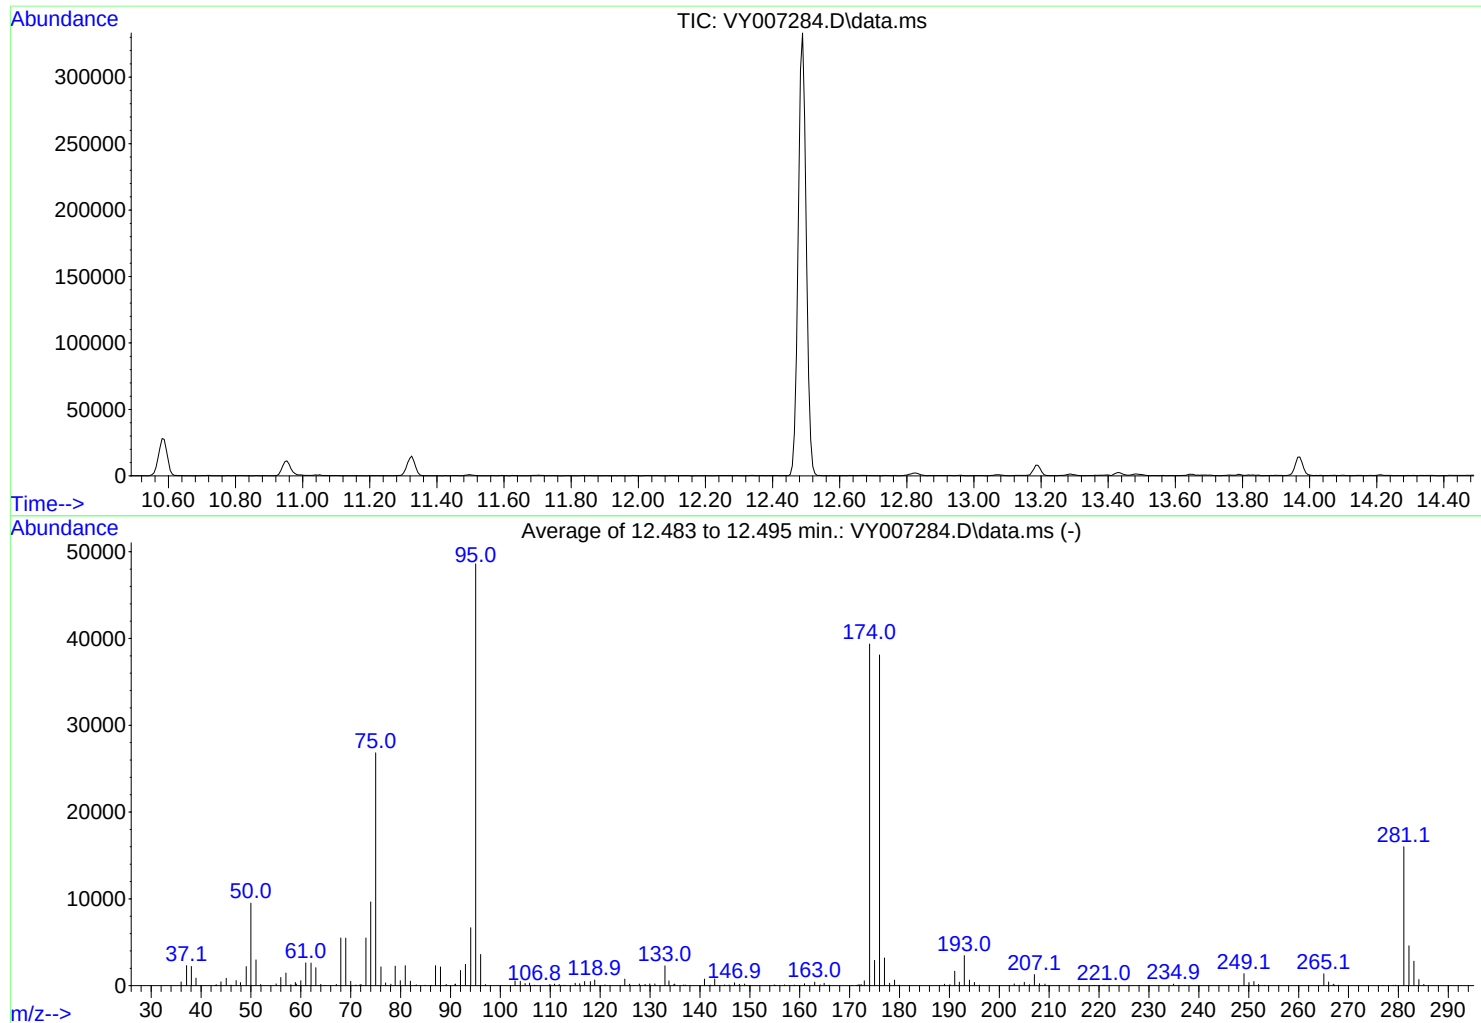

AutoFind: Scans 1749, 1750, 1751; Background Corrected with Scan 1740

| Target<br>Mass | Rel. to<br>Mass | Lower<br>Limit% | Upper<br>Limit% | Rel.<br>Abn% | Raw<br>Abn | Result<br>Pass/Fail |
|----------------|-----------------|-----------------|-----------------|--------------|------------|---------------------|
| 50             | 95              | 15              | 40              | 19.6         | 9515       | PASS                |
| 75             | 95              | 30              | 60              | 55.2         | 26827      | PASS                |
| 95             | 95              | 100             | 100             | 100.0        | 48605      | PASS                |
| 96             | 95              | 5               | 9               | 7.4          | 3590       | PASS                |
| 173            | 174             | 0.00            | 2               | 1.4          | 561        | PASS                |
| 174            | 95              | 50              | 100             | 81.0         | 39373      | PASS                |
| 175            | 174             | 5               | 9               | 7.4          | 2913       | PASS                |
| 176            | 174             | 95              | 101             | 96.8         | 38109      | PASS                |
| 177            | 176             | 5               | 9               | 8.4          | 3198       | PASS                |