
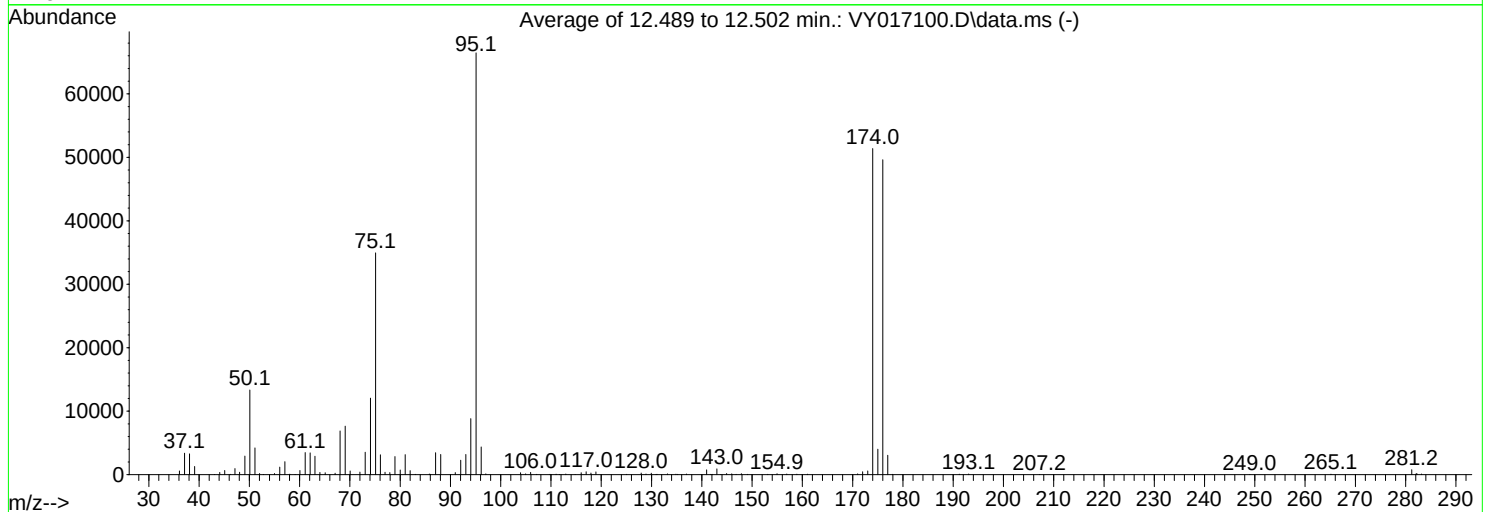


Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY012524\
Data File : VY017100.D
Acq On : 25 Jan 2024 08:52
Operator : SY/MD
Sample : BFB
Misc : 5.00g/5.0mL/MSVOA_Y/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_Y
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y012424S.M
Title : SW846 8260
Last Update : Thu Jan 25 04:44:10 2024

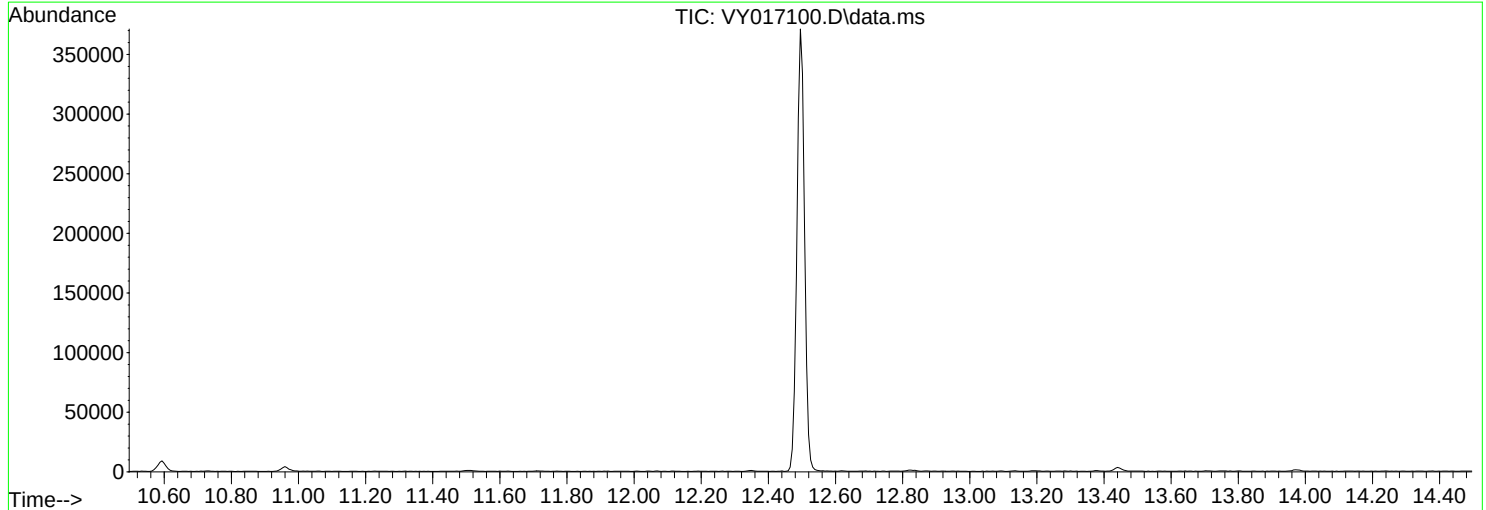

AutoFind: Scans 1750, 1751, 1752; Background Corrected with Scan 1742

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	20.1	13347	PASS
75	95	30	60	52.6	34939	PASS
95	95	100	100	100.0	66469	PASS
96	95	5	9	6.6	4372	PASS
173	174	0.00	2	1.1	572	PASS
174	95	50	100	77.3	51397	PASS
175	174	5	9	7.8	4003	PASS
176	174	95	101	96.6	49627	PASS
177	176	5	9	6.1	3046	PASS