
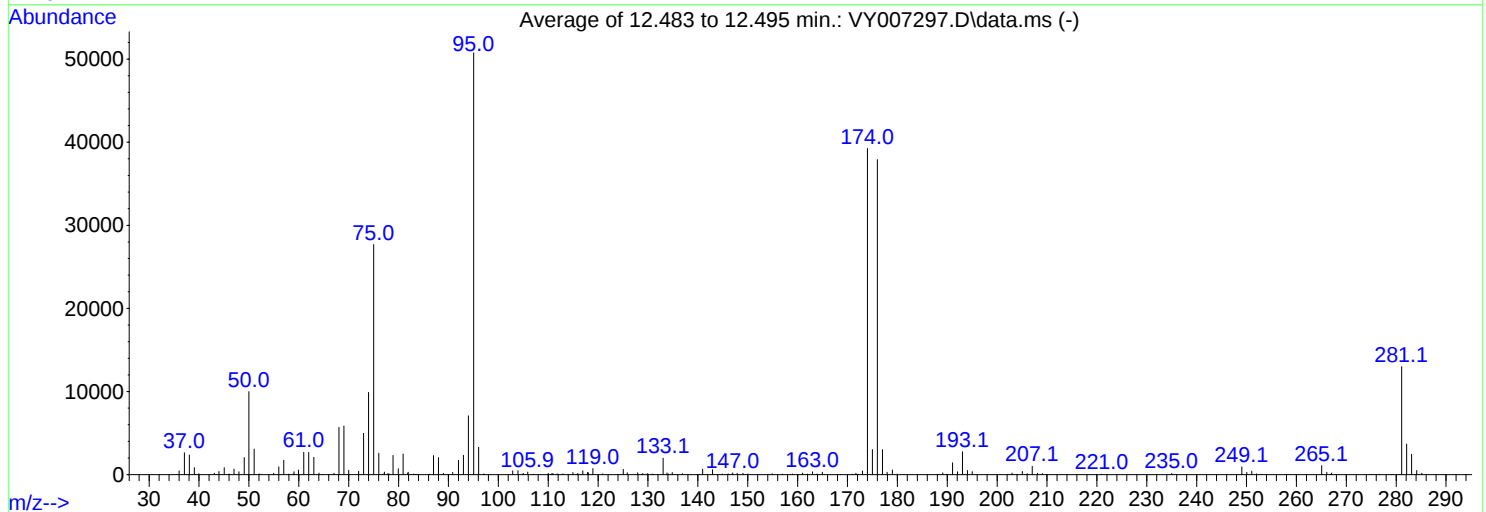


Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY012622\
 Data File : VY007297.D
 Acq On : 26 Jan 2022 08:59
 Operator : SY/MD
 Sample : BFB
 Misc : 5.00g/5.0mL/MSVOA_Y/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_Y
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y011322S.M
 Title : SW846 8260
 Last Update : Fri Jan 14 05:48:29 2022

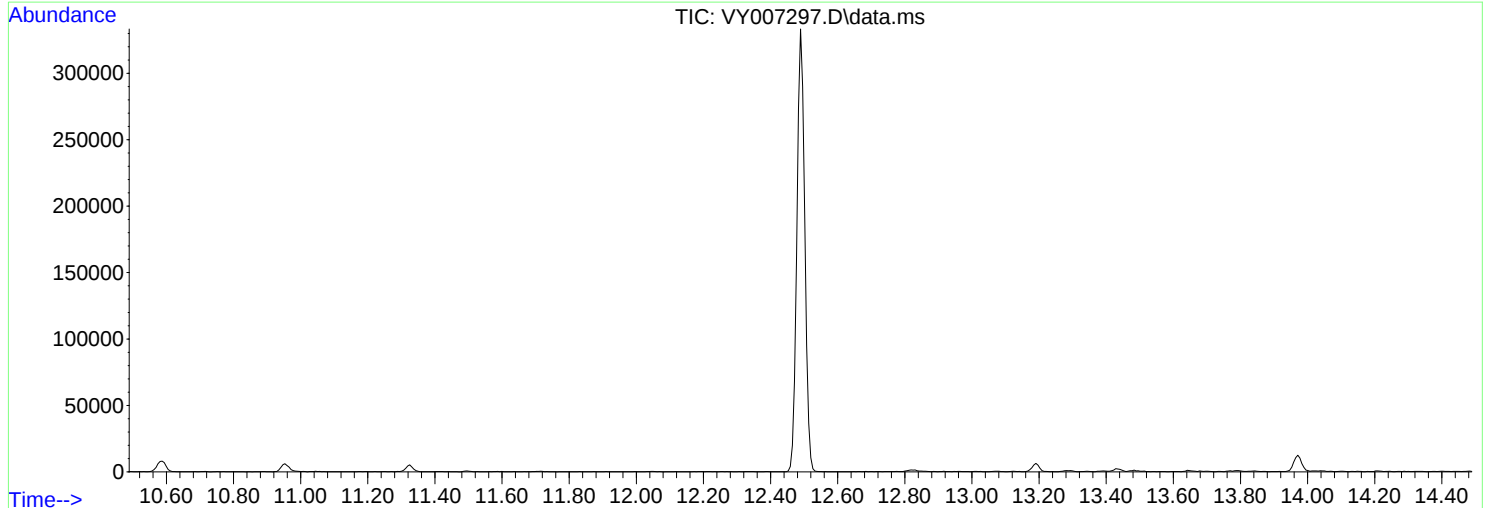

AutoFind: Scans 1749, 1750, 1751; Background Corrected with Scan 1740

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	19.7	10001	PASS
75	95	30	60	54.6	27685	PASS
95	95	100	100	100.0	50749	PASS
96	95	5	9	6.5	3294	PASS
173	174	0.00	2	1.1	440	PASS
174	95	50	100	77.3	39240	PASS
175	174	5	9	7.7	3020	PASS
176	174	95	101	96.6	37904	PASS
177	176	5	9	7.9	2997	PASS