
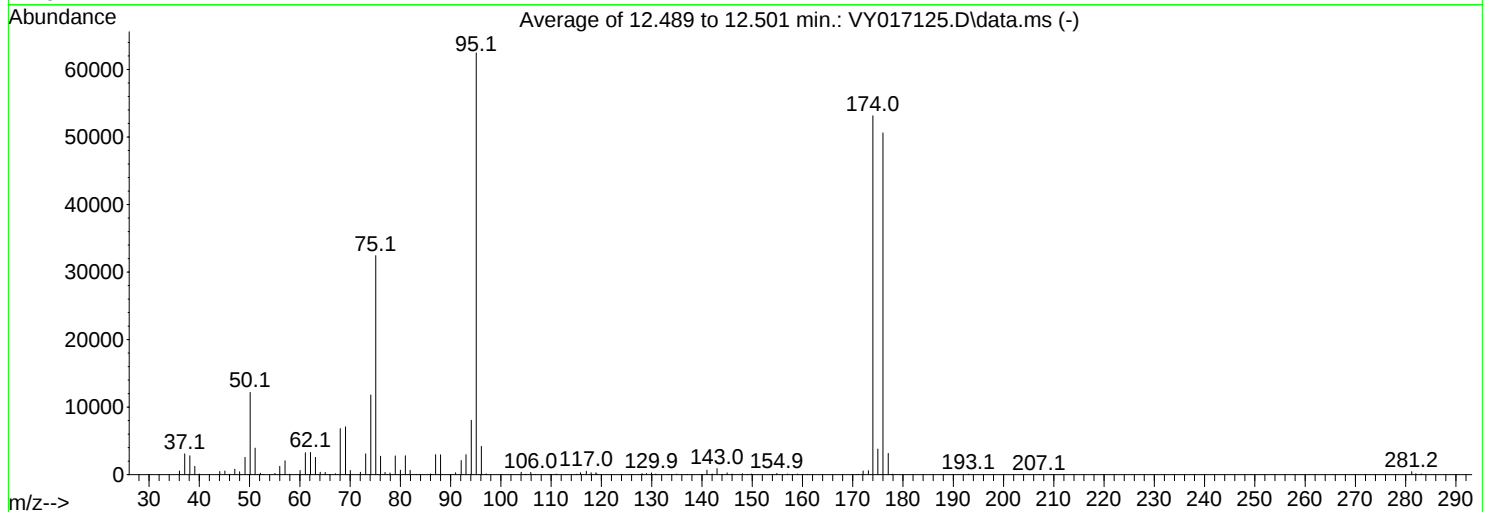


Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY012924\
Data File : VY017125.D
Acq On : 29 Jan 2024 09:12
Operator : SY/MD
Sample : BFB
Misc : 5.00g/5.0mL/MSVOA_Y/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_Y
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y012424S.M
Title : SW846 8260
Last Update : Thu Jan 25 04:44:10 2024

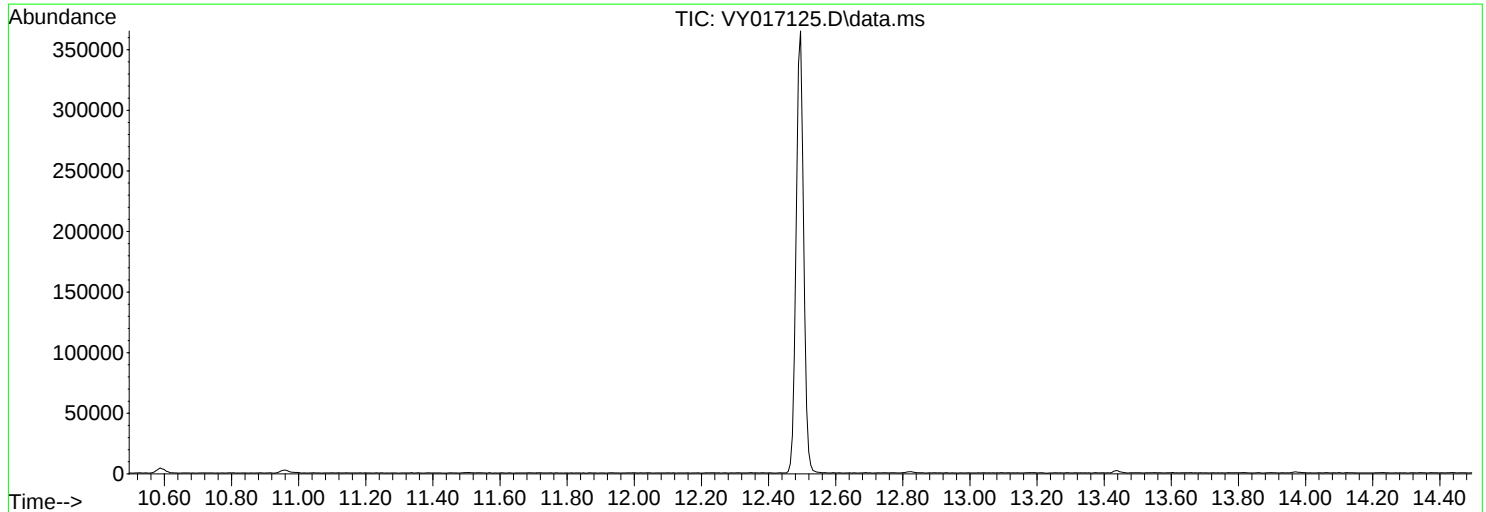

AutoFind: Scans 1750, 1751, 1752; Background Corrected with Scan 1742

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	19.5	12188	PASS
75	95	30	60	51.9	32435	PASS
95	95	100	100	100.0	62467	PASS
96	95	5	9	6.7	4203	PASS
173	174	0.00	2	1.1	589	PASS
174	95	50	100	85.1	53144	PASS
175	174	5	9	7.2	3800	PASS
176	174	95	101	95.2	50608	PASS
177	176	5	9	6.2	3148	PASS