
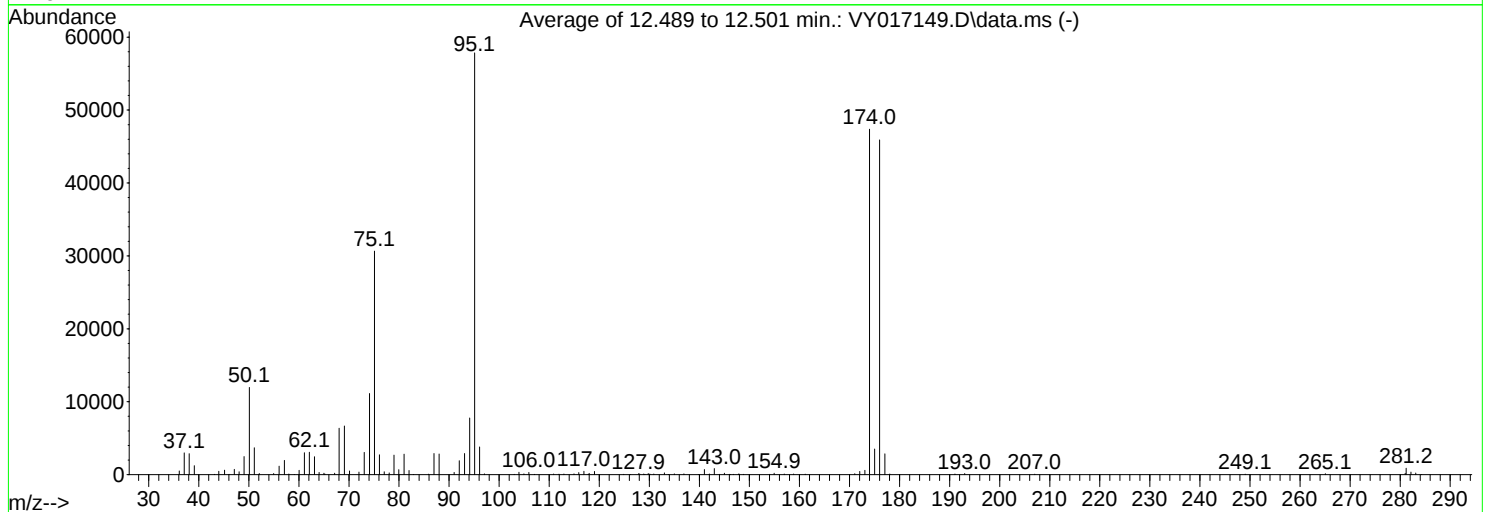


Data Path : Z:\voasrv\HPCHEM1\MSVOA\_Y\Data\VY013124\  
Data File : VY017149.D  
Acq On : 31 Jan 2024 09:17  
Operator : SY/MD  
Sample : BFB  
Misc : 5.00g/5.0mL/MSVOA\_Y/SOIL  
ALS Vial : 1 Sample Multiplier: 1

Instrument :  
MSVOA\_Y  
ClientSampleId :  
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA\_Y\methods\82Y012424S.M  
Title : SW846 8260  
Last Update : Thu Feb 01 16:01:43 2024

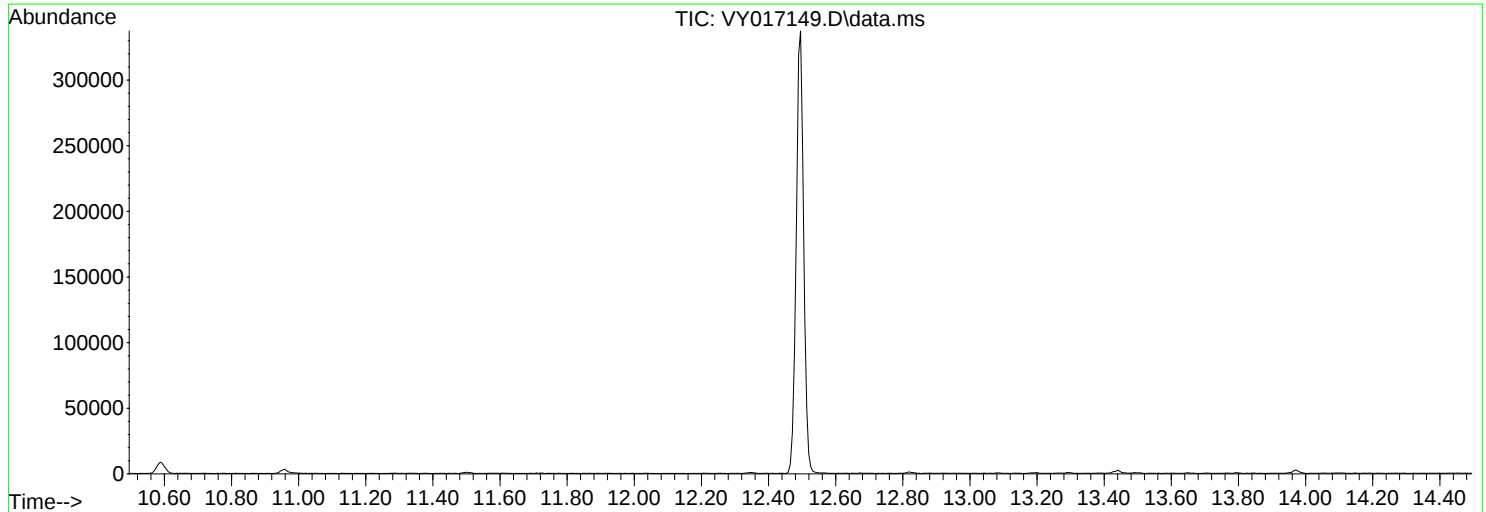

AutoFind: Scans 1750, 1751, 1752; Background Corrected with Scan 1742

| Target<br>Mass | Rel. to<br>Mass | Lower<br>Limit% | Upper<br>Limit% | Rel.<br>Abn% | Raw<br>Abn | Result<br>Pass/Fail |
|----------------|-----------------|-----------------|-----------------|--------------|------------|---------------------|
| 50             | 95              | 15              | 40              | 20.7         | 11965      | PASS                |
| 75             | 95              | 30              | 60              | 53.0         | 30651      | PASS                |
| 95             | 95              | 100             | 100             | 100.0        | 57848      | PASS                |
| 96             | 95              | 5               | 9               | 6.6          | 3791       | PASS                |
| 173            | 174             | 0.00            | 2               | 1.3          | 600        | PASS                |
| 174            | 95              | 50              | 100             | 81.9         | 47376      | PASS                |
| 175            | 174             | 5               | 9               | 7.4          | 3506       | PASS                |
| 176            | 174             | 95              | 101             | 96.9         | 45915      | PASS                |
| 177            | 176             | 5               | 9               | 6.2          | 2844       | PASS                |