
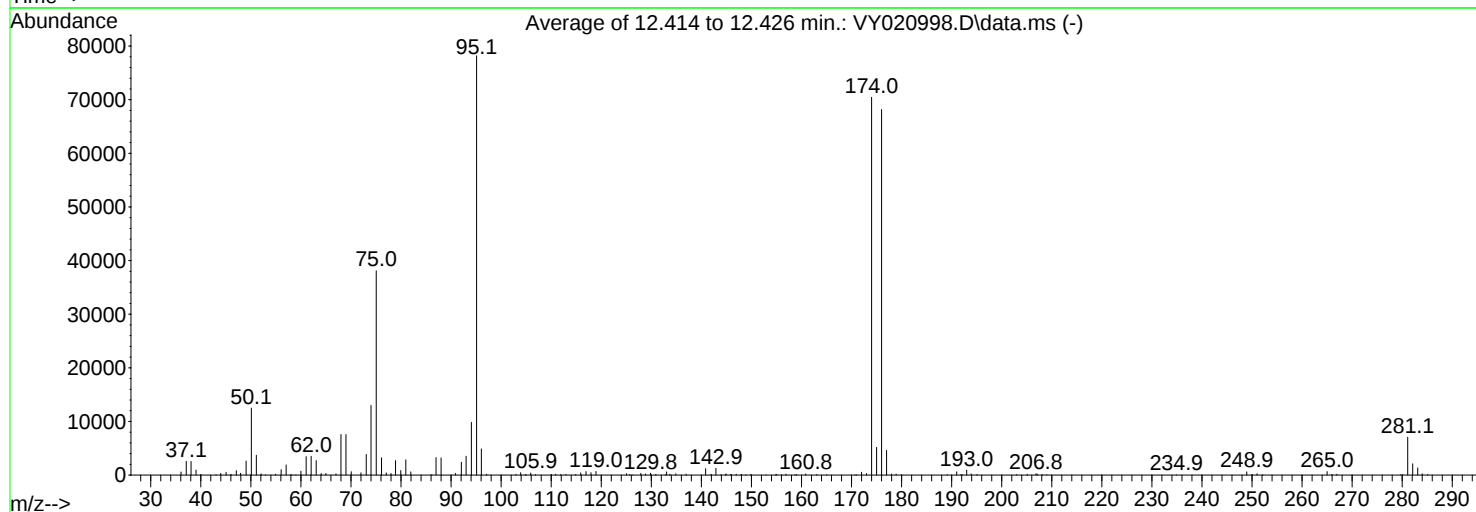


Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY013125\
Data File : VY020998.D
Acq On : 31 Jan 2025 08:34
Operator : SY/MD
Sample : BFB
Misc : 5.00g/5.0mL/MSVOA_Y/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_Y
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y013025S.M
Title : SW846 8260
Last Update : Fri Jan 31 16:50:06 2025

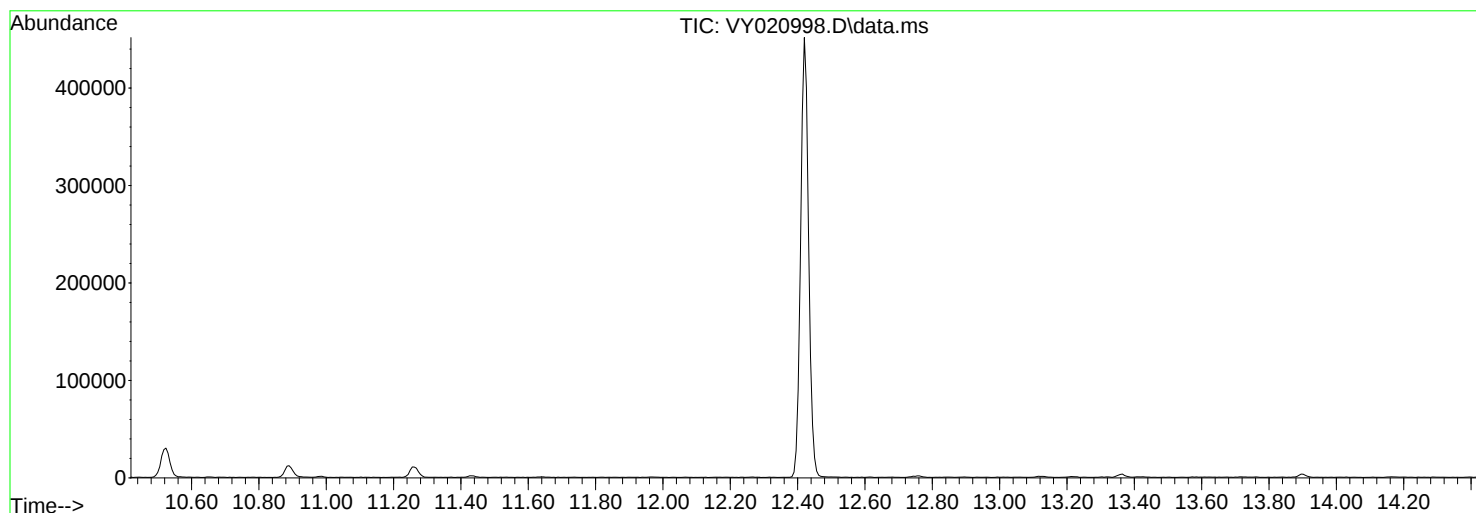

AutoFind: Scans 1754, 1755, 1756; Background Corrected with Scan 1746

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	16.0	12495	PASS
75	95	30	60	48.7	38099	PASS
95	95	100	100	100.0	78197	PASS
96	95	5	9	6.3	4891	PASS
173	174	0.00	2	0.4	304	PASS
174	95	50	100	90.1	70440	PASS
175	174	5	9	7.3	5152	PASS
176	174	95	101	96.8	68163	PASS
177	176	5	9	6.7	4601	PASS