
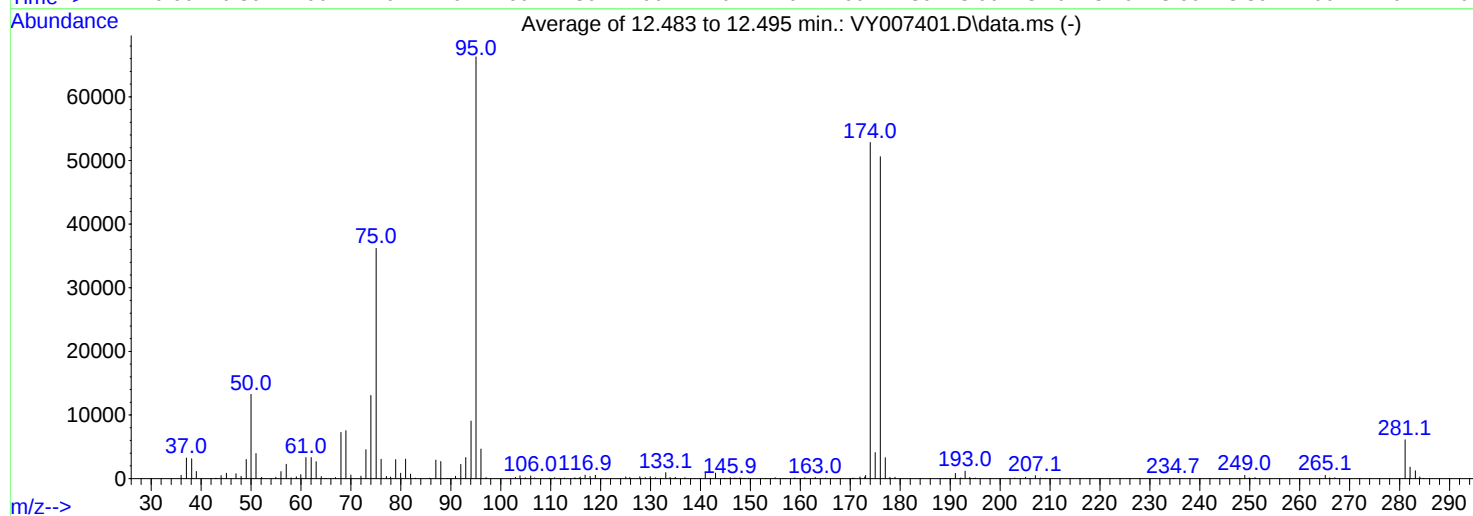


Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY020722\
 Data File : VY007401.D
 Acq On : 07 Feb 2022 09:05
 Operator : SY/MD
 Sample : BFB
 Misc : 5.00g/5.0mL/MSVOA_Y/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_Y
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y020222S.M
 Title : SW846 8260
 Last Update : Thu Feb 03 04:36:48 2022

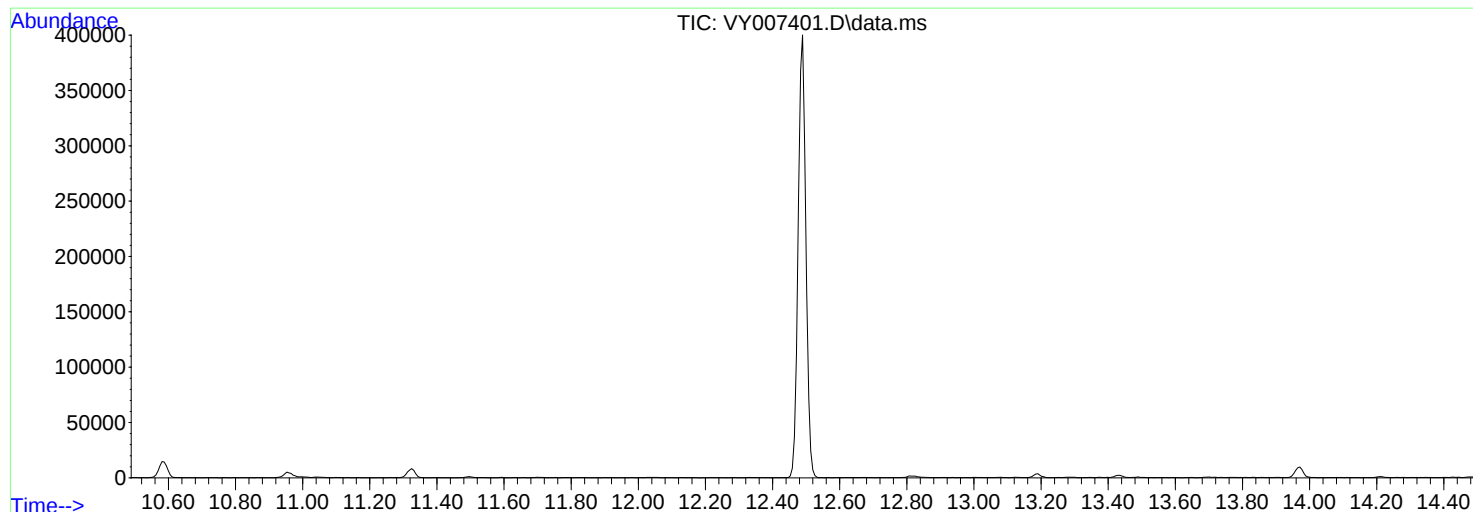

AutoFind: Scans 1749, 1750, 1751; Background Corrected with Scan 1740

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	20.0	13241	PASS
75	95	30	60	54.6	36197	PASS
95	95	100	100	100.0	66288	PASS
96	95	5	9	7.0	4648	PASS
173	174	0.00	2	0.9	501	PASS
174	95	50	100	79.7	52821	PASS
175	174	5	9	7.7	4092	PASS
176	174	95	101	95.8	50603	PASS
177	176	5	9	6.5	3300	PASS