
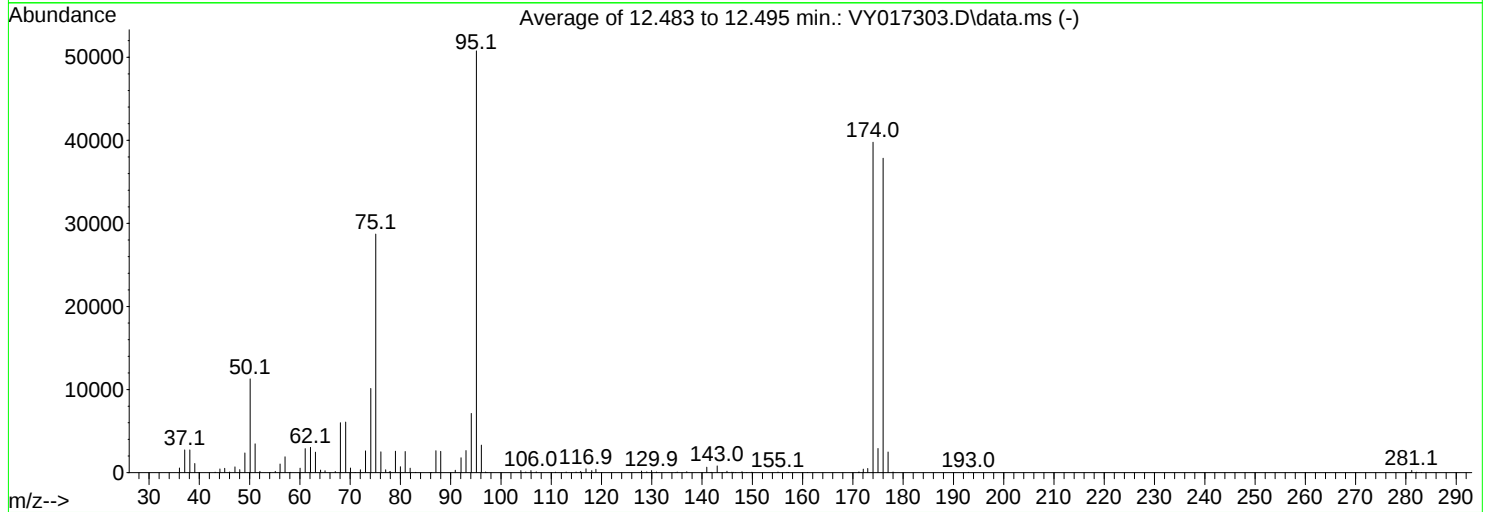


Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY020824\
Data File : VY017303.D
Acq On : 08 Feb 2024 09:43
Operator : SY/MD
Sample : BFB
Misc : 5.00g/5.0mL/MSVOA_Y/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_Y
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y020124S.M
Title : SW846 8260
Last Update : Fri Feb 02 00:56:04 2024

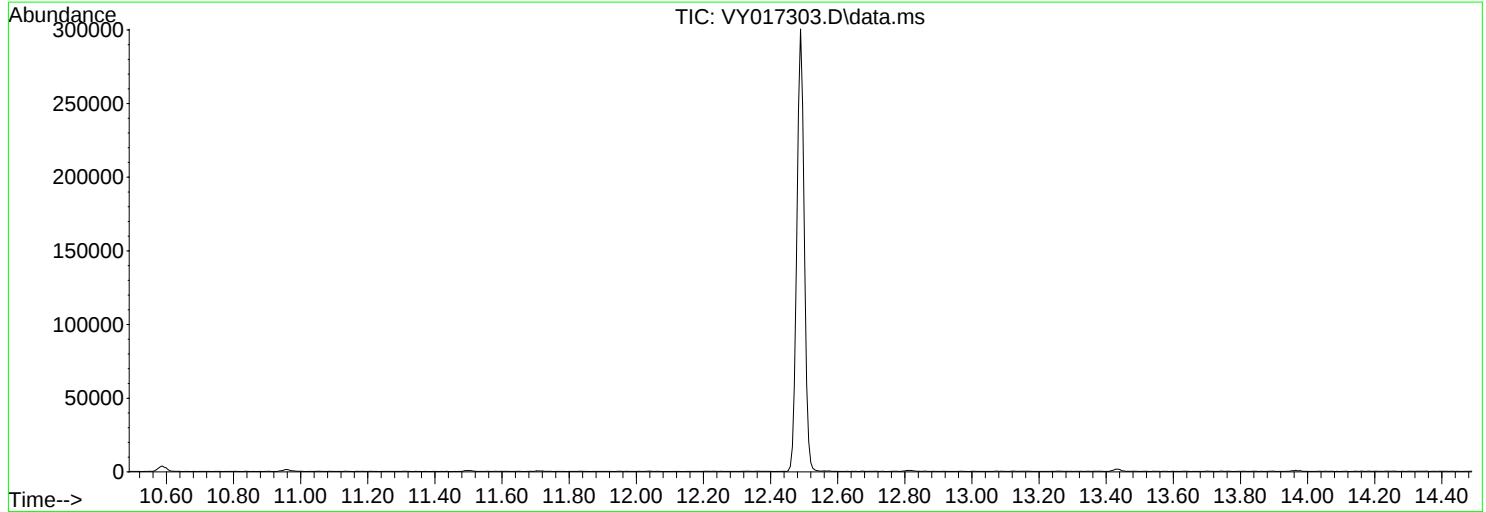

AutoFind: Scans 1749, 1750, 1751; Background Corrected with Scan 1741

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	22.2	11283	PASS
75	95	30	60	56.5	28709	PASS
95	95	100	100	100.0	50771	PASS
96	95	5	9	6.5	3317	PASS
173	174	0.00	2	1.3	511	PASS
174	95	50	100	78.3	39771	PASS
175	174	5	9	7.3	2903	PASS
176	174	95	101	95.1	37837	PASS
177	176	5	9	6.6	2495	PASS