

Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY020924\
 Data File : VY017339.D
 Acq On : 09 Feb 2024 15:08
 Operator : SY/MD
 Sample : P1414-04
 Misc : 5.43g/5.0mL/MSVOA_Y/SOIL/A
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 MSVOA_Y
 ClientSampleId :
 SB-7(12-13)

Quant Time: Feb 09 22:03:46 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y020124S.M
 Quant Title : SW846 8260
 QLast Update : Fri Feb 02 00:56:04 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Pentafluorobenzene	7.783	168	86464	50.000	ug/l	-0.01
34) 1,4-Difluorobenzene	8.685	114	165857	50.000	ug/l	-0.01
63) Chlorobenzene-d5	11.489	117	151993	50.000	ug/l	-0.01
72) 1,4-Dichlorobenzene-d4	13.428	152	59631	50.000	ug/l	0.00

System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.136	65	43033	55.712	ug/l	-0.01
Spiked Amount	50.000	Range	50 - 163	Recovery	=	111.420%
35) Dibromofluoromethane	7.710	113	42939	47.949	ug/l	-0.02
Spiked Amount	50.000	Range	54 - 147	Recovery	=	95.900%
50) Toluene-d8	10.179	98	150729	46.228	ug/l	0.00
Spiked Amount	50.000	Range	58 - 134	Recovery	=	92.460%
62) 4-Bromofluorobenzene	12.483	95	43493	40.720	ug/l	0.00
Spiked Amount	50.000	Range	30 - 143	Recovery	=	81.440%


Target Compounds	Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY020924\
Data File : VY017339.D
Acq On : 09 Feb 2024 15:08
Operator : SY/MD
Sample : P1414-04
Misc : 5.43g/5.0mL/MSVOA_Y/SOIL/A
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_Y
ClientSampleId :
SB-7(12-13)

Quant Time: Feb 09 22:03:46 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y020124S.M
Quant Title : SW846 8260
QLast Update : Fri Feb 02 00:56:04 2024
Response via : Initial Calibration




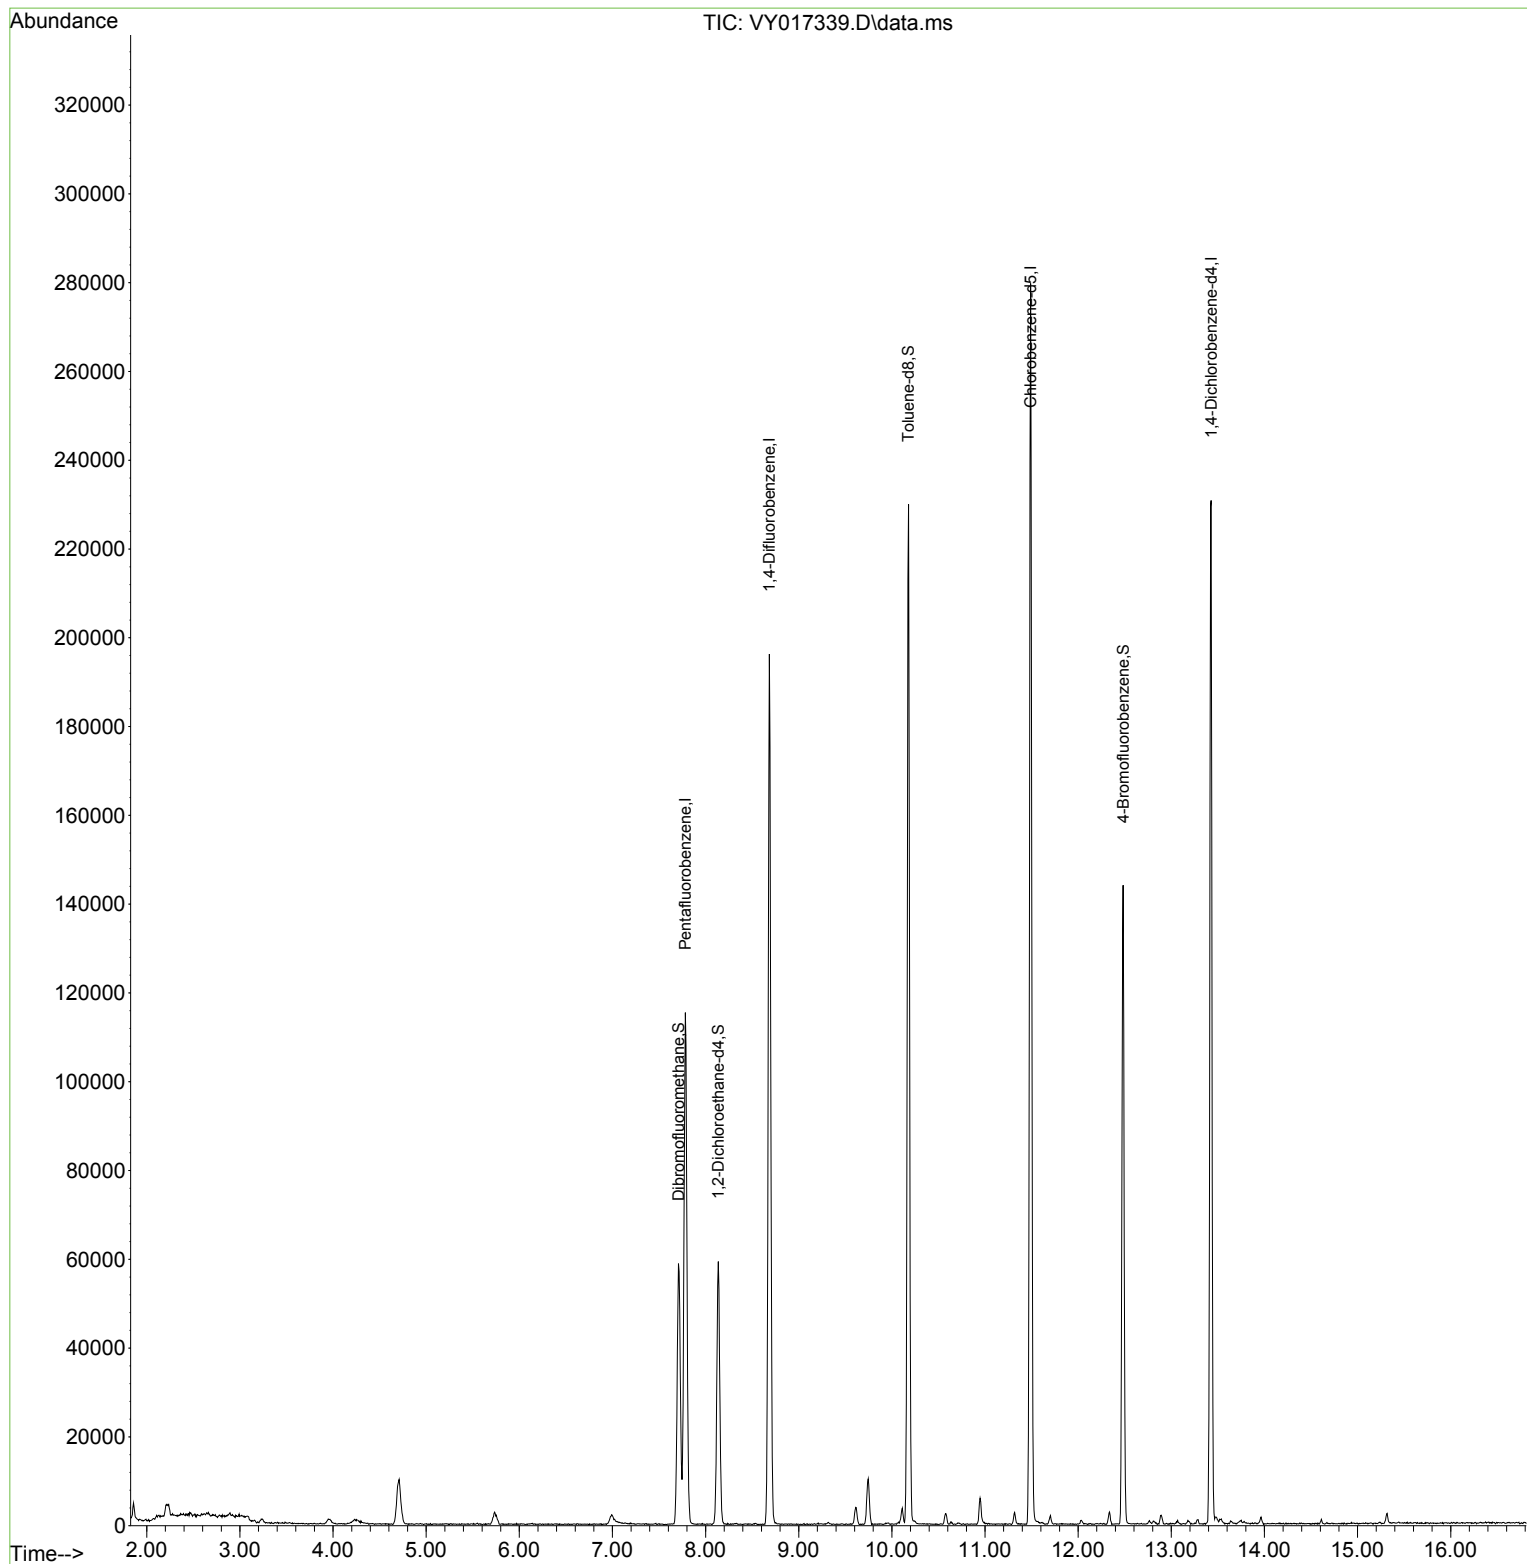


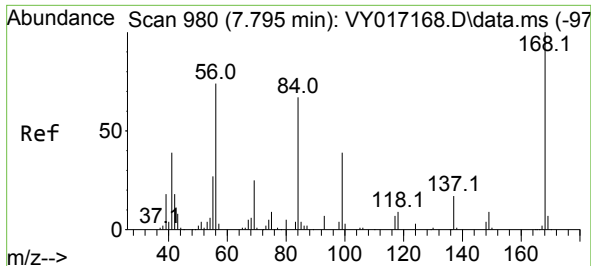

#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 7.783 min Scan# 91
Delta R.T. -0.012 min
Lab File: VY017339.D
Acq: 09 Feb 2024 15:08




Instrument :
MSVOA_Y
ClientSampleId :
SB-7(12-13)


Tgt Ion:168 Resp: 86464
Ion Ratio Lower Upper
168 100
99 55.3 44.2 66.4

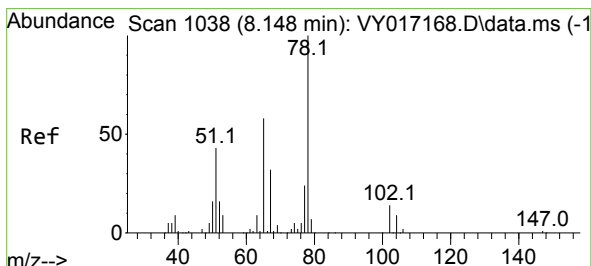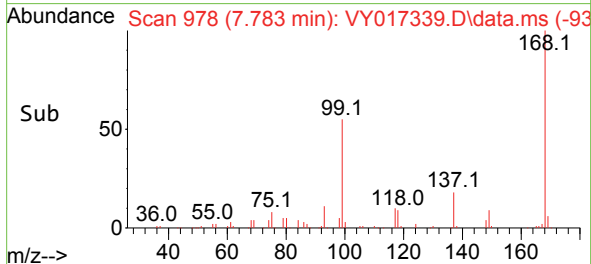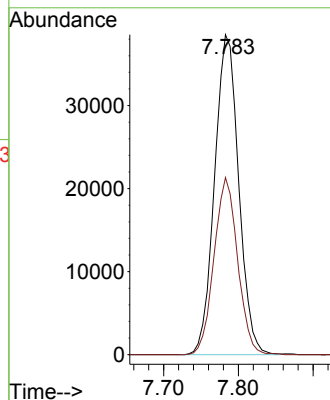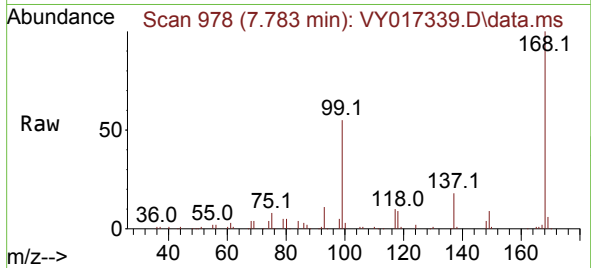

#33
1,2-Dichloroethane-d4
Concen: 55.712 ug/l
RT: 8.136 min Scan# 1036
Delta R.T. -0.012 min
Lab File: VY017339.D
Acq: 09 Feb 2024 15:08

Tgt Ion: 65 Resp: 43033
Ion Ratio Lower Upper
65 100
67 53.2 0.0 109.0

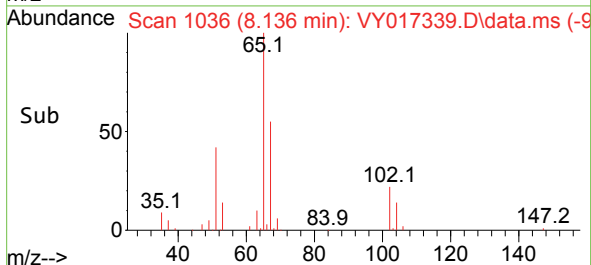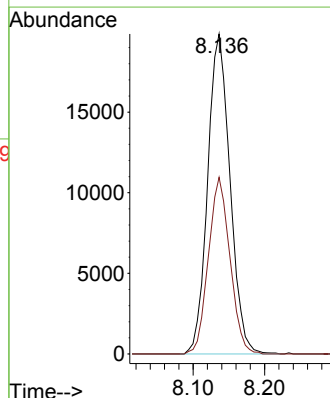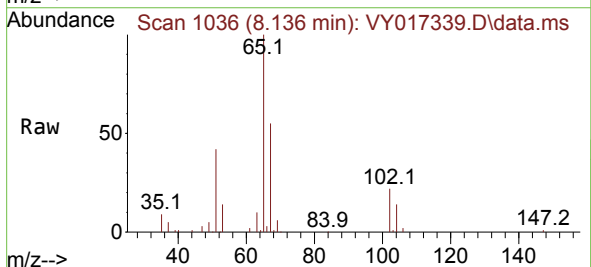

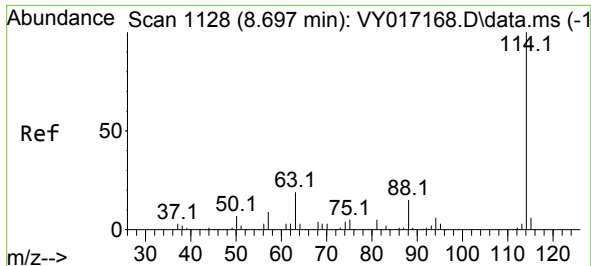

#34

1,4-Difluorobenzene

Concen: 50.000 ug/l

RT: 8.685 min Scan# 1126

Delta R.T. -0.012 min

Lab File: VY017339.D

Acq: 09 Feb 2024 15:08

Instrument :

MSVOA_Y

ClientSampleId :

SB-7(12-13)





Tgt Ion:114 Resp: 165857

Ion Ratio Lower Upper

114 100

63 19.6 0.0 37.4

88 14.3 0.0 29.0

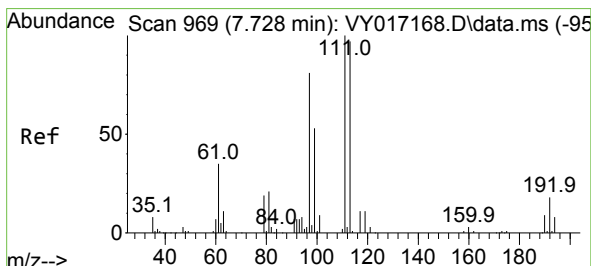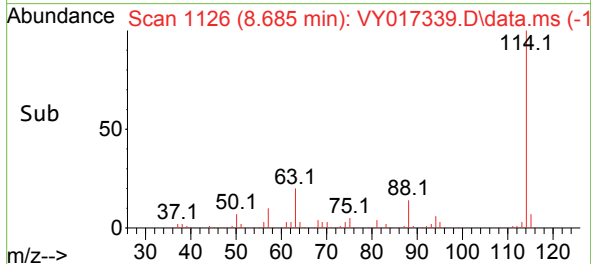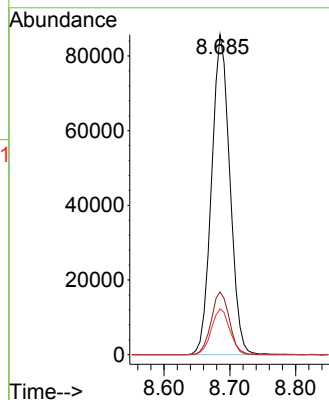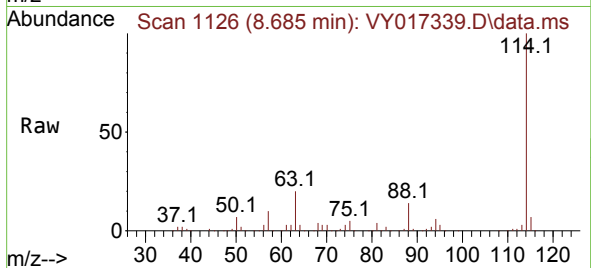

#35

Dibromofluoromethane

Concen: 47.949 ug/l

RT: 7.710 min Scan# 966

Delta R.T. -0.018 min

Lab File: VY017339.D

Acq: 09 Feb 2024 15:08




Tgt Ion:113 Resp: 42939


Ion Ratio Lower Upper

113 100

111 100.4 83.8 125.6

192 18.2 14.5 21.7

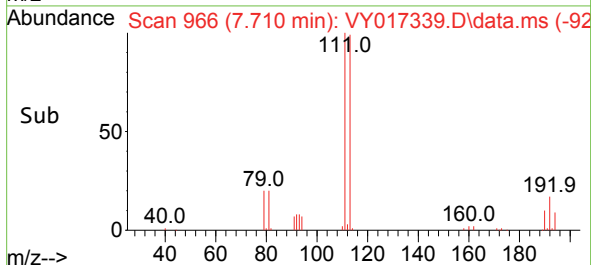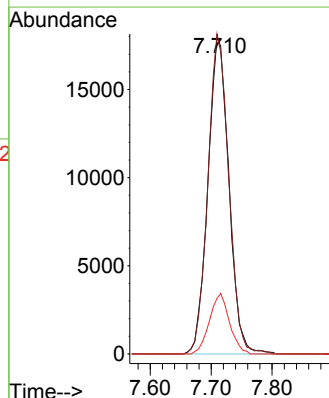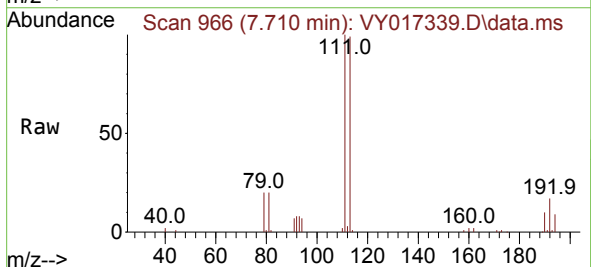

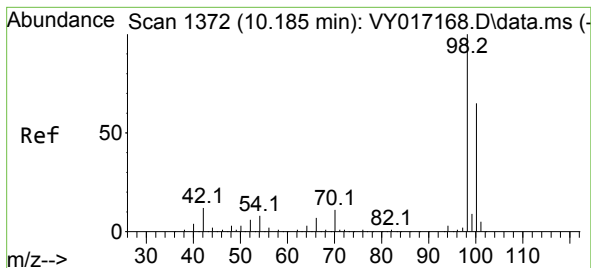

#50

Toluene-d8

Concen: 46.228 ug/l

RT: 10.179 min Scan# 11

Delta R.T. -0.006 min

Lab File: VY017339.D

Acq: 09 Feb 2024 15:08

Instrument :

MSVOA_Y

ClientSampleId :





SB-7(12-13)

Tgt Ion: 98 Resp: 150729

Ion Ratio Lower Upper

98 100

100 64.9 52.3 78.5

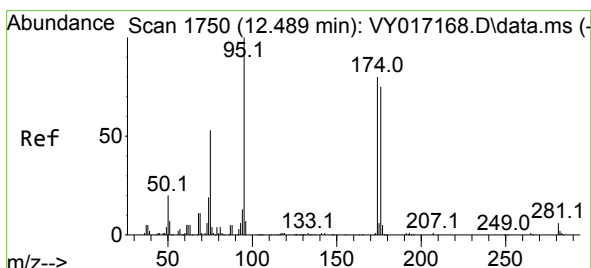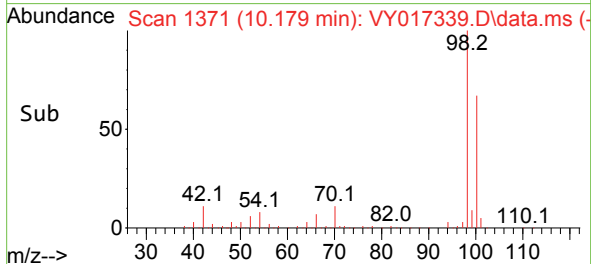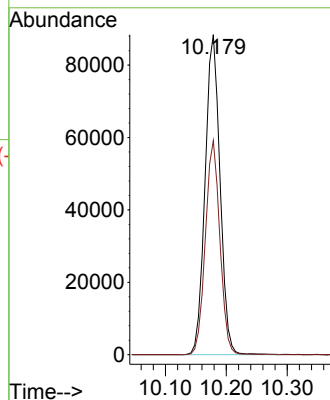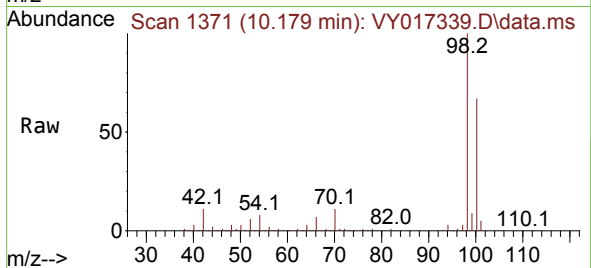

#62

4-Bromofluorobenzene

Concen: 40.720 ug/l

RT: 12.483 min Scan# 1749

Delta R.T. -0.006 min

Lab File: VY017339.D

Acq: 09 Feb 2024 15:08




Tgt Ion: 95 Resp: 43493


Ion Ratio Lower Upper

95 100

174 79.9 0.0 160.0

176 77.3 0.0 151.8

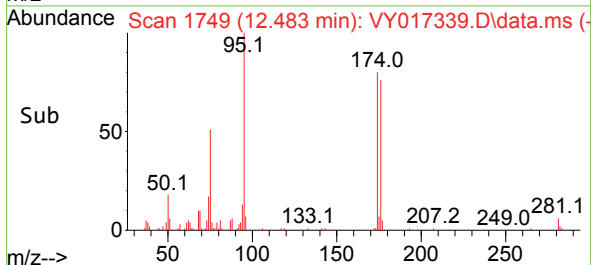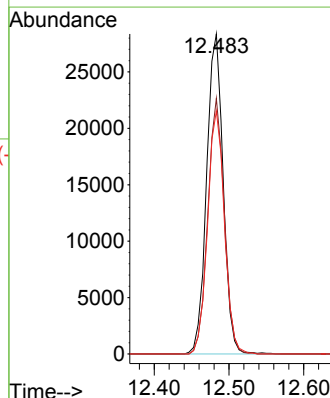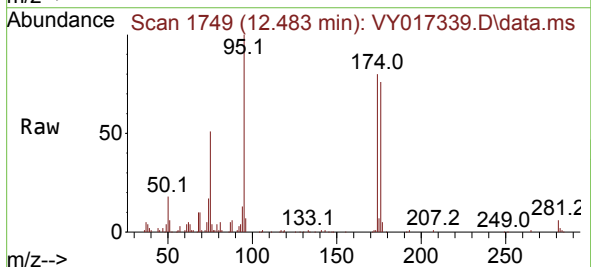

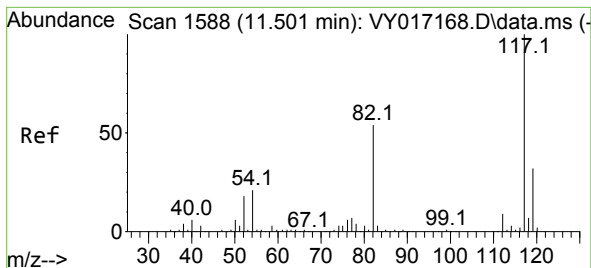

#63

Chlorobenzene-d5

Concen: 50.000 ug/l

RT: 11.489 min Scan# 11

Delta R.T. -0.012 min

Lab File: VY017339.D

Acq: 09 Feb 2024 15:08

Instrument :

MSVOA_Y

ClientSampleId :

SB-7(12-13)





Tgt Ion:117 Resp: 151993

Ion Ratio Lower Upper

117 100

82 53.2 43.8 65.8

119 31.8 26.5 39.7

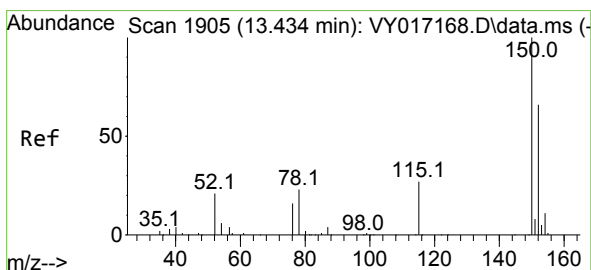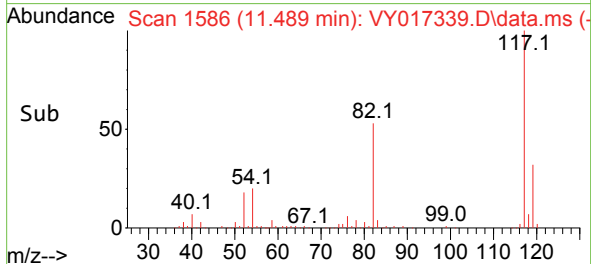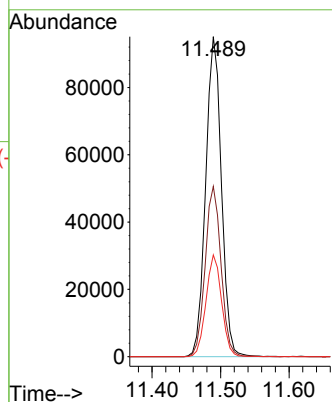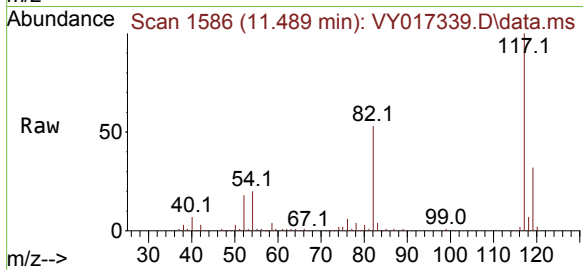

#72

1,4-Dichlorobenzene-d4

Concen: 50.000 ug/l

RT: 13.428 min Scan# 1904

Delta R.T. -0.006 min

Lab File: VY017339.D

Acq: 09 Feb 2024 15:08

Tgt Ion:152 Resp: 59631

Ion Ratio Lower Upper

152 100

115 57.5 30.0 90.0

150 157.5 0.0 344.6

