
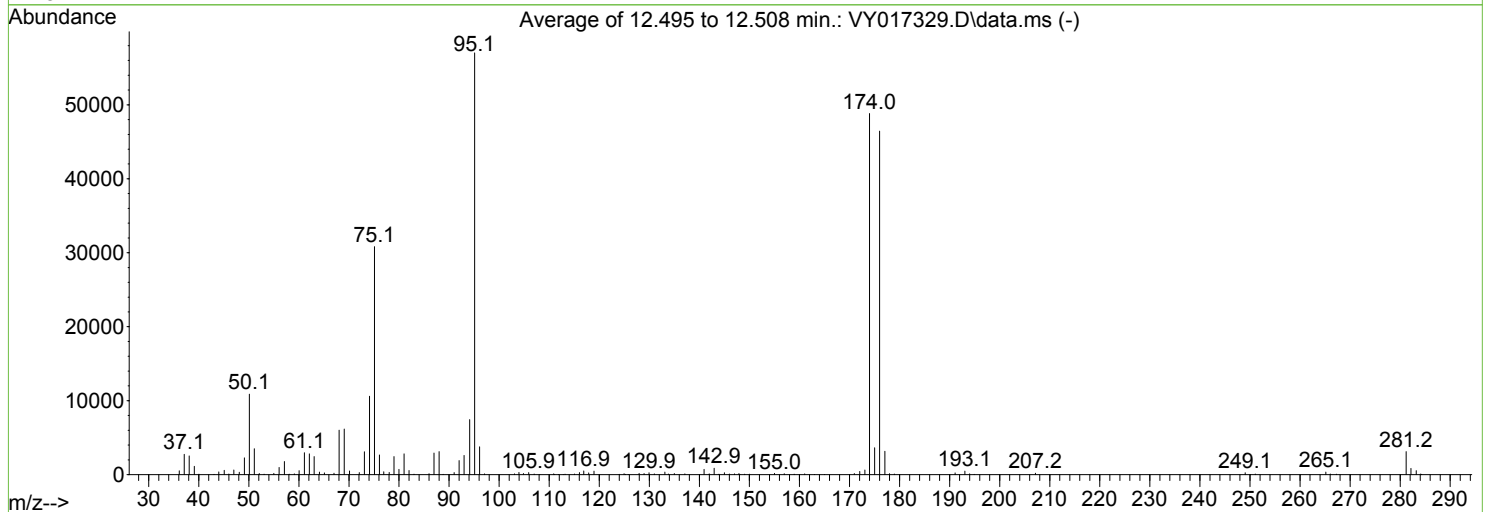


Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY020924\
Data File : VY017329.D
Acq On : 09 Feb 2024 08:19
Operator : SY/MD
Sample : BFB
Misc : 5.00g/5.0mL/MSVOA_Y/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_Y
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y020124S.M
Title : SW846 8260
Last Update : Fri Feb 02 00:56:04 2024

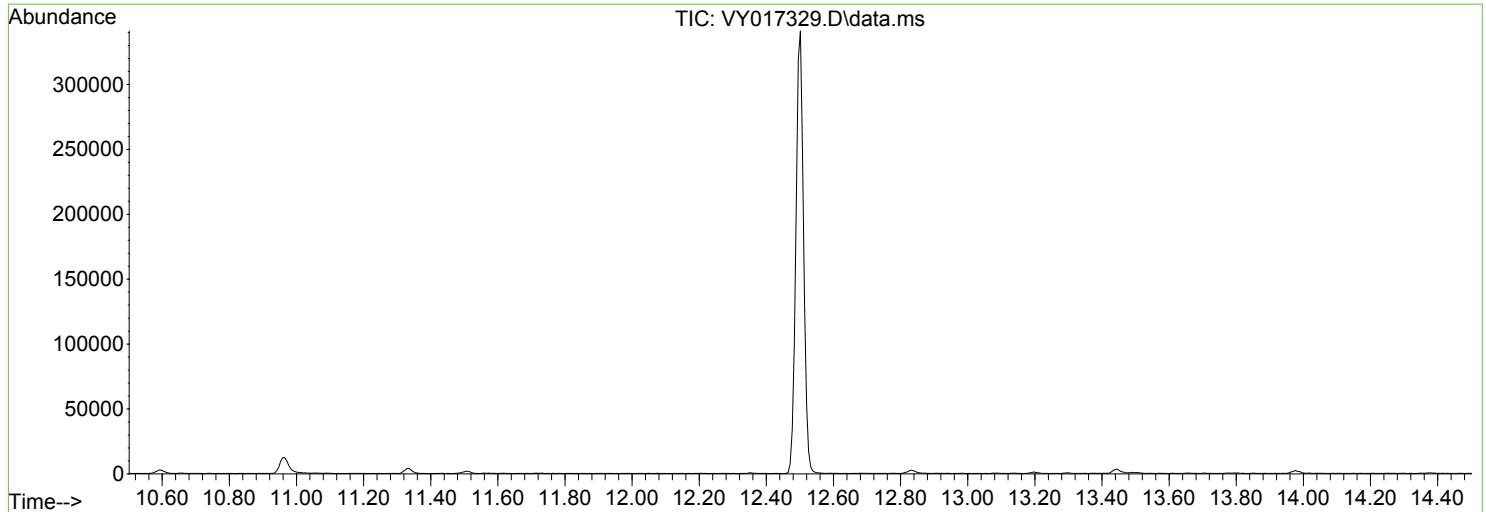

AutoFind: Scans 1751, 1752, 1753; Background Corrected with Scan 1743

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	19.1	10879	PASS
75	95	30	60	54.1	30824	PASS
95	95	100	100	100.0	57027	PASS
96	95	5	9	6.6	3754	PASS
173	174	0.00	2	1.3	638	PASS
174	95	50	100	85.6	48824	PASS
175	174	5	9	7.4	3626	PASS
176	174	95	101	95.1	46443	PASS
177	176	5	9	6.8	3161	PASS