
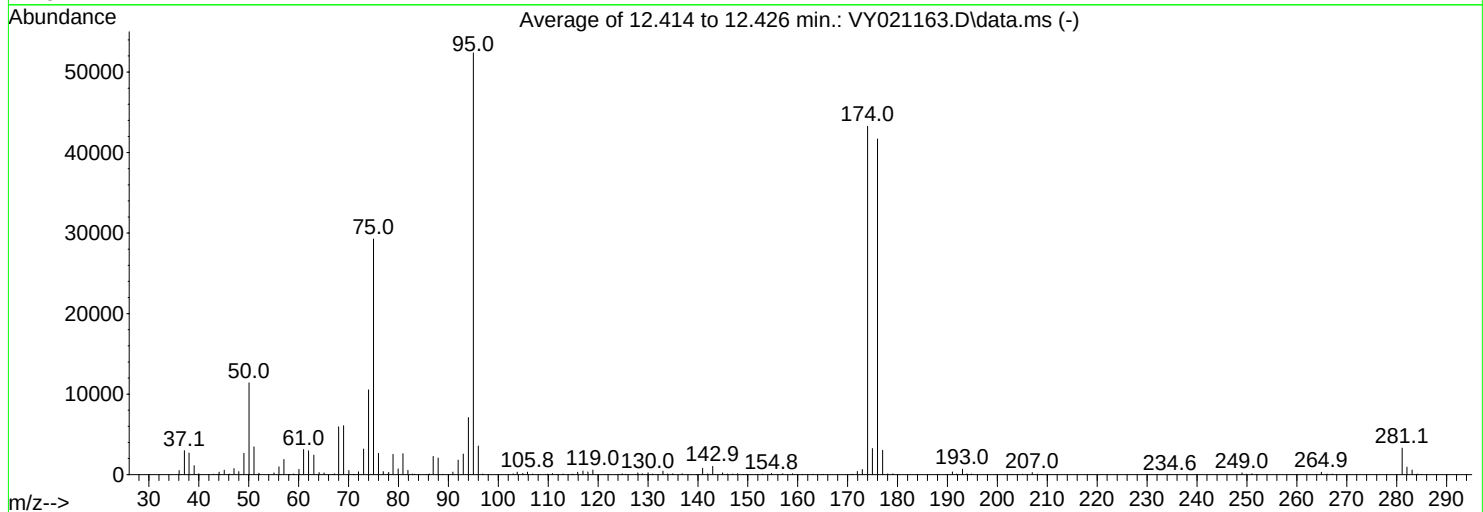


Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY021125\
Data File : VY021163.D
Acq On : 11 Feb 2025 09:08
Operator : SY/MD
Sample : BFB
Misc : 5.00g/5.0mL/MSVOA_Y/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_Y
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y020325S.M
Title : SW846 8260
Last Update : Mon Feb 03 13:08:38 2025

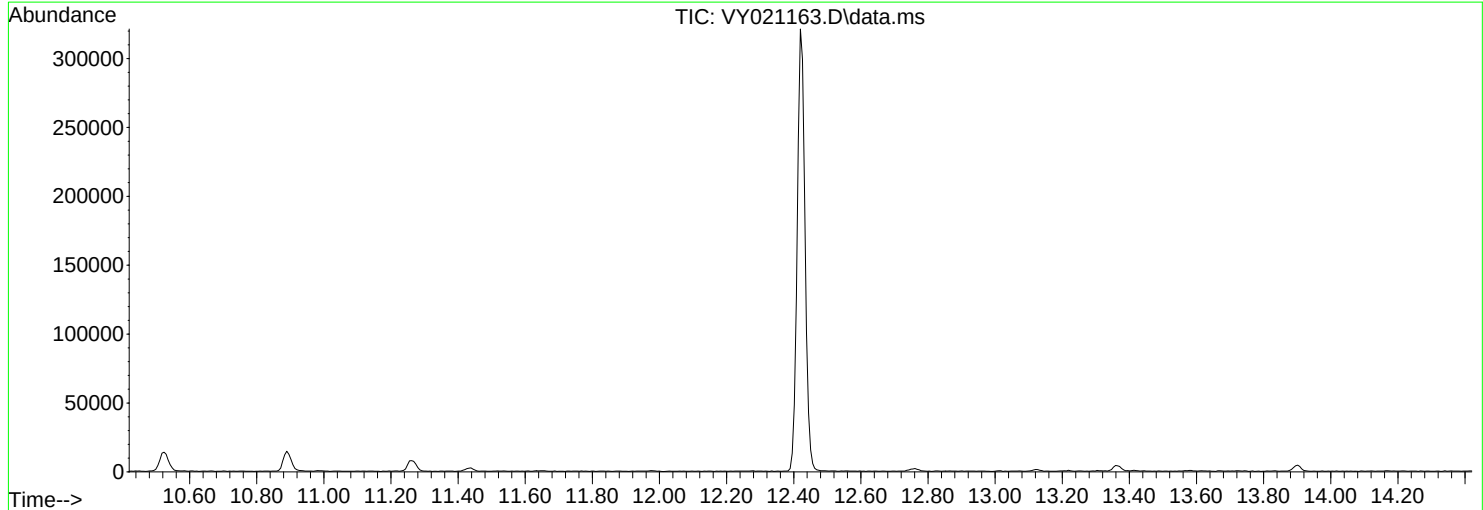

AutoFind: Scans 1754, 1755, 1756; Background Corrected with Scan 1746

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	21.8	11400	PASS
75	95	30	60	55.9	29264	PASS
95	95	100	100	100.0	52389	PASS
96	95	5	9	6.8	3553	PASS
173	174	0.00	2	1.5	637	PASS
174	95	50	100	82.6	43264	PASS
175	174	5	9	7.5	3240	PASS
176	174	95	101	96.4	41693	PASS
177	176	5	9	7.3	3027	PASS