
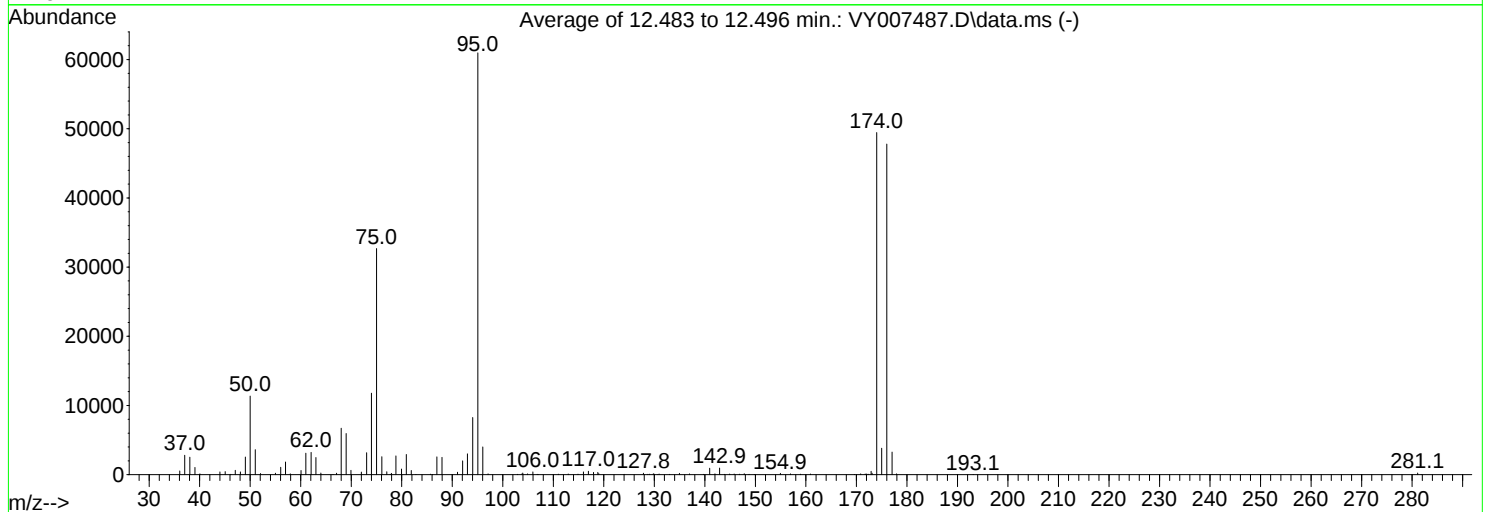


Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY021422\
 Data File : VY007487.D
 Acq On : 14 Feb 2022 08:53
 Operator : SY/MD
 Sample : BFB
 Misc : 5.00g/5.0mL/MSVOA_Y/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_Y
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y021422S.M
 Title : SW846 8260
 Last Update : Tue Feb 15 09:34:50 2022

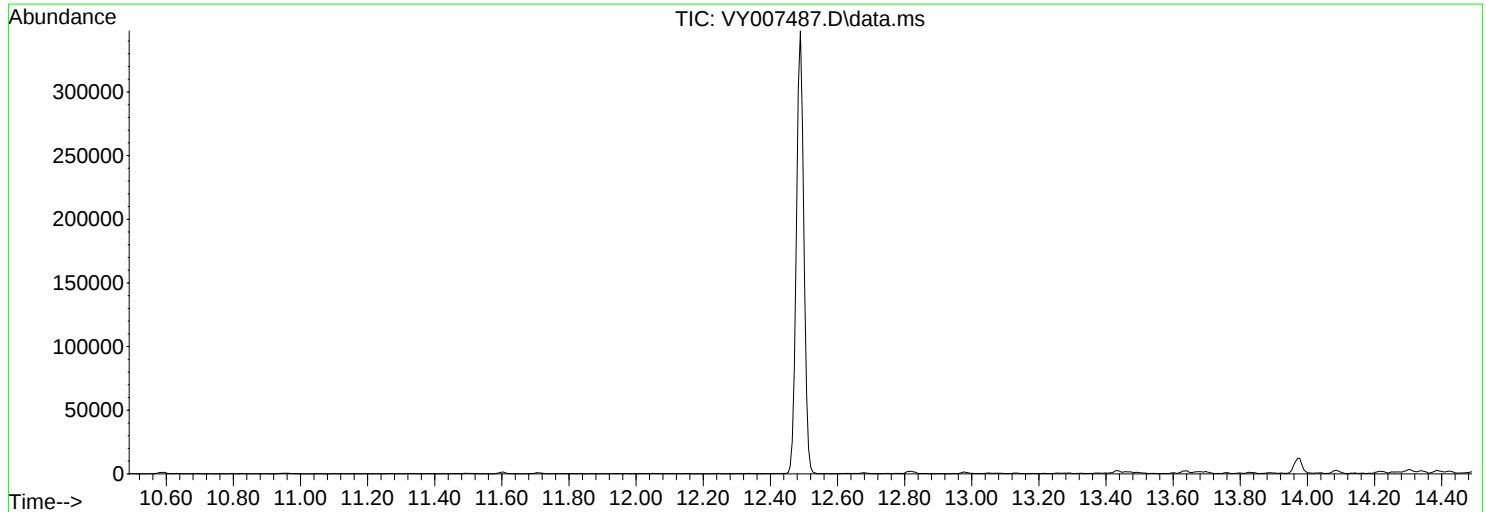

AutoFind: Scans 1749, 1750, 1751; Background Corrected with Scan 1741

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	18.6	11367	PASS
75	95	30	60	53.6	32677	PASS
95	95	100	100	100.0	60973	PASS
96	95	5	9	6.6	3999	PASS
173	174	0.00	2	1.0	499	PASS
174	95	50	100	81.1	49440	PASS
175	174	5	9	7.7	3811	PASS
176	174	95	101	96.6	47781	PASS
177	176	5	9	6.8	3261	PASS