


Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY021622\
Data File : VY007506.D
Acq On : 16 Feb 2022 10:47
Operator : SY/MD
Sample : BFB
Misc : 5.00g/5.0mL/MSVOA_Y/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_Y
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y021422S.M
Title : SW846 8260
Last Update : Tue Feb 15 09:34:50 2022

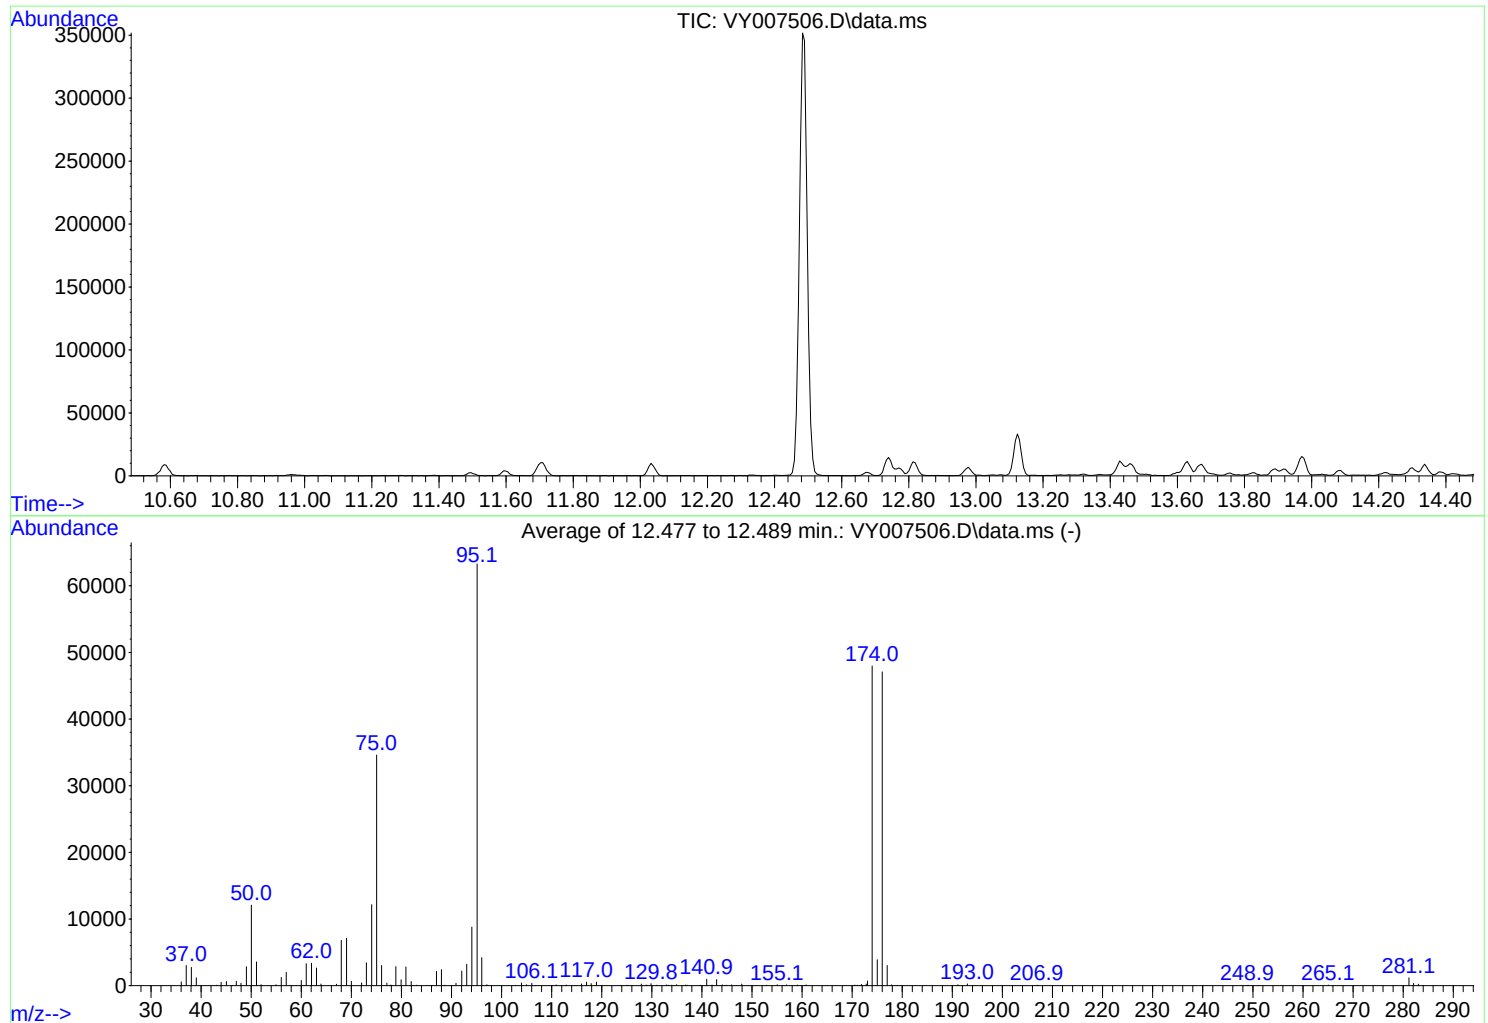

AutoFind: Scans 1748, 1749, 1750; Background Corrected with Scan 1740

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	19.1	12080	PASS
75	95	30	60	54.7	34608	PASS
95	95	100	100	100.0	63299	PASS
96	95	5	9	6.6	4195	PASS
173	174	0.00	2	1.4	690	PASS
174	95	50	100	75.8	47984	PASS
175	174	5	9	8.1	3891	PASS
176	174	95	101	98.1	47093	PASS
177	176	5	9	6.5	3039	PASS