
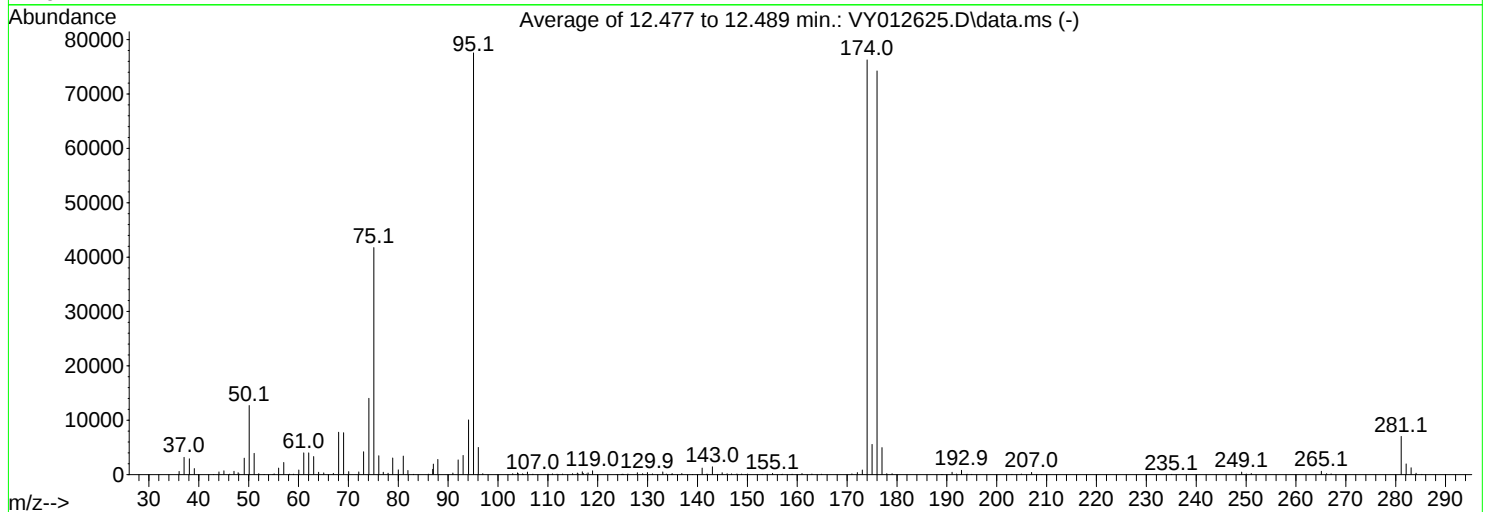


Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY021623\
Data File : VY012625.D
Acq On : 16 Feb 2023 09:04
Operator : KP/MD
Sample : BFB
Misc : 5.00g/5.0mL/MSVOA_Y/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_Y
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y020723S.M
Title : SW846 8260
Last Update : Fri Feb 17 18:08:19 2023

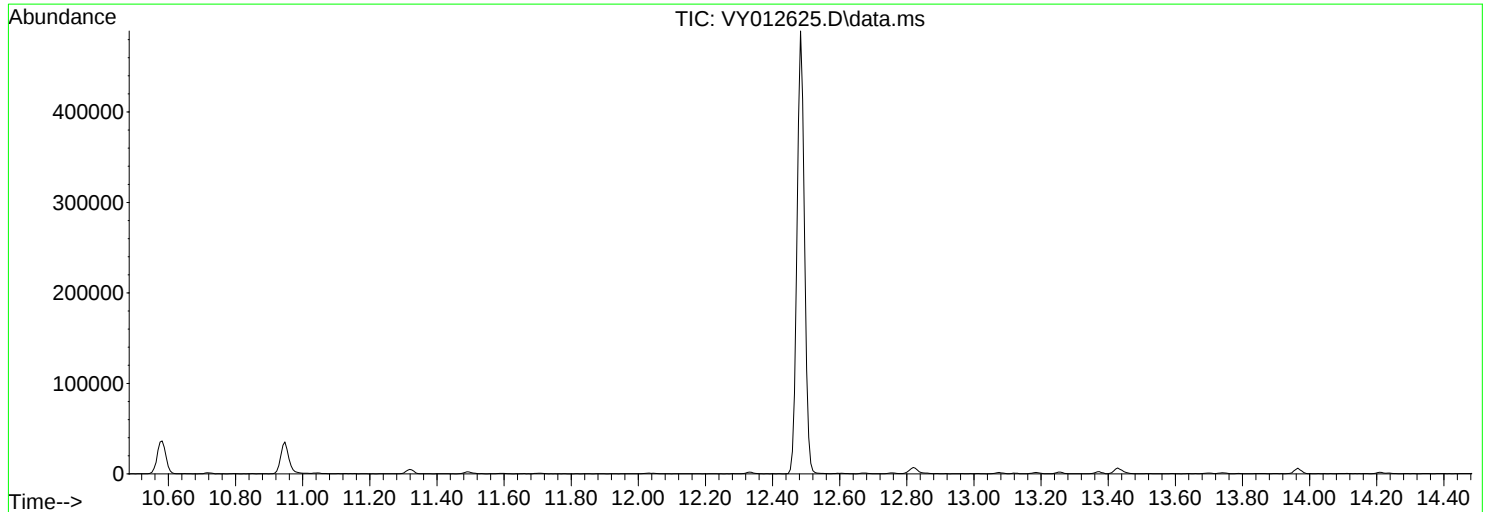

AutoFind: Scans 1748, 1749, 1750; Background Corrected with Scan 1740

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	16.4	12726	PASS
75	95	30	60	53.8	41736	PASS
95	95	100	100	100.0	77563	PASS
96	95	5	9	6.4	4999	PASS
173	174	0.00	2	1.1	854	PASS
174	95	50	100	98.3	76264	PASS
175	174	5	9	7.3	5551	PASS
176	174	95	101	97.3	74229	PASS
177	176	5	9	6.7	4973	PASS