

Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY021722\
 Data File : VY007524.D
 Acq On : 17 Feb 2022 15:51
 Operator : SY/MD
 Sample : N1561-04
 Misc : 3.89g/5.0mL/MSVOA_Y/SOIL
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_Y
 ClientSampleId :
 TP-2-1-2

Quant Time: Feb 18 07:40:28 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y021422S.M
 Quant Title : SW846 8260
 QLast Update : Tue Feb 15 09:34:50 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) Pentafluorobenzene	7.789	168	81254	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	8.691	114	144352	50.000	ug/l	0.00
63) Chlorobenzene-d5	11.489	117	130184	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.422	152	44659	50.000	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.136	65	48925	54.538	ug/l	0.00
Spiked Amount	50.000	Range	50 - 163	Recovery	= 109.080%	
35) Dibromofluoromethane	7.715	113	48468	53.242	ug/l	0.00
Spiked Amount	50.000	Range	54 - 147	Recovery	= 106.480%	
50) Toluene-d8	10.178	98	169728	49.090	ug/l	0.00
Spiked Amount	50.000	Range	49 - 140	Recovery	= 98.180%	
62) 4-Bromofluorobenzene	12.477	95	52269	44.584	ug/l	0.00
Spiked Amount	50.000	Range	25 - 144	Recovery	= 89.160%	
Target Compounds						
68) m/p-Xylenes	11.690	106	5708	2.826	ug/l	98
69) o-Xylene	12.032	106	2088	1.093	ug/l	94


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY021722\
Data File : VY007524.D
Acq On : 17 Feb 2022 15:51
Operator : SY/MD
Sample : N1561-04
Misc : 3.89g/5.0mL/MSVOA_Y/SOIL
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_Y
ClientSampleId :
TP-2-1-2

Quant Time: Feb 18 07:40:28 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y021422S.M
Quant Title : SW846 8260
QLast Update : Tue Feb 15 09:34:50 2022
Response via : Initial Calibration




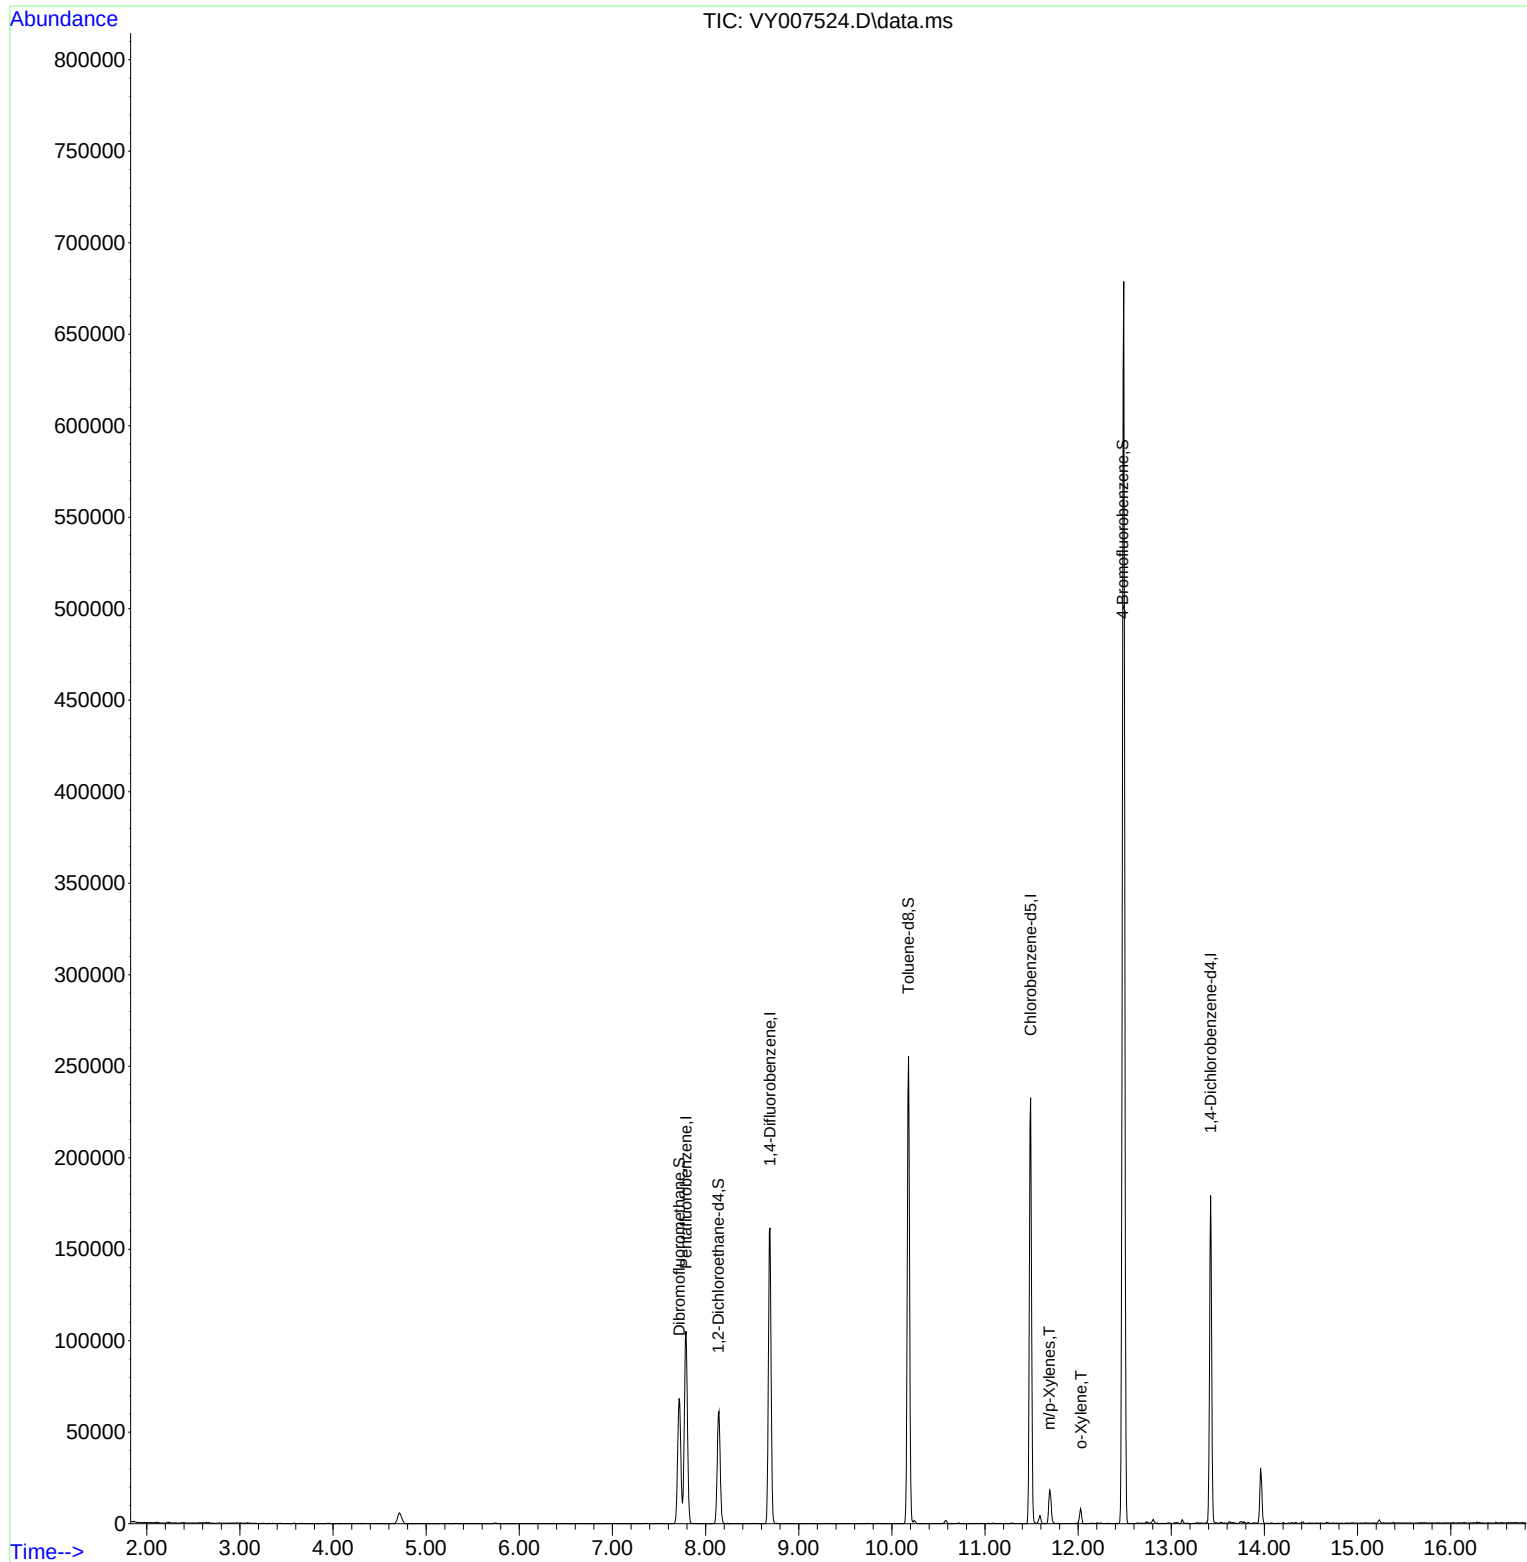


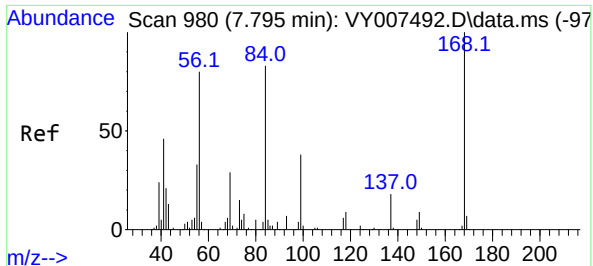

#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 7.789 min Scan# 91
Delta R.T. -0.006 min
Lab File: VY007524.D
Acq: 17 Feb 2022 15:51




Instrument :
MSVOA_Y
ClientSampleId :
TP-2-1-2


Tgt Ion:168 Resp: 81254
Ion Ratio Lower Upper
168 100
99 57.5 46.9 70.3

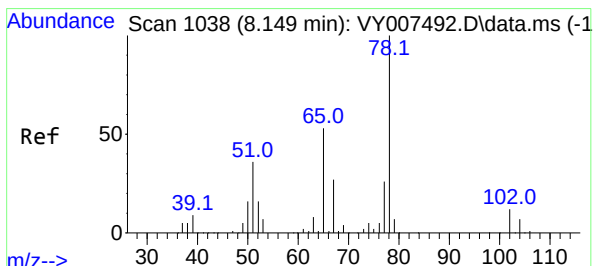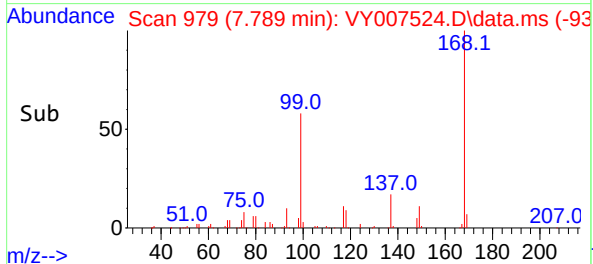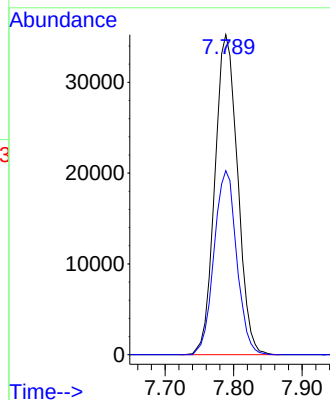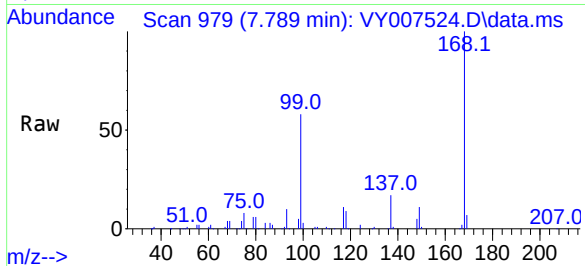

#33
1,2-Dichloroethane-d4
Concen: 54.538 ug/l
RT: 8.136 min Scan# 1036
Delta R.T. -0.007 min
Lab File: VY007524.D
Acq: 17 Feb 2022 15:51

Tgt Ion: 65 Resp: 48925
Ion Ratio Lower Upper
65 100
67 50.3 0.0 99.4

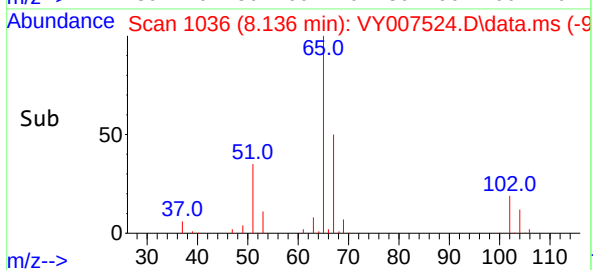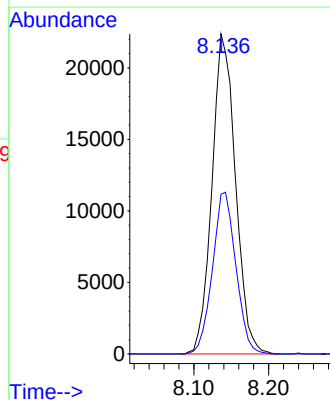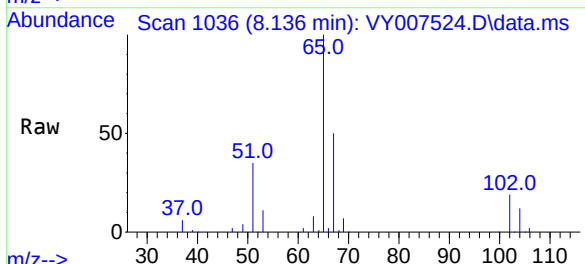

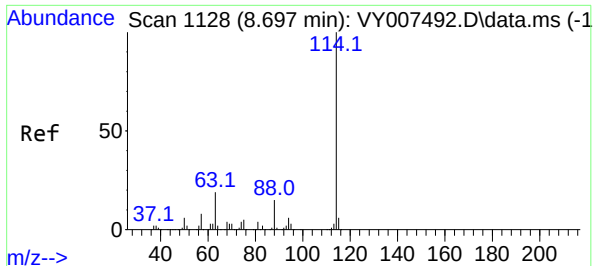

#34

1,4-Difluorobenzene

Concen: 50.000 ug/l

RT: 8.691 min Scan# 1128

Delta R.T. -0.000 min

Lab File: VY007524.D

Acq: 17 Feb 2022 15:51

Instrument :

MSVOA_Y

ClientSampleId :

TP-2-1-2





Tgt Ion:114 Resp: 144352

Ion Ratio Lower Upper

114 100

63 18.2 0.0 43.2

88 13.9 0.0 31.8

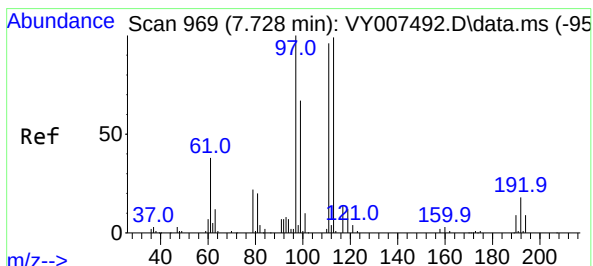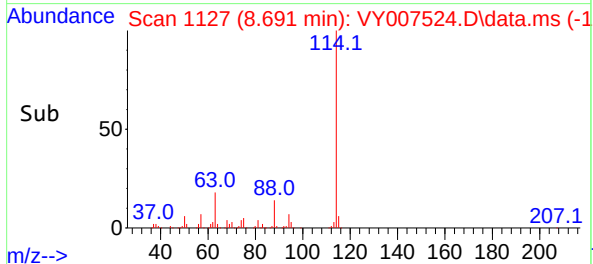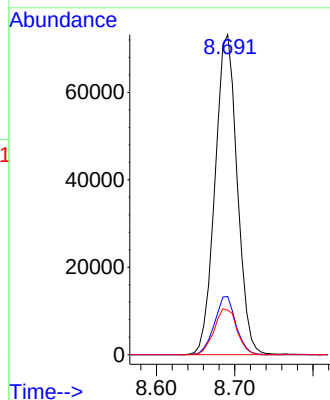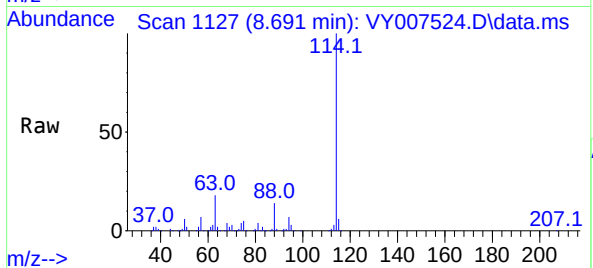

#35

Dibromofluoromethane

Concen: 53.242 ug/l

RT: 7.715 min Scan# 967

Delta R.T. -0.007 min

Lab File: VY007524.D

Acq: 17 Feb 2022 15:51




Tgt Ion:113 Resp: 48468


Ion Ratio Lower Upper

113 100

111 101.4 82.6 124.0

192 18.7 17.6 26.4


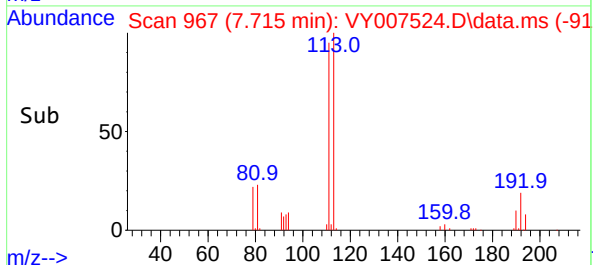
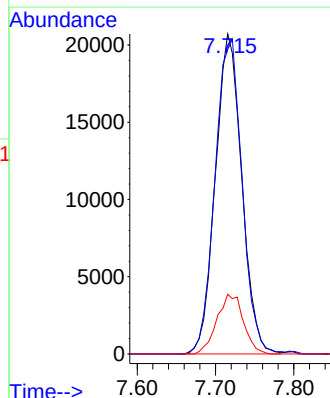
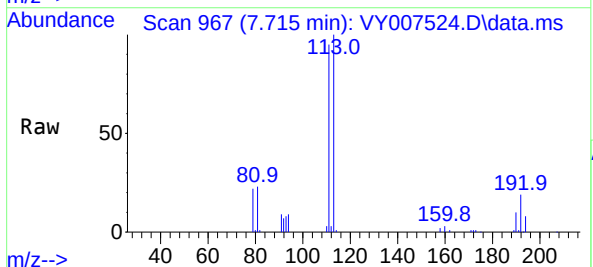


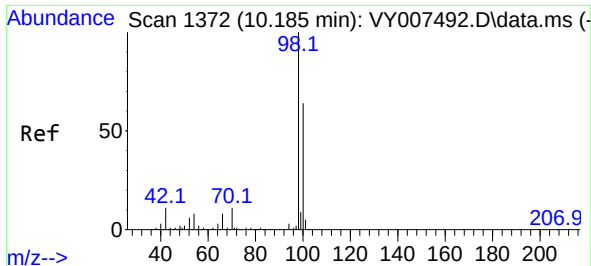

#50
Toluene-d8
Concen: 49.090 ug/l
RT: 10.178 min Scan# 11
Delta R.T. -0.007 min
Lab File: VY007524.D
Acq: 17 Feb 2022 15:51




Instrument :
MSVOA_Y
ClientSampleId :
TP-2-1-2


Tgt Ion: 98 Resp: 169728
Ion Ratio Lower Upper
98 100
100 65.0 50.2 75.2

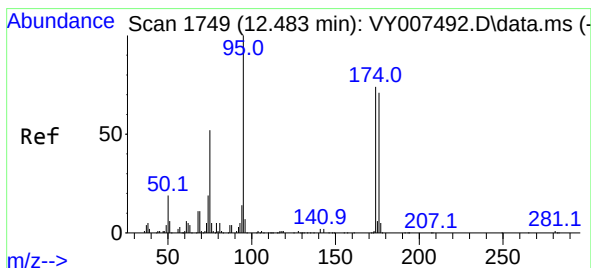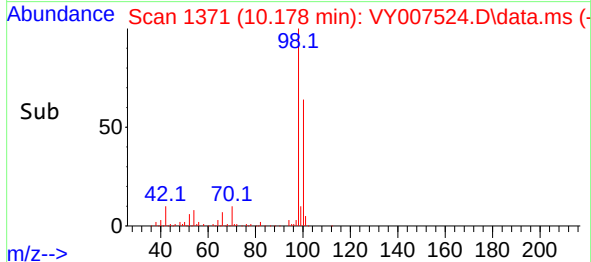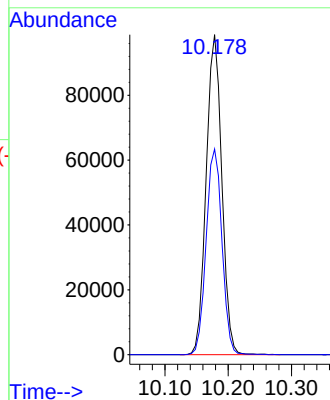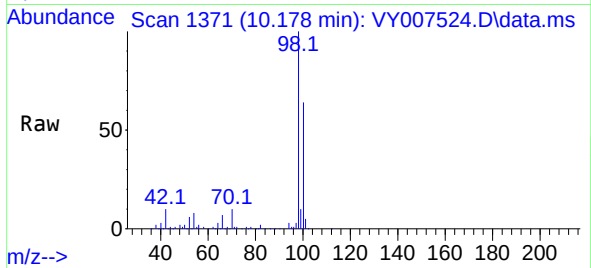

#62
4-Bromofluorobenzene
Concen: 44.584 ug/l
RT: 12.477 min Scan# 1748
Delta R.T. -0.006 min
Lab File: VY007524.D
Acq: 17 Feb 2022 15:51

Tgt Ion: 95 Resp: 52269
Ion Ratio Lower Upper
95 100
174 85.3 0.0 177.0
176 86.1 0.0 175.8


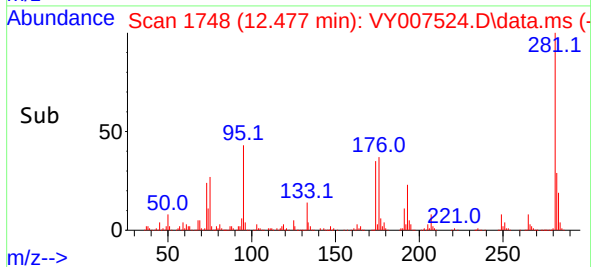
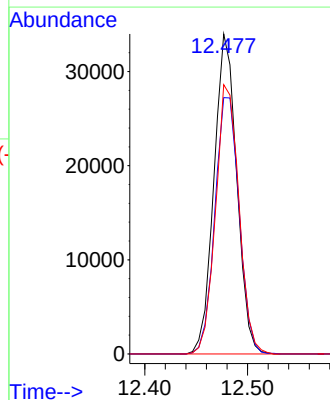
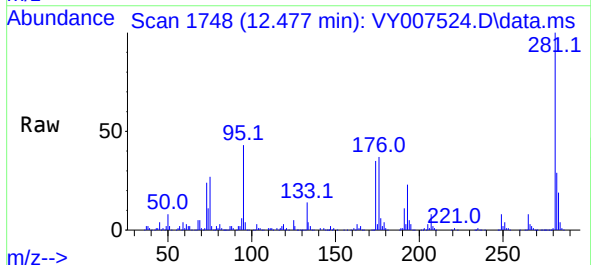


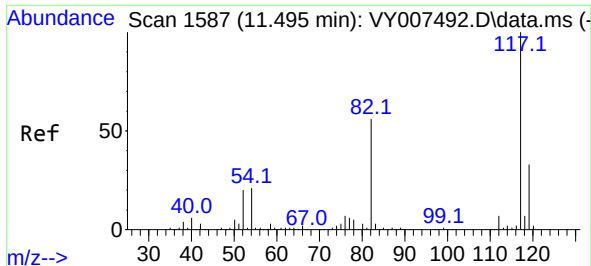

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 11.489 min Scan# 11
Delta R.T. -0.000 min
Lab File: VY007524.D
Acq: 17 Feb 2022 15:51




Instrument :
MSVOA_Y
ClientSampleId :
TP-2-1-2


Tgt Ion:117 Resp: 130184
Ion Ratio Lower Upper
117 100
82 53.5 43.0 64.4
119 32.7 25.4 38.0

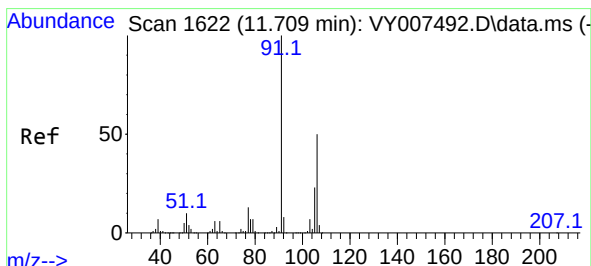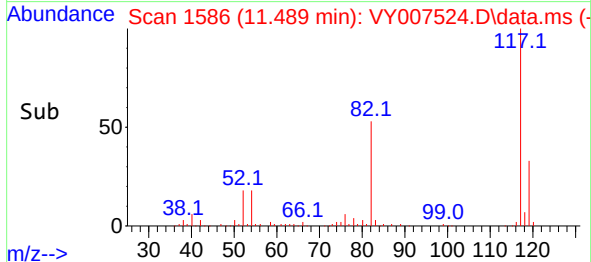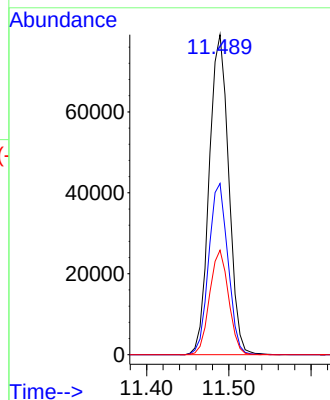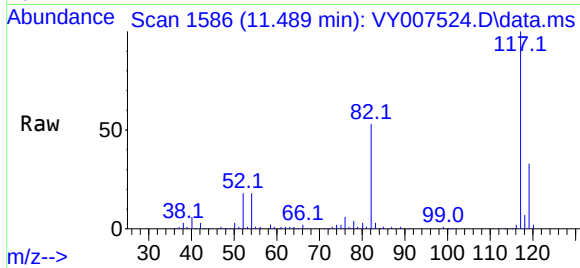

#68
m/p-Xylenes
Concen: 2.826 ug/l
RT: 11.690 min Scan# 1619
Delta R.T. -0.013 min
Lab File: VY007524.D
Acq: 17 Feb 2022 15:51

Tgt Ion:106 Resp: 5708
Ion Ratio Lower Upper
106 100
91 205.7 166.6 249.8


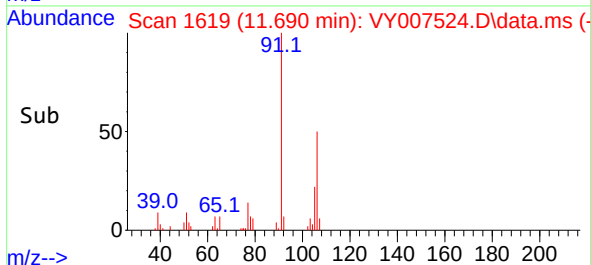
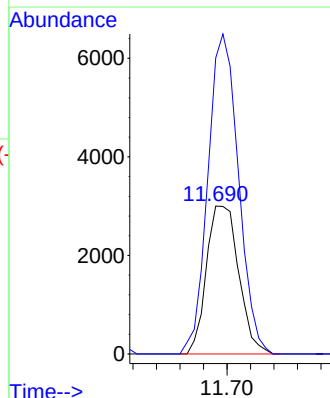
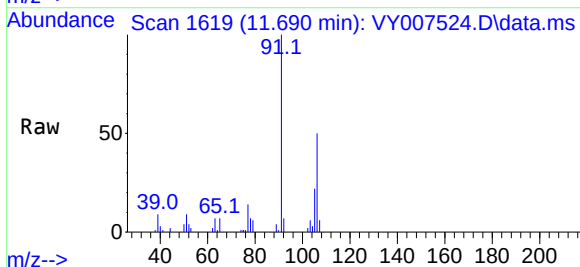


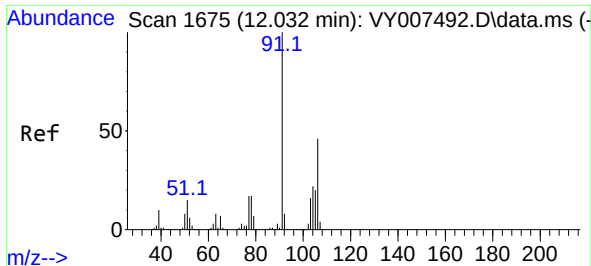

#69
o-Xylene
Concen: 1.093 ug/l
RT: 12.032 min Scan# 1
Delta R.T. -0.000 min
Lab File: VY007524.D
Acq: 17 Feb 2022 15:51

Instrument :
MSVOA_Y
ClientSampleId :
TP-2-1-2

Tgt Ion:106 Resp: 2088
Ion Ratio Lower Upper
106 100
91 211.8 110.3 331.0

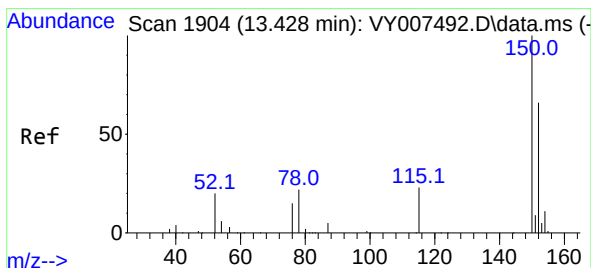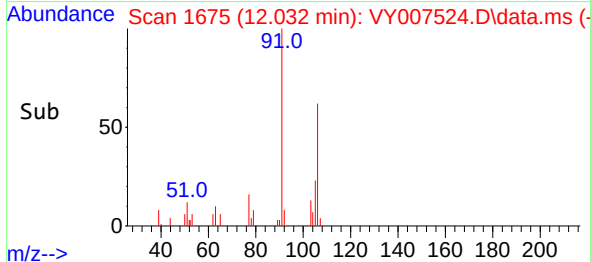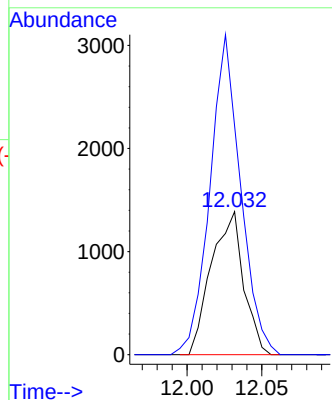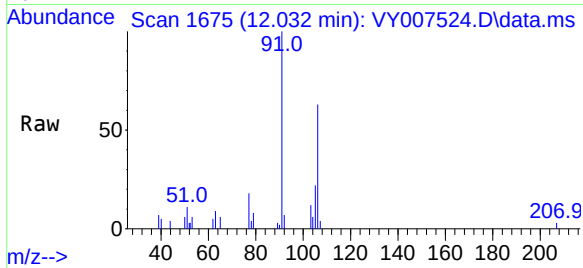

#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 13.422 min Scan# 1903
Delta R.T. -0.000 min
Lab File: VY007524.D
Acq: 17 Feb 2022 15:51

Tgt Ion:152 Resp: 44659
Ion Ratio Lower Upper
152 100
115 58.6 28.2 84.7
150 161.2 0.0 347.6

