
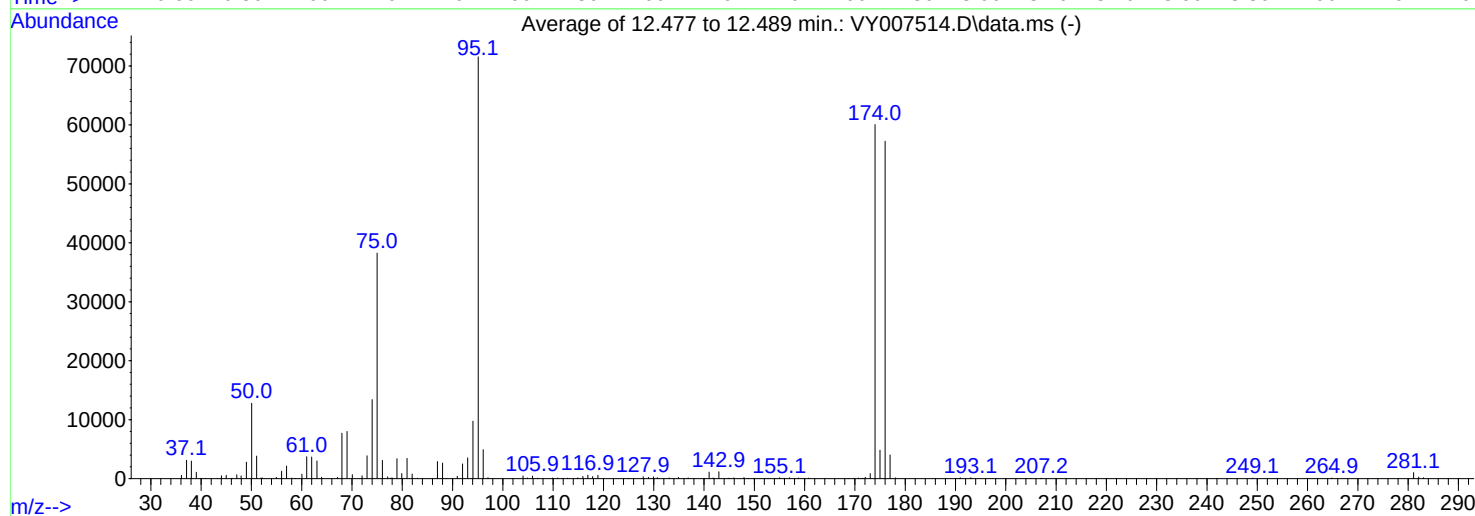


Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY021722\
 Data File : VY007514.D
 Acq On : 17 Feb 2022 10:41
 Operator : SY/MD
 Sample : BFB
 Misc : 5.00g/5.0mL/MSVOA_Y/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_Y
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y021422S.M
 Title : SW846 8260
 Last Update : Tue Feb 15 09:34:50 2022

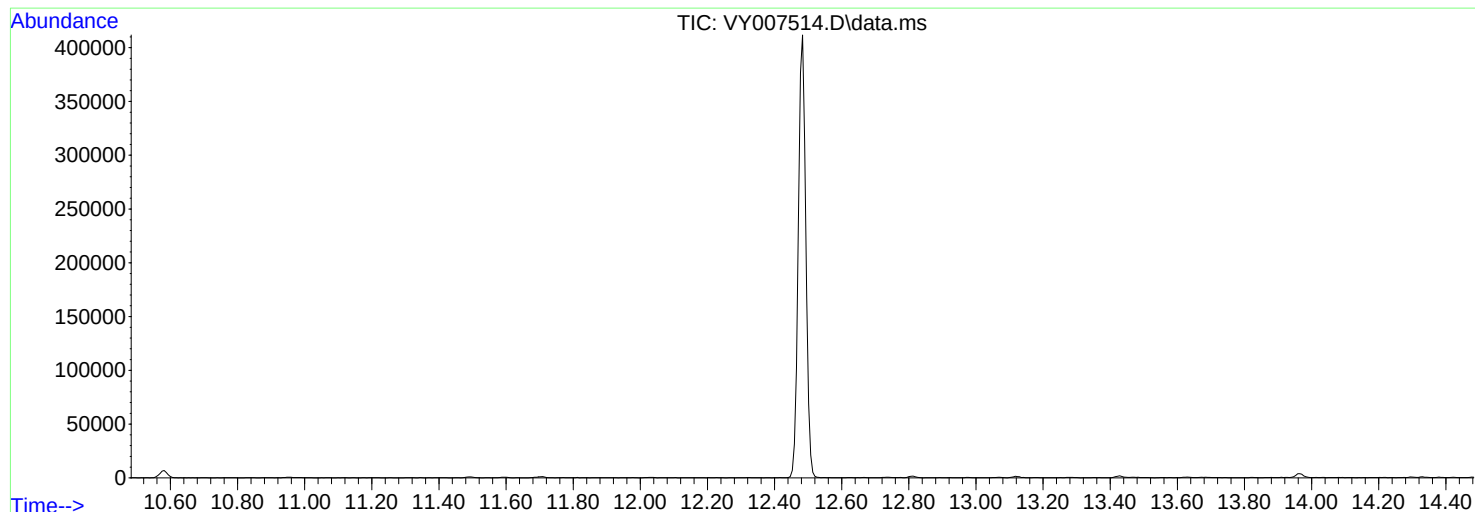

AutoFind: Scans 1748, 1749, 1750; Background Corrected with Scan 1740

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	17.9	12782	PASS
75	95	30	60	53.5	38275	PASS
95	95	100	100	100.0	71541	PASS
96	95	5	9	6.9	4921	PASS
173	174	0.00	2	1.5	880	PASS
174	95	50	100	84.0	60067	PASS
175	174	5	9	8.1	4838	PASS
176	174	95	101	95.3	57235	PASS
177	176	5	9	7.0	4017	PASS