

Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY021723\
 Data File : VY012640.D
 Acq On : 17 Feb 2023 11:01
 Operator : KP/MD
 Sample : VY0217SBL01
 Misc : 5.00g/5.0mL/MSVOA_Y/SOIL
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_Y
 ClientSampleId :
 VY0217SBL01

Quant Time: Feb 17 11:46:57 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y020723S.M
 Quant Title : SW846 8260
 QLast Update : Wed Feb 08 01:09:03 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Pentafluorobenzene	7.789	168	104755	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	8.685	114	160532	50.000	ug/l	0.00
63) Chlorobenzene-d5	11.489	117	147029	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.428	152	78703	50.000	ug/l	0.00

System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.136	65	81505	61.186	ug/l	0.00
Spiked Amount	50.000	Range	50 - 163	Recovery	=	122.380%
35) Dibromofluoromethane	7.715	113	67681	57.892	ug/l	0.00
Spiked Amount	50.000	Range	54 - 147	Recovery	=	115.780%
50) Toluene-d8	10.178	98	262894	54.026	ug/l	0.00
Spiked Amount	50.000	Range	49 - 140	Recovery	=	108.060%
62) 4-Bromofluorobenzene	12.477	95	86331	50.863	ug/l	0.00
Spiked Amount	50.000	Range	25 - 144	Recovery	=	101.720%


Target Compounds	Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY021723\
Data File : VY012640.D
Acq On : 17 Feb 2023 11:01
Operator : KP/MD
Sample : VY0217SBL01
Misc : 5.00g/5.0mL/MSVOA_Y/SOIL
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_Y
ClientSampleId :
VY0217SBL01

Quant Time: Feb 17 11:46:57 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y020723S.M
Quant Title : SW846 8260
QLast Update : Wed Feb 08 01:09:03 2023
Response via : Initial Calibration




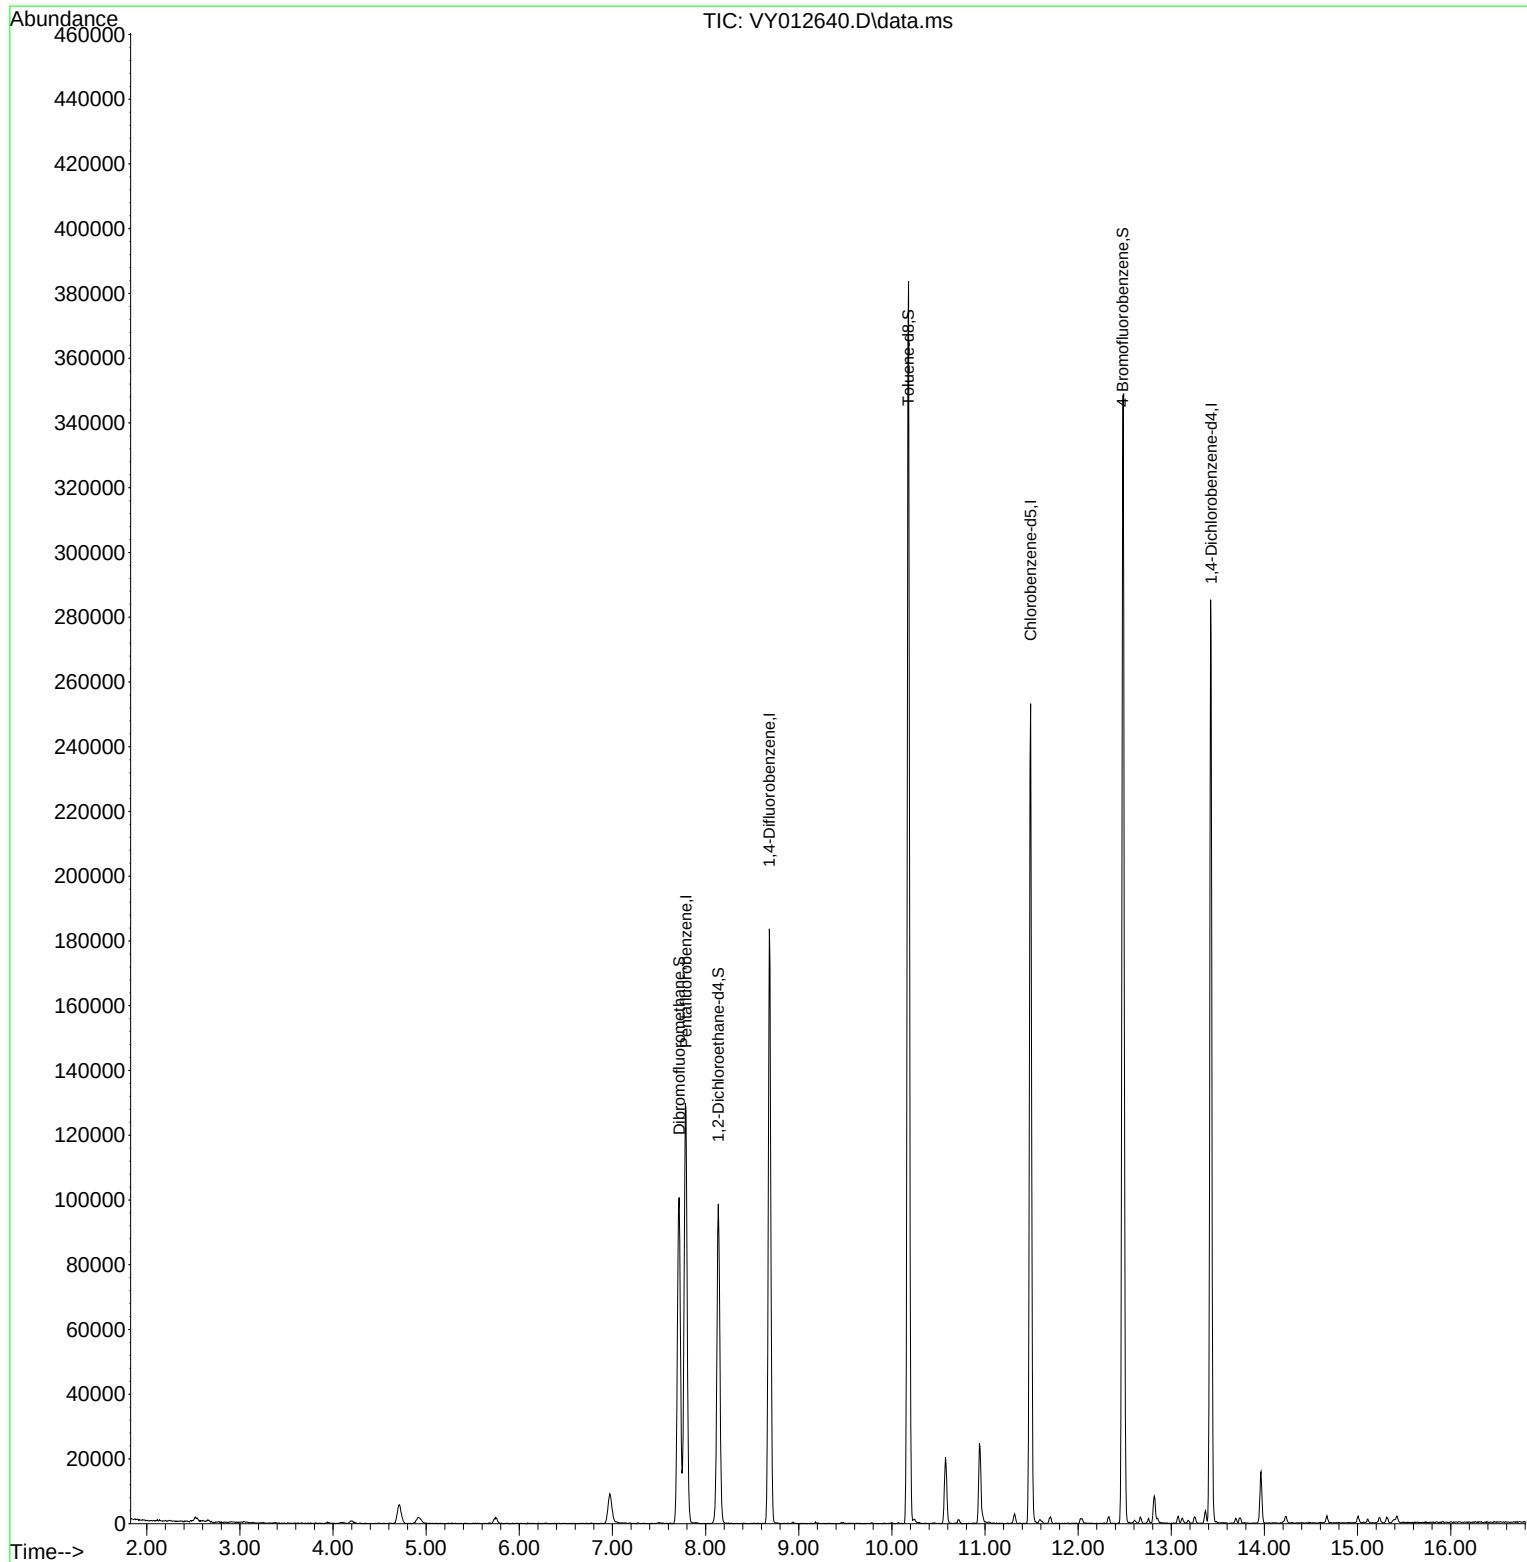


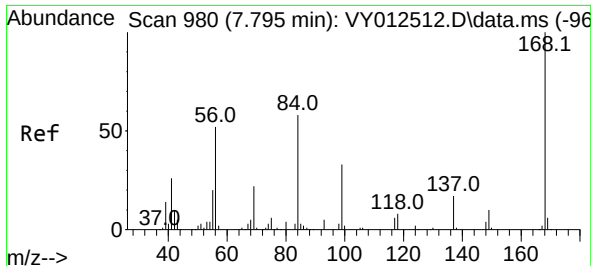

#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 7.789 min Scan# 91
Delta R.T. -0.006 min
Lab File: VY012640.D
Acq: 17 Feb 2023 11:01




Instrument :
MSVOA_Y
ClientSampleId :
VY0217SBL01


Tgt Ion:168 Resp: 104755
Ion Ratio Lower Upper
168 100
99 53.3 40.8 61.2

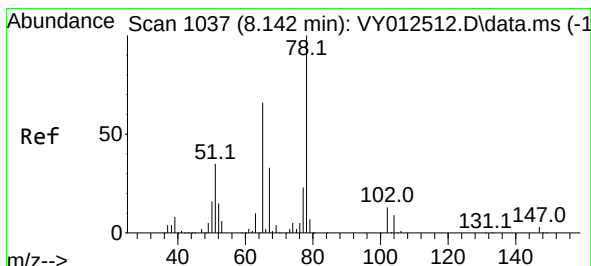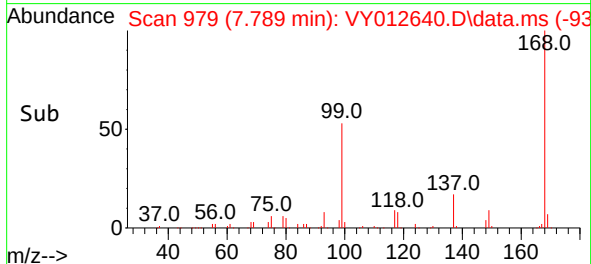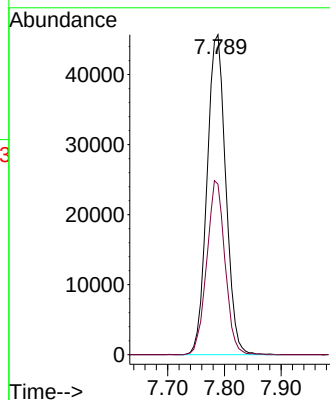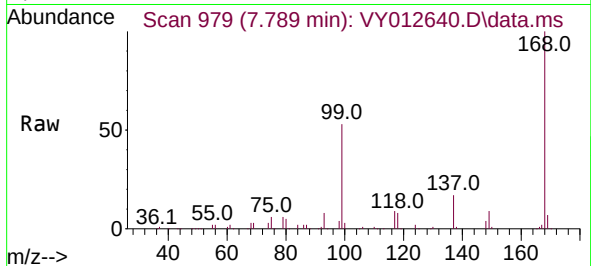

#33
1,2-Dichloroethane-d4
Concen: 61.186 ug/l
RT: 8.136 min Scan# 1036
Delta R.T. -0.006 min
Lab File: VY012640.D
Acq: 17 Feb 2023 11:01

Tgt Ion: 65 Resp: 81505
Ion Ratio Lower Upper
65 100
67 49.3 0.0 98.6

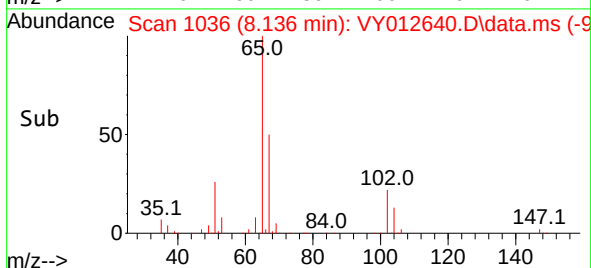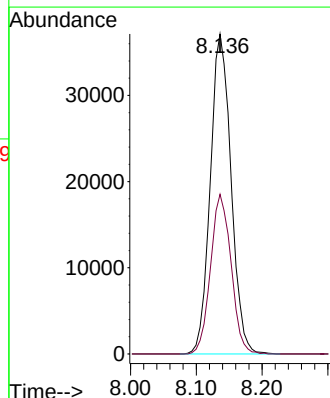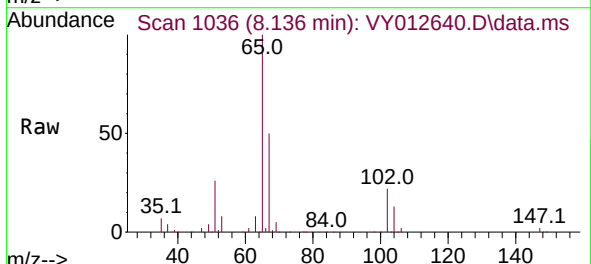

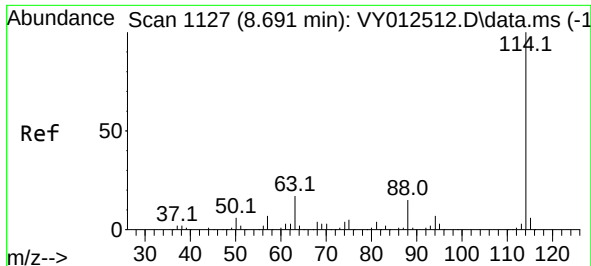

#34

1,4-Difluorobenzene

Concen: 50.000 ug/l

RT: 8.685 min Scan# 1126

Delta R.T. -0.006 min

Lab File: VY012640.D

Acq: 17 Feb 2023 11:01

Instrument :

MSVOA_Y

ClientSampleId :

VY0217SBL01





Tgt Ion:114 Resp: 160532

Ion Ratio Lower Upper

114 100

63 16.9 0.0 33.6

88 15.3 0.0 29.8

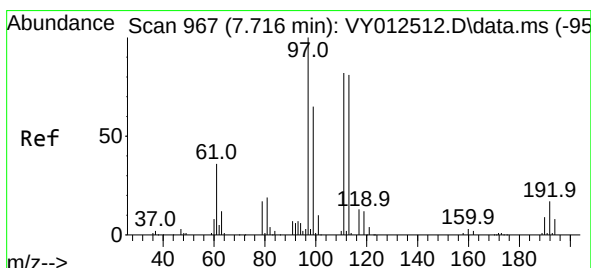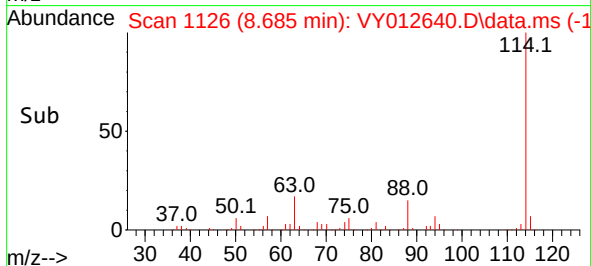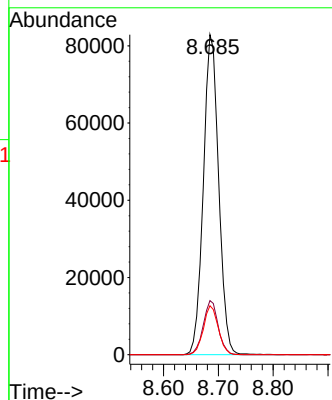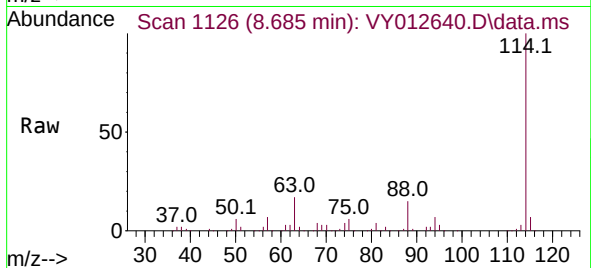

#35

Dibromofluoromethane

Concen: 57.892 ug/l

RT: 7.715 min Scan# 967

Delta R.T. -0.000 min

Lab File: VY012640.D

Acq: 17 Feb 2023 11:01




Tgt Ion:113 Resp: 67681


Ion Ratio Lower Upper

113 100

111 102.3 81.9 122.9

192 22.6 17.5 26.3


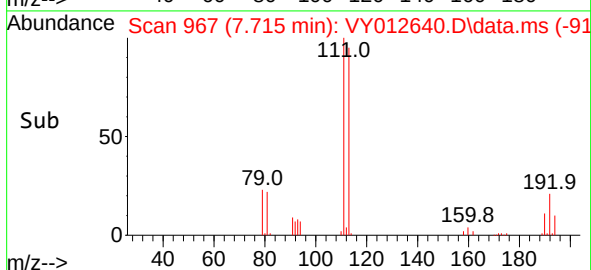
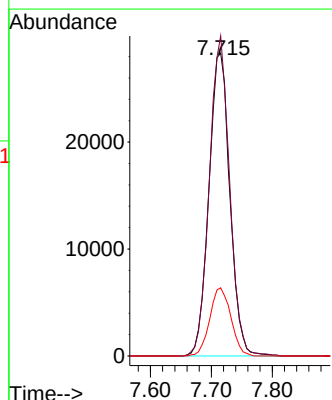
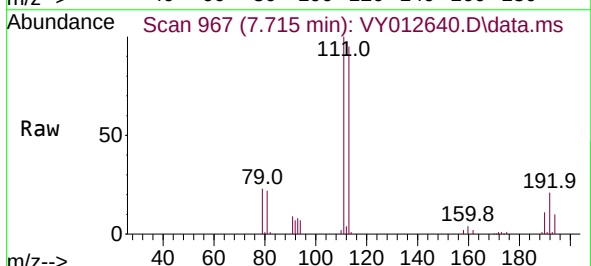


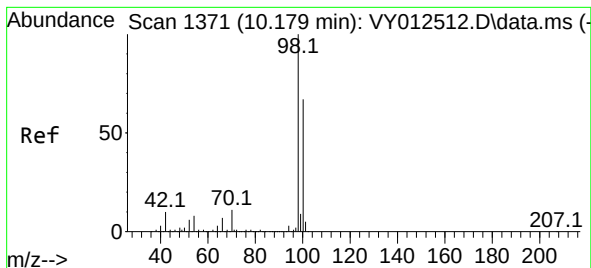

#50
Toluene-d8
Concen: 54.026 ug/l
RT: 10.178 min Scan# 11
Delta R.T. -0.000 min
Lab File: VY012640.D
Acq: 17 Feb 2023 11:01




Instrument :
MSVOA_Y
ClientSampleId :
VY0217SBL01


Tgt Ion: 98 Resp: 262894
Ion Ratio Lower Upper
98 100
100 65.0 52.2 78.2

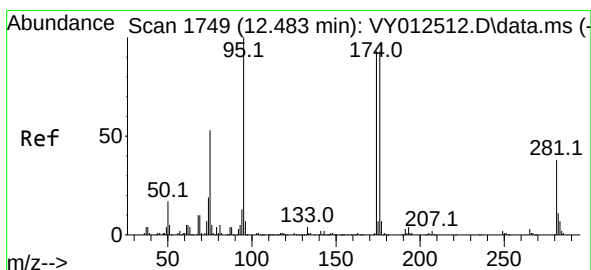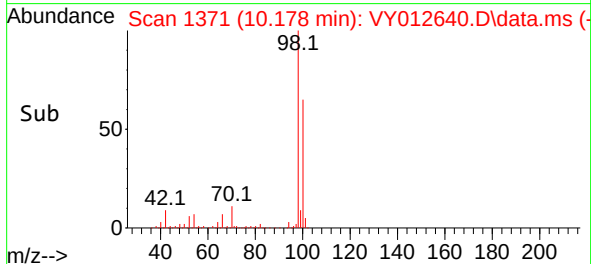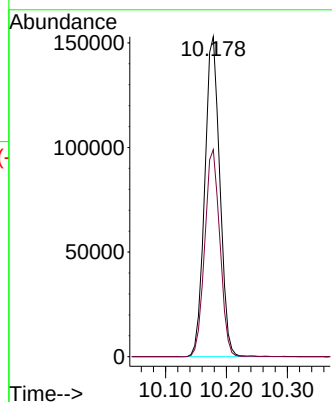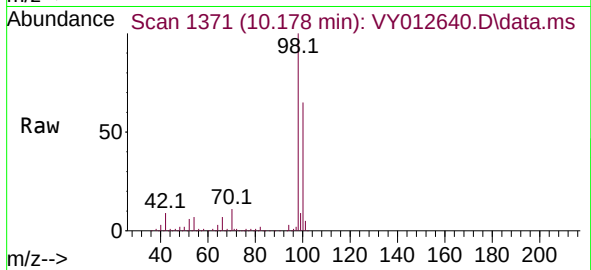

#62
4-Bromofluorobenzene
Concen: 50.863 ug/l
RT: 12.477 min Scan# 1748
Delta R.T. -0.006 min
Lab File: VY012640.D
Acq: 17 Feb 2023 11:01

Tgt Ion: 95 Resp: 86331
Ion Ratio Lower Upper
95 100
174 97.8 0.0 188.0
176 94.5 0.0 183.6


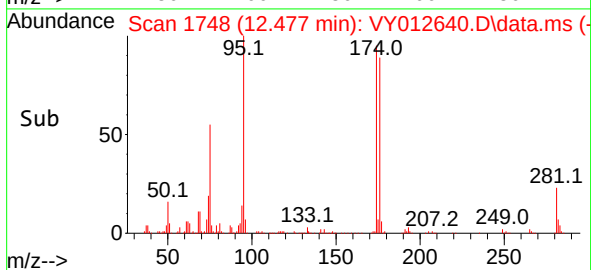
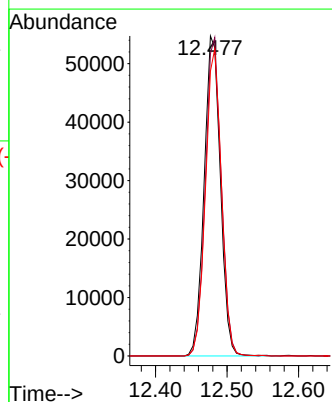
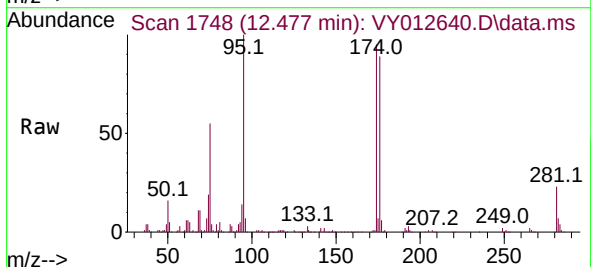


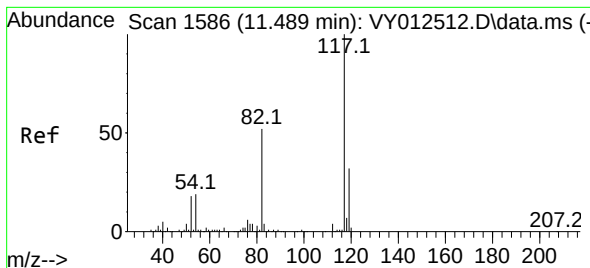

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 11.489 min Scan# 11
Delta R.T. -0.000 min
Lab File: VY012640.D
Acq: 17 Feb 2023 11:01

Instrument :
MSVOA_Y
ClientSampleId :
VY0217SBL01

Tgt Ion:117 Resp: 147029
Ion Ratio Lower Upper
117 100
82 48.4 41.7 62.5
119 31.9 25.8 38.8

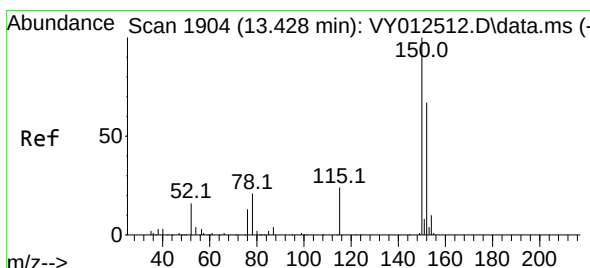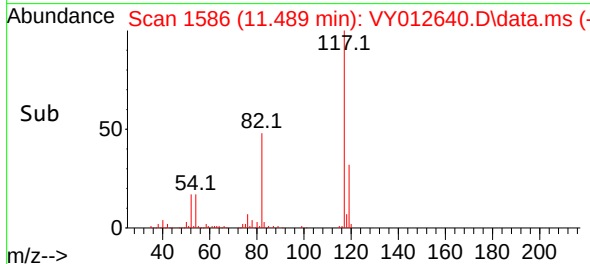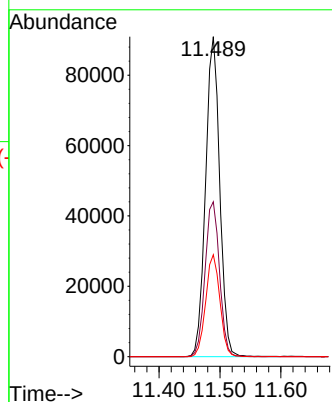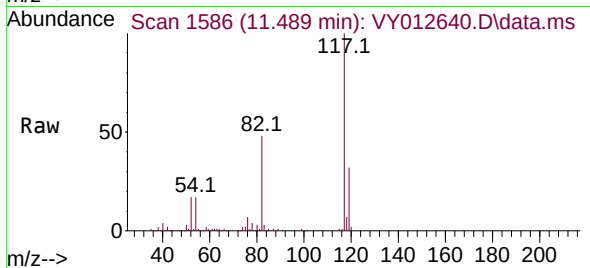

#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 13.428 min Scan# 1904
Delta R.T. -0.000 min
Lab File: VY012640.D
Acq: 17 Feb 2023 11:01

Tgt Ion:152 Resp: 78703
Ion Ratio Lower Upper
152 100
115 56.1 28.1 84.3
150 155.1 0.0 351.0

