

Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY021723\
 Data File : VY012645.D
 Acq On : 17 Feb 2023 12:58
 Operator : KP/MD
 Sample : 01595-01
 Misc : 5.02g/5.0mL/MSVOA_Y/SOIL
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 MSVOA_Y
 ClientSampleId :
 S-322-1

Quant Time: Feb 17 14:59:34 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y020723S.M
 Quant Title : SW846 8260
 QLast Update : Wed Feb 08 01:09:03 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Pentafluorobenzene	7.789	168	150796	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	8.685	114	250097	50.000	ug/l	0.00
63) Chlorobenzene-d5	11.490	117	260739	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.422	152	132160	50.000	ug/l	0.00

System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.136	65	86857	45.296	ug/l	0.00
Spiked Amount	50.000	Range	50 - 163	Recovery	=	90.600%
35) Dibromofluoromethane	7.710	113	75035	41.197	ug/l	0.00
Spiked Amount	50.000	Range	54 - 147	Recovery	=	82.400%
50) Toluene-d8	10.179	98	300065	39.581	ug/l	0.00
Spiked Amount	50.000	Range	49 - 140	Recovery	=	79.160%
62) 4-Bromofluorobenzene	12.477	95	108047	40.861	ug/l	0.00
Spiked Amount	50.000	Range	25 - 144	Recovery	=	81.720%


Target Compounds	Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY021723\
Data File : VY012645.D
Acq On : 17 Feb 2023 12:58
Operator : KP/MD
Sample : 01595-01
Misc : 5.02g/5.0mL/MSVOA_Y/SOIL
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_Y
ClientSampleId :
S-322-1

Quant Time: Feb 17 14:59:34 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y020723S.M
Quant Title : SW846 8260
QLast Update : Wed Feb 08 01:09:03 2023
Response via : Initial Calibration




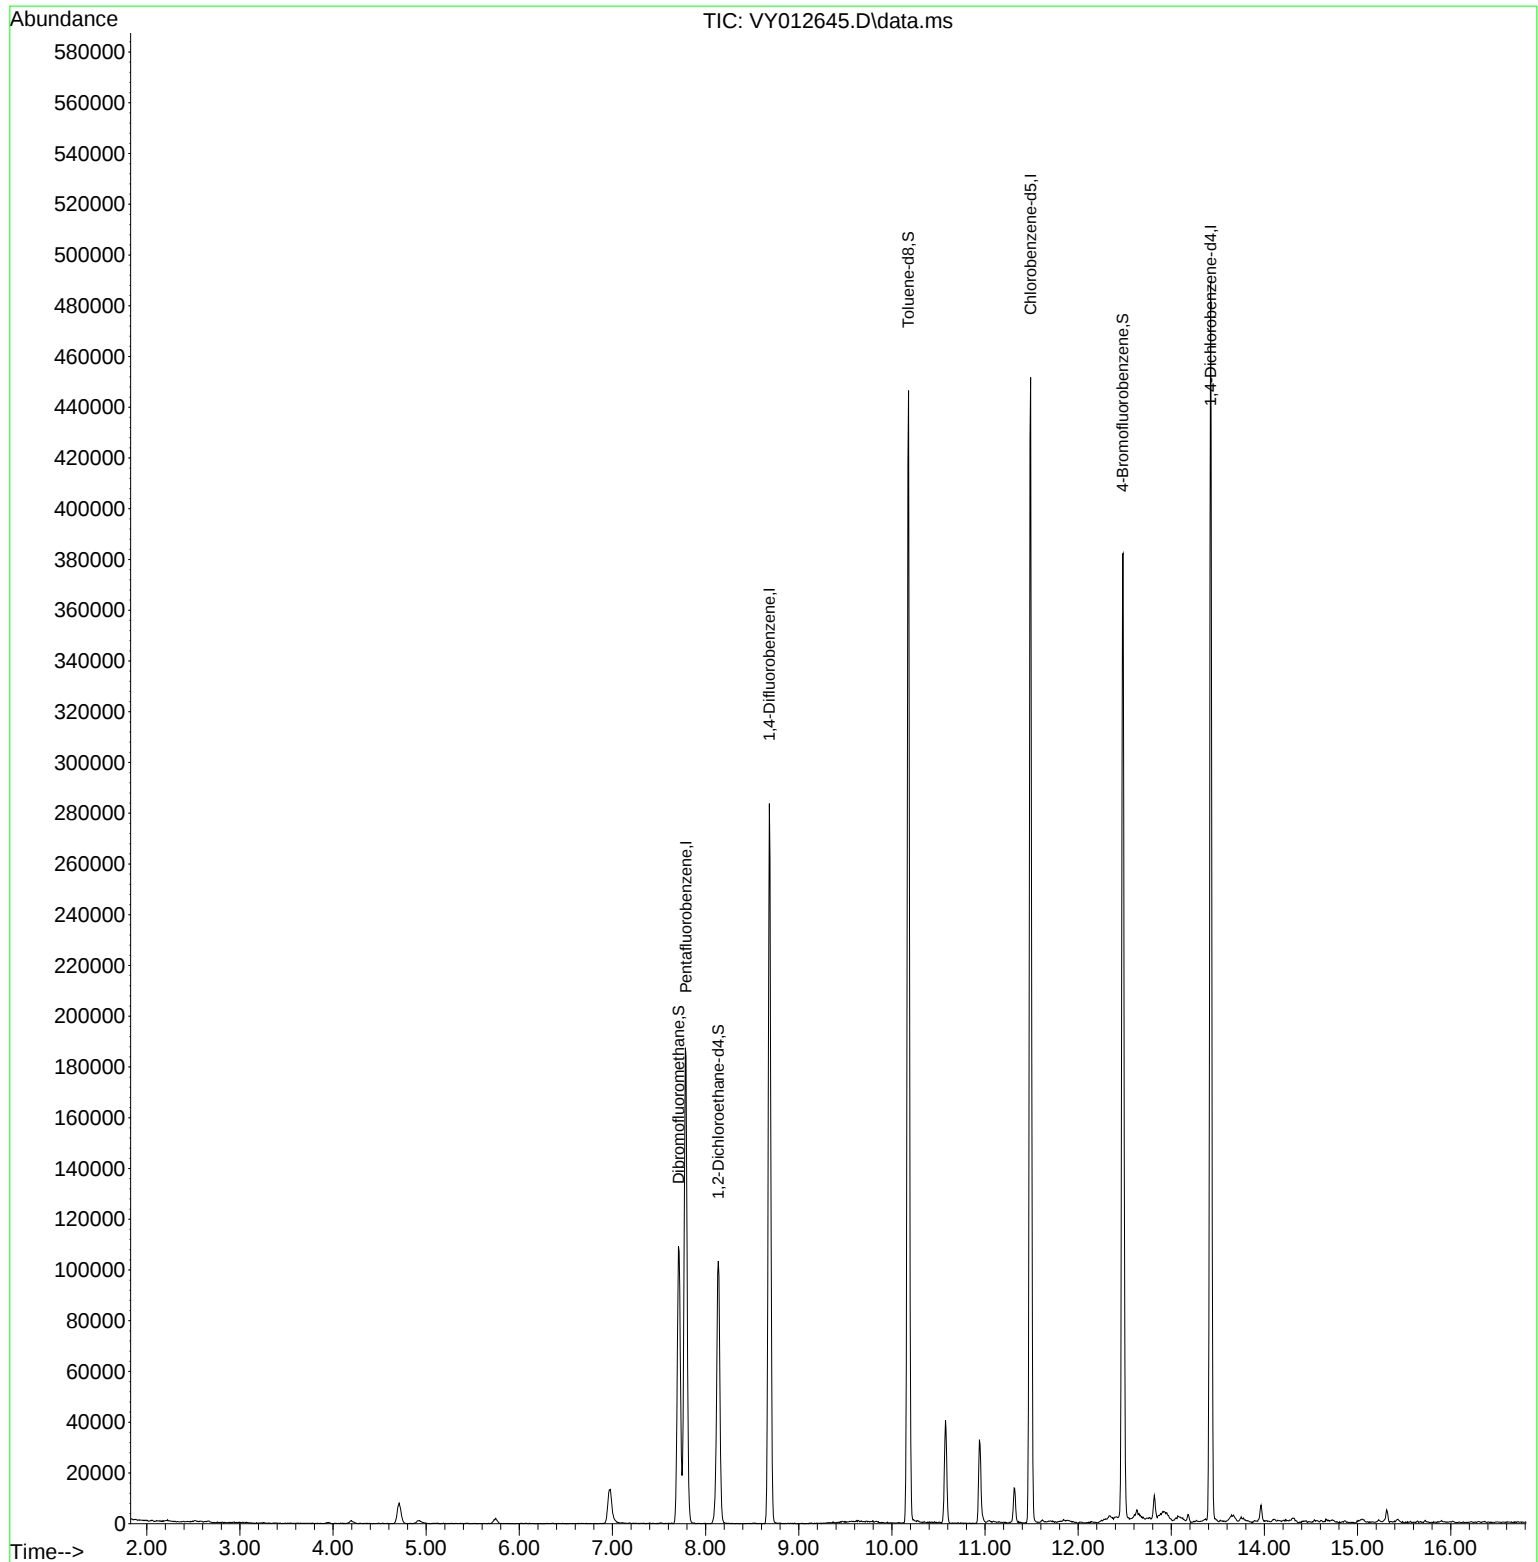


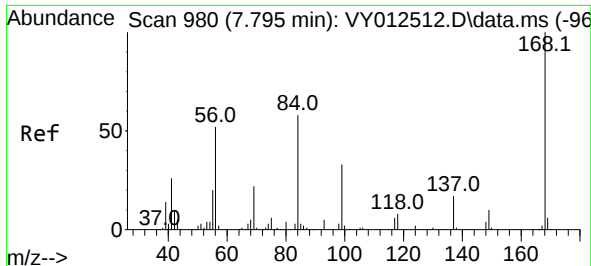

#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 7.789 min Scan# 91
Delta R.T. -0.006 min
Lab File: VY012645.D
Acq: 17 Feb 2023 12:58




Instrument :
MSVOA_Y
ClientSampleId :
S-322-1


Tgt Ion:168 Resp: 150796
Ion Ratio Lower Upper
168 100
99 52.0 40.8 61.2

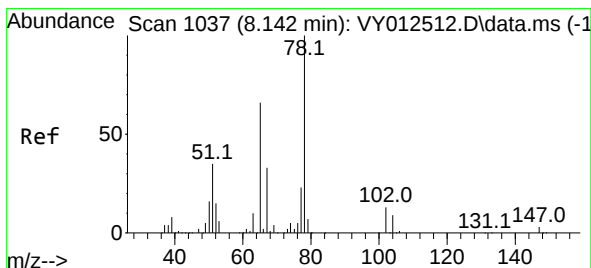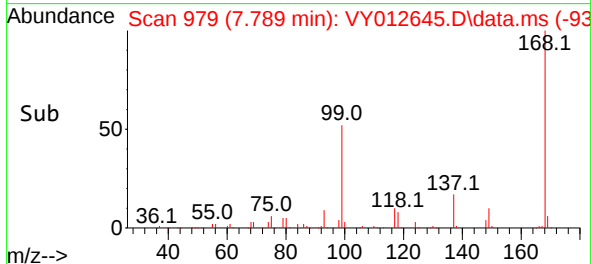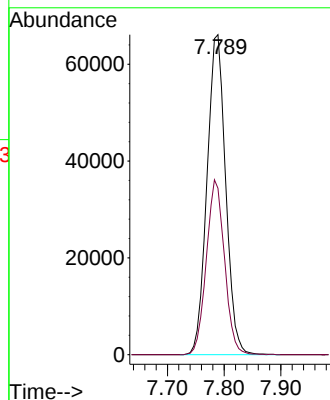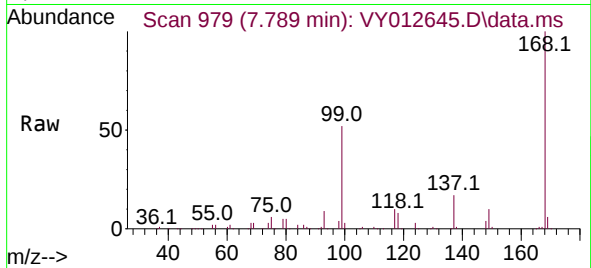

#33
1,2-Dichloroethane-d4
Concen: 45.296 ug/l
RT: 8.136 min Scan# 1036
Delta R.T. -0.006 min
Lab File: VY012645.D
Acq: 17 Feb 2023 12:58

Tgt Ion: 65 Resp: 86857
Ion Ratio Lower Upper
65 100
67 49.9 0.0 98.6

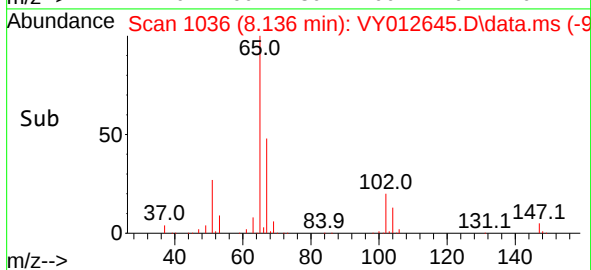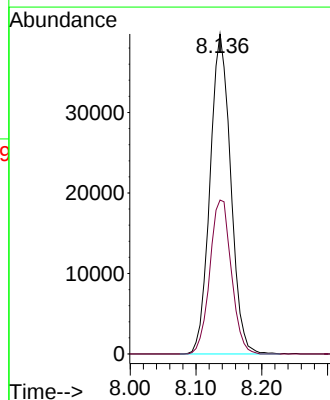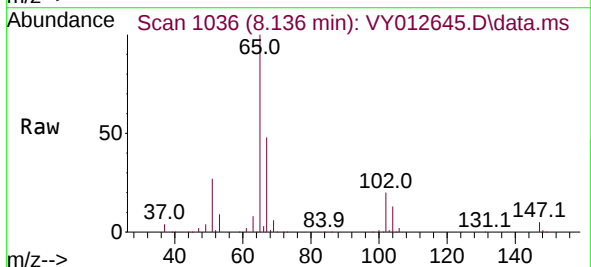

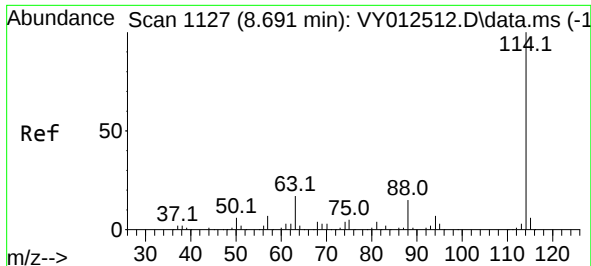

#34

1,4-Difluorobenzene

Concen: 50.000 ug/l

RT: 8.685 min Scan# 1126

Delta R.T. -0.006 min

Lab File: VY012645.D

Acq: 17 Feb 2023 12:58

Instrument :

MSVOA_Y

ClientSampleId :

S-322-1





Tgt Ion:114 Resp: 250097

Ion Ratio Lower Upper

114 100

63 16.6 0.0 33.6

88 15.2 0.0 29.8

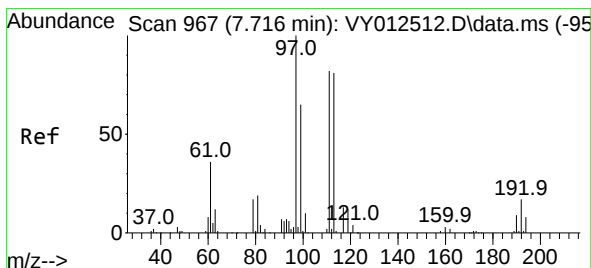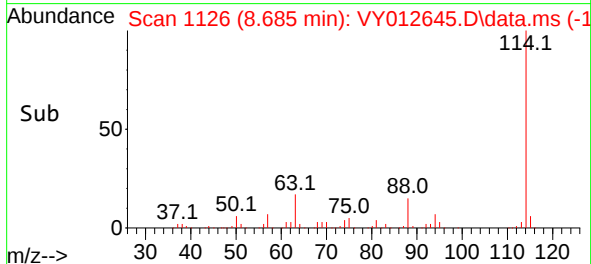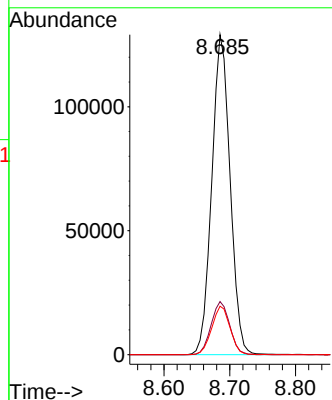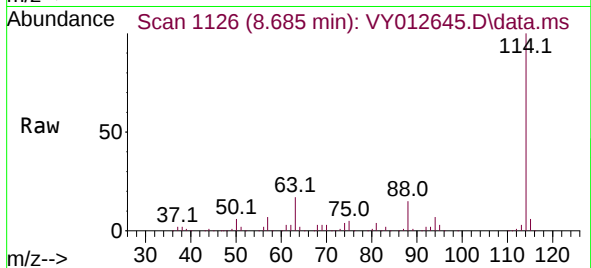

#35

Dibromofluoromethane

Concen: 41.197 ug/l

RT: 7.710 min Scan# 966

Delta R.T. -0.006 min

Lab File: VY012645.D

Acq: 17 Feb 2023 12:58




Tgt Ion:113 Resp: 75035


Ion Ratio Lower Upper

113 100

111 101.6 81.9 122.9

192 21.8 17.5 26.3


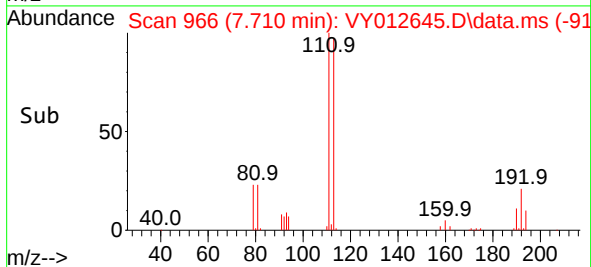
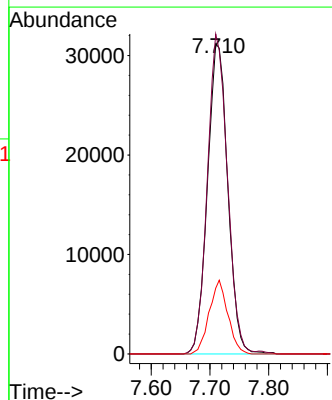
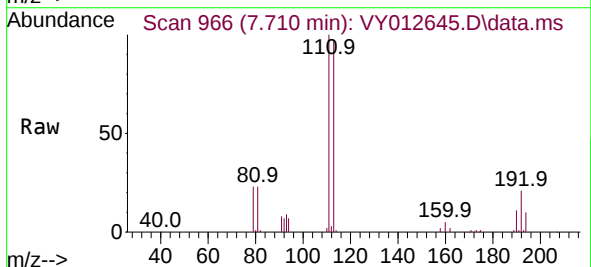


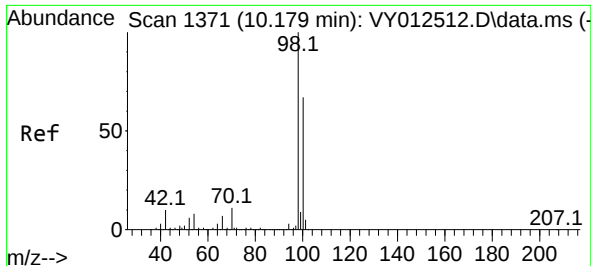

#50
Toluene-d8
Concen: 39.581 ug/l
RT: 10.179 min Scan# 11
Delta R.T. 0.000 min
Lab File: VY012645.D
Acq: 17 Feb 2023 12:58




Instrument :
MSVOA_Y
ClientSampleId :
S-322-1


Tgt Ion: 98 Resp: 300065
Ion Ratio Lower Upper
98 100
100 65.3 52.2 78.2

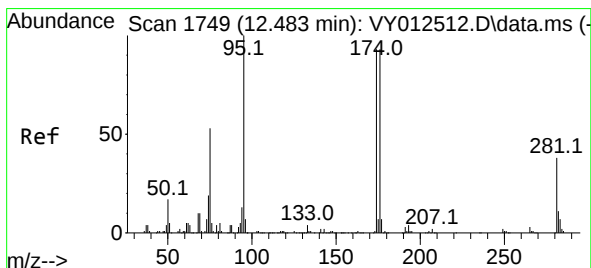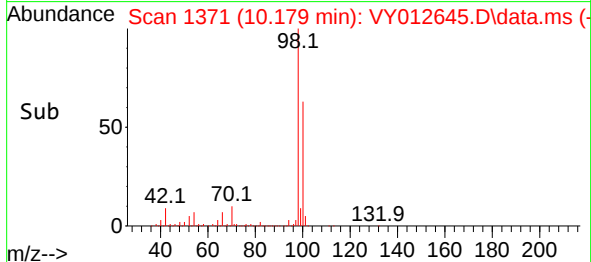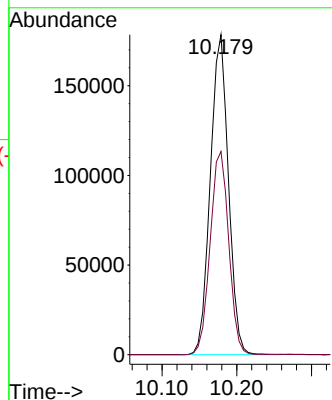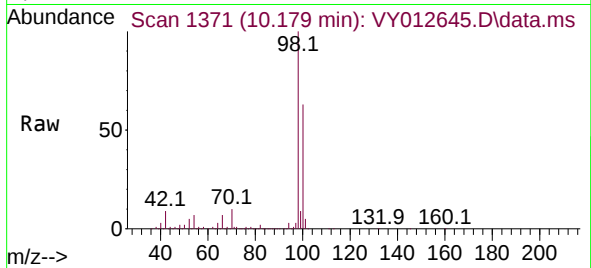

#62
4-Bromofluorobenzene
Concen: 40.861 ug/l
RT: 12.477 min Scan# 1748
Delta R.T. -0.006 min
Lab File: VY012645.D
Acq: 17 Feb 2023 12:58

Tgt Ion: 95 Resp: 108047
Ion Ratio Lower Upper
95 100
174 97.9 0.0 188.0
176 94.6 0.0 183.6

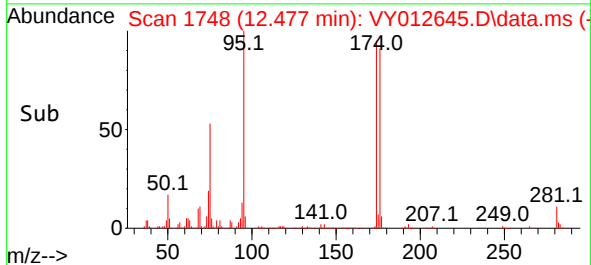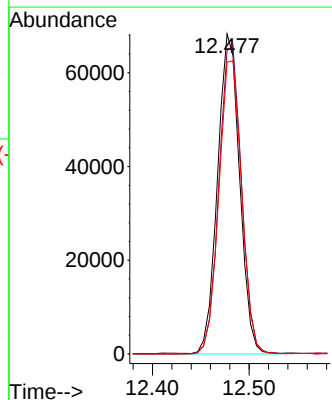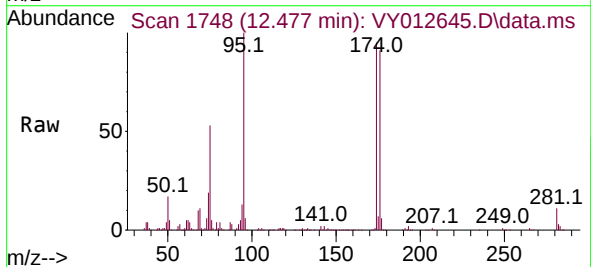

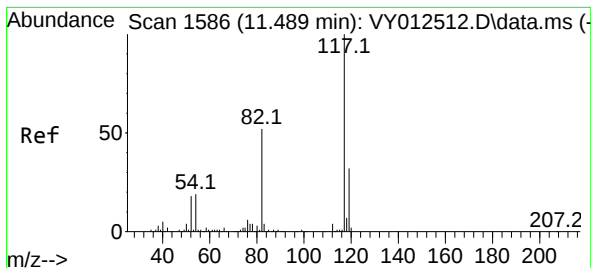

#63

Chlorobenzene-d5

Concen: 50.000 ug/l

RT: 11.490 min Scan# 11

Delta R.T. 0.000 min

Lab File: VY012645.D

Acq: 17 Feb 2023 12:58

Instrument :

MSVOA_Y

ClientSampleId :

S-322-1





Tgt Ion:117 Resp: 260739

Ion Ratio Lower Upper

117 100

82 49.7 41.7 62.5

119 31.5 25.8 38.8

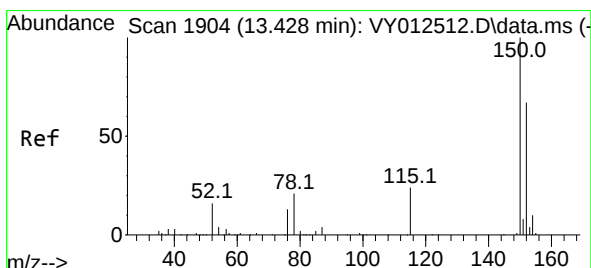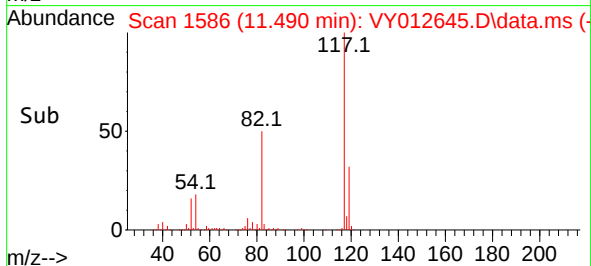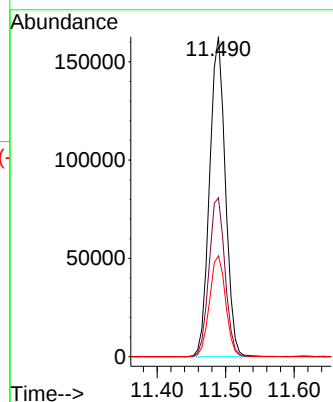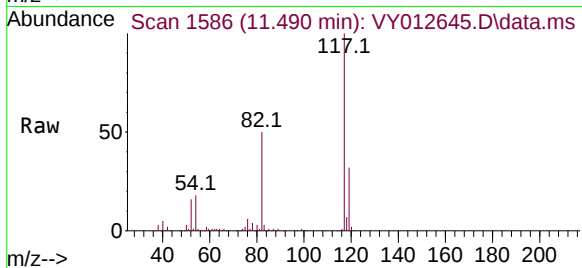

#72

1,4-Dichlorobenzene-d4

Concen: 50.000 ug/l

RT: 13.422 min Scan# 1903

Delta R.T. -0.006 min

Lab File: VY012645.D

Acq: 17 Feb 2023 12:58

Tgt Ion:152 Resp: 132160

Ion Ratio Lower Upper

152 100

115 54.8 28.1 84.3

150 155.7 0.0 351.0

