

Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY021723\
 Data File : VY012648.D
 Acq On : 17 Feb 2023 14:08
 Operator : KP/MD
 Sample : 01559-03RE
 Misc : 5.07g/5.0mL/MSVOA_Y/SOIL
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 MSVOA_Y
 ClientSampleId :
 BP-VPB-RW10-GW-798-800RE

Quant Time: Feb 17 15:00:19 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y020723S.M
 Quant Title : SW846 8260
 QLast Update : Wed Feb 08 01:09:03 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Pentafluorobenzene	7.789	168	149974	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	8.685	114	249696	50.000	ug/l	0.00
63) Chlorobenzene-d5	11.490	117	252340	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.422	152	129164	50.000	ug/l	0.00

System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.137	65	92555	48.532	ug/l	0.00
Spiked Amount	50.000	Range	50 - 163	Recovery	=	97.060%
35) Dibromofluoromethane	7.716	113	74259	40.837	ug/l	0.00
Spiked Amount	50.000	Range	54 - 147	Recovery	=	81.680%
50) Toluene-d8	10.179	98	295041	38.981	ug/l	0.00
Spiked Amount	50.000	Range	49 - 140	Recovery	=	77.960%
62) 4-Bromofluorobenzene	12.477	95	107902	40.871	ug/l	0.00
Spiked Amount	50.000	Range	25 - 144	Recovery	=	81.740%


Target Compounds	Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY021723\
Data File : VY012648.D
Acq On : 17 Feb 2023 14:08
Operator : KP/MD
Sample : 01559-03RE
Misc : 5.07g/5.0mL/MSVOA_Y/SOIL
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_Y
ClientSampleId :
BP-VPB-RW10-GW-798-800RE

Quant Time: Feb 17 15:00:19 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y020723S.M
Quant Title : SW846 8260
QLast Update : Wed Feb 08 01:09:03 2023
Response via : Initial Calibration




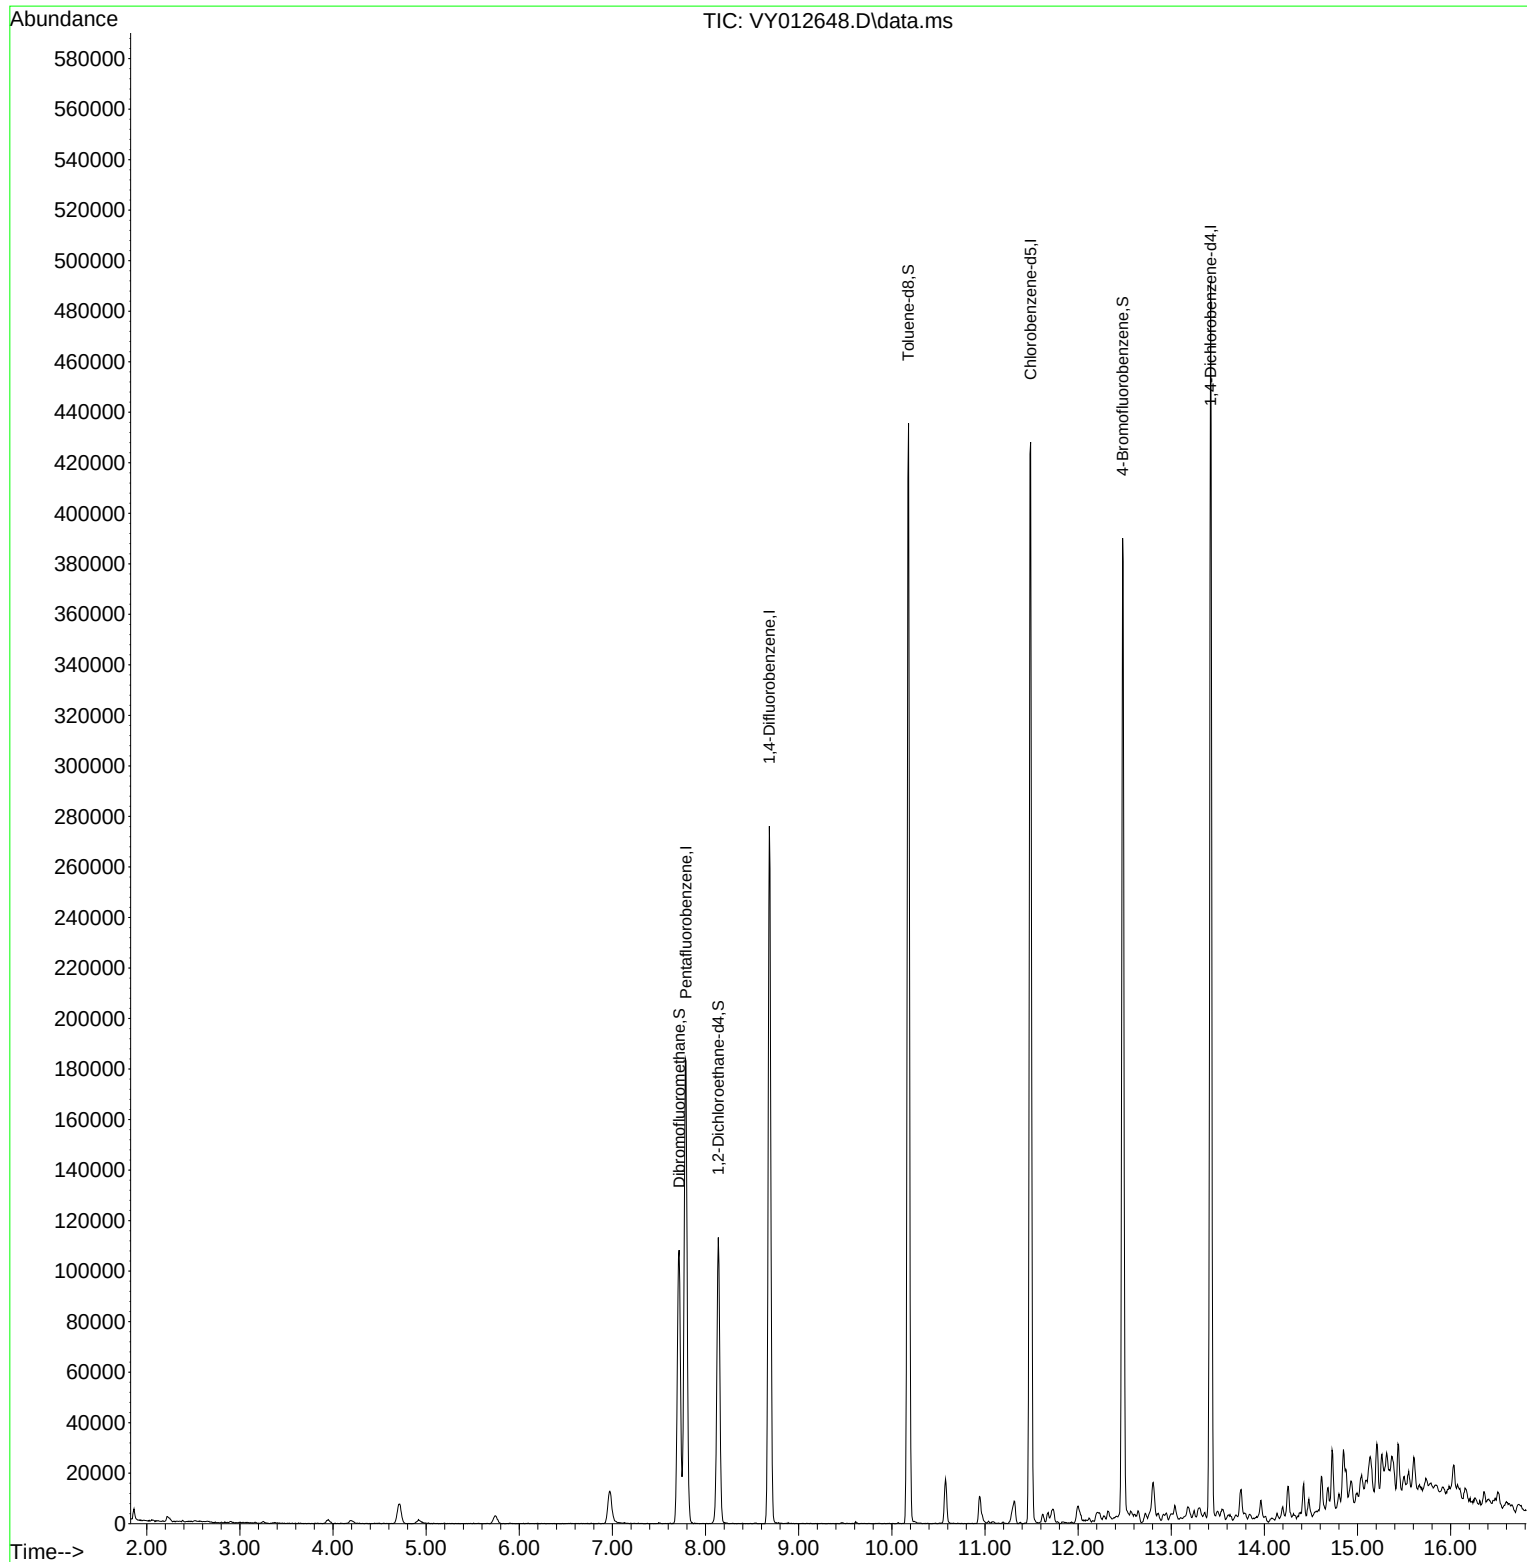


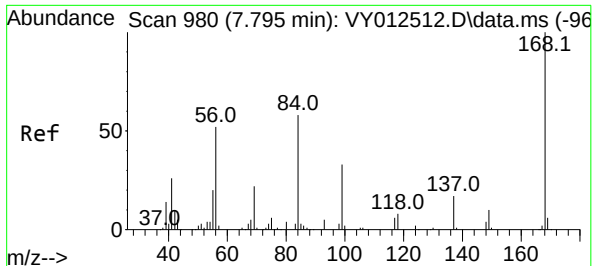

#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 7.789 min Scan# 91
Delta R.T. -0.006 min
Lab File: VY012648.D
Acq: 17 Feb 2023 14:08




Instrument :
MSVOA_Y
ClientSampleId :
BP-VPB-RW10-GW-798-800RE


Tgt Ion:168 Resp: 149974
Ion Ratio Lower Upper
168 100
99 49.9 40.8 61.2

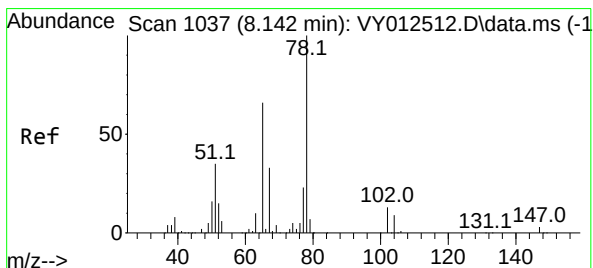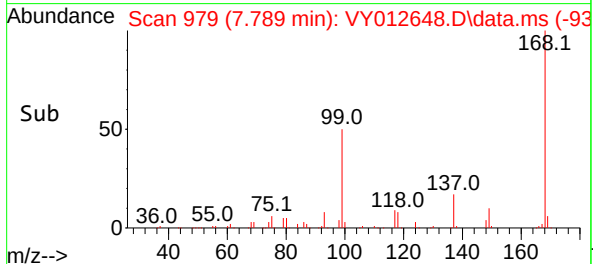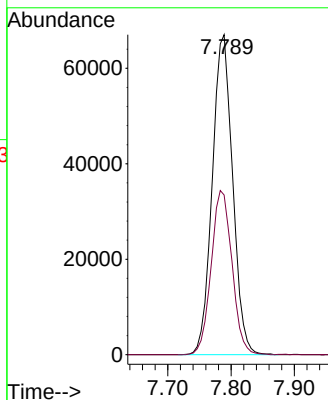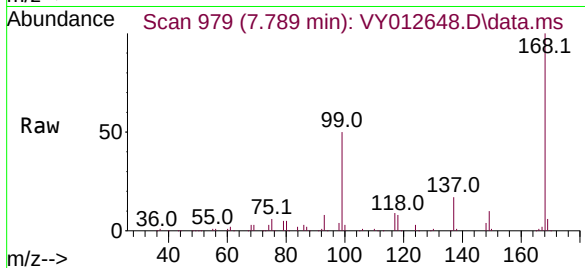

#33
1,2-Dichloroethane-d4
Concen: 48.532 ug/l
RT: 8.137 min Scan# 1036
Delta R.T. -0.006 min
Lab File: VY012648.D
Acq: 17 Feb 2023 14:08

Tgt Ion: 65 Resp: 92555
Ion Ratio Lower Upper
65 100
67 49.0 0.0 98.6

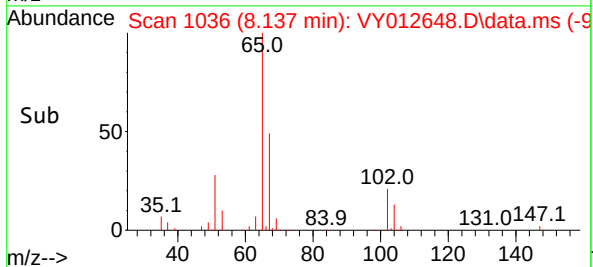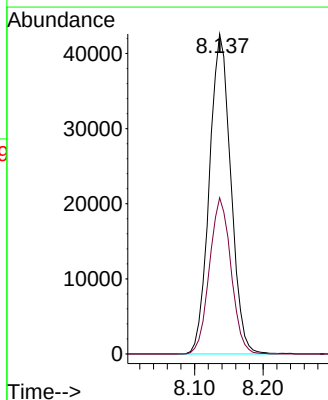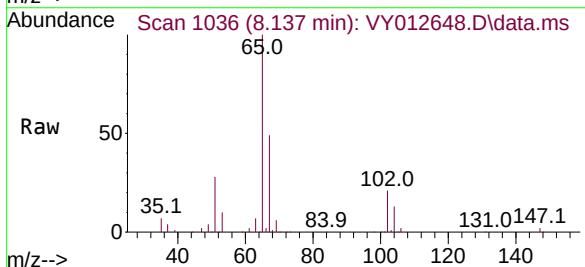

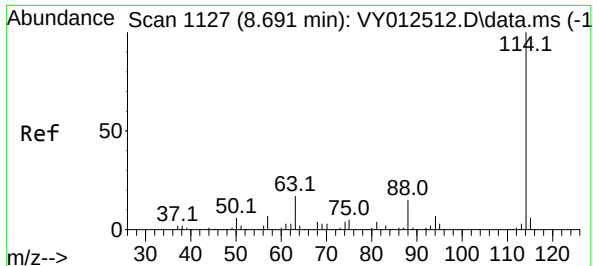

#34

1,4-Difluorobenzene

Concen: 50.000 ug/l

RT: 8.685 min Scan# 1126

Delta R.T. -0.006 min

Lab File: VY012648.D

Acq: 17 Feb 2023 14:08

Instrument :

MSVOA_Y

ClientSampleId :

BP-VPB-RW10-GW-798-800RE





Tgt Ion:114 Resp: 249696

Ion Ratio Lower Upper

114 100

63 17.3 0.0 33.6

88 14.7 0.0 29.8

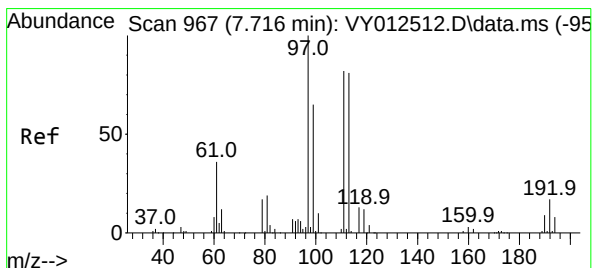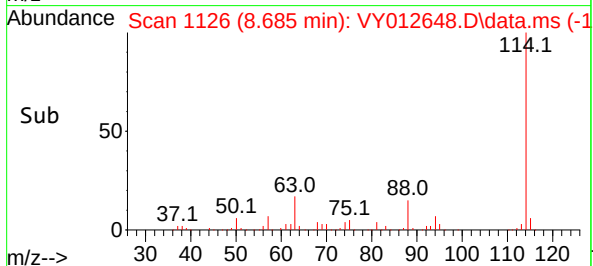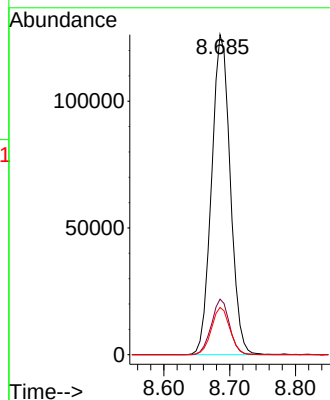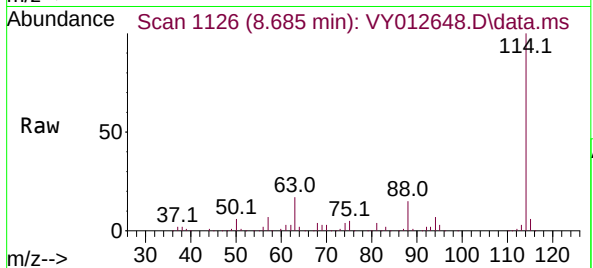

#35

Dibromofluoromethane

Concen: 40.837 ug/l

RT: 7.716 min Scan# 967

Delta R.T. 0.000 min

Lab File: VY012648.D

Acq: 17 Feb 2023 14:08




Tgt Ion:113 Resp: 74259


Ion Ratio Lower Upper

113 100

111 103.0 81.9 122.9

192 23.0 17.5 26.3


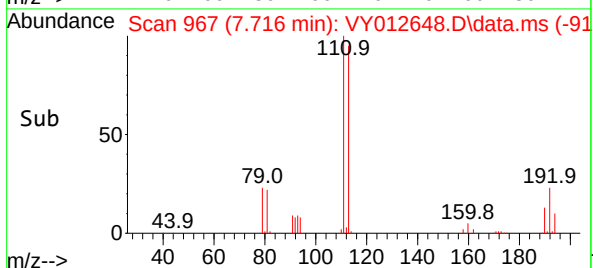
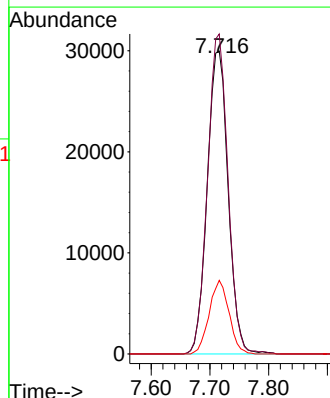
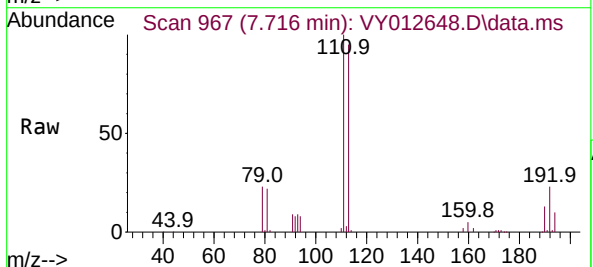


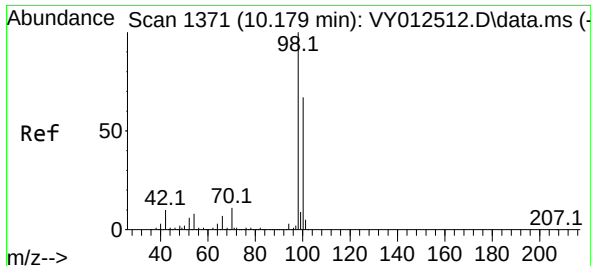

#50
Toluene-d8
Concen: 38.981 ug/l
RT: 10.179 min Scan# 11
Delta R.T. 0.000 min
Lab File: VY012648.D
Acq: 17 Feb 2023 14:08




Instrument :
MSVOA_Y
ClientSampleId :
BP-VPB-RW10-GW-798-800RE


Tgt Ion: 98 Resp: 295041
Ion Ratio Lower Upper
98 100
100 64.8 52.2 78.2

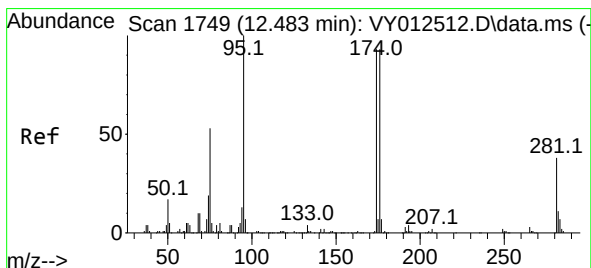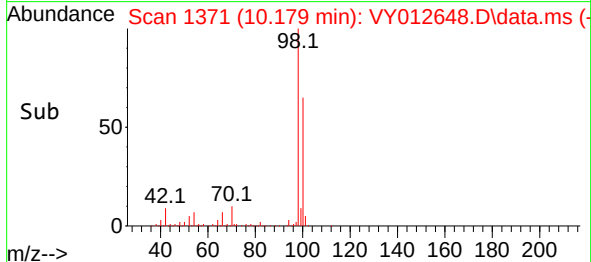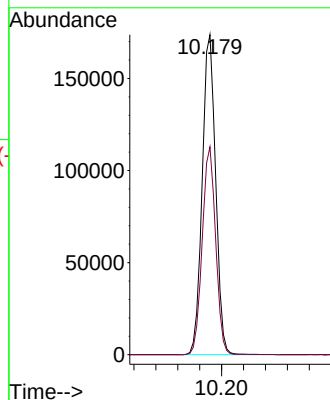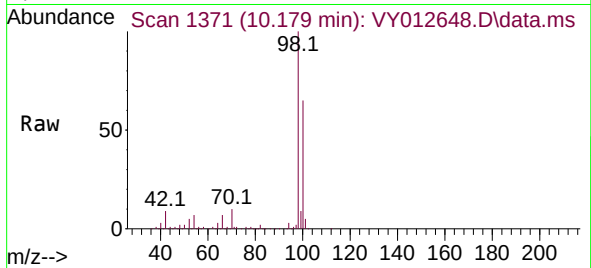

#62
4-Bromofluorobenzene
Concen: 40.871 ug/l
RT: 12.477 min Scan# 1748
Delta R.T. -0.006 min
Lab File: VY012648.D
Acq: 17 Feb 2023 14:08

Tgt Ion: 95 Resp: 107902
Ion Ratio Lower Upper
95 100
174 98.3 0.0 188.0
176 94.1 0.0 183.6

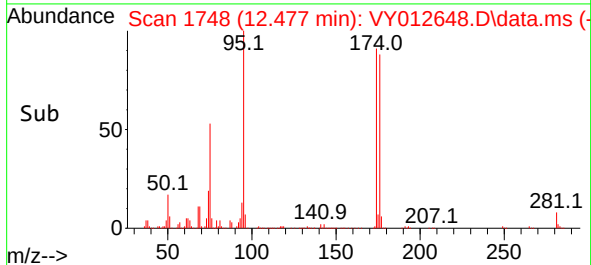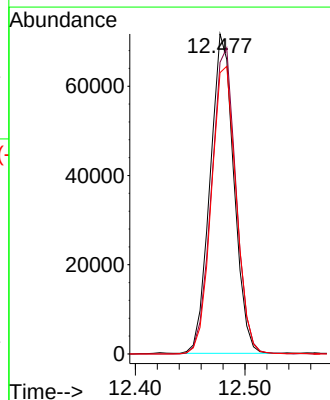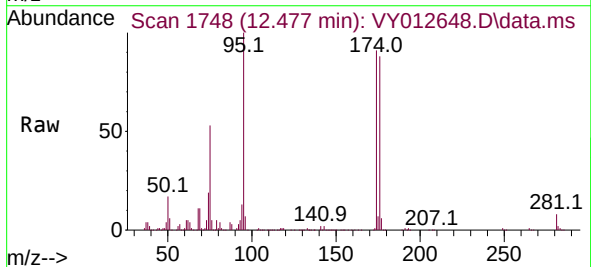

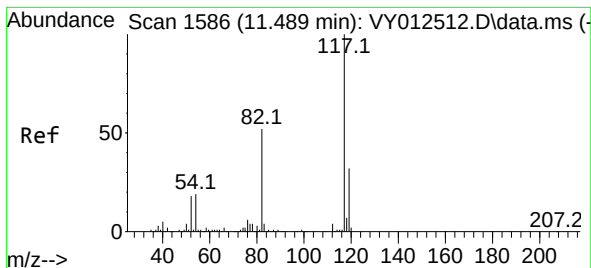

#63

Chlorobenzene-d5

Concen: 50.000 ug/l

RT: 11.490 min Scan# 11

Delta R.T. 0.000 min

Lab File: VY012648.D

Acq: 17 Feb 2023 14:08

Instrument :

MSVOA_Y

ClientSampleId :

BP-VPB-RW10-GW-798-800RE





Tgt Ion:117 Resp: 252340

Ion Ratio Lower Upper

117 100

82 50.2 41.7 62.5

119 32.8 25.8 38.8

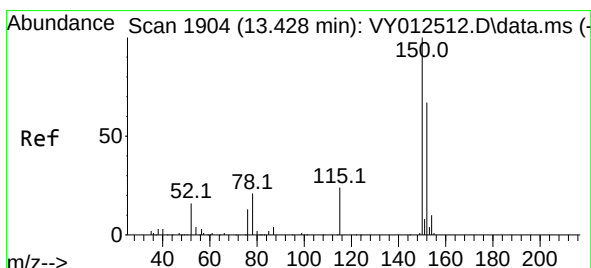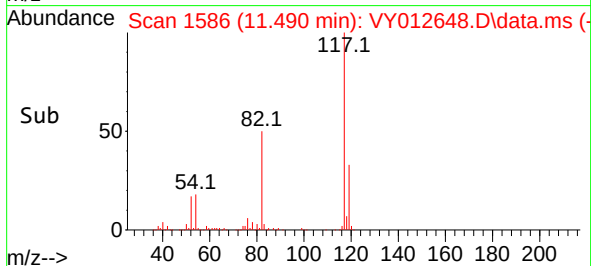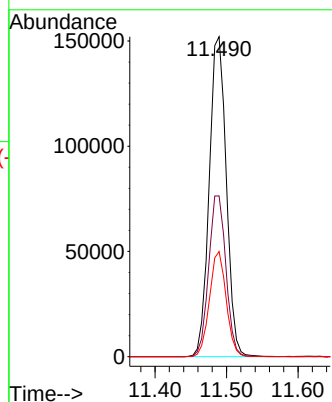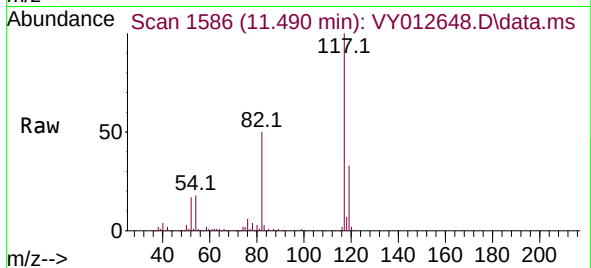

#72

1,4-Dichlorobenzene-d4

Concen: 50.000 ug/l

RT: 13.422 min Scan# 1903

Delta R.T. -0.006 min

Lab File: VY012648.D

Acq: 17 Feb 2023 14:08

Tgt Ion:152 Resp: 129164

Ion Ratio Lower Upper

152 100

115 56.9 28.1 84.3

150 157.4 0.0 351.0

