

Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY021822\
 Data File : VY007551.D
 Acq On : 18 Feb 2022 17:38
 Operator : SY/MD
 Sample : N1600-04
 Misc : 5.21g/5.0mL/MSVOA_Y/SOIL
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 MSVOA_Y
 ClientSampleId :
 C0AA4

Quant Time: Feb 19 04:35:19 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y021422S.M
 Quant Title : SW846 8260
 QLast Update : Tue Feb 15 09:34:50 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Pentafluorobenzene	7.789	168	67875	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	8.691	114	120659	50.000	ug/l	0.00
63) Chlorobenzene-d5	11.489	117	116872	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.428	152	47858	50.000	ug/l	0.00

System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.142	65	43640	58.235	ug/l	0.00
Spiked Amount	50.000	Range	50 - 163	Recovery	= 116.480%	
35) Dibromofluoromethane	7.722	113	40122	52.729	ug/l	0.00
Spiked Amount	50.000	Range	54 - 147	Recovery	= 105.460%	
50) Toluene-d8	10.179	98	148073	51.236	ug/l	0.00
Spiked Amount	50.000	Range	49 - 140	Recovery	= 102.480%	
62) 4-Bromofluorobenzene	12.477	95	51702	52.760	ug/l	0.00
Spiked Amount	50.000	Range	25 - 144	Recovery	= 105.520%	


Target Compounds				Qvalue		
3) Chloromethane	2.119	50	126	Below Cal	#	44
16) Acetone	3.948	43	49305	247.990	ug/l	96
18) Methyl Acetate	4.466	43	60	1.505	ug/l #	56
20) Methylene Chloride	4.710	84	920	1.129	ug/l #	62
31) Cyclohexane	7.783	56	2384	1.799	ug/l #	53
36) 1,1-Dichloropropene	7.789	75	5556	4.507	ug/l #	51
38) Carbon Tetrachloride	7.789	117	7585	5.415	ug/l #	14
39) Methylcyclohexane	9.185	83	7694	4.807	ug/l #	82
55) 1,1,2-Trichloroethane	10.618	97	6946	10.464	ug/l #	20
56) Ethyl methacrylate	10.514	69	1615	1.809	ug/l #	74
59) 2-Hexanone	10.801	43	4307	10.618	ug/l #	31
66) 1,1,1,2-Tetrachloroethane	11.599	131	1194	1.235	ug/l #	9
67) Ethyl Benzene	11.593	91	11705	2.443	ug/l	97
68) m/p-Xylenes	11.697	106	7963	4.392	ug/l	91
69) o-Xylene	12.026	106	13340	7.776	ug/l	97
73) Isopropylbenzene	12.331	105	8294	1.956	ug/l	92
75) 1,1,2,2-Tetrachloroethane	12.532	83	762	1.049	ug/l #	44
76) 1,2,3-Trichloropropane	12.477	75	28816	52.111	ug/l #	100
78) n-propylbenzene	12.666	91	12783	2.506	ug/l	95
79) 2-Chlorotoluene	12.733	91	4447	1.581	ug/l #	44
80) 1,3,5-Trimethylbenzene	12.812	105	28344	8.071	ug/l	96
81) trans-1,4-Dichloro-2-b...	12.477	75	28816	108.310	ug/l #	8
82) 4-Chlorotoluene	12.806	91	3584	1.243	ug/l #	63
83) tert-Butylbenzene	13.123	119	4597	1.498	ug/l #	67
84) 1,2,4-Trimethylbenzene	13.117	105	34825	10.227	ug/l	99
85) sec-Butylbenzene	13.251	105	10962	2.423	ug/l	84
86) p-Isopropyltoluene	13.367	119	4209	1.129	ug/l	94
89) n-Butylbenzene	13.696	91	6281	1.772	ug/l #	50
90) Hexachloroethane	13.971	117	5570	7.821	ug/l #	6
92) 1,2-Dibromo-3-Chloropr...	14.336	75	593	4.810	ug/l #	6
95) Naphthalene	15.202	128	4100	2.014	ug/l #	1
96) 1,2,3-Trichlorobenzene	15.446	180	2934	3.630	ug/l #	1


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY021822\
Data File : VY007551.D
Acq On : 18 Feb 2022 17:38
Operator : SY/MD
Sample : N1600-04
Misc : 5.21g/5.0mL/MSVOA_Y/SOIL
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_Y
ClientSampleId :
C0AA4

Quant Time: Feb 19 04:35:19 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y021422S.M
Quant Title : SW846 8260
QLast Update : Tue Feb 15 09:34:50 2022
Response via : Initial Calibration




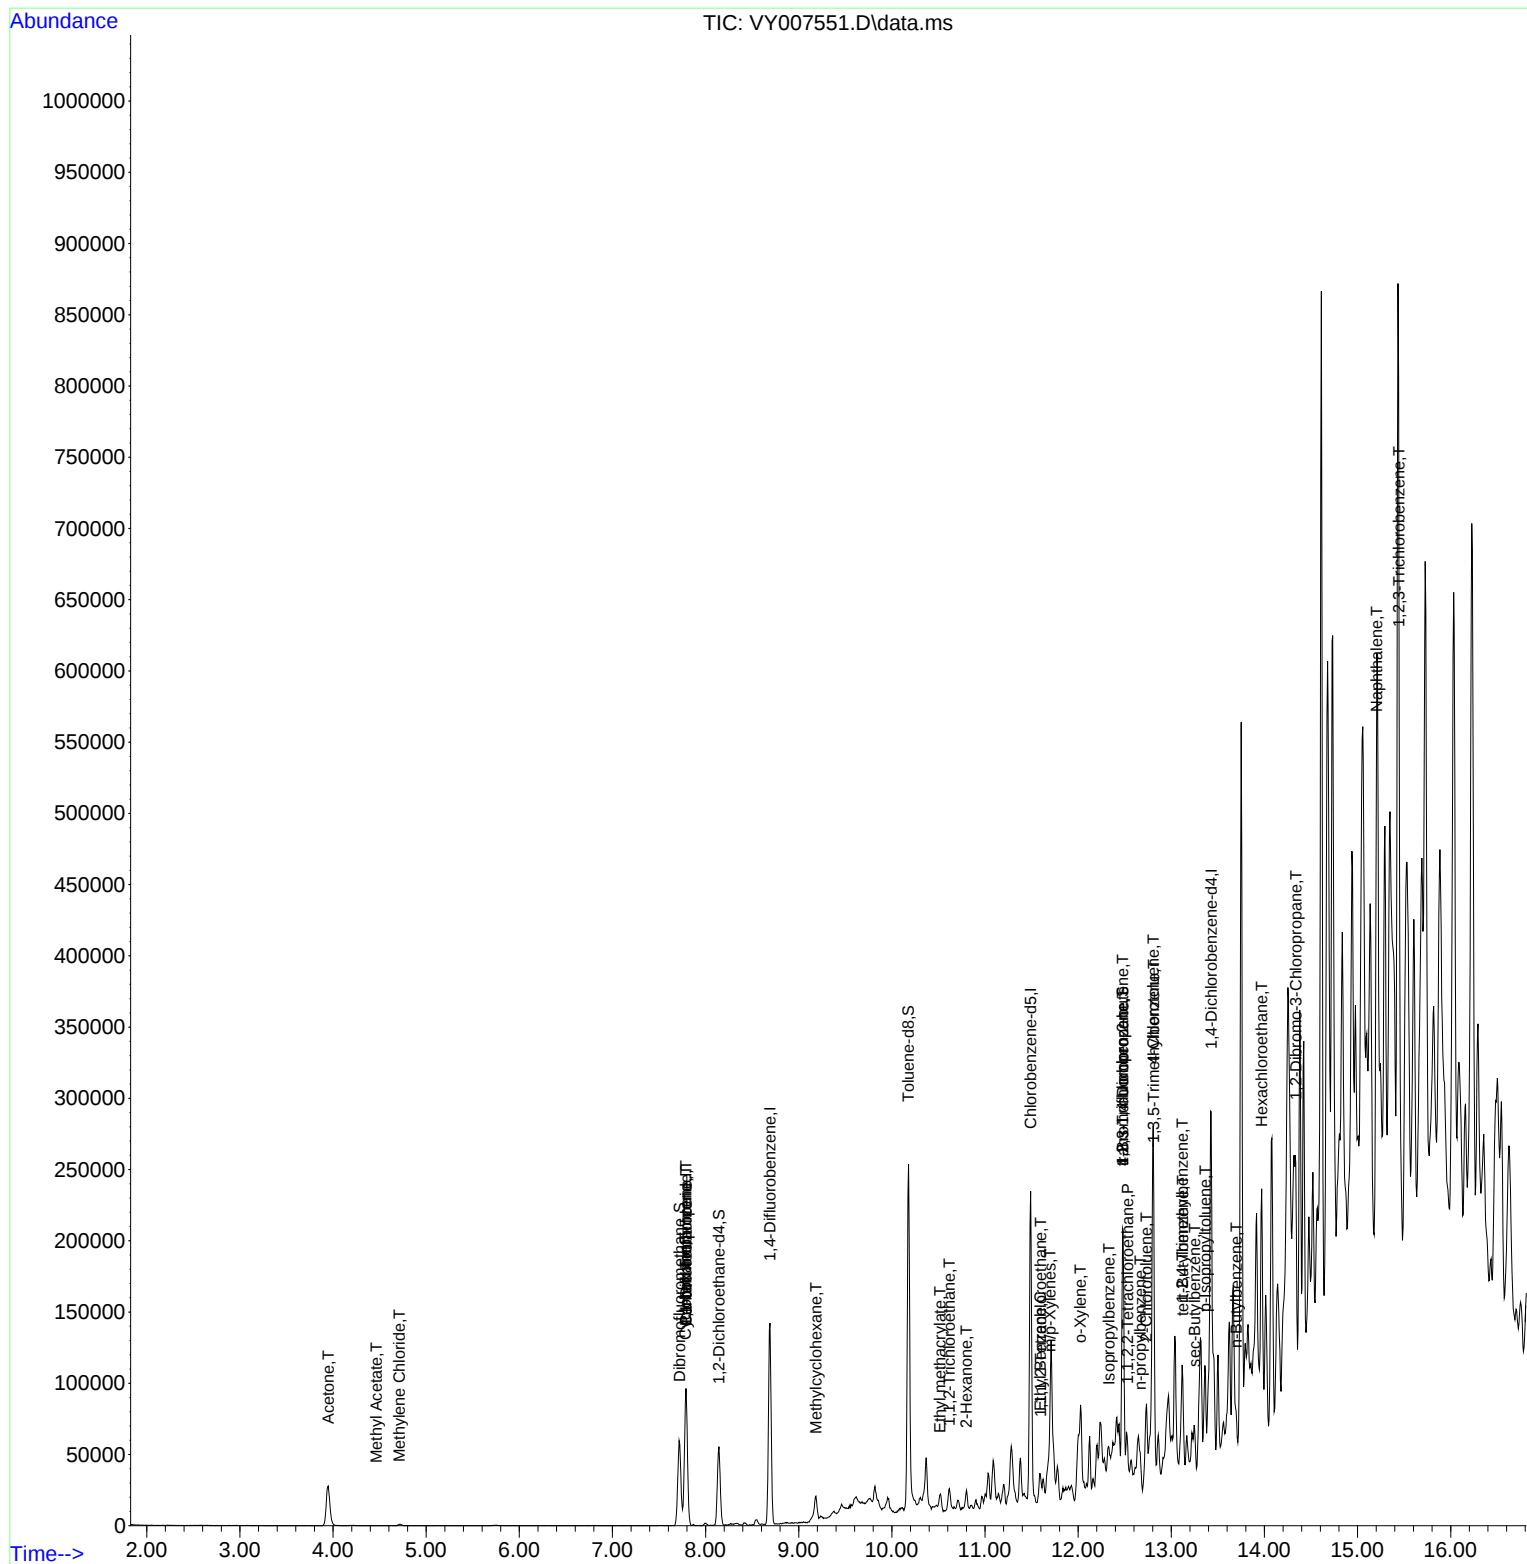


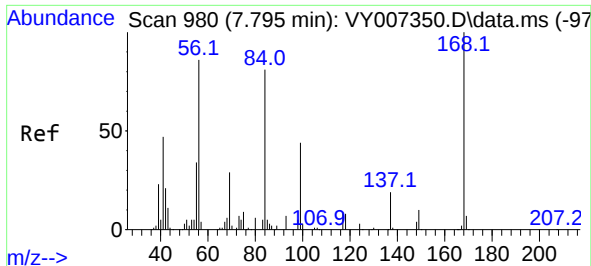

#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 7.789 min Scan# 91
Delta R.T. -0.006 min
Lab File: VY007551.D
Acq: 18 Feb 2022 17:38




Instrument :
MSVOA_Y
ClientSampleId :
C0AA4


Tgt Ion:168 Resp: 67875
Ion Ratio Lower Upper
168 100
99 62.5 46.9 70.3



#16
Acetone
Concen: 247.990 ug/l
RT: 3.948 min Scan# 349
Delta R.T. 0.000 min
Lab File: VY007551.D
Acq: 18 Feb 2022 17:38

Tgt Ion: 43 Resp: 49305
Ion Ratio Lower Upper
43 100
58 29.8 22.0 33.0

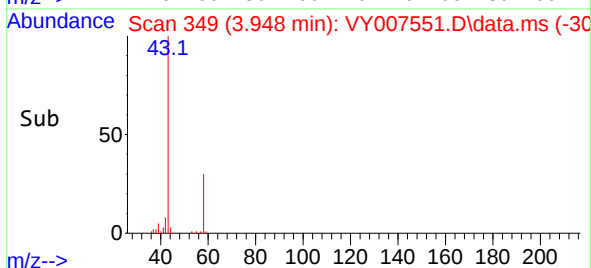

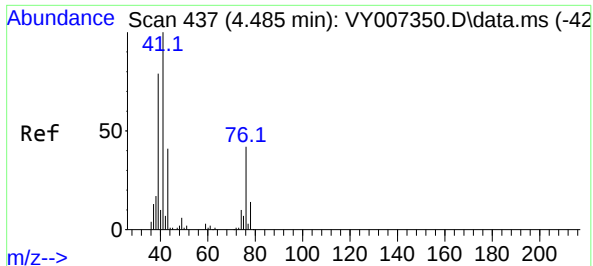

#18

Methyl Acetate

Concen: 1.505 ug/l

RT: 4.466 min Scan# 41

Delta R.T. -0.019 min

Lab File: VY007551.D

Acq: 18 Feb 2022 17:38

Instrument :

MSVOA_Y

ClientSampleId :





C0AA4

Tgt Ion: 43 Resp: 60

Ion Ratio Lower Upper

43 100

74 0.0 16.6 24.8#

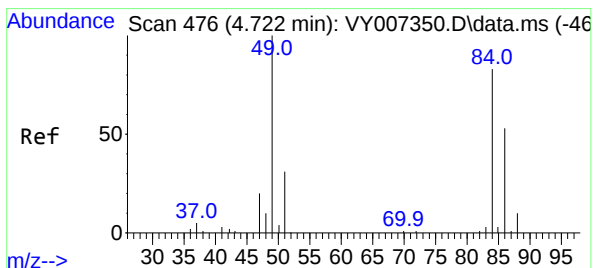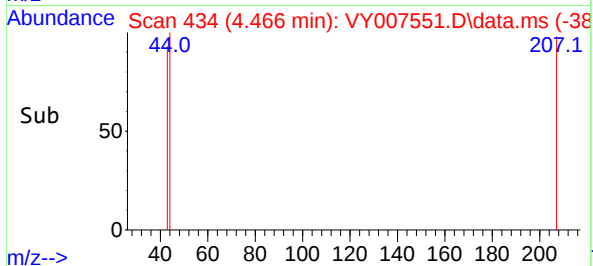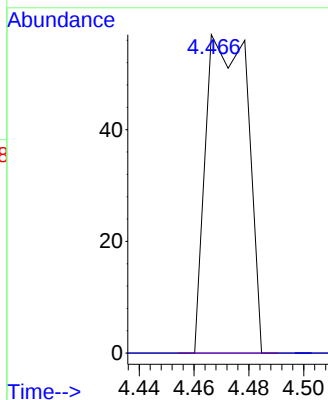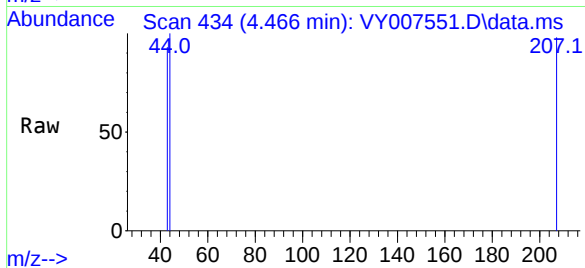

#20

Methylene Chloride

Concen: 1.129 ug/l

RT: 4.710 min Scan# 474

Delta R.T. -0.012 min

Lab File: VY007551.D

Acq: 18 Feb 2022 17:38

Tgt Ion: 84 Resp: 920




Ion Ratio Lower Upper


84 100

49 70.9 114.4 171.6#

51 40.7 35.3 52.9

86 55.7 53.7 80.5


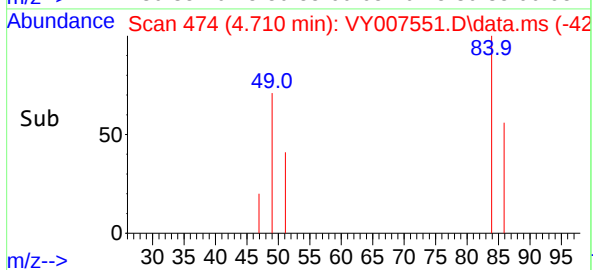
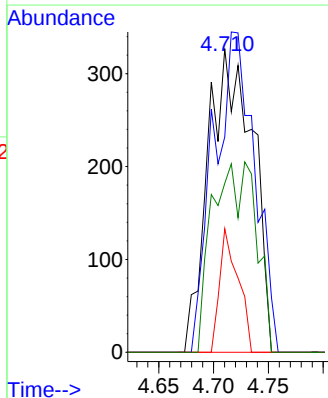
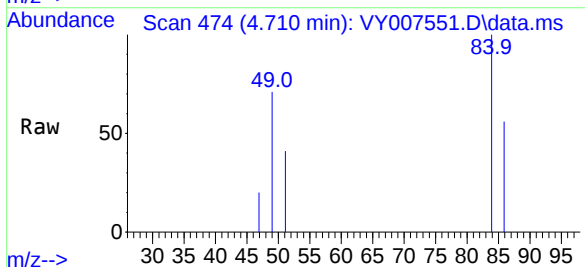




#31
Cyclohexane
Concen: 1.799 ug/l
RT: 7.783 min Scan# 91
Delta R.T. -0.006 min
Lab File: VY007551.D
Acq: 18 Feb 2022 17:38




Instrument :
MSVOA_Y
ClientSampleId :
C0AA4


Tgt Ion: 56 Resp: 2384
Ion Ratio Lower Upper
56 100
69 105.3 26.7 40.1#
84 97.9 67.2 100.8

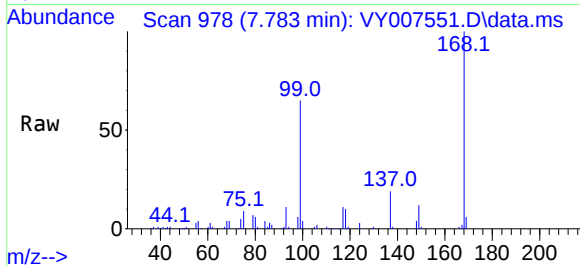

#33
1,2-Dichloroethane-d4
Concen: 58.235 ug/l
RT: 8.142 min Scan# 1037
Delta R.T. -0.001 min
Lab File: VY007551.D
Acq: 18 Feb 2022 17:38

Tgt Ion: 65 Resp: 43640
Ion Ratio Lower Upper
65 100
67 50.7 0.0 99.4

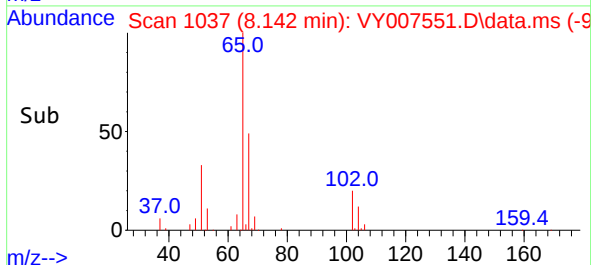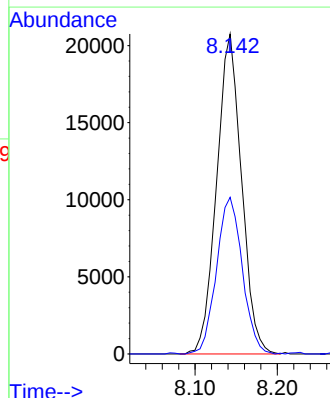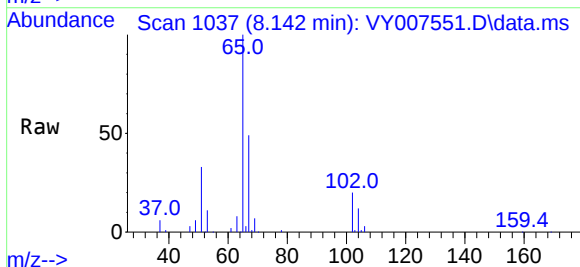



#34

1,4-Difluorobenzene

Concen: 50.000 ug/l

RT: 8.691 min Scan# 1127

Delta R.T. -0.000 min

Lab File: VY007551.D

Acq: 18 Feb 2022 17:38

Instrument :

MSVOA_Y

ClientSampleId :

C0AA4





Tgt Ion:114 Resp: 120659

Ion Ratio Lower Upper

114 100

63 17.6 0.0 43.2

88 14.6 0.0 31.8

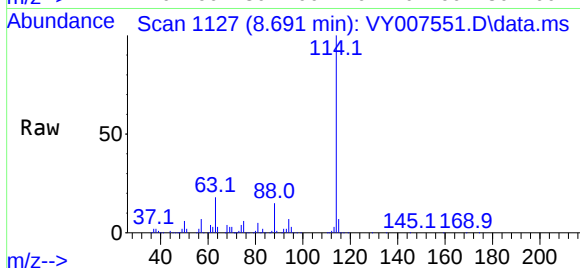

#35

Dibromofluoromethane

Concen: 52.729 ug/l

RT: 7.722 min Scan# 968

Delta R.T. -0.000 min

Lab File: VY007551.D

Acq: 18 Feb 2022 17:38




Tgt Ion:113 Resp: 40122


Ion Ratio Lower Upper

113 100

111 103.4 82.6 124.0

192 20.0 17.6 26.4


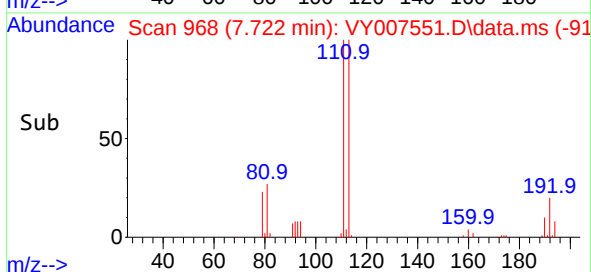

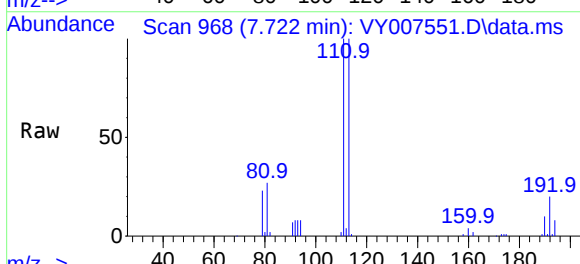


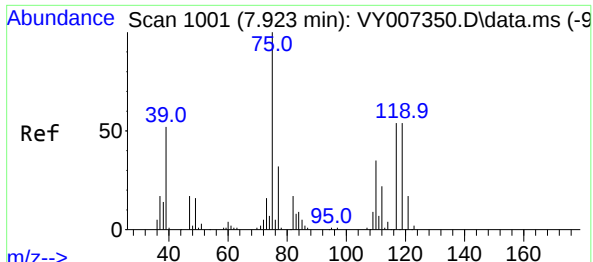

#36
1,1-Dichloropropene
Concen: 4.507 ug/l
RT: 7.789 min Scan# 91
Delta R.T. -0.134 min
Lab File: VY007551.D
Acq: 18 Feb 2022 17:38




Instrument :
MSVOA_Y
ClientSampleId :
C0AA4


Tgt Ion: 75 Resp: 5556
Ion Ratio Lower Upper
75 100
110 9.8 17.1 51.2#
77 0.0 24.4 36.6#

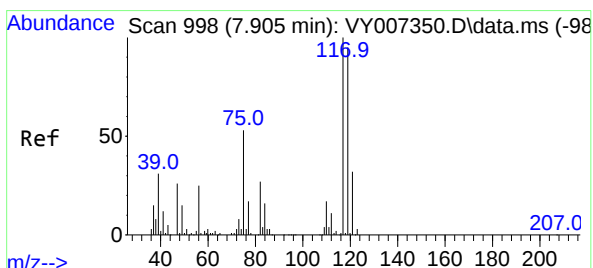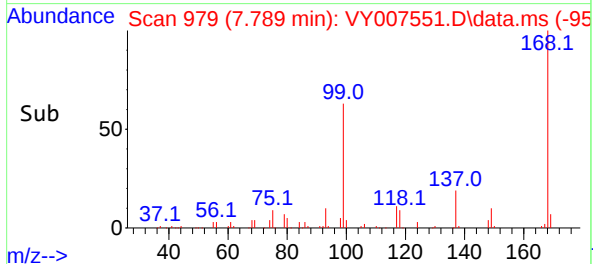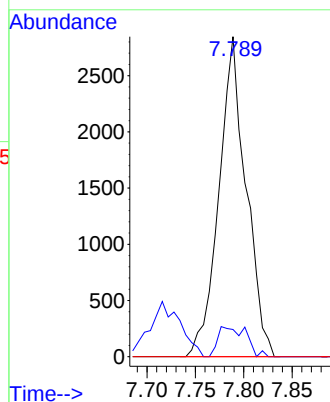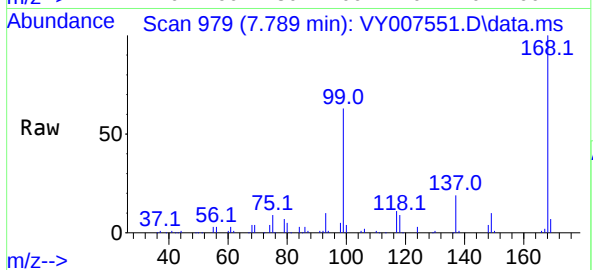

#38
Carbon Tetrachloride
Concen: 5.415 ug/l
RT: 7.789 min Scan# 979
Delta R.T. -0.116 min
Lab File: VY007551.D
Acq: 18 Feb 2022 17:38

Tgt Ion: 117 Resp: 7585
Ion Ratio Lower Upper
117 100
119 4.0 77.9 116.9#
121 0.0 24.8 37.2#

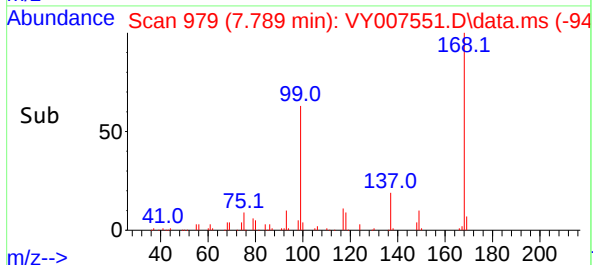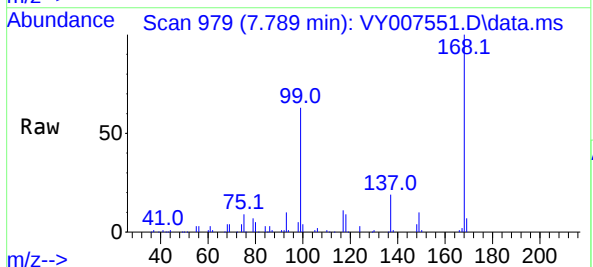

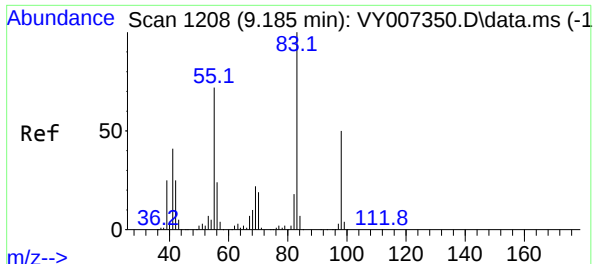

#39

Methylcyclohexane

Concen: 4.807 ug/l

RT: 9.185 min Scan# 11

Delta R.T. -0.000 min

Lab File: VY007551.D

Acq: 18 Feb 2022 17:38

Instrument :

MSVOA_Y

ClientSampleId :

C0AA4





Tgt Ion: 83 Resp: 7694

Ion Ratio Lower Upper

83 100

55 61.1 66.5 99.7#

98 52.2 37.9 56.9

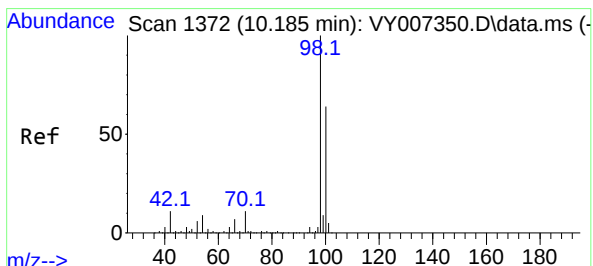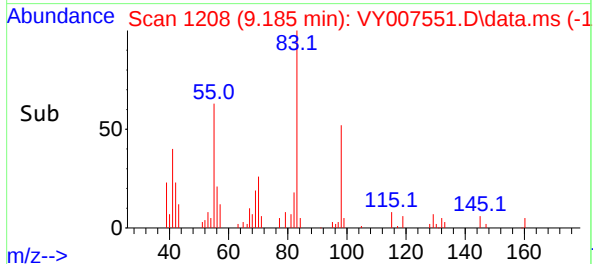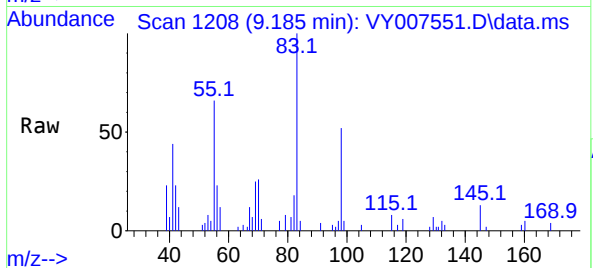

#50

Toluene-d8

Concen: 51.236 ug/l

RT: 10.179 min Scan# 1371

Delta R.T. -0.006 min

Lab File: VY007551.D




Acq: 18 Feb 2022 17:38


Tgt Ion: 98 Resp: 148073

Ion Ratio Lower Upper

98 100

100 63.7 50.2 75.2


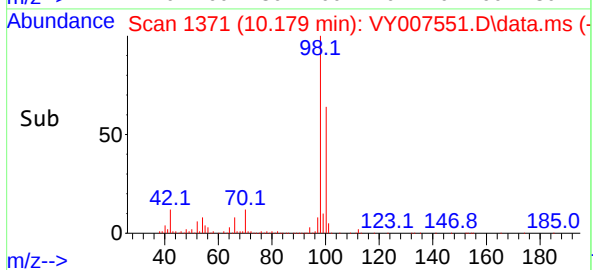

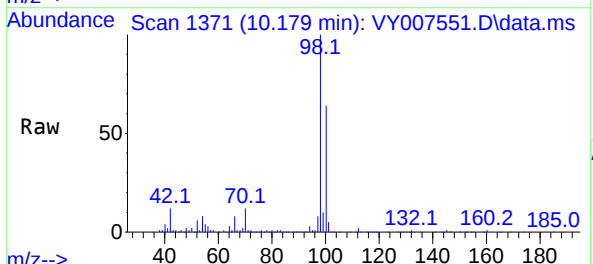




#55
1,1,2-Trichloroethane
Concen: 10.464 ug/l
RT: 10.618 min Scan# 1443
Delta R.T. -0.030 min
Lab File: VY007551.D
Acq: 18 Feb 2022 17:38




Instrument :
MSVOA_Y
ClientSampleId :
C0AA4


Tgt Ion: 97	Resp: 6946
Ion Ratio	Lower Upper
97 100	
83 9.0	69.8 104.8#
85 1.8	44.3 66.5#
99 0.0	49.8 74.6#

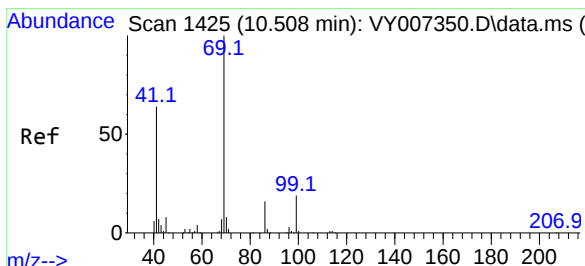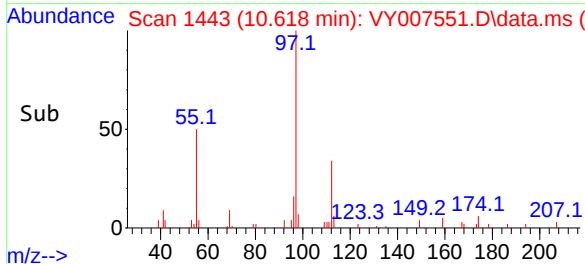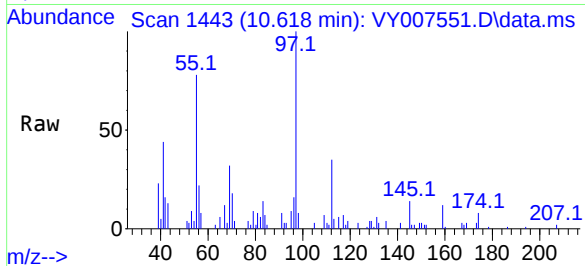

#56
Ethyl methacrylate
Concen: 1.809 ug/l
RT: 10.514 min Scan# 1426
Delta R.T. 0.006 min
Lab File: VY007551.D
Acq: 18 Feb 2022 17:38

Tgt Ion: 69	Resp: 1615		
Ion Ratio	Lower	Upper	
69 100			
41 105.7	63.4	95.0#	
39 56.2	35.8	53.8#	


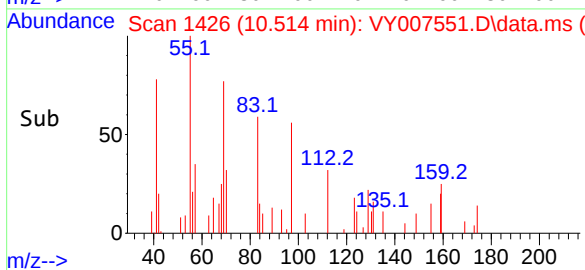

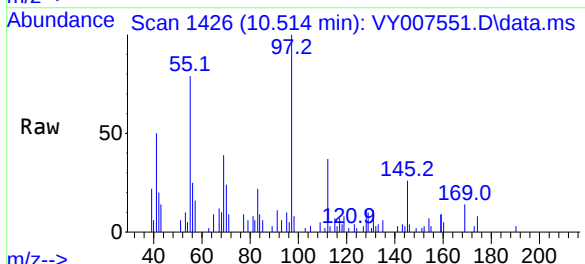




#59
2-Hexanone
Concen: 10.618 ug/l
RT: 10.801 min Scan# 1478
Delta R.T. -0.030 min
Lab File: VY007551.D
Acq: 18 Feb 2022 17:38




Instrument :
MSVOA_Y
ClientSampleId :
C0AA4


Tgt Ion: 43 Resp: 4307
Ion Ratio Lower Upper
43 100
58 2.1 24.4 73.4#

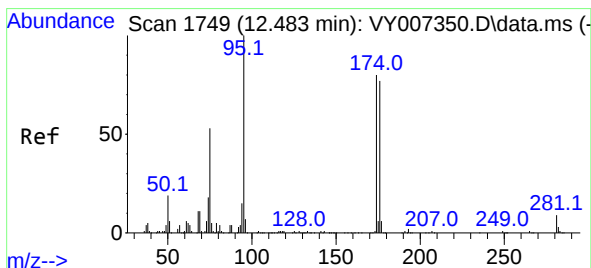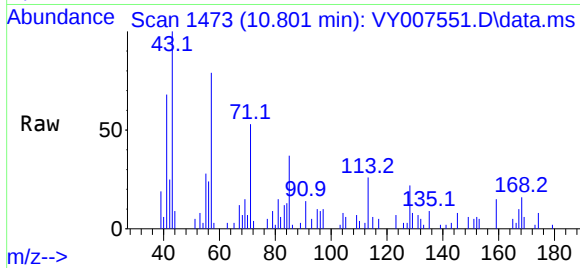

#62
4-Bromofluorobenzene
Concen: 52.760 ug/l
RT: 12.477 min Scan# 1748
Delta R.T. -0.006 min
Lab File: VY007551.D
Acq: 18 Feb 2022 17:38

Tgt Ion: 95 Resp: 51702
Ion Ratio Lower Upper
95 100
174 83.5 0.0 177.0
176 79.9 0.0 175.8

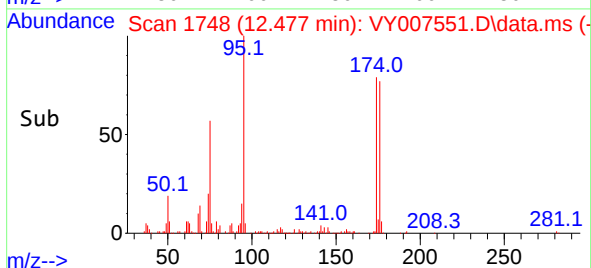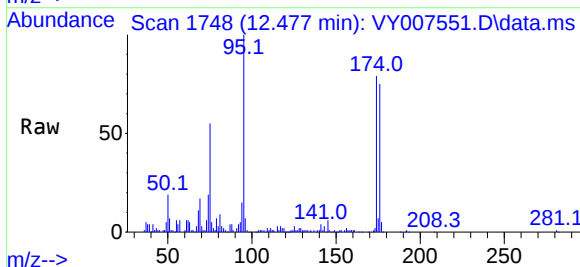



#63

Chlorobenzene-d5

Concen: 50.000 ug/l

RT: 11.489 min Scan# 11

Delta R.T. -0.000 min

Lab File: VY007551.D

Acq: 18 Feb 2022 17:38

Instrument :

MSVOA_Y

ClientSampleId :

C0AA4





Tgt Ion:117 Resp: 116872

Ion Ratio Lower Upper

117 100

82 53.0 43.0 64.4

119 32.7 25.4 38.0

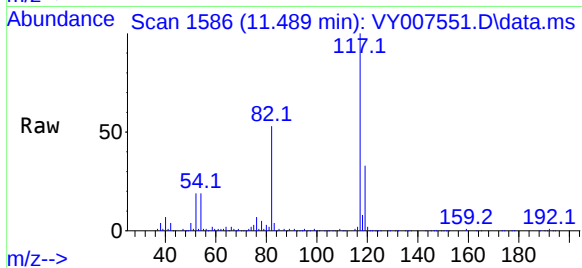

#66

1,1,1,2-Tetrachloroethane

Concen: 1.235 ug/l

RT: 11.599 min Scan# 1604

Delta R.T. 0.006 min

Lab File: VY007551.D

Acq: 18 Feb 2022 17:38




Tgt Ion:131 Resp: 1194


Ion Ratio Lower Upper

131 100

133 0.0 47.9 143.6#

119 0.0 30.8 92.3#

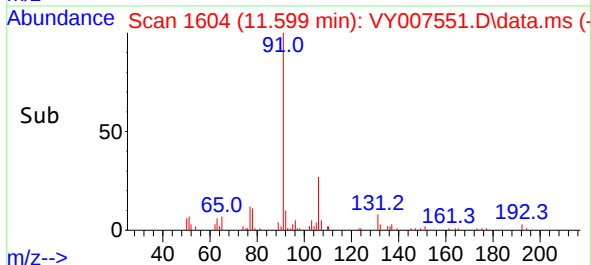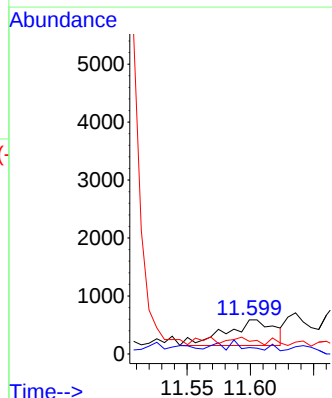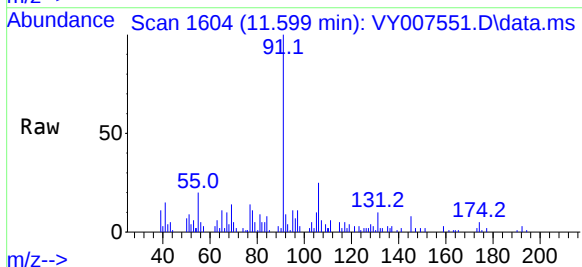



#67

Ethyl Benzene

Concen: 2.443 ug/l

RT: 11.593 min Scan# 1

Delta R.T. 0.000 min

Lab File: VY007551.D

Acq: 18 Feb 2022 17:38

Instrument :

MSVOA_Y

ClientSampleId :





C0AA4

Tgt Ion: 91 Resp: 11705

Ion Ratio Lower Upper

91 100

106 32.4 24.5 36.7

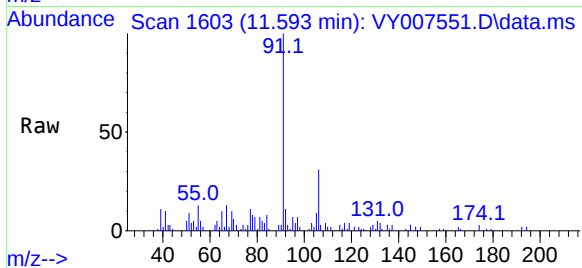

#68

m/p-Xylenes

Concen: 4.392 ug/l

RT: 11.697 min Scan# 1620

Delta R.T. -0.006 min

Lab File: VY007551.D




Acq: 18 Feb 2022 17:38


Tgt Ion:106 Resp: 7963

Ion Ratio Lower Upper

106 100

91 194.0 166.6 249.8


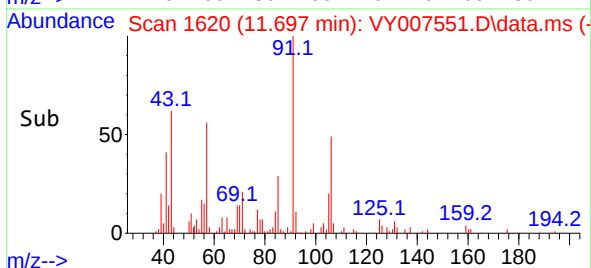
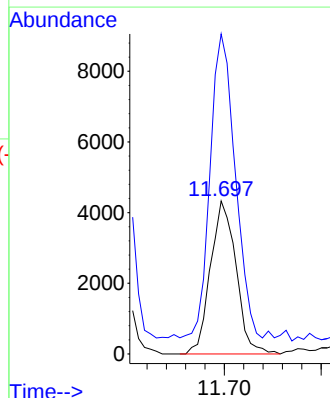
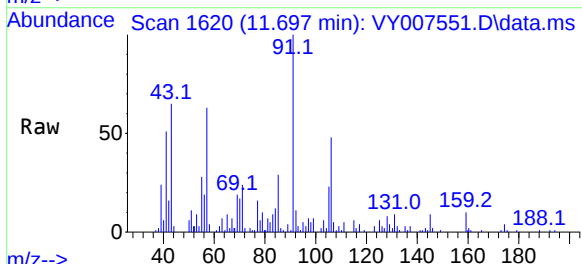




#69
o-Xylene
Concen: 7.776 ug/l
RT: 12.026 min Scan# 11
Delta R.T. -0.006 min
Lab File: VY007551.D
Acq: 18 Feb 2022 17:38




Instrument :
MSVOA_Y
ClientSampleId :
C0AA4


Tgt Ion:106 Resp: 13340
Ion Ratio Lower Upper
106 100
91 225.2 110.3 331.0

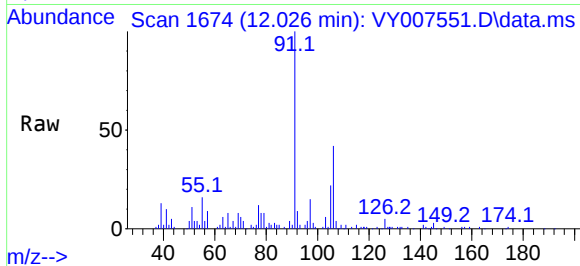

#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 13.428 min Scan# 1904
Delta R.T. 0.006 min
Lab File: VY007551.D
Acq: 18 Feb 2022 17:38

Tgt Ion:152 Resp: 47858
Ion Ratio Lower Upper
152 100
115 65.0 28.2 84.7
150 156.8 0.0 347.6


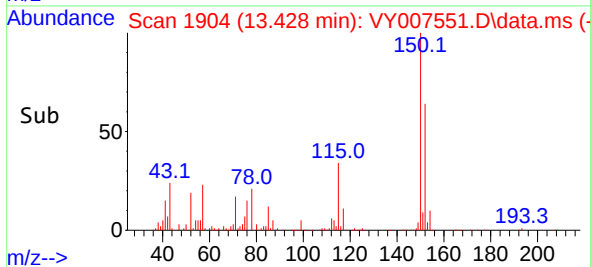

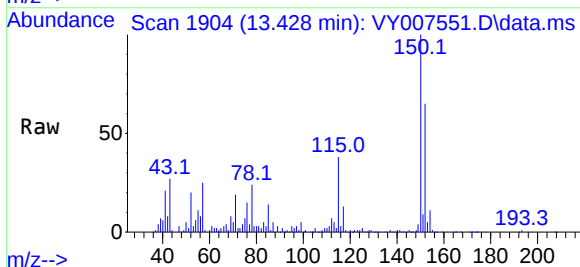




#73
Isopropylbenzene
Concen: 1.956 ug/l
RT: 12.331 min Scan# 1724
Delta R.T. -0.000 min
Lab File: VY007551.D
Acq: 18 Feb 2022 17:38




Instrument :
MSVOA_Y
ClientSampleId :
C0AA4


Tgt Ion:105 Resp: 8294
Ion Ratio Lower Upper
105 100
120 30.9 13.4 40.2

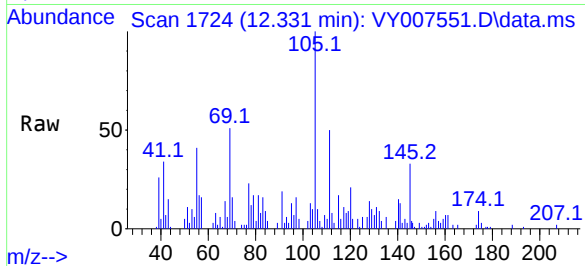

#75
1,1,2,2-Tetrachloroethane
Concen: 1.049 ug/l
RT: 12.532 min Scan# 1757
Delta R.T. -0.049 min
Lab File: VY007551.D
Acq: 18 Feb 2022 17:38

Tgt Ion: 83 Resp: 762
Ion Ratio Lower Upper
83 100
131 20.5 5.6 16.8#
85 113.0 32.3 96.8#


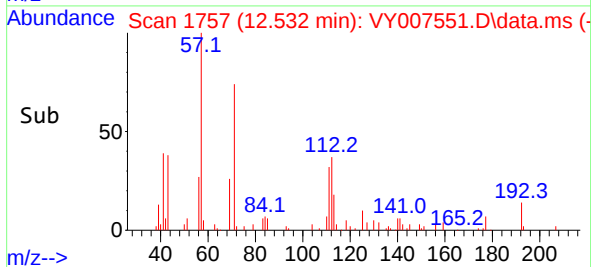

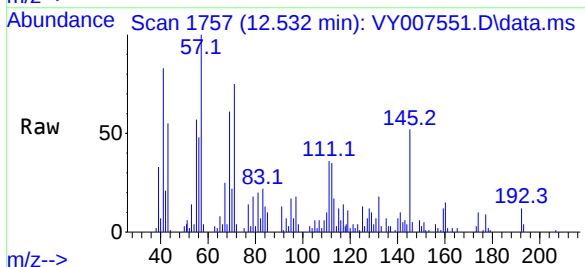




#76
1,2,3-Trichloropropane
Concen: 52.111 ug/l
RT: 12.477 min Scan# 1774
Delta R.T. -0.159 min
Lab File: VY007551.D
Acq: 18 Feb 2022 17:38




Instrument :
MSVOA_Y
ClientSampleId :
C0AA4


Tgt Ion: 75 Resp: 28816
Ion Ratio Lower Upper
75 100
77 0.9 0.0 0.0#

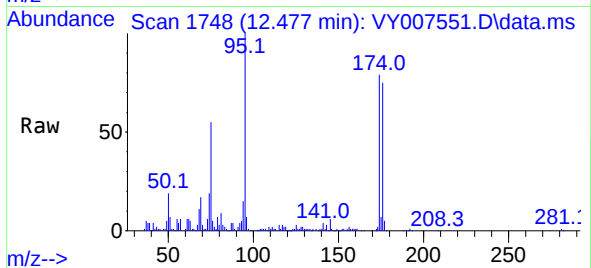

#78
n-propylbenzene
Concen: 2.506 ug/l
RT: 12.666 min Scan# 1779
Delta R.T. -0.006 min
Lab File: VY007551.D
Acq: 18 Feb 2022 17:38

Tgt Ion: 91 Resp: 12783
Ion Ratio Lower Upper
91 100
120 25.1 11.3 33.9

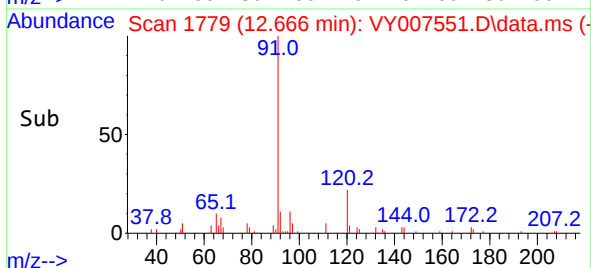



#79

2-Chlorotoluene

Concen: 1.581 ug/l

RT: 12.733 min Scan# 1

Delta R.T. -0.025 min

Lab File: VY007551.D

Acq: 18 Feb 2022 17:38

Instrument :

MSVOA_Y

ClientSampleId :





C0AA4

Tgt Ion: 91 Resp: 4447

Ion Ratio Lower Upper

91 100

126 1.5 16.9 50.6#

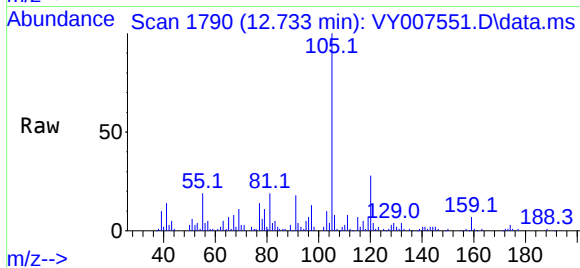

#80

1,3,5-Trimethylbenzene

Concen: 8.071 ug/l

RT: 12.812 min Scan# 1803

Delta R.T. 0.000 min

Lab File: VY007551.D




Acq: 18 Feb 2022 17:38


Tgt Ion: 105 Resp: 28344

Ion Ratio Lower Upper

105 100

120 46.2 24.4 73.4


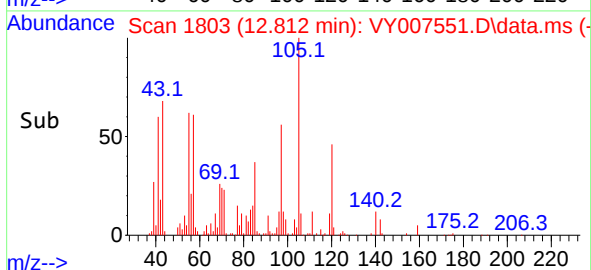

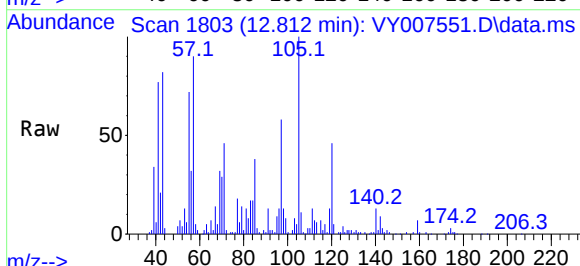




#81
trans-1,4-Dichloro-2-butene
Concen: 108.310 ug/l
RT: 12.477 min Scan# 11
Delta R.T. 0.097 min
Lab File: VY007551.D
Acq: 18 Feb 2022 17:38




Instrument :
MSVOA_Y
ClientSampleId :
C0AA4


Tgt Ion: 75 Resp: 28816
Ion Ratio Lower Upper
75 100
53 0.9 85.3 127.9#
89 1.0 37.0 55.4#



#82
4-Chlorotoluene
Concen: 1.243 ug/l
RT: 12.806 min Scan# 1802
Delta R.T. -0.049 min
Lab File: VY007551.D
Acq: 18 Feb 2022 17:38

Tgt Ion: 91 Resp: 3584
Ion Ratio Lower Upper
91 100
126 13.1 17.0 51.0#


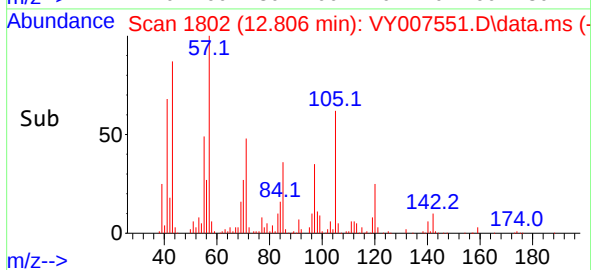






#83
tert-Butylbenzene
Concen: 1.498 ug/l
RT: 13.123 min Scan# 1854
Delta R.T. 0.048 min
Lab File: VY007551.D
Acq: 18 Feb 2022 17:38




Instrument :
MSVOA_Y
ClientSampleId :
C0AA4


Tgt Ion:119 Resp: 4597
Ion Ratio Lower Upper
119 100
91 90.8 34.8 104.4
134 0.0 13.3 39.9#

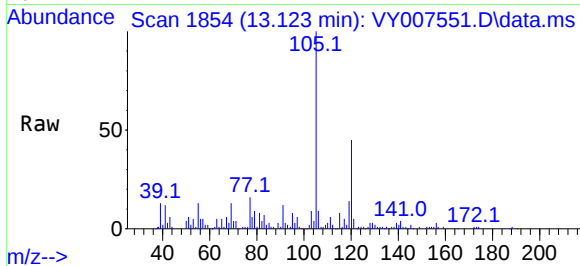

#84
1,2,4-Trimethylbenzene
Concen: 10.227 ug/l
RT: 13.117 min Scan# 1853
Delta R.T. 0.000 min
Lab File: VY007551.D
Acq: 18 Feb 2022 17:38

Tgt Ion:105 Resp: 34825
Ion Ratio Lower Upper
105 100
120 44.2 22.3 66.9


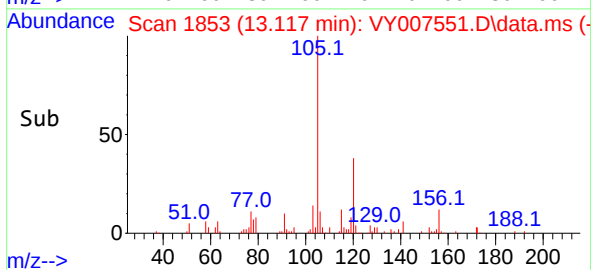

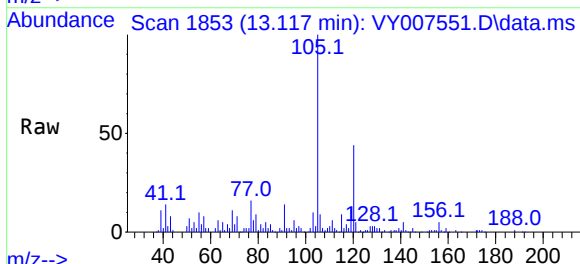




#85
 sec-Butylbenzene
 Concen: 2.423 ug/l
 RT: 13.251 min Scan# 1875
 Delta R.T. 0.000 min
 Lab File: VY007551.D
 Acq: 18 Feb 2022 17:38




Instrument :
 MSVOA_Y
 ClientSampleId :
 C0AA4


Tgt Ion:105 Resp: 10962
 Ion Ratio Lower Upper
 105 100
 134 27.7 10.2 30.4

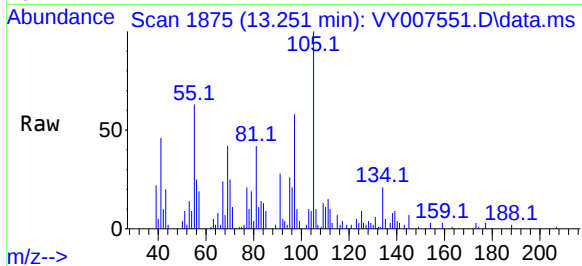

#86
 p-Isopropyltoluene
 Concen: 1.129 ug/l
 RT: 13.367 min Scan# 1894
 Delta R.T. 0.000 min
 Lab File: VY007551.D
 Acq: 18 Feb 2022 17:38

Tgt Ion:119 Resp: 4209
 Ion Ratio Lower Upper
 119 100
 134 28.2 13.2 39.5
 91 29.2 12.4 37.2


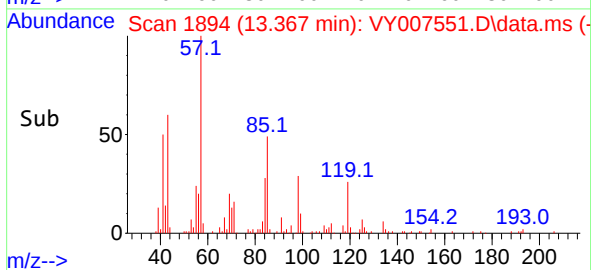

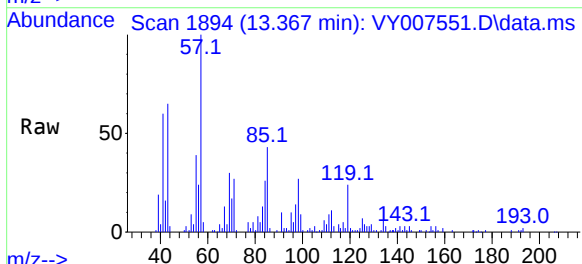




#89
n-Butylbenzene
Concen: 1.772 ug/l
RT: 13.696 min Scan# 1948
Delta R.T. 0.000 min
Lab File: VY007551.D
Acq: 18 Feb 2022 17:38




Instrument :
MSVOA_Y
ClientSampleId :
C0AA4


Tgt Ion: 91 Resp: 6281
Ion Ratio Lower Upper
91 100
92 87.5 26.3 78.9#
134 0.0 13.0 38.9#

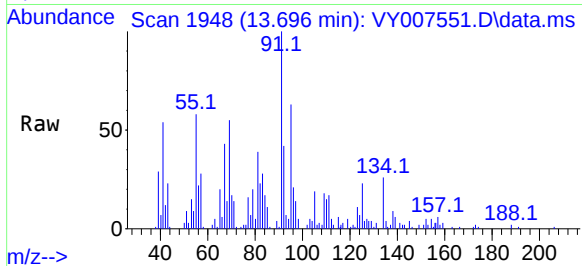

#90
Hexachloroethane
Concen: 7.821 ug/l
RT: 13.971 min Scan# 1993
Delta R.T. 0.012 min
Lab File: VY007551.D
Acq: 18 Feb 2022 17:38

Tgt Ion: 117 Resp: 5570
Ion Ratio Lower Upper
117 100
201 0.0 43.0 128.8#


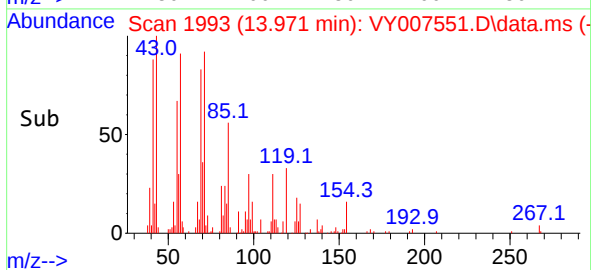

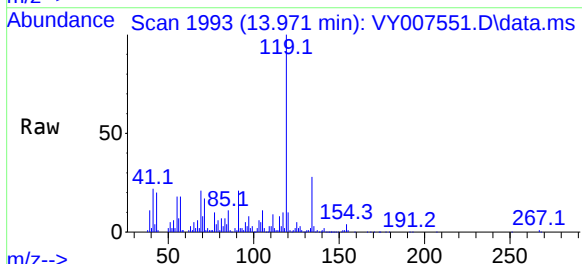




#92
1,2-Dibromo-3-Chloropropane
Concen: 4.810 ug/l
RT: 14.336 min Scan# 2053
Delta R.T. -0.019 min
Lab File: VY007551.D
Acq: 18 Feb 2022 17:38




Instrument :
MSVOA_Y
ClientSampleId :
C0AA4


Tgt Ion: 75 Resp: 593
Ion Ratio Lower Upper
75 100
155 0.0 38.0 113.9#
157 0.0 47.8 143.3#

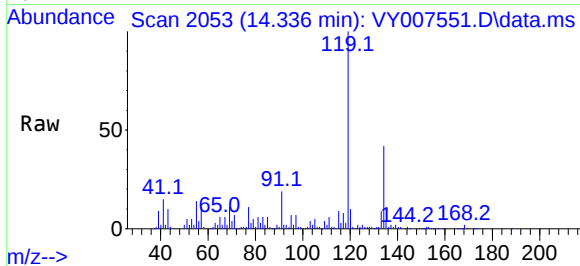

#95
Naphthalene
Concen: 2.014 ug/l
RT: 15.202 min Scan# 2195
Delta R.T. -0.031 min
Lab File: VY007551.D
Acq: 18 Feb 2022 17:38


Tgt Ion: 128 Resp: 4100
Ion Ratio Lower Upper
128 100
127 107.6 11.0 16.4#
129 111.2 8.4 12.6#

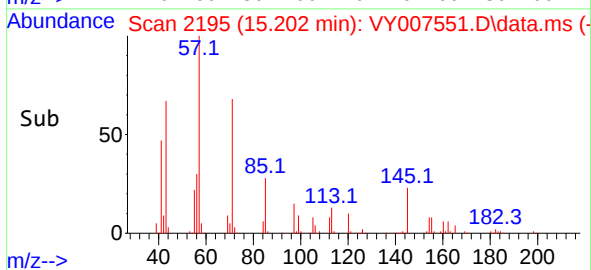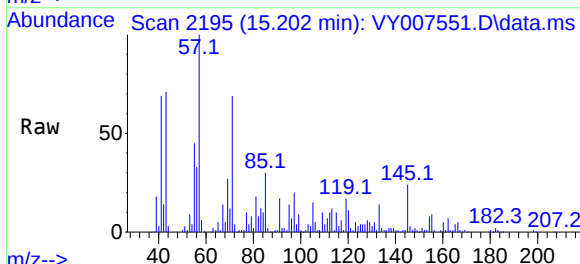



#96
 1,2,3-Trichlorobenzene
 Concen: 3.630 ug/l
 RT: 15.446 min Scan# 21
 Delta R.T. 0.024 min
 Lab File: VY007551.D
 Acq: 18 Feb 2022 17:38

Instrument :
 MSVOA_Y
 ClientSampleId :
 C0AA4

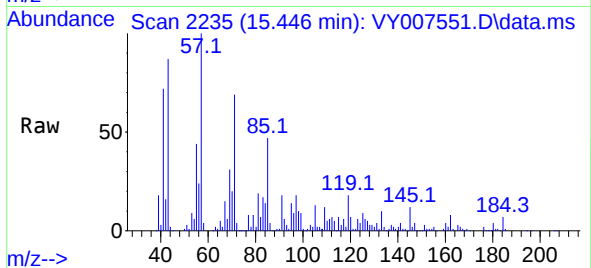

Tgt Ion:180 Resp: 2934
 Ion Ratio Lower Upper
 180 100
 182 0.0 47.3 141.9#
 145 1152.3 15.3 45.9#

