

Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY021925\
 Data File : VY021244.D
 Acq On : 19 Feb 2025 18:09
 Operator : SY/MD
 Sample : Q1382-05
 Misc : 5.42g/5.0mL/MSVOA_Y/SOIL/A
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_Y
 ClientSampleId :
 OU4-PCS-TC-03-021725

Quant Time: Feb 20 00:21:41 2025
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y020325S.M
 Quant Title : SW846 8260
 QLast Update : Mon Feb 03 13:08:38 2025
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Pentafluorobenzene	7.713	168	207032	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	8.622	114	397674	50.000	ug/l	0.00
63) Chlorobenzene-d5	11.420	117	367484	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.353	152	147214	50.000	ug/l	0.00

System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.067	65	129525	61.062	ug/l	0.00
Spiked Amount	50.000	Range	50 - 163	Recovery	=	122.120%
35) Dibromofluoromethane	7.640	113	130403	51.167	ug/l	0.00
Spiked Amount	50.000	Range	54 - 147	Recovery	=	102.340%
50) Toluene-d8	10.109	98	483051	49.786	ug/l	0.00
Spiked Amount	50.000	Range	58 - 134	Recovery	=	99.580%
62) 4-Bromofluorobenzene	12.414	95	160823	50.736	ug/l	0.00
Spiked Amount	50.000	Range	30 - 143	Recovery	=	101.480%


Target Compounds	Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY021925\
Data File : VY021244.D
Acq On : 19 Feb 2025 18:09
Operator : SY/MD
Sample : Q1382-05
Misc : 5.42g/5.0mL/MSVOA_Y/SOIL/A
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_Y
ClientSampleId :
OU4-PCS-TC-03-021725

Quant Time: Feb 20 00:21:41 2025
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y020325S.M
Quant Title : SW846 8260
QLast Update : Mon Feb 03 13:08:38 2025
Response via : Initial Calibration




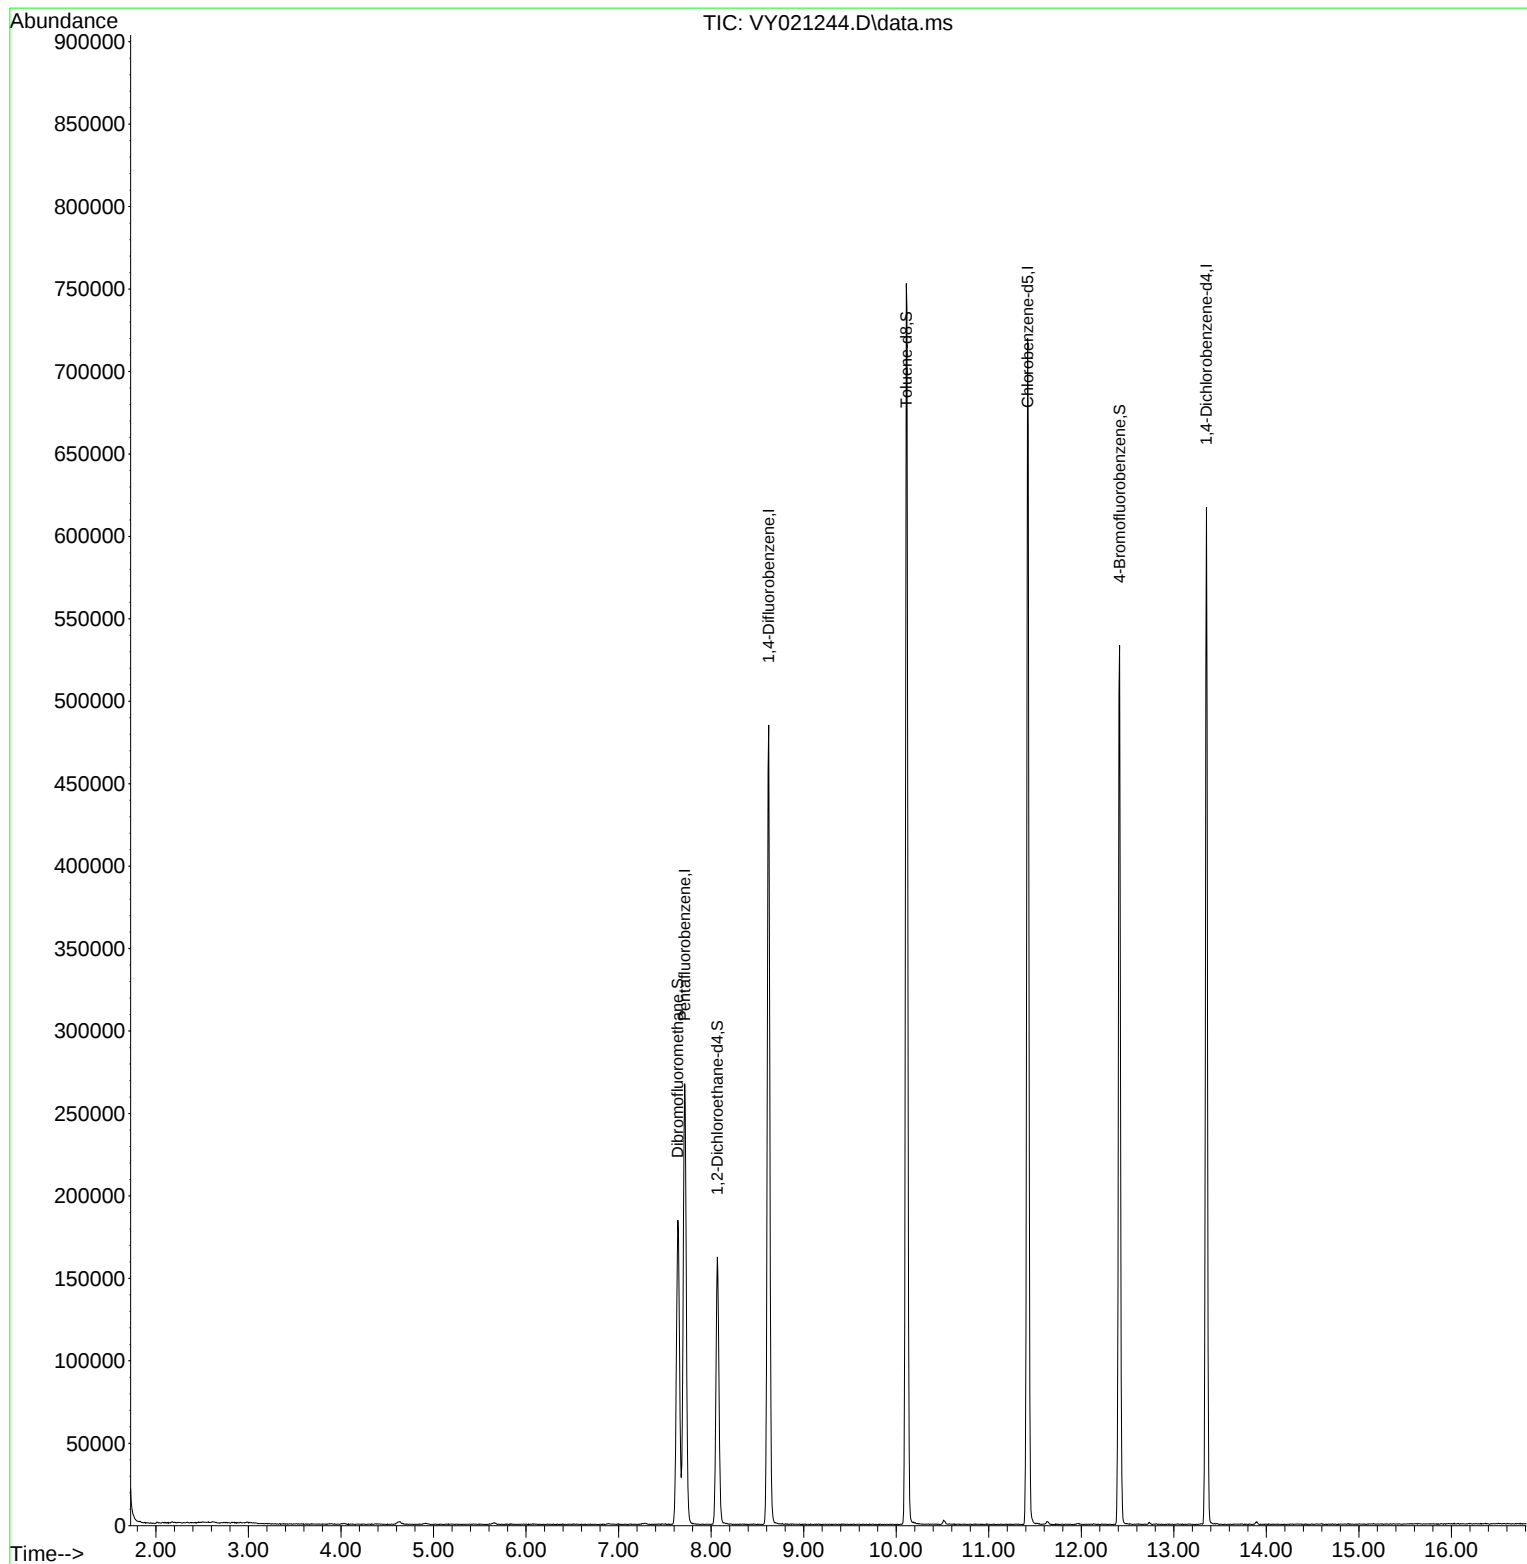




#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 7.713 min Scan# 91
Delta R.T. 0.000 min
Lab File: VY021244.D
Acq: 19 Feb 2025 18:09




Instrument :
MSVOA_Y
ClientSampleId :
OU4-PCS-TC-03-021725


Tgt Ion:168 Resp: 207032
Ion Ratio Lower Upper
168 100
99 56.4 44.2 66.4

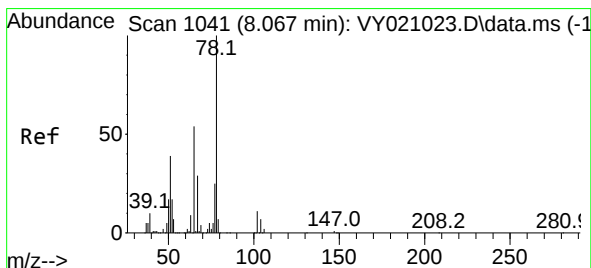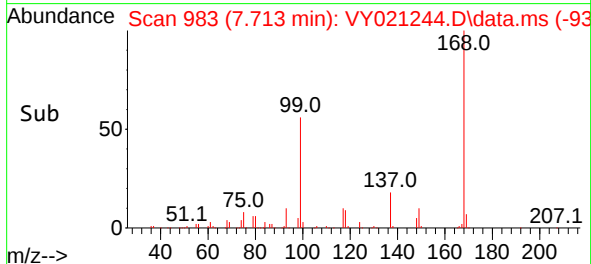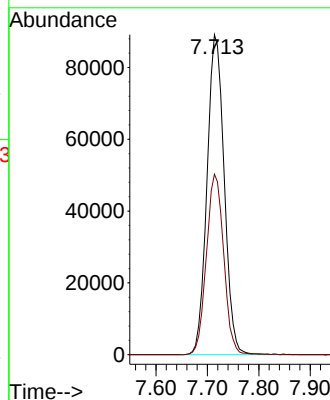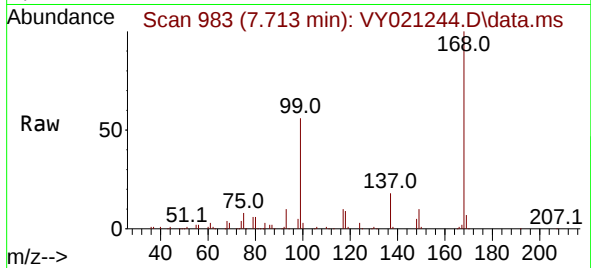

#33
1,2-Dichloroethane-d4
Concen: 61.062 ug/l
RT: 8.067 min Scan# 1041
Delta R.T. 0.000 min
Lab File: VY021244.D
Acq: 19 Feb 2025 18:09

Tgt Ion: 65 Resp: 129525
Ion Ratio Lower Upper
65 100
67 51.8 0.0 109.0


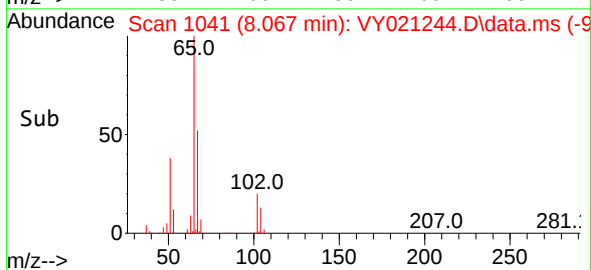
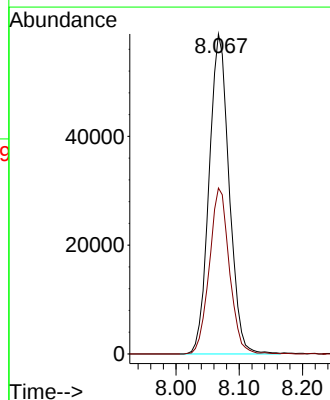
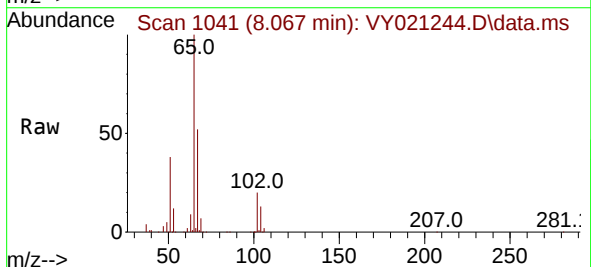


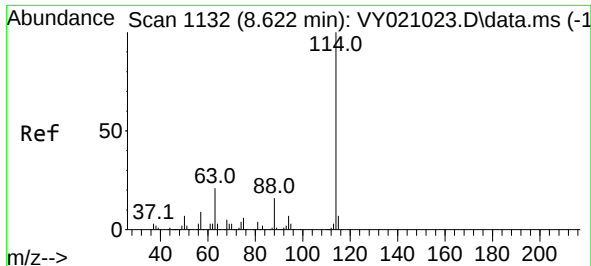

#34
 1,4-Difluorobenzene
 Concen: 50.000 ug/l
 RT: 8.622 min Scan# 1132
 Delta R.T. 0.000 min
 Lab File: VY021244.D
 Acq: 19 Feb 2025 18:09




Instrument :
 MSVOA_Y
 ClientSampleId :
 OU4-PCS-TC-03-021725

Tgt Ion:114 Resp: 397674
 Ion Ratio Lower Upper
 114 100
 63 19.7 0.0 37.4
 88 15.5 0.0 29.0

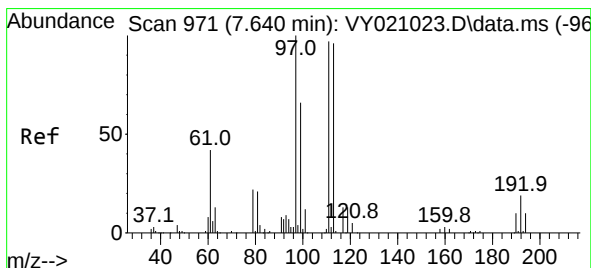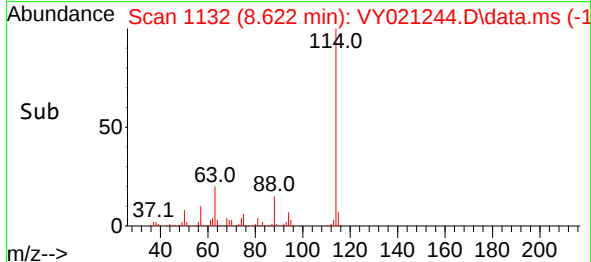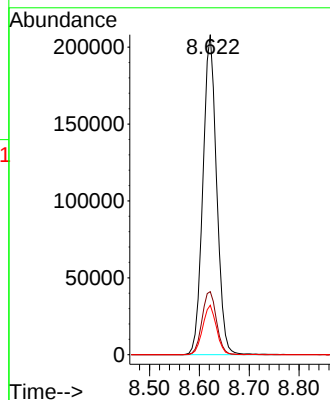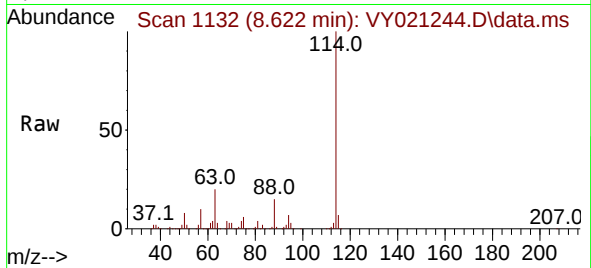

#35
 Dibromofluoromethane
 Concen: 51.167 ug/l
 RT: 7.640 min Scan# 971
 Delta R.T. 0.000 min
 Lab File: VY021244.D
 Acq: 19 Feb 2025 18:09

Tgt Ion:113 Resp: 130403
 Ion Ratio Lower Upper
 113 100
 111 102.9 83.8 125.6
 192 19.5 14.5 21.7

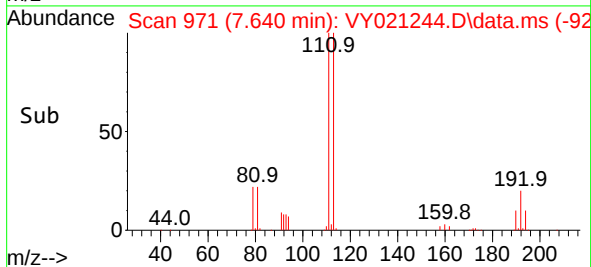
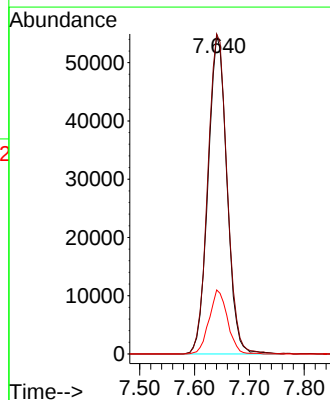
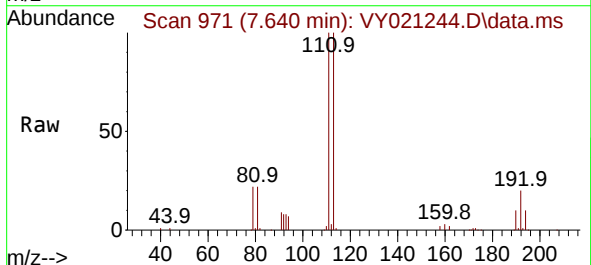




#50
Toluene-d8
Concen: 49.786 ug/l
RT: 10.109 min Scan# 1376
Delta R.T. 0.000 min
Lab File: VY021244.D
Acq: 19 Feb 2025 18:09




Instrument :
MSVOA_Y
ClientSampleId :
OU4-PCS-TC-03-021725


Tgt Ion: 98 Resp: 483051
Ion Ratio Lower Upper
98 100
100 64.4 52.3 78.5

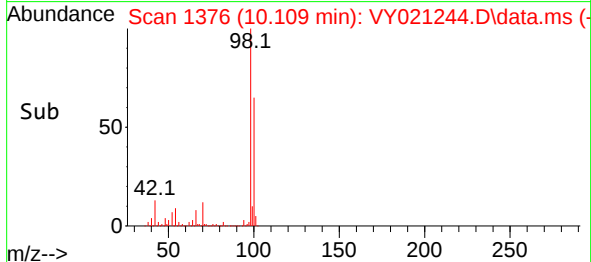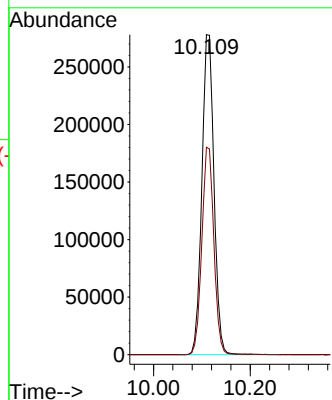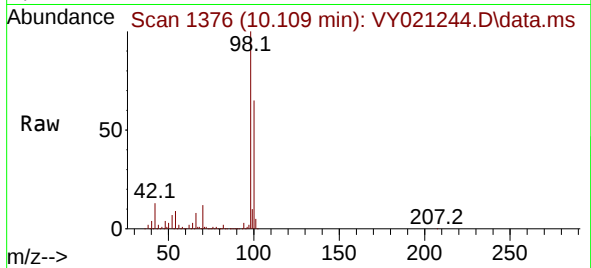

#62
4-Bromofluorobenzene
Concen: 50.736 ug/l
RT: 12.414 min Scan# 1754
Delta R.T. 0.000 min
Lab File: VY021244.D
Acq: 19 Feb 2025 18:09

Tgt Ion: 95 Resp: 160823
Ion Ratio Lower Upper
95 100
174 83.9 0.0 160.0
176 80.2 0.0 151.8

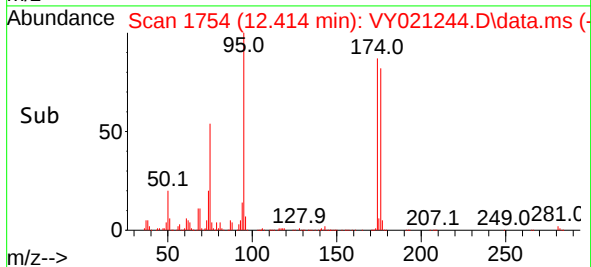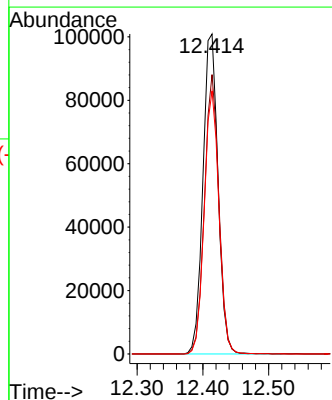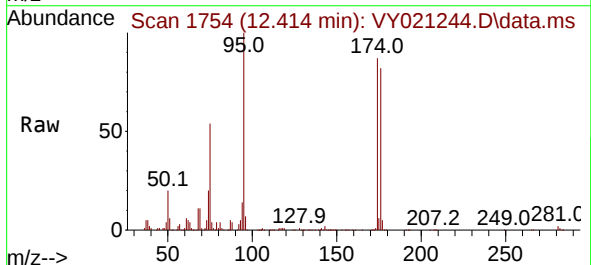

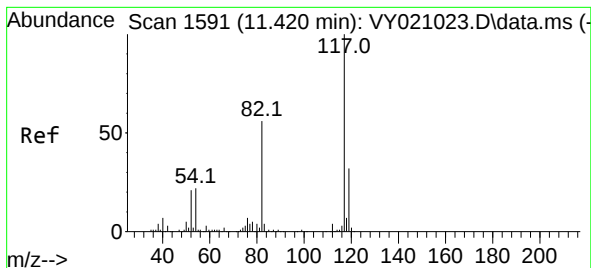

#63

Chlorobenzene-d5

Concen: 50.000 ug/l

RT: 11.420 min Scan# 11

Delta R.T. -0.000 min

Lab File: VY021244.D

Acq: 19 Feb 2025 18:09

Instrument :

MSVOA_Y

ClientSampleId :

OU4-PCS-TC-03-021725





Tgt Ion:117 Resp: 367484

Ion Ratio Lower Upper

117 100

82 57.4 43.8 65.8

119 32.4 26.5 39.7

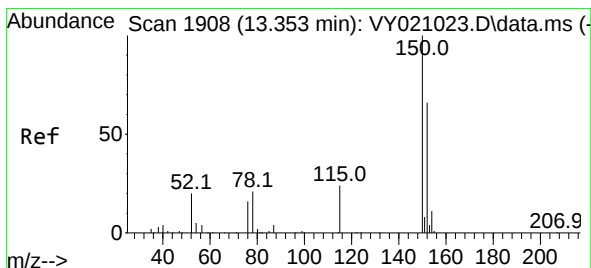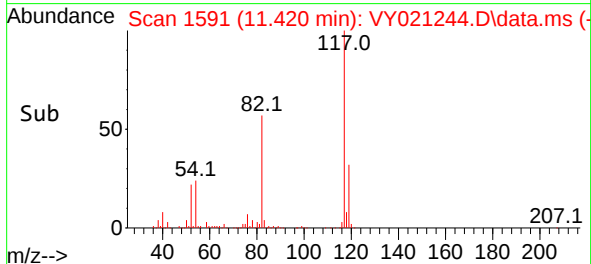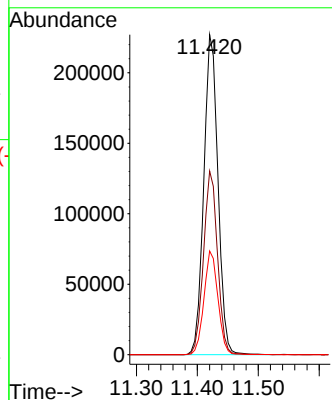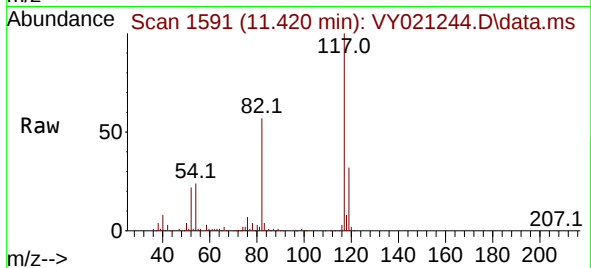

#72

1,4-Dichlorobenzene-d4

Concen: 50.000 ug/l

RT: 13.353 min Scan# 1908

Delta R.T. 0.000 min

Lab File: VY021244.D

Acq: 19 Feb 2025 18:09

Tgt Ion:152 Resp: 147214

Ion Ratio Lower Upper

152 100

115 58.6 30.0 90.0

150 155.9 0.0 344.6

