
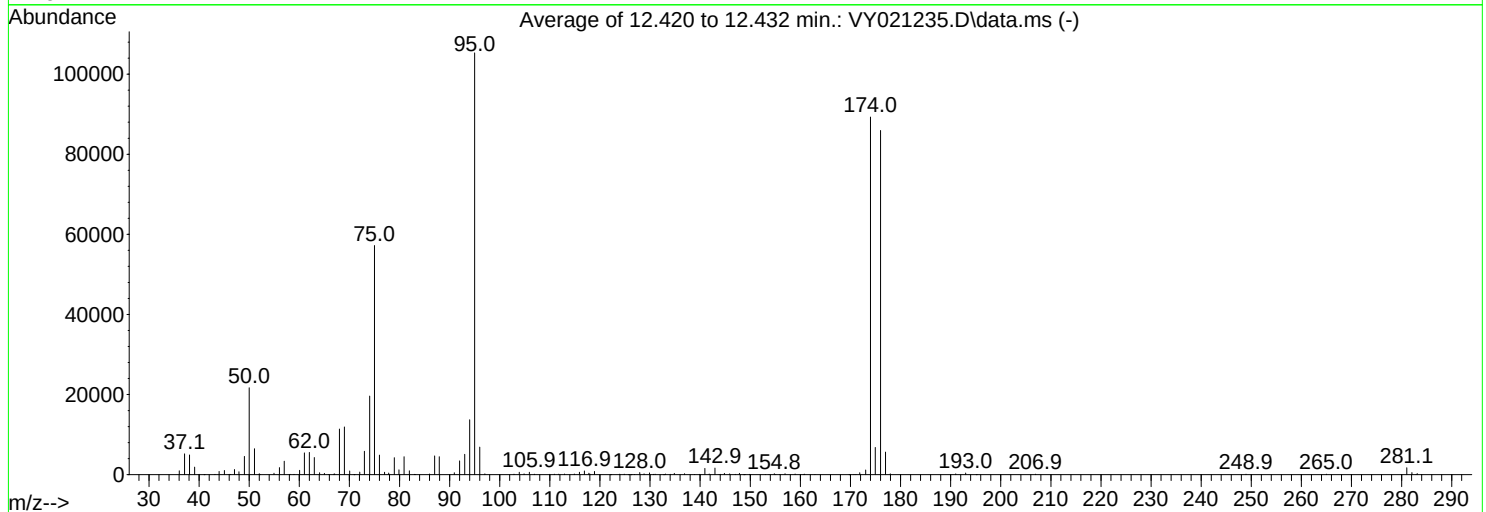


Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY021925\
Data File : VY021235.D
Acq On : 19 Feb 2025 09:09
Operator : SY/MD
Sample : BFB
Misc : 5.00g/5.0mL/MSVOA_Y/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_Y
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y020325S.M
Title : SW846 8260
Last Update : Mon Feb 03 13:08:38 2025

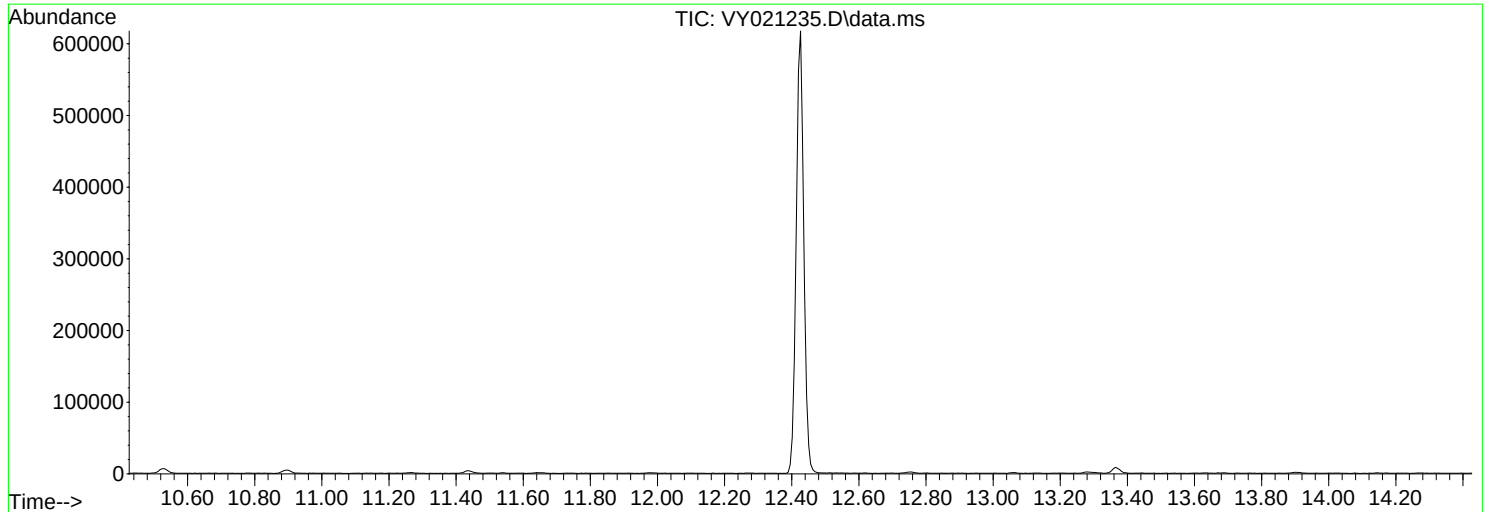

AutoFind: Scans 1755, 1756, 1757; Background Corrected with Scan 1747

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	20.6	21704	PASS
75	95	30	60	54.3	57235	PASS
95	95	100	100	100.0	105325	PASS
96	95	5	9	6.5	6876	PASS
173	174	0.00	2	1.3	1142	PASS
174	95	50	100	84.8	89280	PASS
175	174	5	9	7.6	6780	PASS
176	174	95	101	96.3	85939	PASS
177	176	5	9	6.6	5654	PASS