
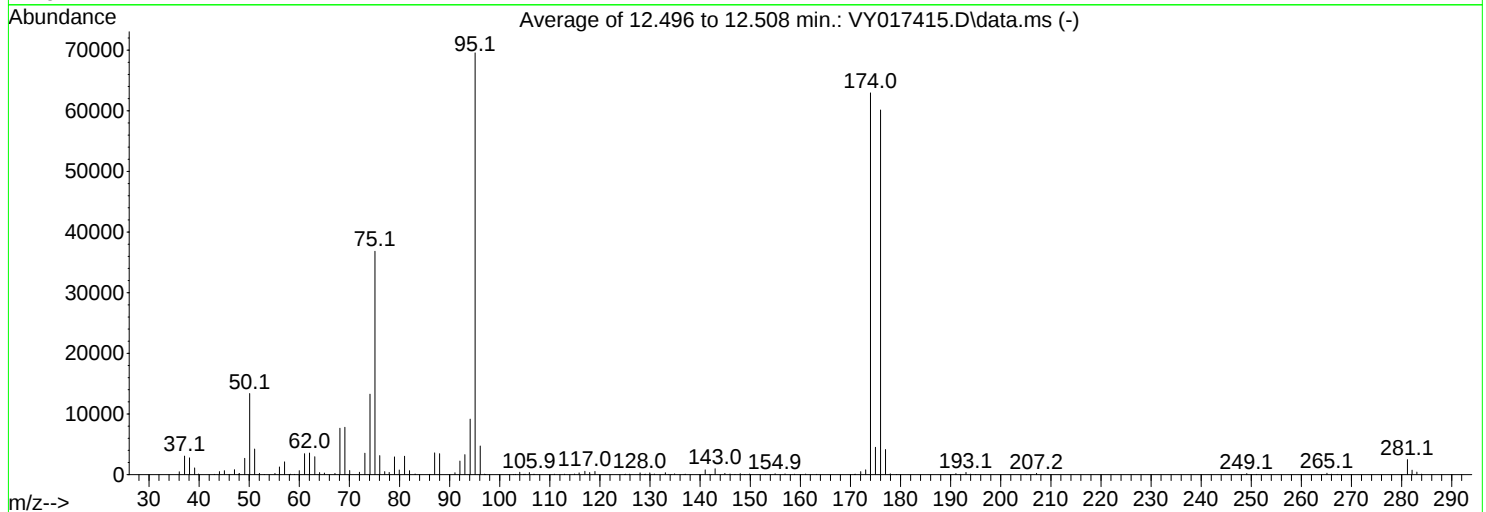


Data Path : Z:\voasrv\HPCHEM1\MSVOA\_Y\Data\VY022024\  
Data File : VY017415.D  
Acq On : 20 Feb 2024 08:46  
Operator : SY/MD  
Sample : BFB  
Misc : 5.00g/5.0mL/MSVOA\_Y/SOIL  
ALS Vial : 1 Sample Multiplier: 1

Instrument :  
MSVOA\_Y  
ClientSampleId :  
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA\_Y\methods\82Y021924S.M  
Title : SW846 8260  
Last Update : Tue Feb 20 06:16:24 2024

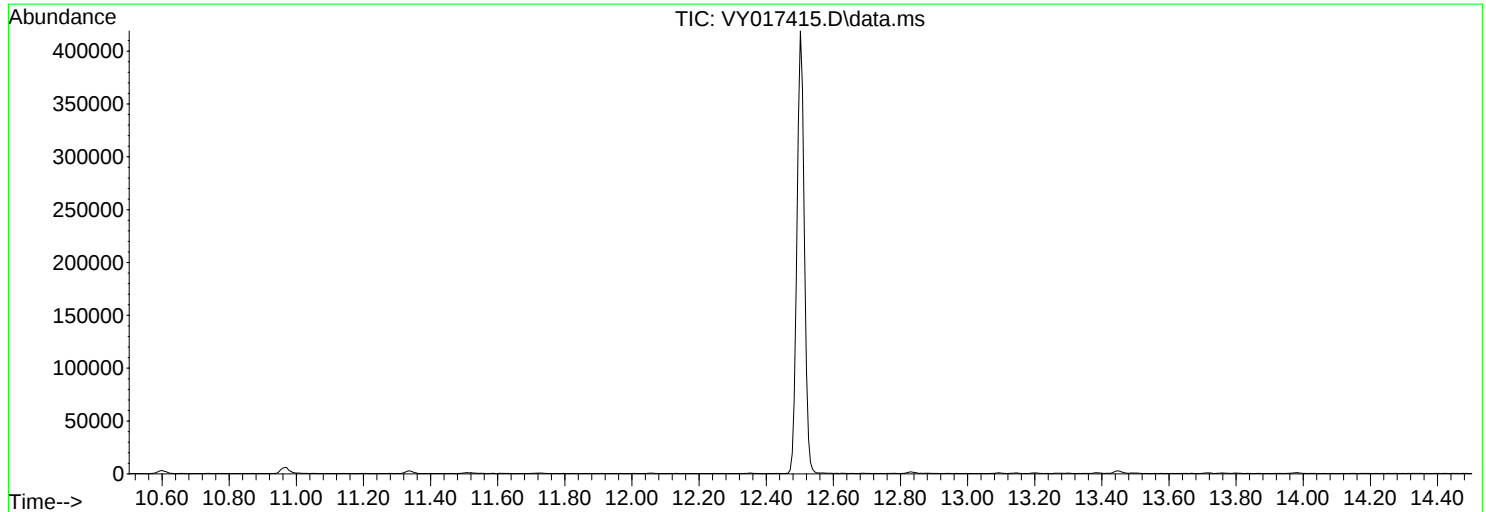

AutoFind: Scans 1751, 1752, 1753; Background Corrected with Scan 1743

| Target | Rel. to | Lower  | Upper  | Rel.  | Raw   | Result    |
|--------|---------|--------|--------|-------|-------|-----------|
| Mass   | Mass    | Limit% | Limit% | Abn%  | Abn   | Pass/Fail |
| 50     | 95      | 15     | 40     | 19.2  | 13381 | PASS      |
| 75     | 95      | 30     | 60     | 52.9  | 36829 | PASS      |
| 95     | 95      | 100    | 100    | 100.0 | 69555 | PASS      |
| 96     | 95      | 5      | 9      | 6.8   | 4737  | PASS      |
| 173    | 174     | 0.00   | 2      | 1.3   | 788   | PASS      |
| 174    | 95      | 50     | 100    | 90.5  | 62965 | PASS      |
| 175    | 174     | 5      | 9      | 7.2   | 4523  | PASS      |
| 176    | 174     | 95     | 101    | 95.5  | 60123 | PASS      |
| 177    | 176     | 5      | 9      | 6.9   | 4153  | PASS      |