

Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY022025\
 Data File : VY021251.D
 Acq On : 20 Feb 2025 15:55
 Operator : SY/MD
 Sample : Q1383-01
 Misc : 5.53g/5.0mL/MSVOA_Y/SOIL/A
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_Y
 ClientSampleId :
 OU4-PCS-TC-11-021725

Quant Time: Feb 21 02:42:32 2025
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y020325S.M
 Quant Title : SW846 8260
 QLast Update : Mon Feb 03 13:08:38 2025
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) Pentafluorobenzene	7.725	168	221666	50.000	ug/l	0.01
34) 1,4-Difluorobenzene	8.628	114	419656	50.000	ug/l	0.00
63) Chlorobenzene-d5	11.432	117	374382	50.000	ug/l	0.01
72) 1,4-Dichlorobenzene-d4	13.359	152	140750	50.000	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.079	65	125705	55.349	ug/l	0.01
Spiked Amount	50.000	Range	50 - 163	Recovery	=	110.700%
35) Dibromofluoromethane	7.652	113	135920	50.538	ug/l	0.01
Spiked Amount	50.000	Range	54 - 147	Recovery	=	101.080%
50) Toluene-d8	10.121	98	507425	49.559	ug/l	0.01
Spiked Amount	50.000	Range	58 - 134	Recovery	=	99.120%
62) 4-Bromofluorobenzene	12.420	95	155739	46.559	ug/l	0.00
Spiked Amount	50.000	Range	30 - 143	Recovery	=	93.120%
Target Compounds						
16) Acetone	3.891	43	20672	58.366	ug/l	Qvalue # 85


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY022025\
Data File : VY021251.D
Acq On : 20 Feb 2025 15:55
Operator : SY/MD
Sample : Q1383-01
Misc : 5.53g/5.0mL/MSVOA_Y/SOIL/A
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_Y
ClientSampleId :
OU4-PCS-TC-11-021725

Quant Time: Feb 21 02:42:32 2025
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y020325S.M
Quant Title : SW846 8260
QLast Update : Mon Feb 03 13:08:38 2025
Response via : Initial Calibration




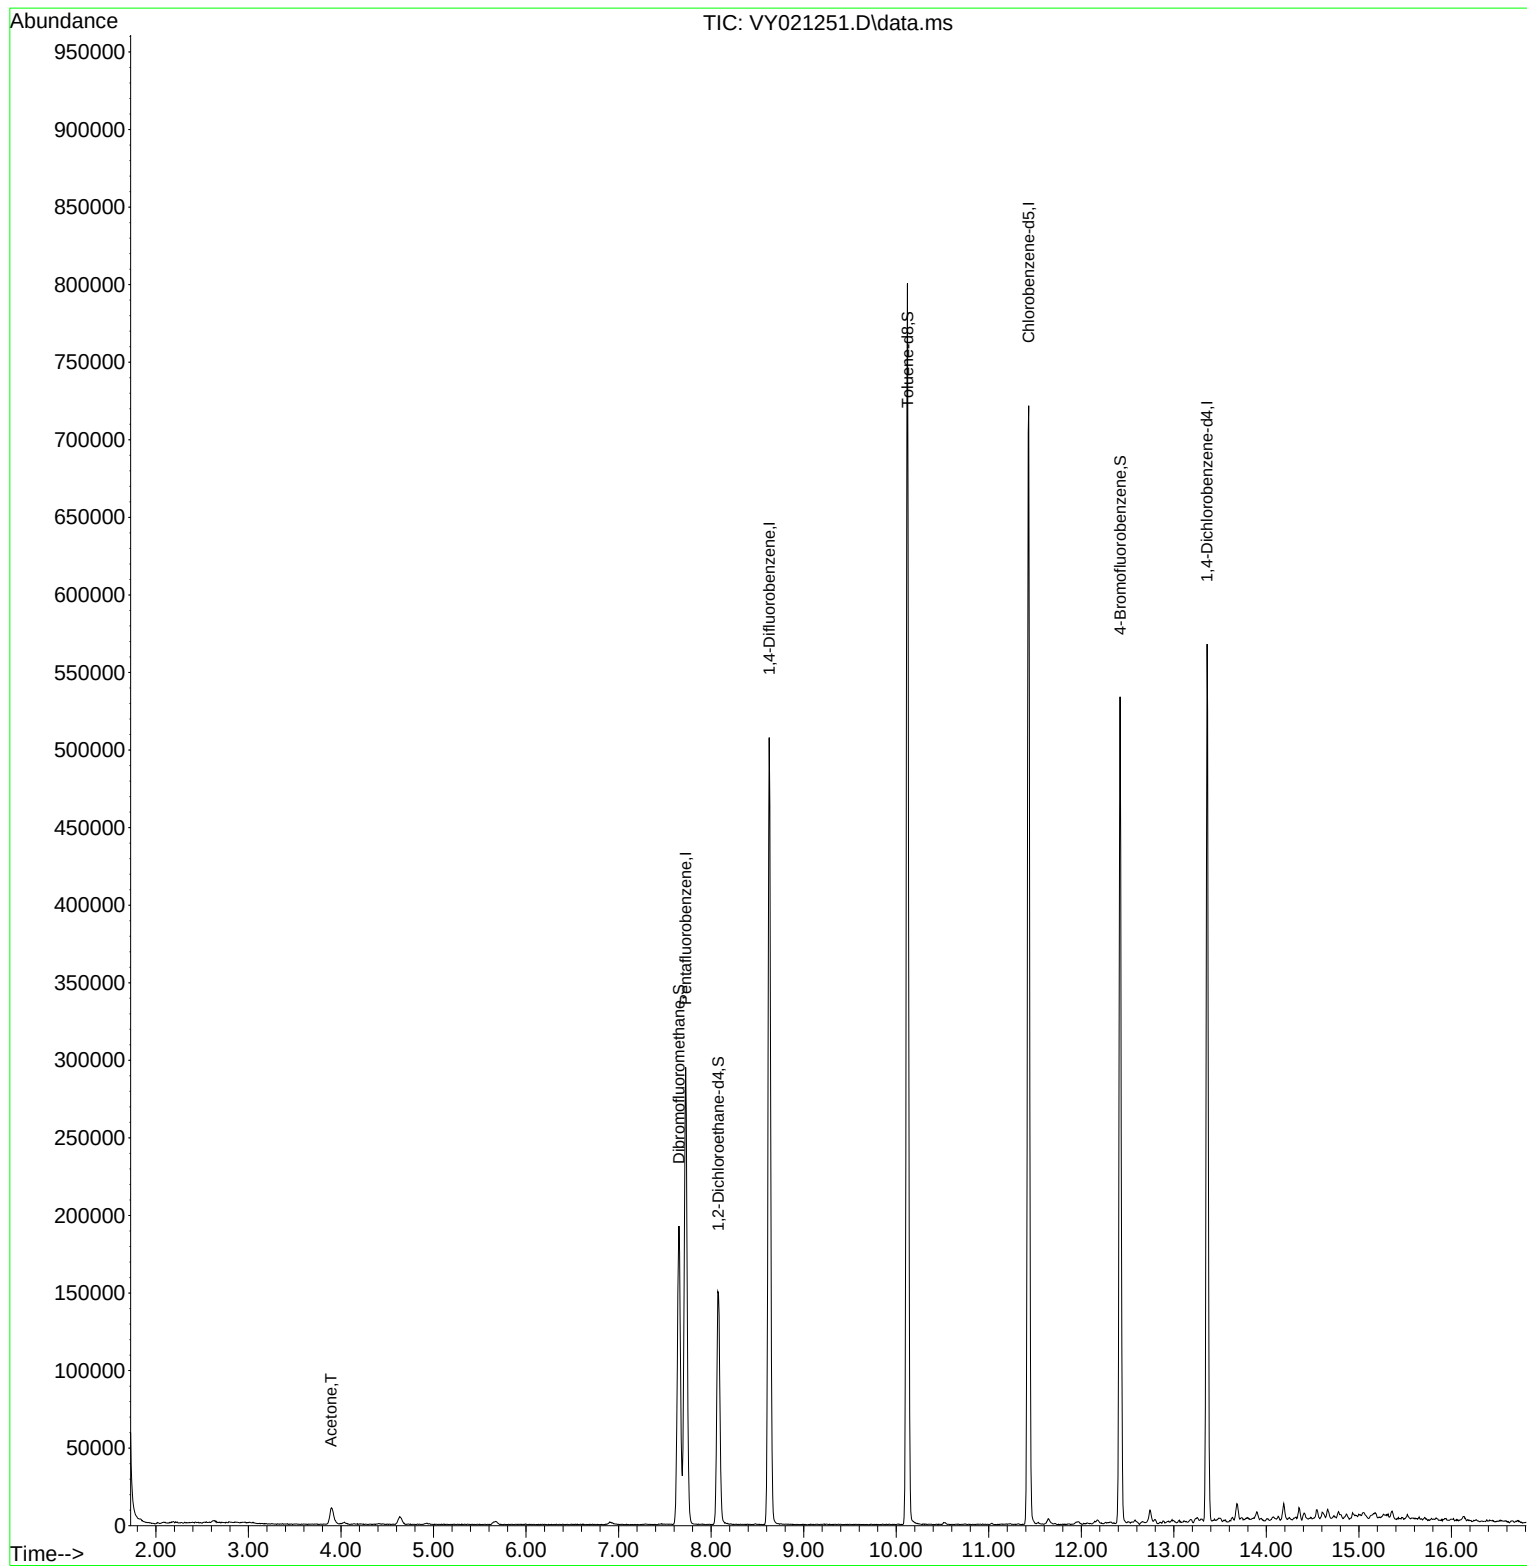


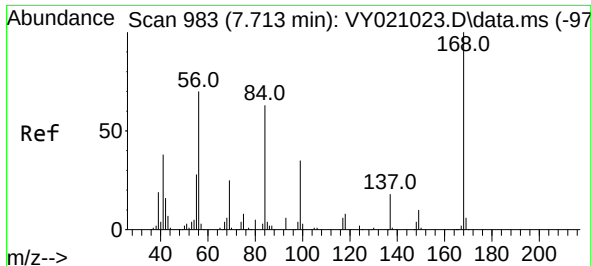

#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 7.725 min Scan# 983
Delta R.T. 0.012 min
Lab File: VY021251.D
Acq: 20 Feb 2025 15:55




Instrument :
MSVOA_Y
ClientSampleId :
OU4-PCS-TC-11-021725


Tgt Ion:168 Resp: 221666
Ion Ratio Lower Upper
168 100
99 57.8 44.2 66.4

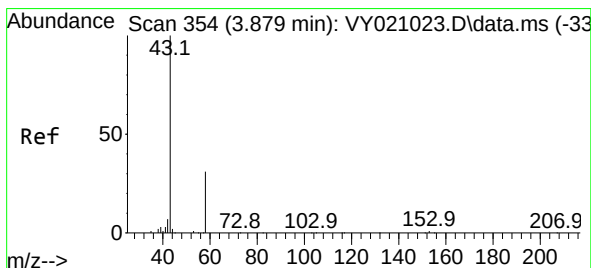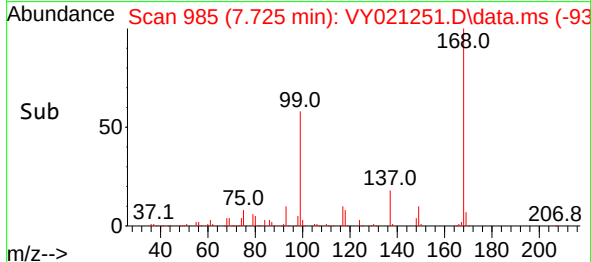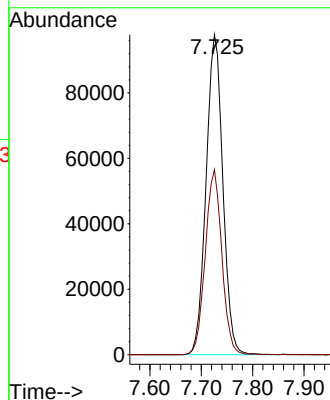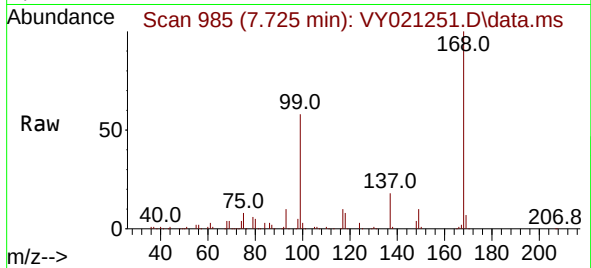

#16
Acetone
Concen: 58.366 ug/l
RT: 3.891 min Scan# 356
Delta R.T. 0.012 min
Lab File: VY021251.D
Acq: 20 Feb 2025 15:55

Tgt Ion: 43 Resp: 20672
Ion Ratio Lower Upper
43 100
58 24.9 26.6 39.8#

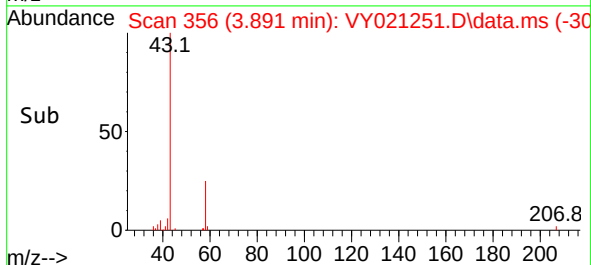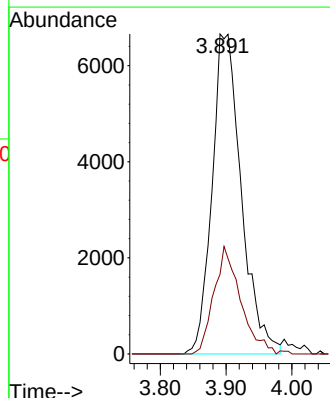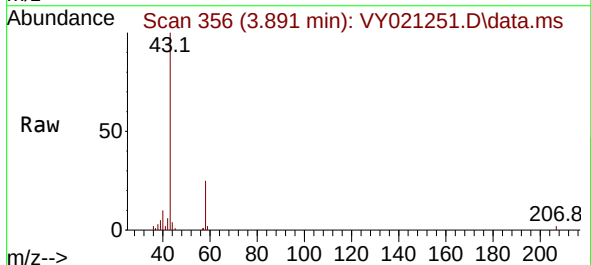

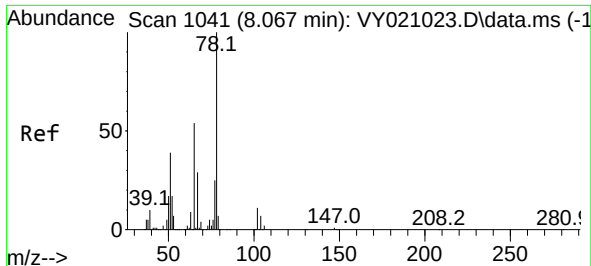

#33

1,2-Dichloroethane-d4

Concen: 55.349 ug/l

RT: 8.079 min Scan# 1104

Delta R.T. 0.012 min

Lab File: VY021251.D

Acq: 20 Feb 2025 15:55

Instrument :

MSVOA_Y

ClientSampleId :





OU4-PCS-TC-11-021725

Tgt Ion: 65 Resp: 125705

Ion Ratio Lower Upper

65 100

67 51.4 0.0 109.0

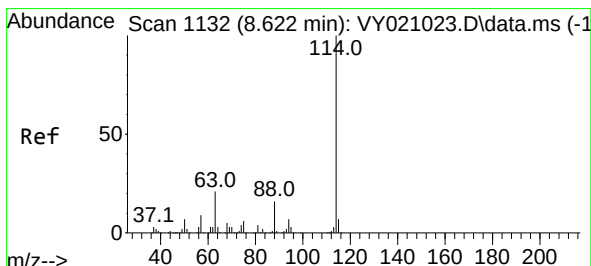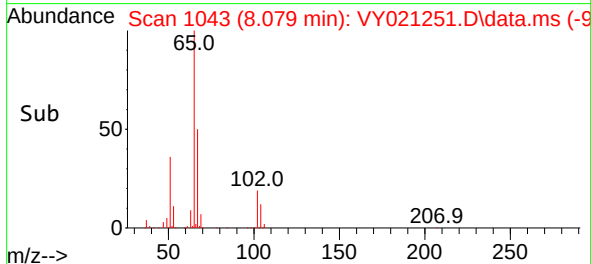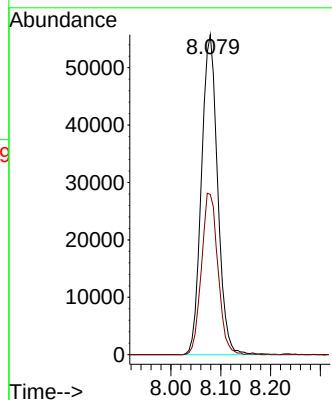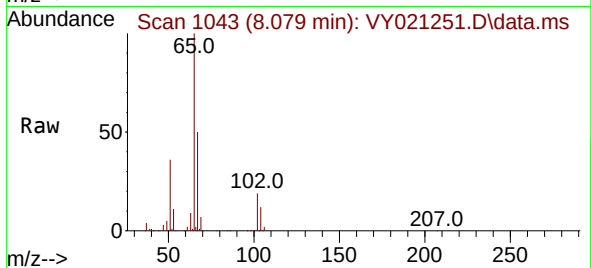

#34

1,4-Difluorobenzene

Concen: 50.000 ug/l

RT: 8.628 min Scan# 1133

Delta R.T. 0.006 min

Lab File: VY021251.D

Acq: 20 Feb 2025 15:55




Tgt Ion: 114 Resp: 419656


Ion Ratio Lower Upper

114 100

63 21.9 0.0 37.4

88 15.4 0.0 29.0


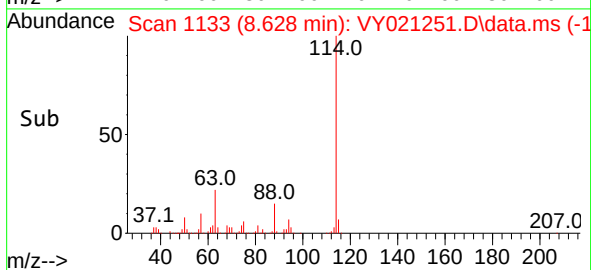
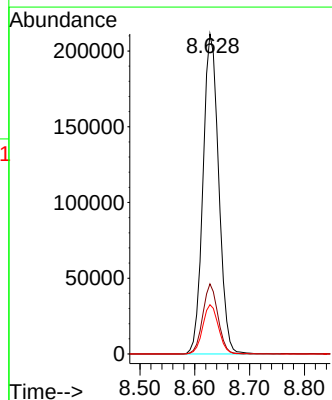
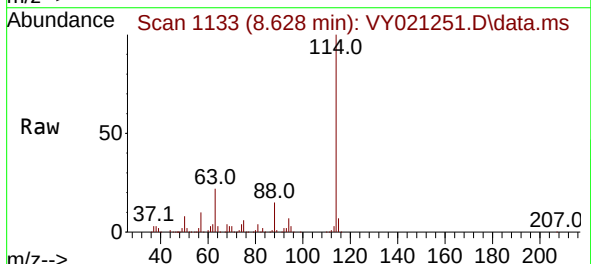


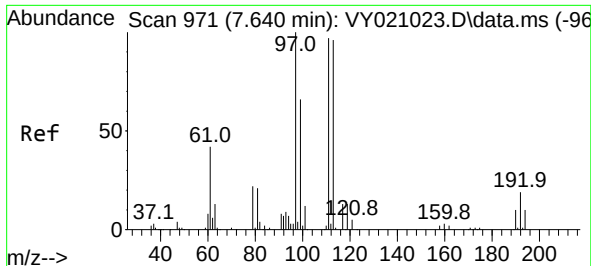

#35
 Dibromofluoromethane
 Concen: 50.538 ug/l
 RT: 7.652 min Scan# 91
 Delta R.T. 0.012 min
 Lab File: VY021251.D
 Acq: 20 Feb 2025 15:55




Instrument :
 MSVOA_Y
 ClientSampleId :
 OU4-PCS-TC-11-021725


Tgt Ion:113 Resp: 135920
 Ion Ratio Lower Upper
 113 100
 111 102.6 83.8 125.6
 192 19.8 14.5 21.7

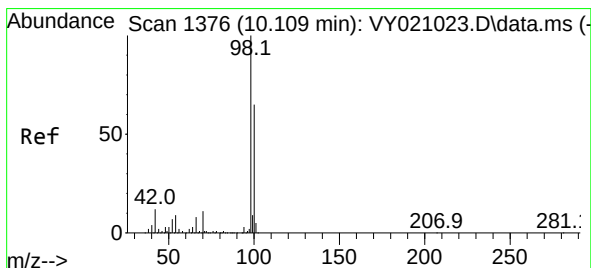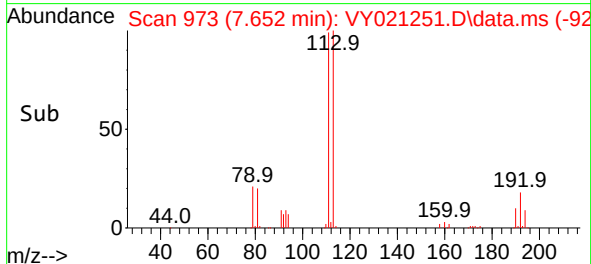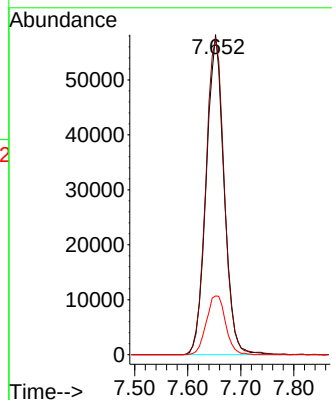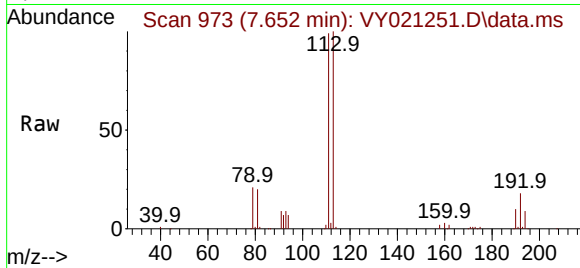

#50
 Toluene-d8
 Concen: 49.559 ug/l
 RT: 10.121 min Scan# 1378
 Delta R.T. 0.012 min
 Lab File: VY021251.D
 Acq: 20 Feb 2025 15:55

Tgt Ion: 98 Resp: 507425
 Ion Ratio Lower Upper
 98 100
 100 64.4 52.3 78.5


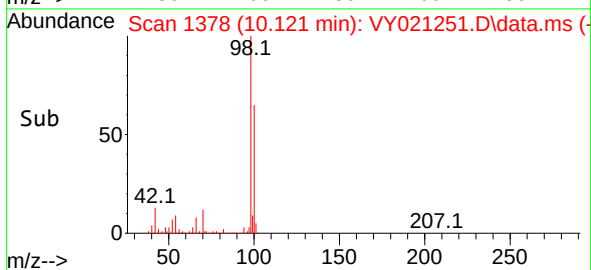
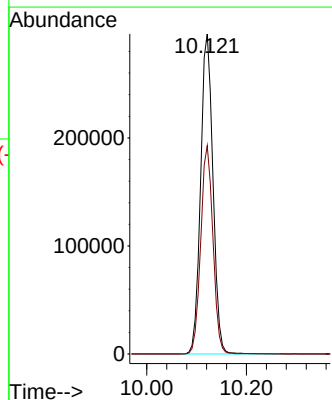
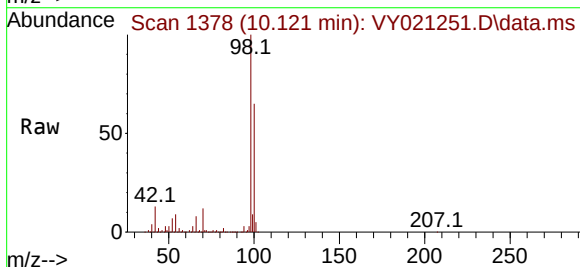


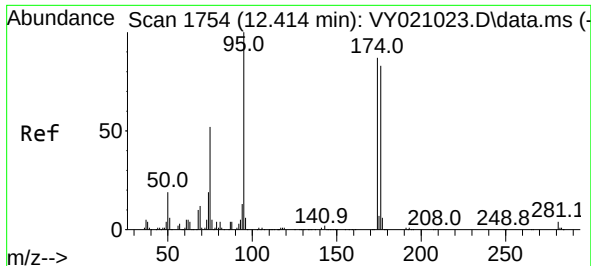

#62
4-Bromofluorobenzene
Concen: 46.559 ug/l
RT: 12.420 min Scan# 1755
Delta R.T. 0.006 min
Lab File: VY021251.D
Acq: 20 Feb 2025 15:55




Instrument :
MSVOA_Y
ClientSampleId :
OU4-PCS-TC-11-021725


Tgt Ion: 95 Resp: 155739
Ion Ratio Lower Upper
95 100
174 83.7 0.0 160.0
176 81.6 0.0 151.8

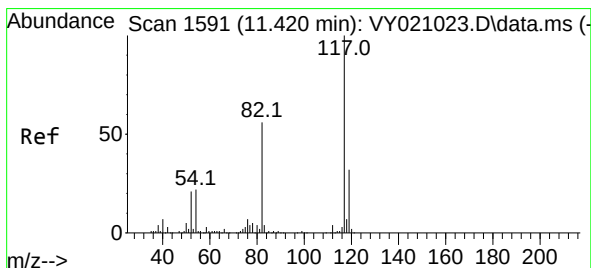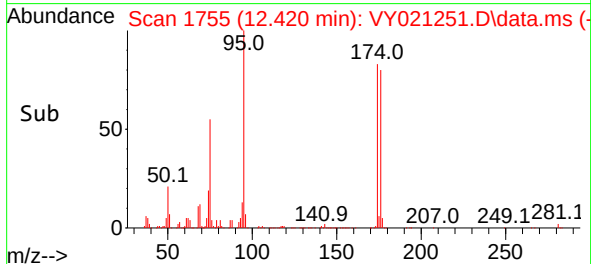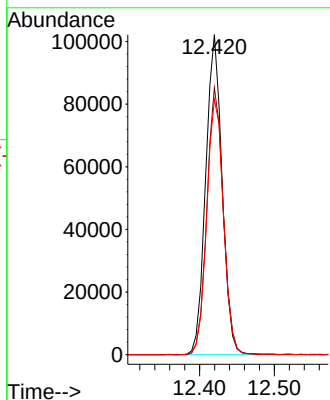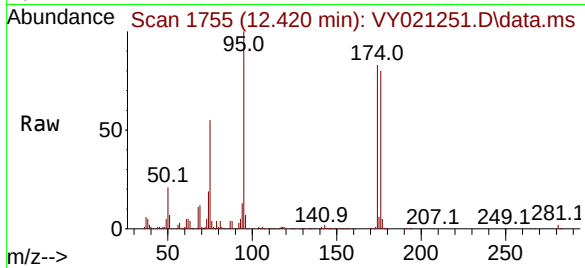

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 11.432 min Scan# 1593
Delta R.T. 0.012 min
Lab File: VY021251.D
Acq: 20 Feb 2025 15:55

Tgt Ion: 117 Resp: 374382
Ion Ratio Lower Upper
117 100
82 57.1 43.8 65.8
119 33.2 26.5 39.7

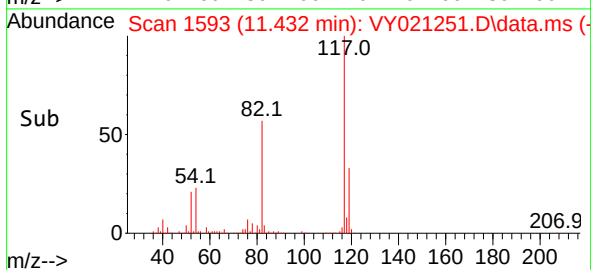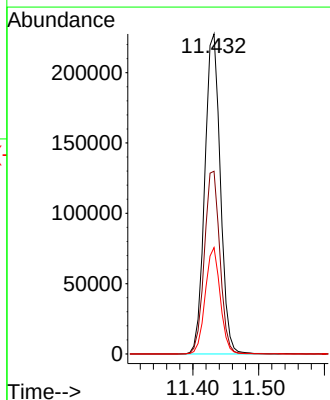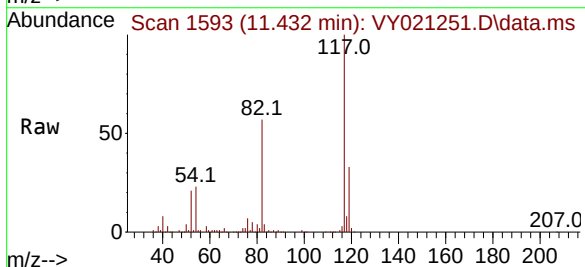

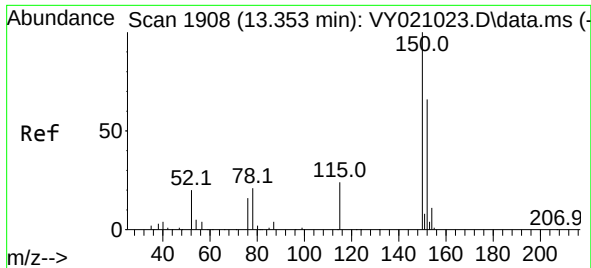

#72

1,4-Dichlorobenzene-d4

Concen: 50.000 ug/l

RT: 13.359 min Scan# 1909

Delta R.T. 0.006 min

Lab File: VY021251.D


Acq: 20 Feb 2025 15:55

Instrument :

MSVOA_Y

ClientSampleId :

OU4-PCS-TC-11-021725

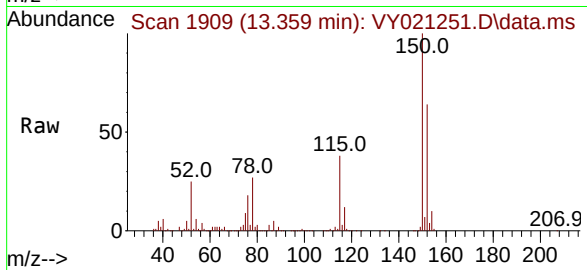

Tgt Ion:152 Resp: 140750

Ion Ratio Lower Upper

152 100

115 58.5 30.0 90.0

150 153.7 0.0 344.6

