

Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY022025\
 Data File : VY021256.D
 Acq On : 20 Feb 2025 17:52
 Operator : SY/MD
 Sample : Q1383-11
 Misc : 5.29g/5.0mL/MSVOA_Y/SOIL/A
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_Y
 ClientSampleId :
 OU4-PCS-TC-16-021725

Quant Time: Feb 21 02:44:20 2025
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y020325S.M
 Quant Title : SW846 8260
 QLast Update : Mon Feb 03 13:08:38 2025
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) Pentafluorobenzene	7.720	168	197039	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	8.628	114	374580	50.000	ug/l	0.00
63) Chlorobenzene-d5	11.426	117	340962	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.359	152	132279	50.000	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.073	65	113314	56.129	ug/l	0.00
Spiked Amount	50.000	Range	50 - 163	Recovery	= 112.260%	
35) Dibromofluoromethane	7.646	113	121526	50.624	ug/l	0.00
Spiked Amount	50.000	Range	54 - 147	Recovery	= 101.240%	
50) Toluene-d8	10.115	98	460913	50.433	ug/l	0.00
Spiked Amount	50.000	Range	58 - 134	Recovery	= 100.860%	
62) 4-Bromofluorobenzene	12.414	95	141716	47.465	ug/l	0.00
Spiked Amount	50.000	Range	30 - 143	Recovery	= 94.920%	
Target Compounds						Qvalue
16) Acetone	3.897	43	4152	13.188	ug/l	95

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY022025\
Data File : VY021256.D
Acq On : 20 Feb 2025 17:52
Operator : SY/MD
Sample : Q1383-11
Misc : 5.29g/5.0mL/MSVOA_Y/SOIL/A
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_Y
ClientSampleId :
OU4-PCS-TC-16-021725

Quant Time: Feb 21 02:44:20 2025
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y020325S.M
Quant Title : SW846 8260
QLast Update : Mon Feb 03 13:08:38 2025
Response via : Initial Calibration




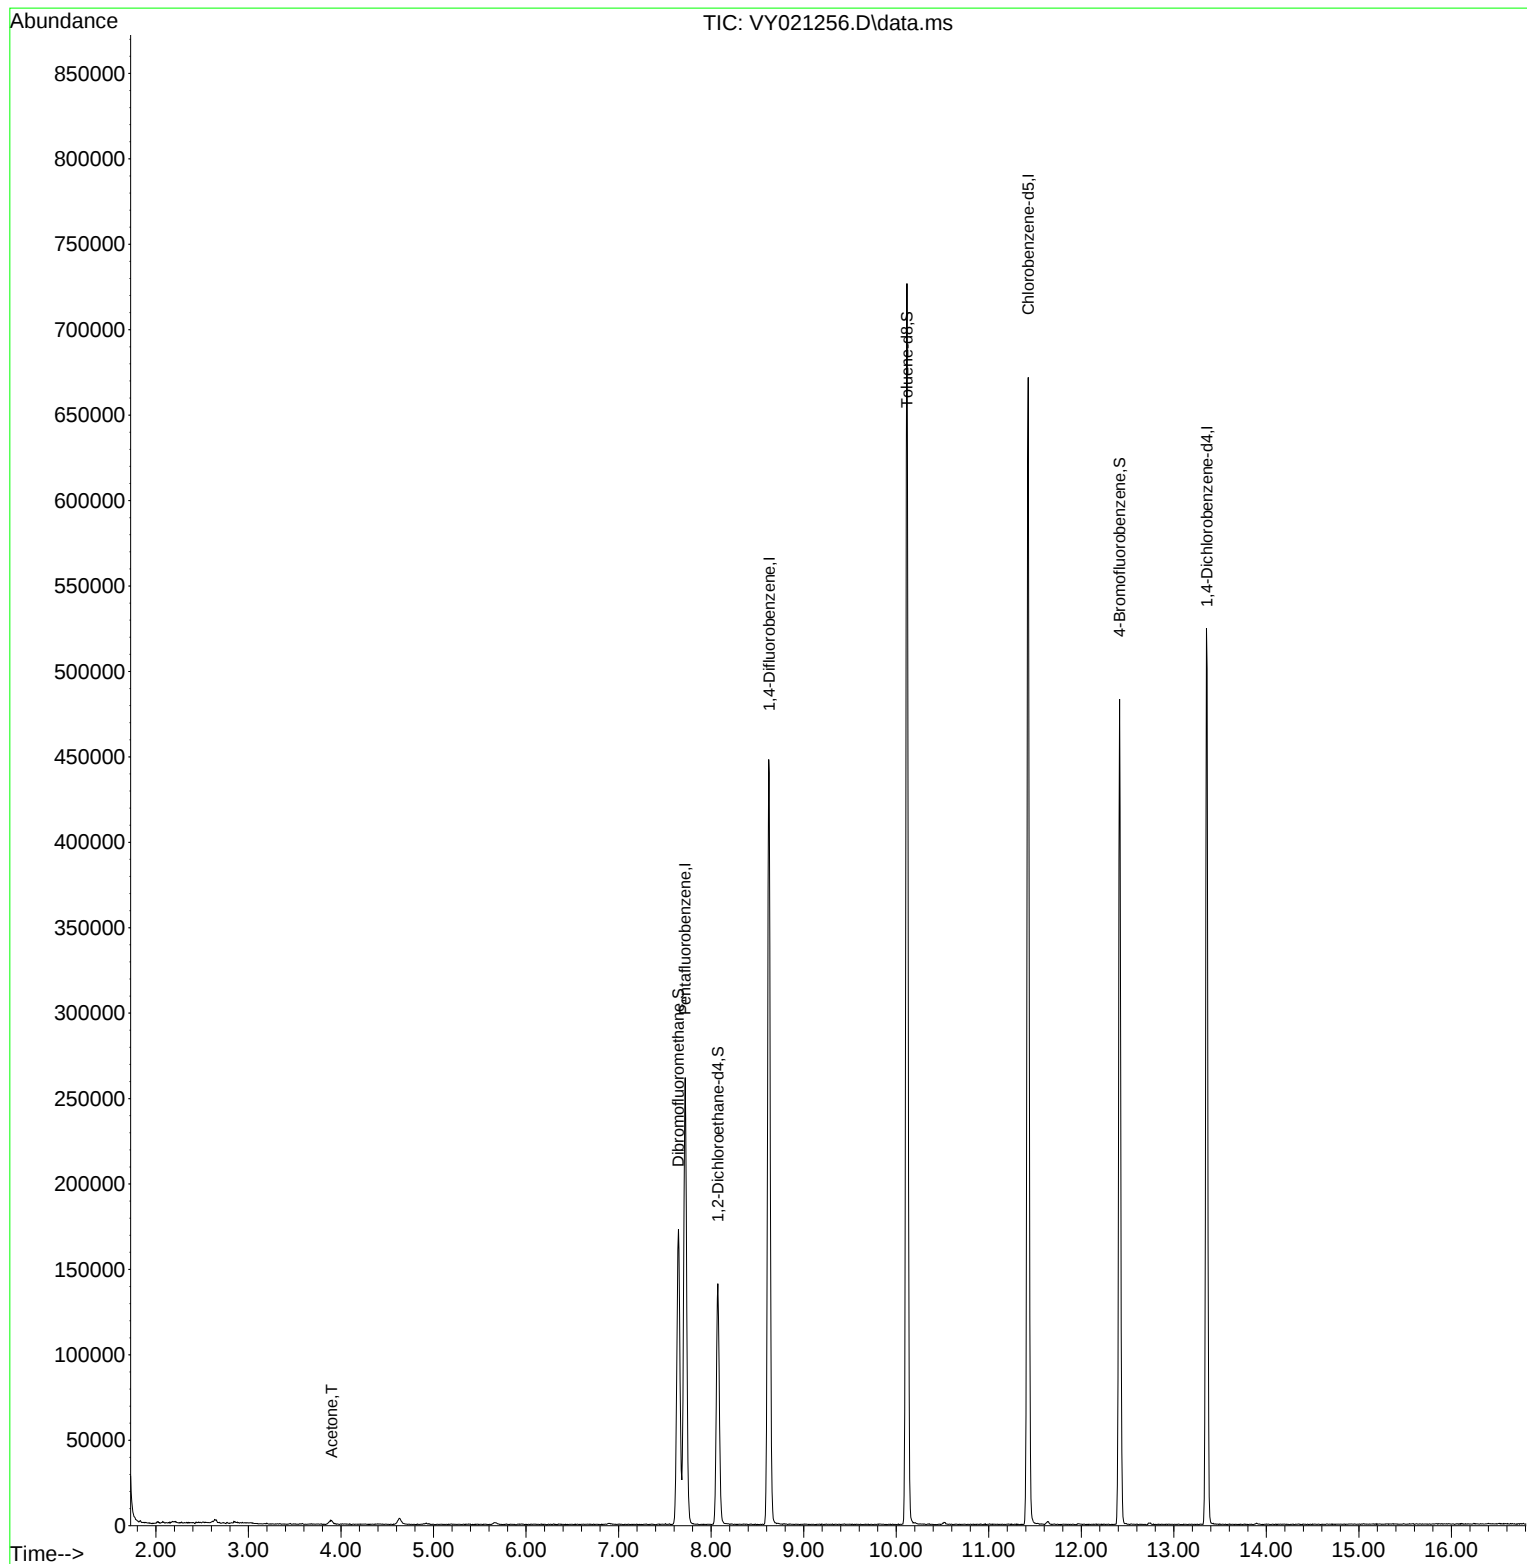




#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 7.720 min Scan# 91
Delta R.T. 0.007 min
Lab File: VY021256.D
Acq: 20 Feb 2025 17:52




Instrument :
MSVOA_Y
ClientSampleId :
OU4-PCS-TC-16-021725


Tgt Ion:168 Resp: 197039
Ion Ratio Lower Upper
168 100
99 56.0 44.2 66.4

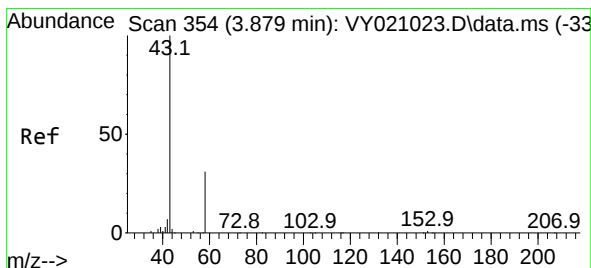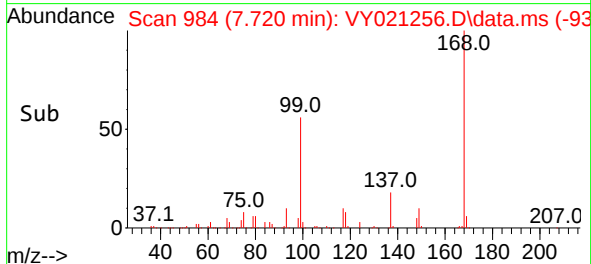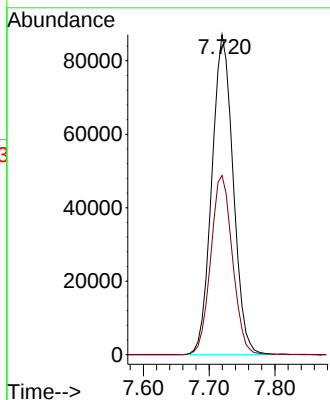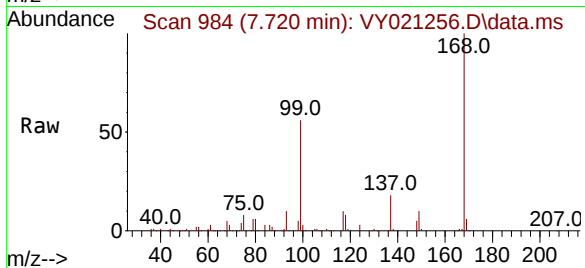

#16
Acetone
Concen: 13.188 ug/l
RT: 3.897 min Scan# 357
Delta R.T. 0.018 min
Lab File: VY021256.D
Acq: 20 Feb 2025 17:52

Tgt Ion: 43 Resp: 4152
Ion Ratio Lower Upper
43 100
58 30.6 26.6 39.8

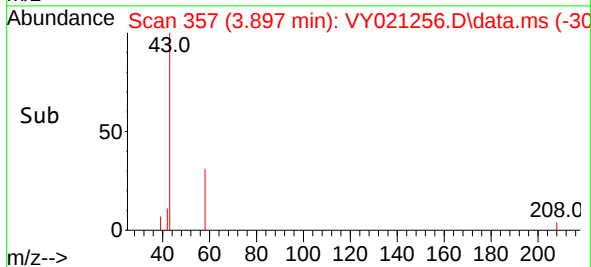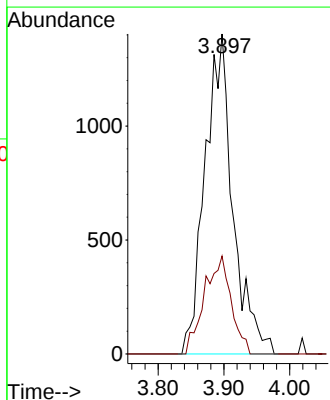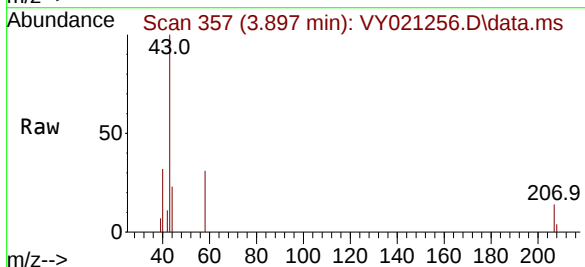

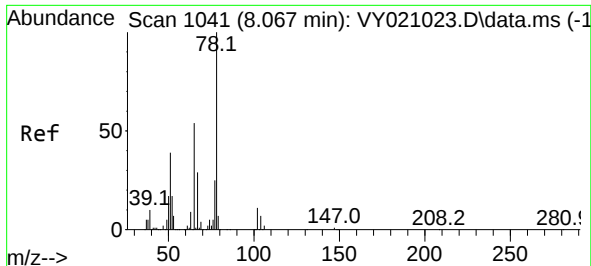

#33

1,2-Dichloroethane-d4

Concen: 56.129 ug/l

RT: 8.073 min Scan# 110

Delta R.T. 0.006 min

Lab File: VY021256.D

Acq: 20 Feb 2025 17:52

Instrument :

MSVOA_Y

ClientSampleId :





OU4-PCS-TC-16-021725

Tgt Ion: 65 Resp: 113314

Ion Ratio Lower Upper

65 100

67 51.9 0.0 109.0

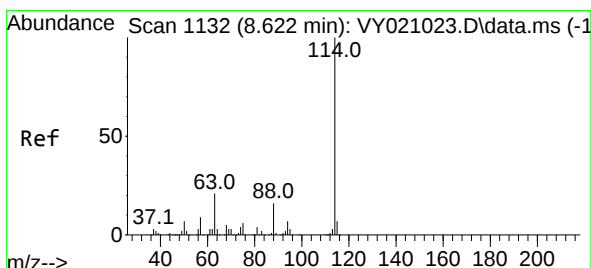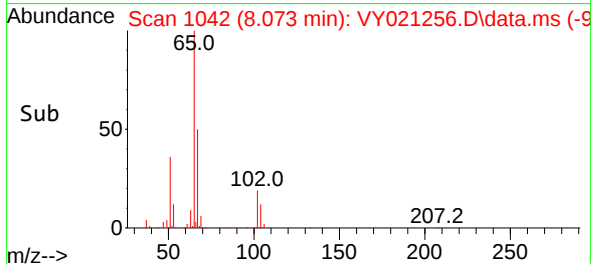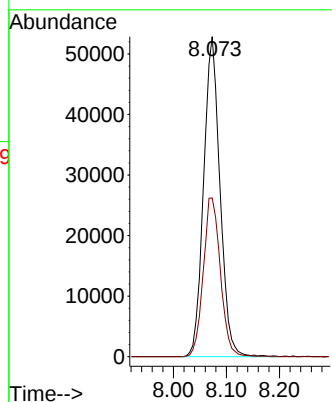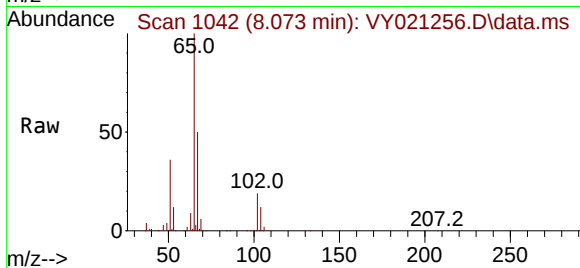

#34

1,4-Difluorobenzene

Concen: 50.000 ug/l

RT: 8.628 min Scan# 1133

Delta R.T. 0.006 min

Lab File: VY021256.D

Acq: 20 Feb 2025 17:52




Tgt Ion: 114 Resp: 374580


Ion Ratio Lower Upper

114 100

63 21.2 0.0 37.4

88 15.6 0.0 29.0


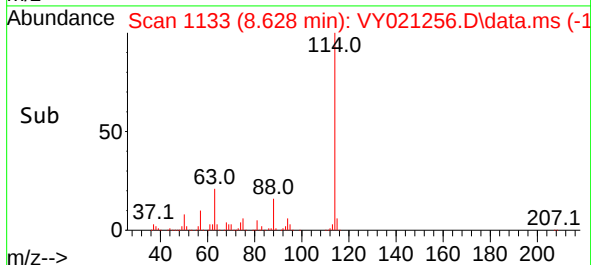
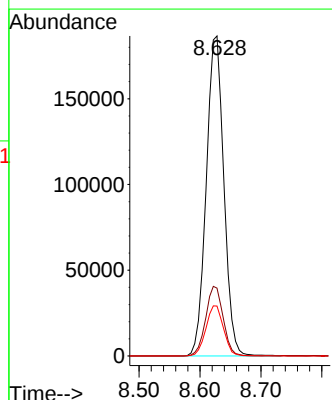
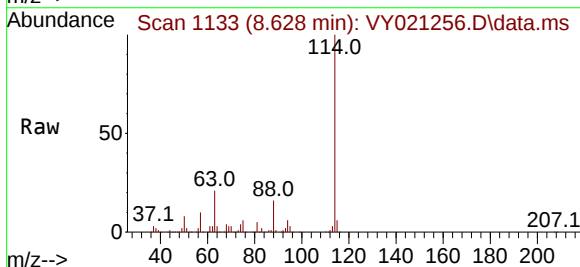


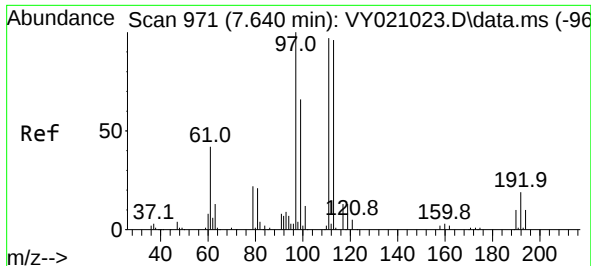

#35
Dibromofluoromethane
Concen: 50.624 ug/l
RT: 7.646 min Scan# 91
Delta R.T. 0.006 min
Lab File: VY021256.D
Acq: 20 Feb 2025 17:52




Instrument :
MSVOA_Y
ClientSampleId :
OU4-PCS-TC-16-021725


Tgt Ion:113 Resp: 121526
Ion Ratio Lower Upper
113 100
111 103.2 83.8 125.6
192 19.6 14.5 21.7

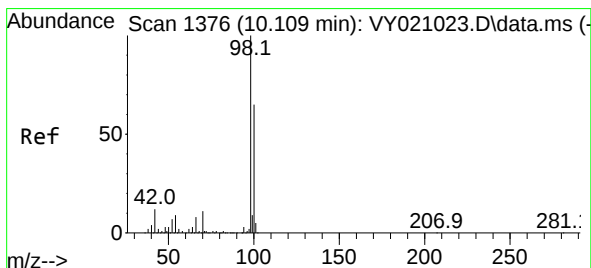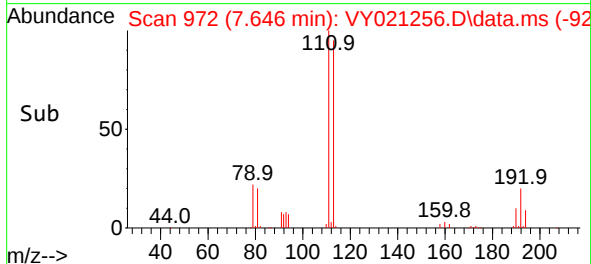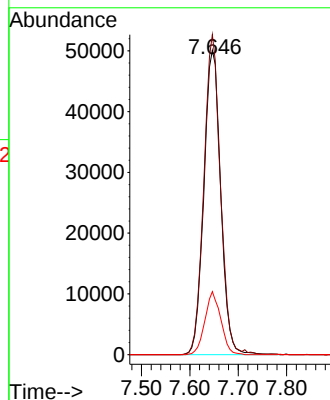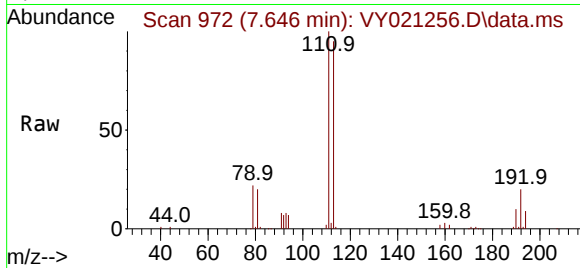

#50
Toluene-d8
Concen: 50.433 ug/l
RT: 10.115 min Scan# 1377
Delta R.T. 0.006 min
Lab File: VY021256.D
Acq: 20 Feb 2025 17:52

Tgt Ion: 98 Resp: 460913
Ion Ratio Lower Upper
98 100
100 63.7 52.3 78.5


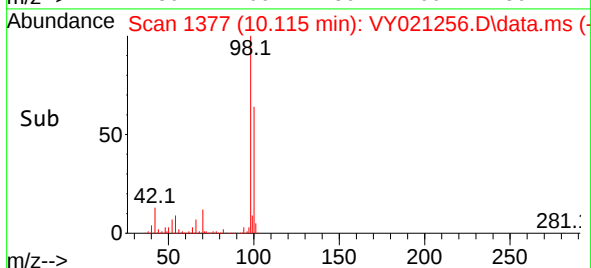
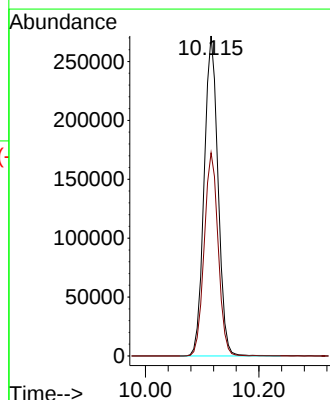
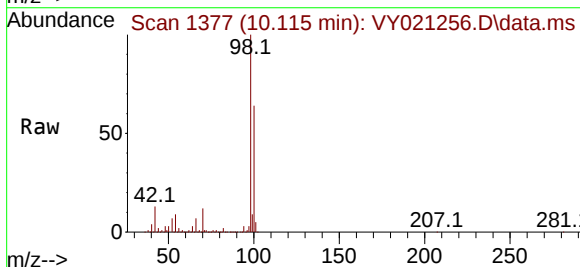


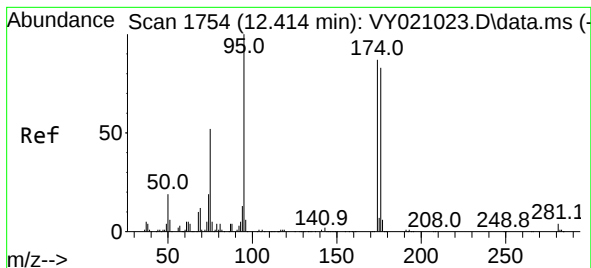

#62
4-Bromofluorobenzene
Concen: 47.465 ug/l
RT: 12.414 min Scan# 11
Delta R.T. 0.000 min
Lab File: VY021256.D
Acq: 20 Feb 2025 17:52




Instrument :
MSVOA_Y
ClientSampleId :
OU4-PCS-TC-16-021725


Tgt Ion: 95 Resp: 141716
Ion Ratio Lower Upper
95 100
174 84.5 0.0 160.0
176 80.8 0.0 151.8

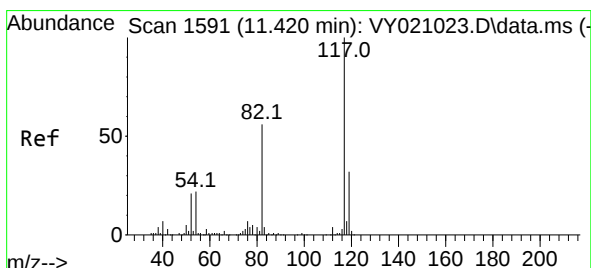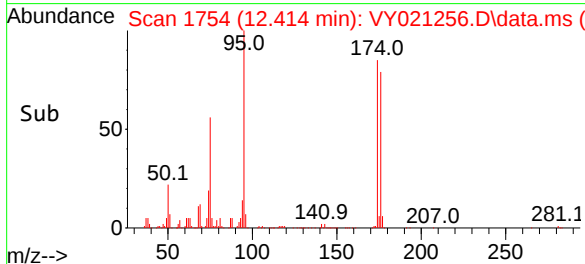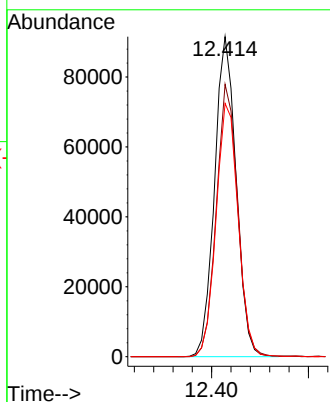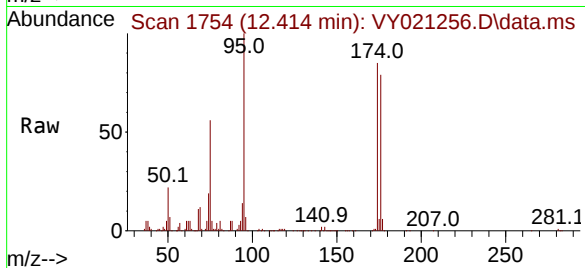

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 11.426 min Scan# 1592
Delta R.T. 0.006 min
Lab File: VY021256.D
Acq: 20 Feb 2025 17:52


Tgt Ion: 117 Resp: 340962
Ion Ratio Lower Upper
117 100
82 56.4 43.8 65.8
119 31.9 26.5 39.7

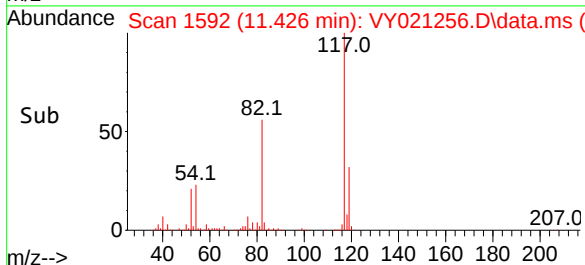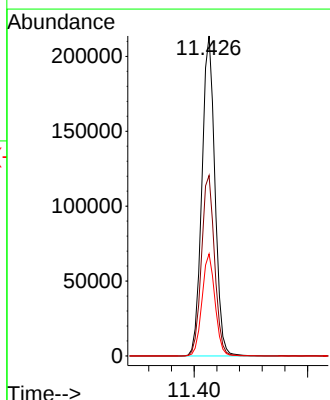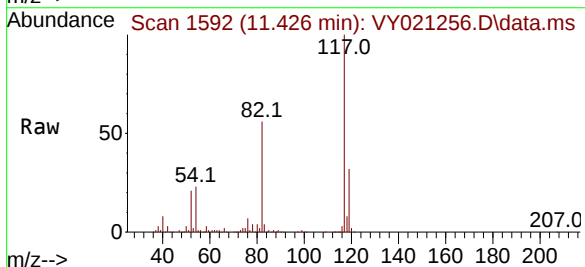

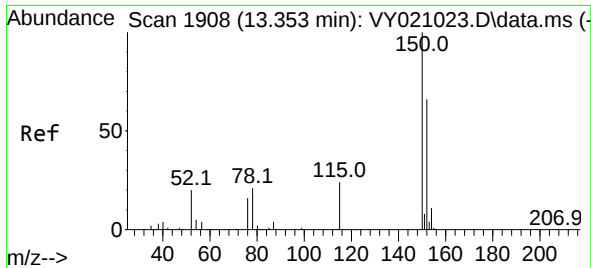

#72
 1,4-Dichlorobenzene-d4
 Concen: 50.000 ug/l
 RT: 13.359 min Scan# 1909
 Delta R.T. 0.006 min
 Lab File: VY021256.D
 Acq: 20 Feb 2025 17:52

Instrument :
 MSVOA_Y
 ClientSampleId :
 OU4-PCS-TC-16-021725

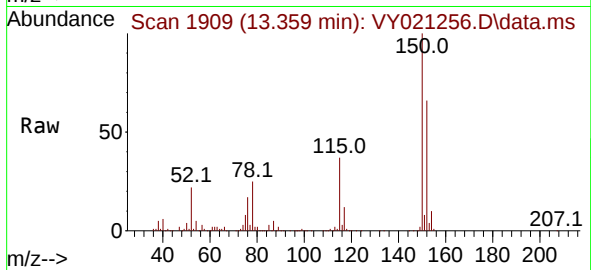

Tgt Ion:152 Resp: 132279
 Ion Ratio Lower Upper
 152 100
 115 57.9 30.0 90.0
 150 155.6 0.0 344.6

