

Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY022025\
 Data File : VY021262.D
 Acq On : 20 Feb 2025 20:13
 Operator : SY/MD
 Sample : Q1382-07
 Misc : 5.61g/5.0mL/MSVOA_Y/SOIL/A
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 MSVOA_Y
 ClientSampleId :
 OU4-PCS-TC-04-021725

Quant Time: Feb 21 02:46:23 2025
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y020325S.M
 Quant Title : SW846 8260
 QLast Update : Mon Feb 03 13:08:38 2025
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Pentafluorobenzene	7.719	168	173272	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	8.622	114	337765	50.000	ug/l	0.00
63) Chlorobenzene-d5	11.426	117	312885	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.359	152	121569	50.000	ug/l	0.00

System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.073	65	106301	59.877	ug/l	0.00
Spiked Amount	50.000	Range	50 - 163	Recovery	=	119.760%
35) Dibromofluoromethane	7.646	113	110503	51.050	ug/l	0.00
Spiked Amount	50.000	Range	54 - 147	Recovery	=	102.100%
50) Toluene-d8	10.115	98	412123	50.010	ug/l	0.00
Spiked Amount	50.000	Range	58 - 134	Recovery	=	100.020%
62) 4-Bromofluorobenzene	12.414	95	132214	49.109	ug/l	0.00
Spiked Amount	50.000	Range	30 - 143	Recovery	=	98.220%


Target Compounds	Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY022025\
Data File : VY021262.D
Acq On : 20 Feb 2025 20:13
Operator : SY/MD
Sample : Q1382-07
Misc : 5.61g/5.0mL/MSVOA_Y/SOIL/A
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_Y
ClientSampleId :
OU4-PCS-TC-04-021725

Quant Time: Feb 21 02:46:23 2025
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y020325S.M
Quant Title : SW846 8260
QLast Update : Mon Feb 03 13:08:38 2025
Response via : Initial Calibration




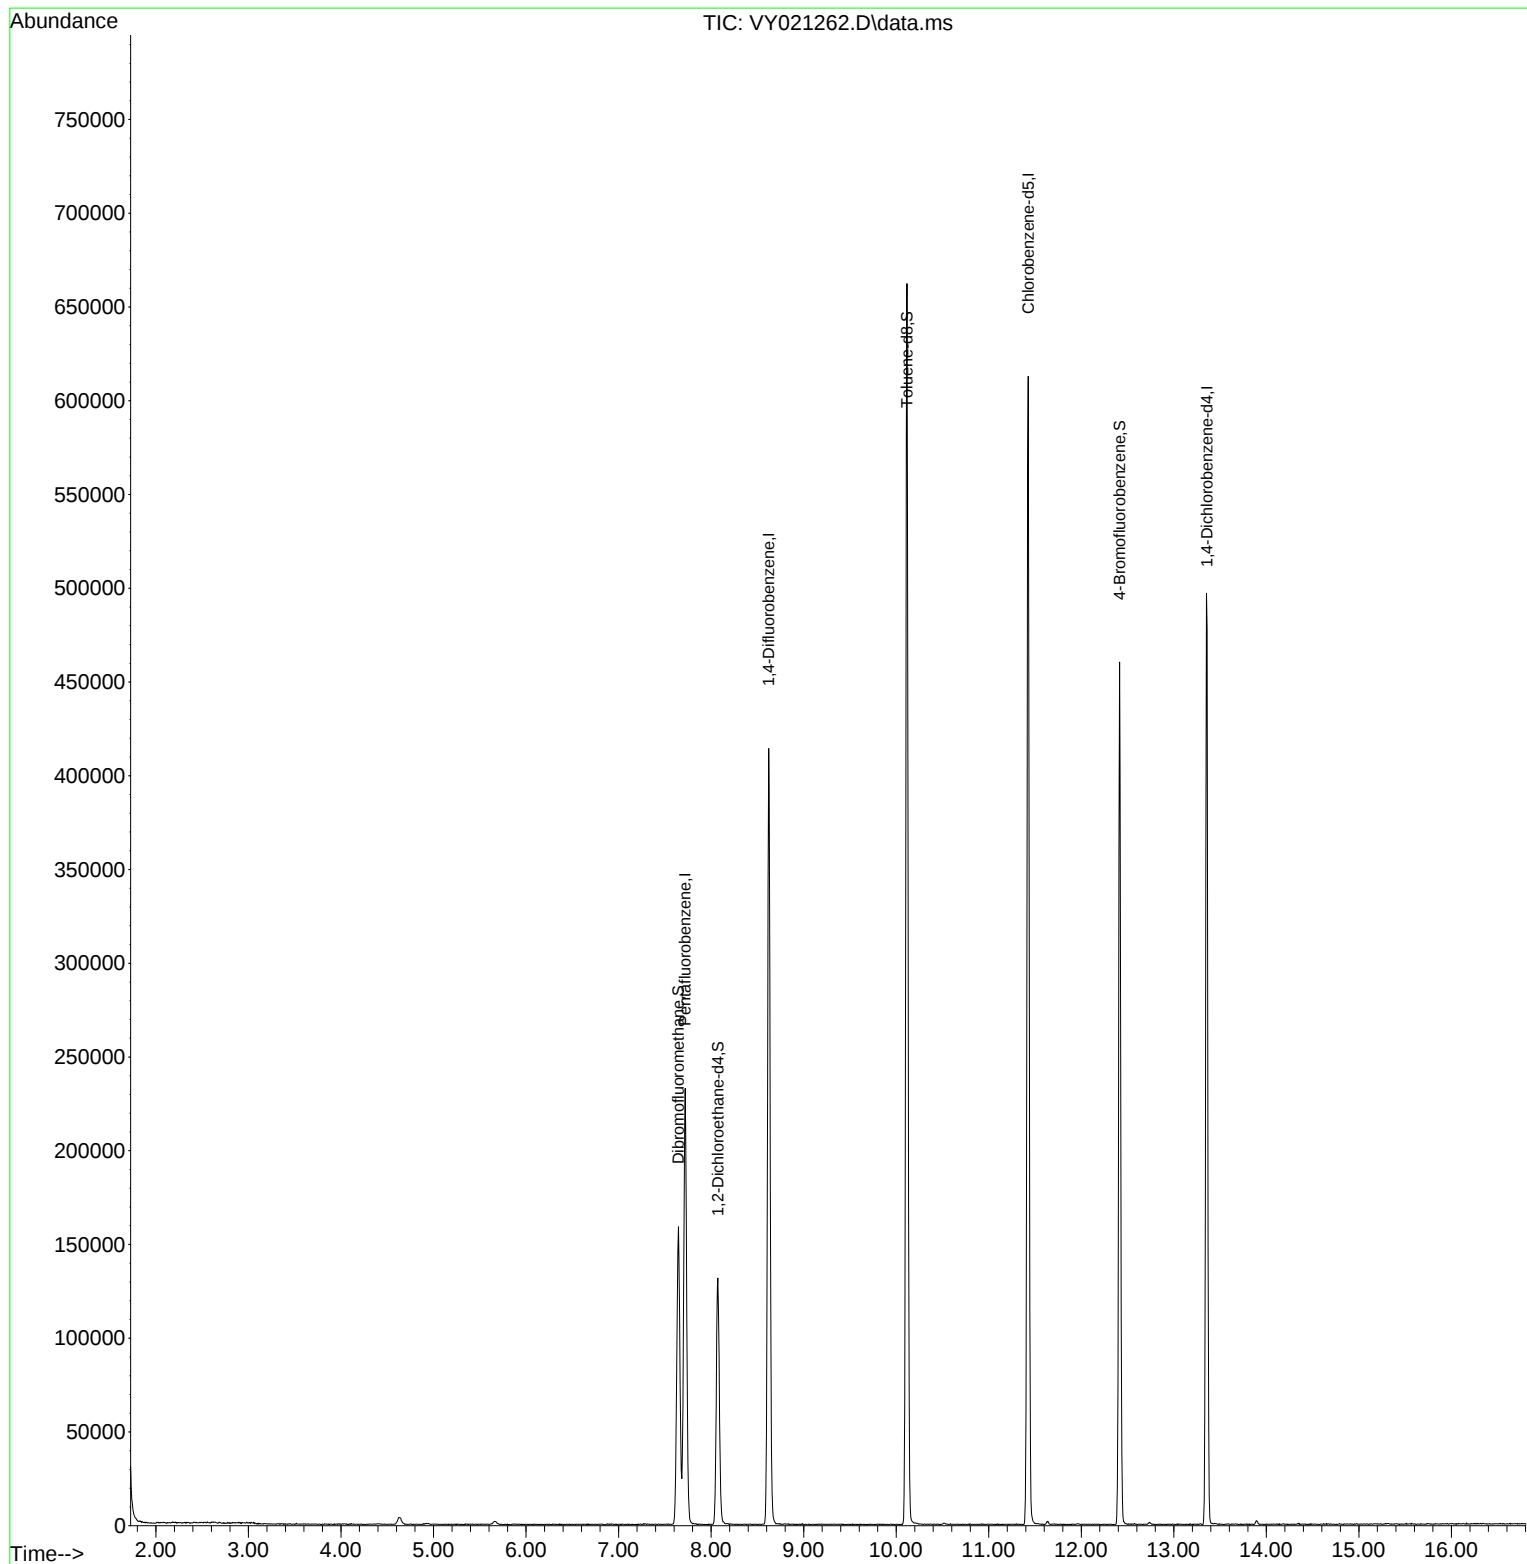


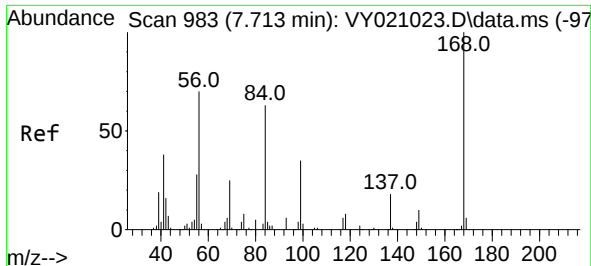

#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 7.719 min Scan# 983
Delta R.T. 0.006 min
Lab File: VY021262.D
Acq: 20 Feb 2025 20:13




Instrument :
MSVOA_Y
ClientSampleId :
OU4-PCS-TC-04-021725


Tgt Ion:168 Resp: 173272
Ion Ratio Lower Upper
168 100
99 57.4 44.2 66.4

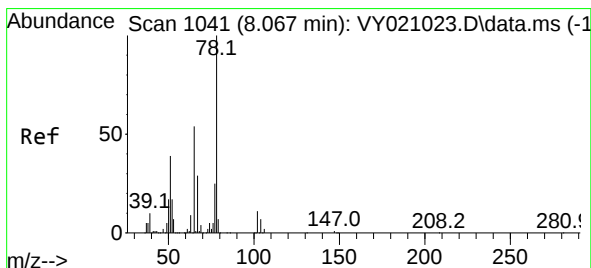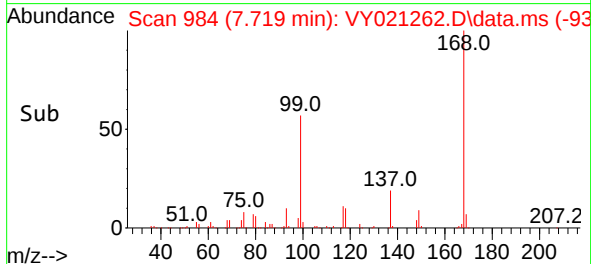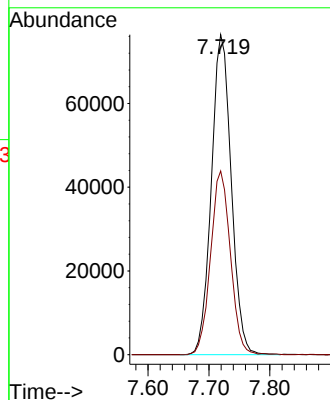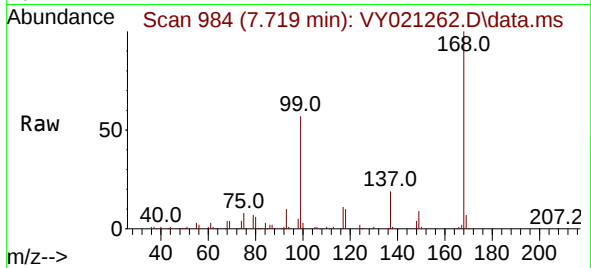

#33
1,2-Dichloroethane-d4
Concen: 59.877 ug/l
RT: 8.073 min Scan# 1042
Delta R.T. 0.006 min
Lab File: VY021262.D
Acq: 20 Feb 2025 20:13

Tgt Ion: 65 Resp: 106301
Ion Ratio Lower Upper
65 100
67 52.6 0.0 109.0

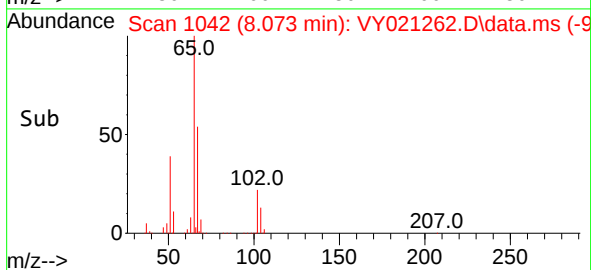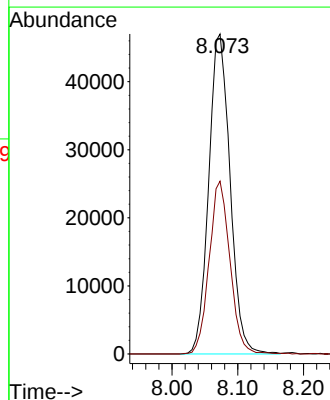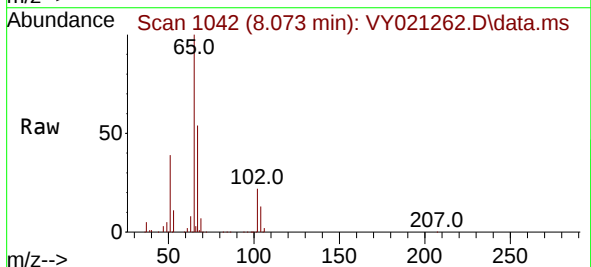

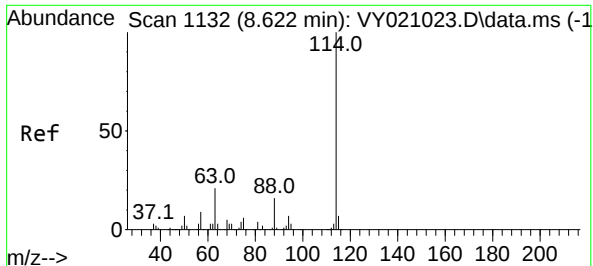

#34

1,4-Difluorobenzene

Concen: 50.000 ug/l

RT: 8.622 min Scan# 1132

Delta R.T. -0.000 min

Lab File: VY021262.D

Acq: 20 Feb 2025 20:13

Instrument :

MSVOA_Y

ClientSampleId :

OU4-PCS-TC-04-021725





Tgt Ion:114 Resp: 337765

Ion Ratio Lower Upper

114 100

63 22.1 0.0 37.4

88 16.2 0.0 29.0

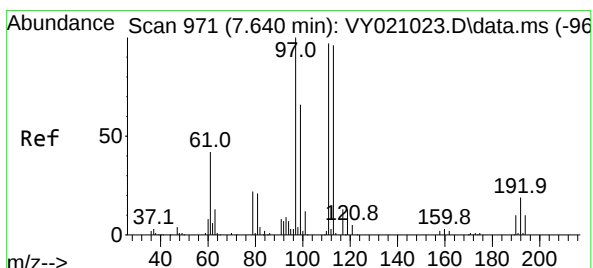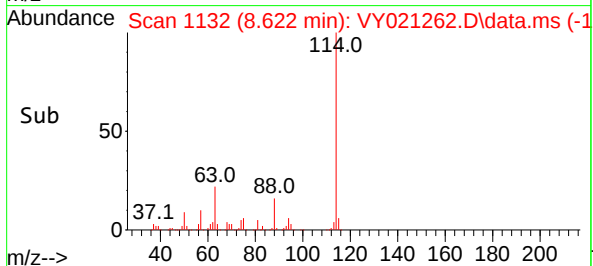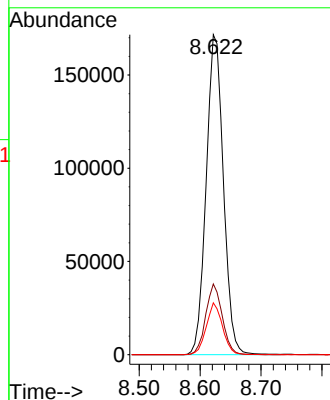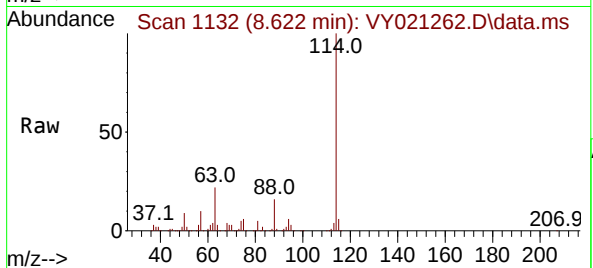

#35

Dibromofluoromethane

Concen: 51.050 ug/l

RT: 7.646 min Scan# 972

Delta R.T. 0.006 min

Lab File: VY021262.D

Acq: 20 Feb 2025 20:13




Tgt Ion:113 Resp: 110503

Ion Ratio Lower Upper

113 100

111 102.8 83.8 125.6

192 19.6 14.5 21.7

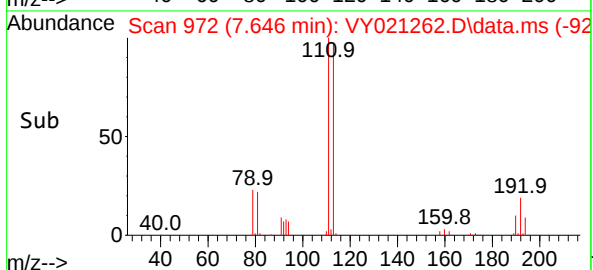
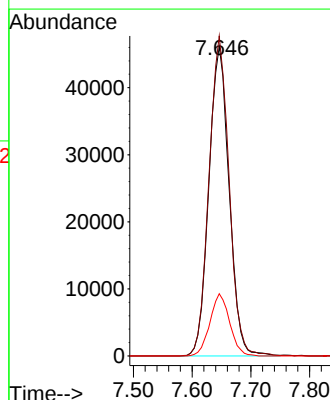
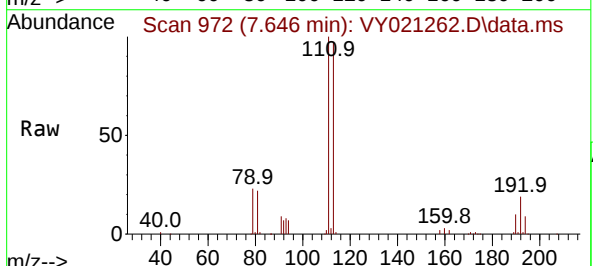




#50
Toluene-d8
Concen: 50.010 ug/l
RT: 10.115 min Scan# 11
Delta R.T. 0.006 min
Lab File: VY021262.D
Acq: 20 Feb 2025 20:13




Instrument :
MSVOA_Y
ClientSampleId :
OU4-PCS-TC-04-021725


Tgt Ion: 98 Resp: 412123
Ion Ratio Lower Upper
98 100
100 64.8 52.3 78.5

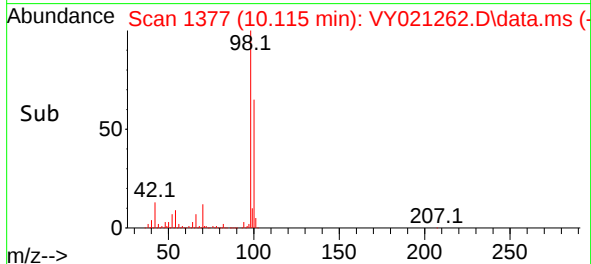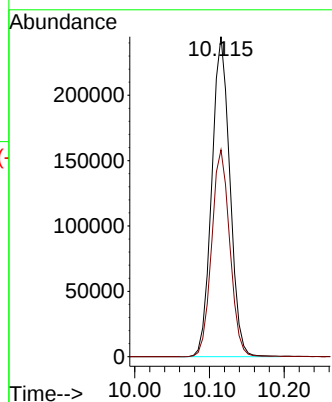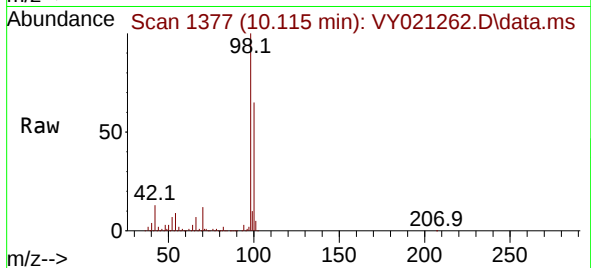

#62
4-Bromofluorobenzene
Concen: 49.109 ug/l
RT: 12.414 min Scan# 1754
Delta R.T. -0.000 min
Lab File: VY021262.D
Acq: 20 Feb 2025 20:13

Tgt Ion: 95 Resp: 132214
Ion Ratio Lower Upper
95 100
174 84.3 0.0 160.0
176 81.1 0.0 151.8

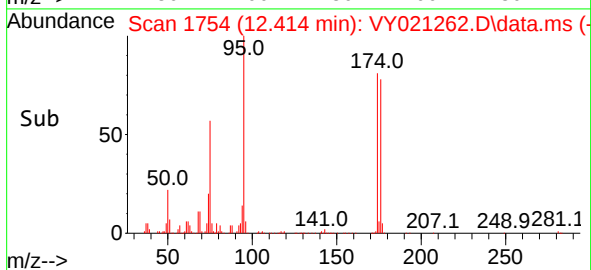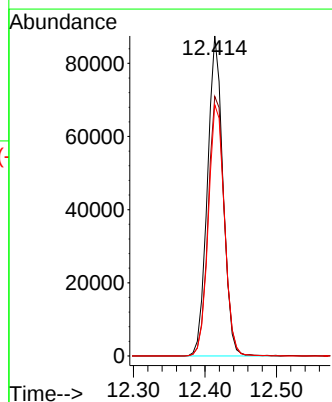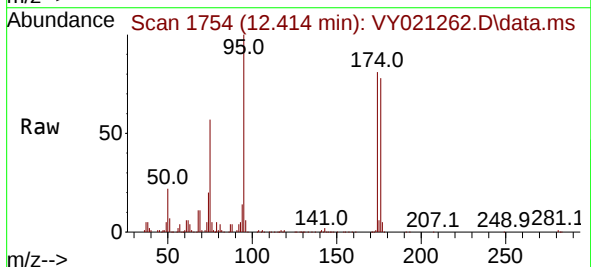

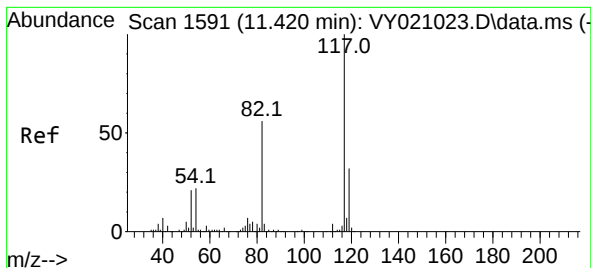

#63

Chlorobenzene-d5

Concen: 50.000 ug/l

RT: 11.426 min Scan# 11

Delta R.T. 0.006 min

Lab File: VY021262.D

Acq: 20 Feb 2025 20:13

Instrument :

MSVOA_Y

ClientSampleId :

OU4-PCS-TC-04-021725





Tgt Ion:117 Resp: 312885

Ion Ratio Lower Upper

117 100

82 55.9 43.8 65.8

119 32.0 26.5 39.7

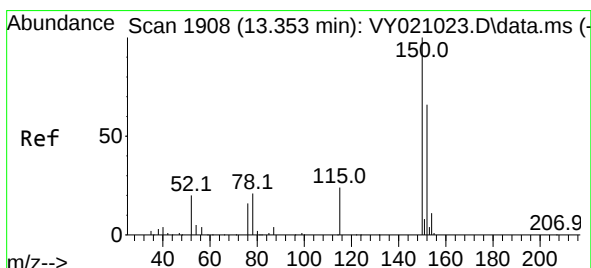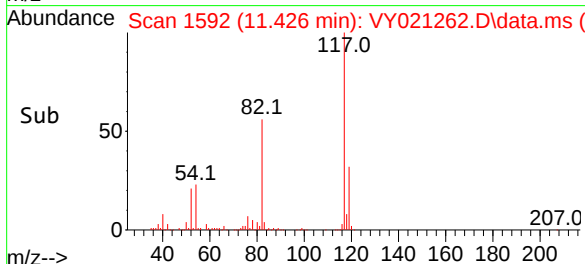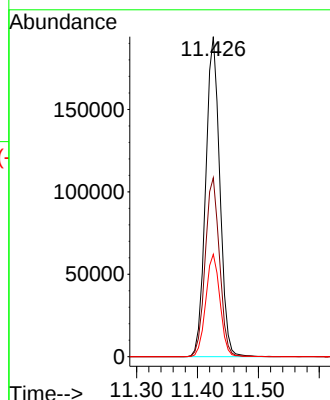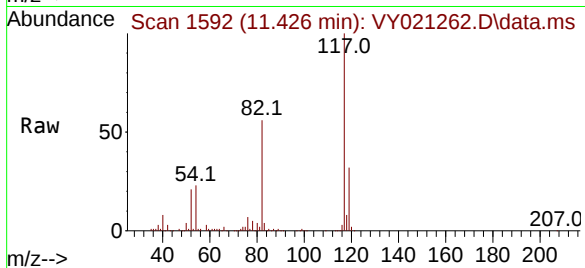

#72

1,4-Dichlorobenzene-d4

Concen: 50.000 ug/l

RT: 13.359 min Scan# 1909

Delta R.T. 0.006 min

Lab File: VY021262.D

Acq: 20 Feb 2025 20:13

Tgt Ion:152 Resp: 121569

Ion Ratio Lower Upper

152 100

115 59.0 30.0 90.0

150 158.7 0.0 344.6

